

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121319\
 Data File : PS008039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2019 10:52
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 17:34:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
12) T	2,4,5-T	7.403	7.205	71090183	66775721	7.681 16.407 #
15) T	Picloram	8.951	8.893	303.2E6	163.1E6	25.077 26.406
16) T	DCPA	0.000	8.835	0	7930290	N.D. 1.382



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121319\
Data File : PS008039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2019 10:52
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 17:34:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

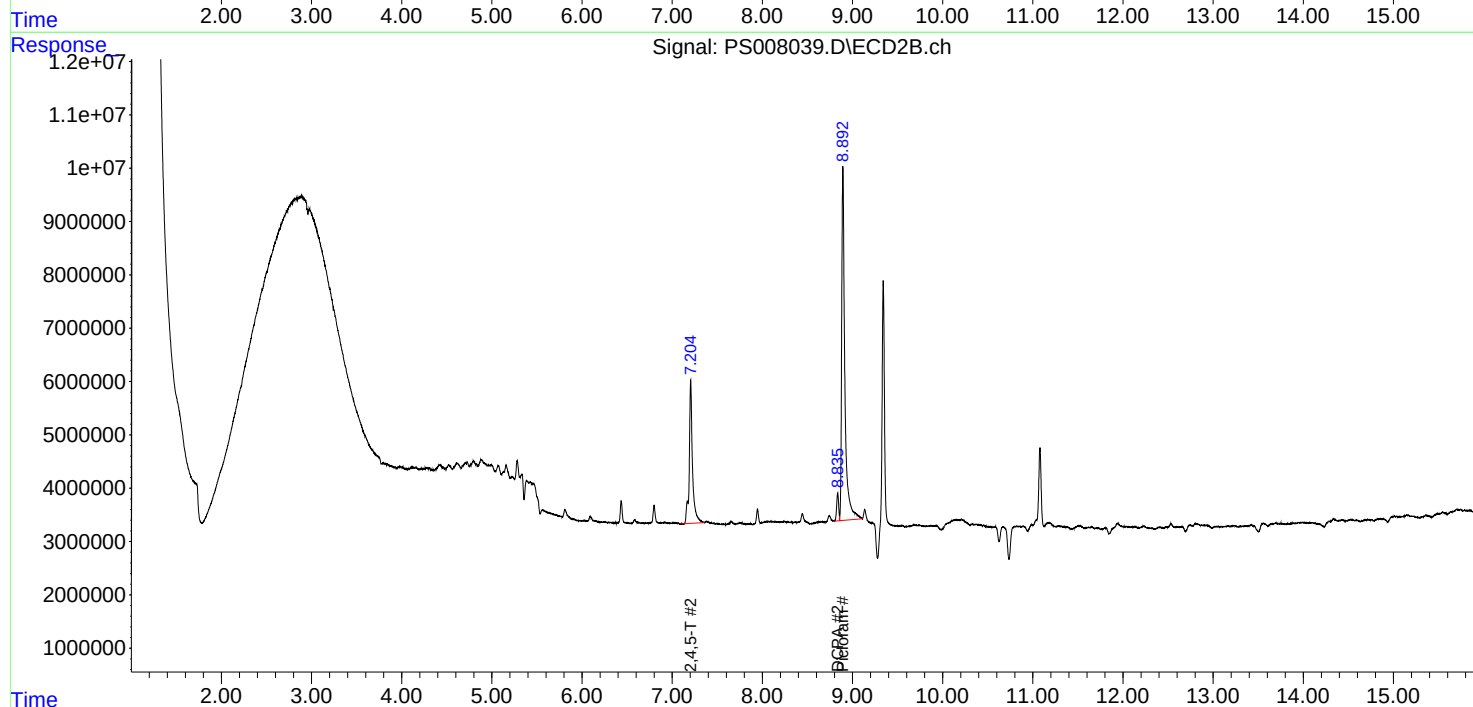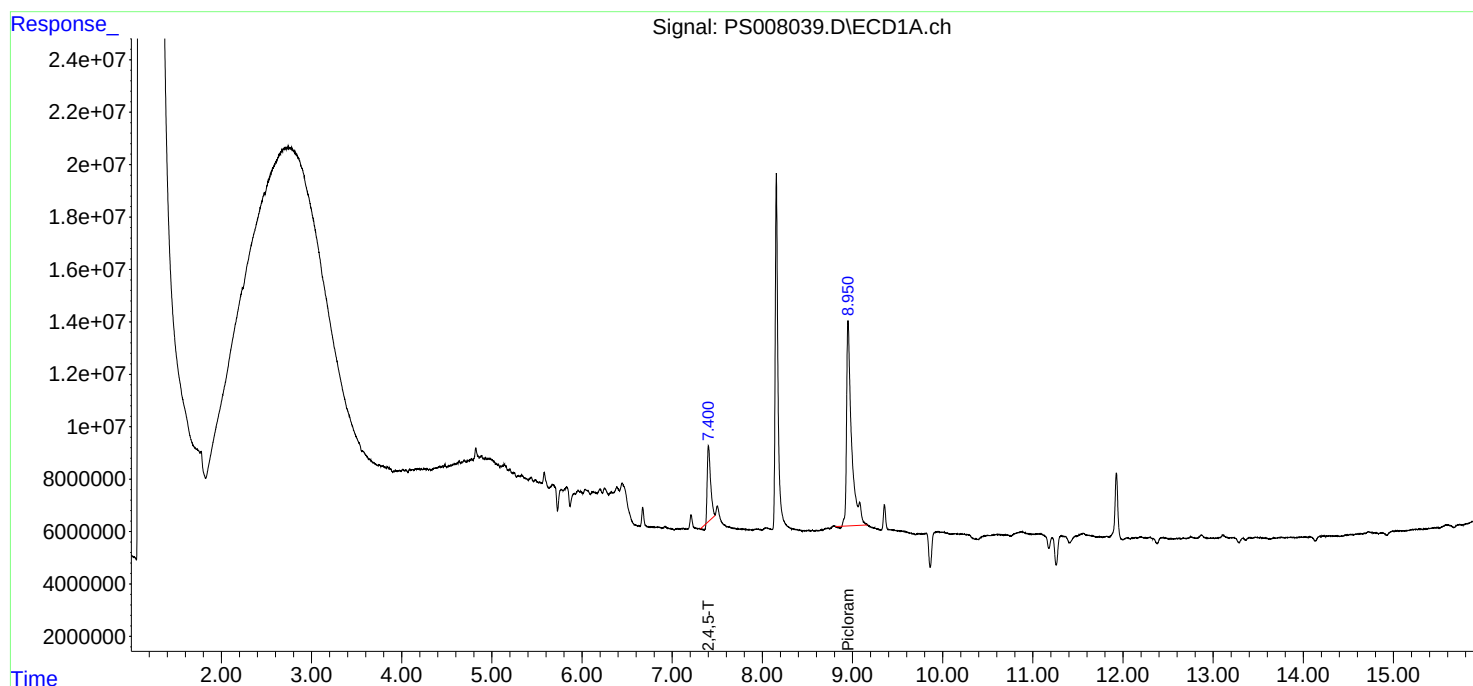


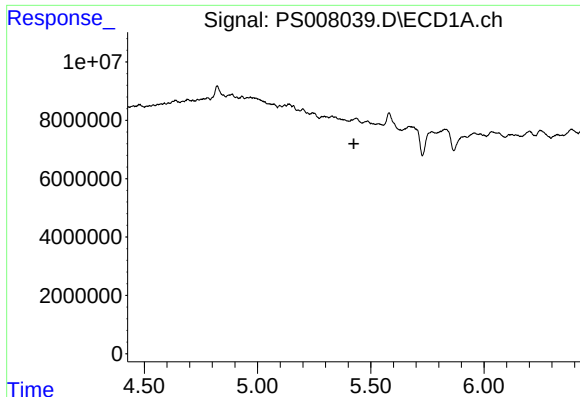

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.425 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

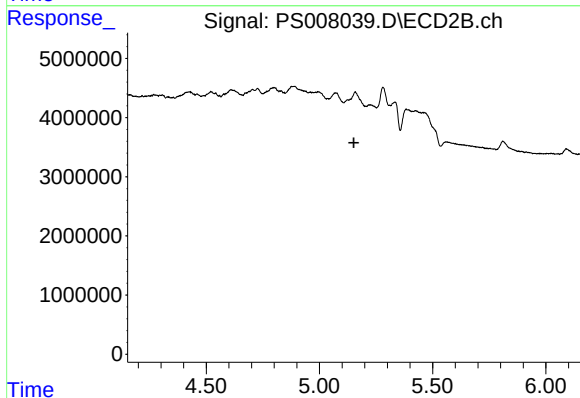


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.152 min
Response: 0
Conc: N.D.

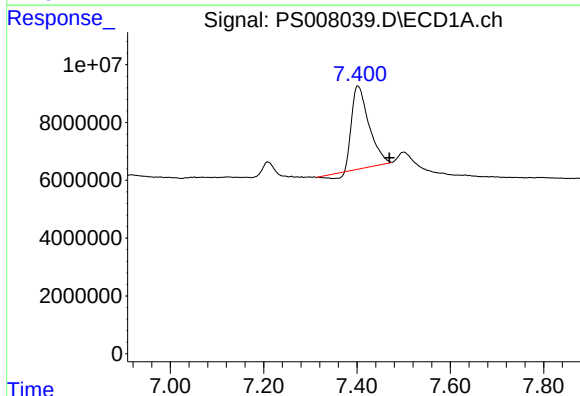


#12 2,4,5-T

R.T.: 7.403 min
Delta R.T.: -0.067 min
Response: 71090183
Conc: 7.68 ng/ml

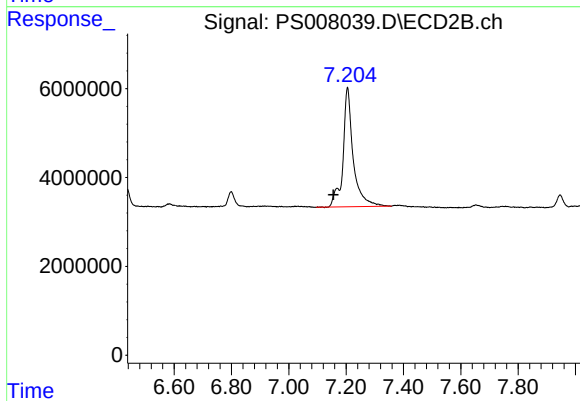

#12 2,4,5-T


R.T.: 7.205 min
Delta R.T.: 0.050 min
Response: 66775721
Conc: 16.41 ng/ml

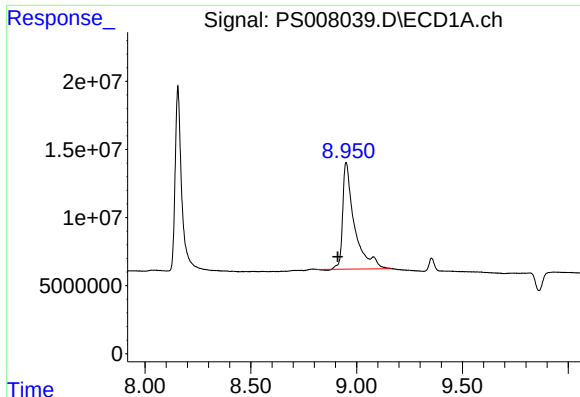

#15 Picloram


R.T.: 8.951 min
Delta R.T.: 0.041 min
Response: 303196917
Conc: 25.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

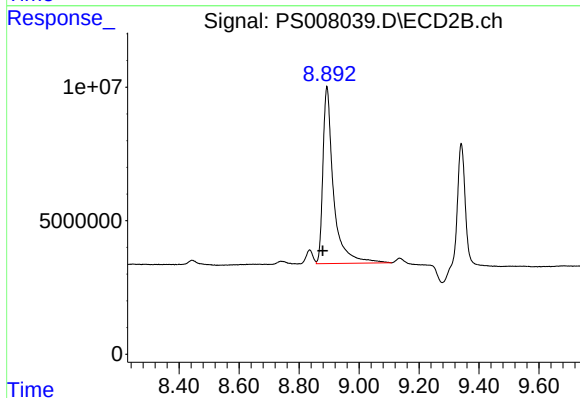


#15 Picloram

R.T.: 8.893 min
Delta R.T.: 0.014 min
Response: 163098235
Conc: 26.41 ng/ml

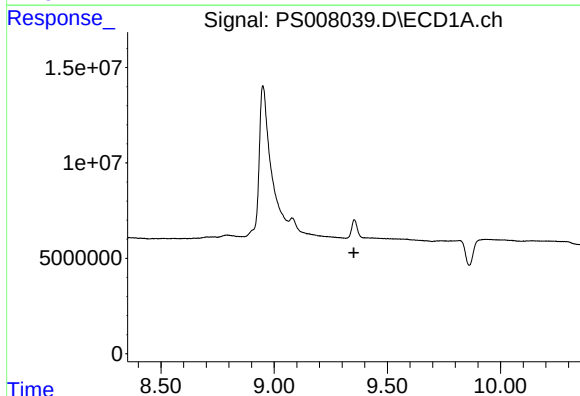

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.352 min
Response: 0
Conc: N.D.

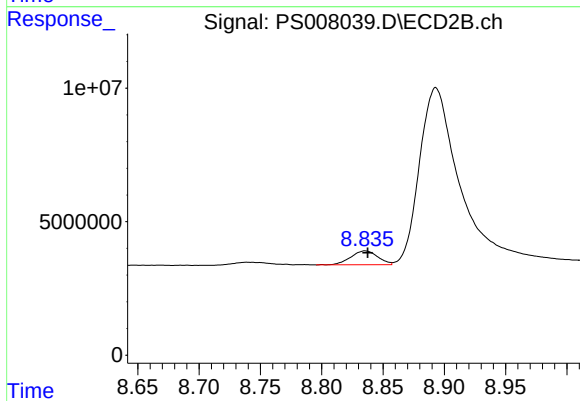

#16 DCPA

R.T.: 8.835 min
Delta R.T.: -0.002 min
Response: 7930290
Conc: 1.38 ng/ml