

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121322\
 Data File : PS021440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2022 08:30
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 20:40:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.387	0.000	809473	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.518	0.000	766267	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.757	0.000	665610	0	<MDL	N.D. #
3) T	4-Nitroph...	6.221	0.000	1448428	0	<MDL	N.D. #
5) T	DICAMBA	6.527	6.983	963320	1351703	<MDL	<MDL #
6) T	MCPD	6.732f	0.000	3281400	0	<MDL	N.D. #
7) T	MCPA	6.834	0.000	485331	0	<MDL	N.D. #
8) T	DICHLORPROP	7.113	7.627	485982	2284036	<MDL	1.160 #
9) T	2,4-D	7.321	7.903	1107735	672614	<MDL	<MDL #
10) T	Pentachlo...	7.556	8.317	2510065	1902682	<MDL	<MDL #
11) T	2,4,5-TP ...	8.086	8.680	3039400	1284297	<MDL	<MDL #
12) T	2,4,5-T	8.360	9.067	6957849	2568988	<MDL	<MDL #
13) T	2,4-DB	8.873	9.586	988325	824561	<MDL	<MDL #
14) T	DINOSEB	9.905	9.893	7664118	636250	<MDL	<MDL #
15) T	Picloram	9.774	10.876	123.2E6	75048132	4.301	4.615
16) T	DCPA	10.175	10.817	1392117	10505380	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121322\
Data File : PS021440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2022 08:30
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 20:40:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

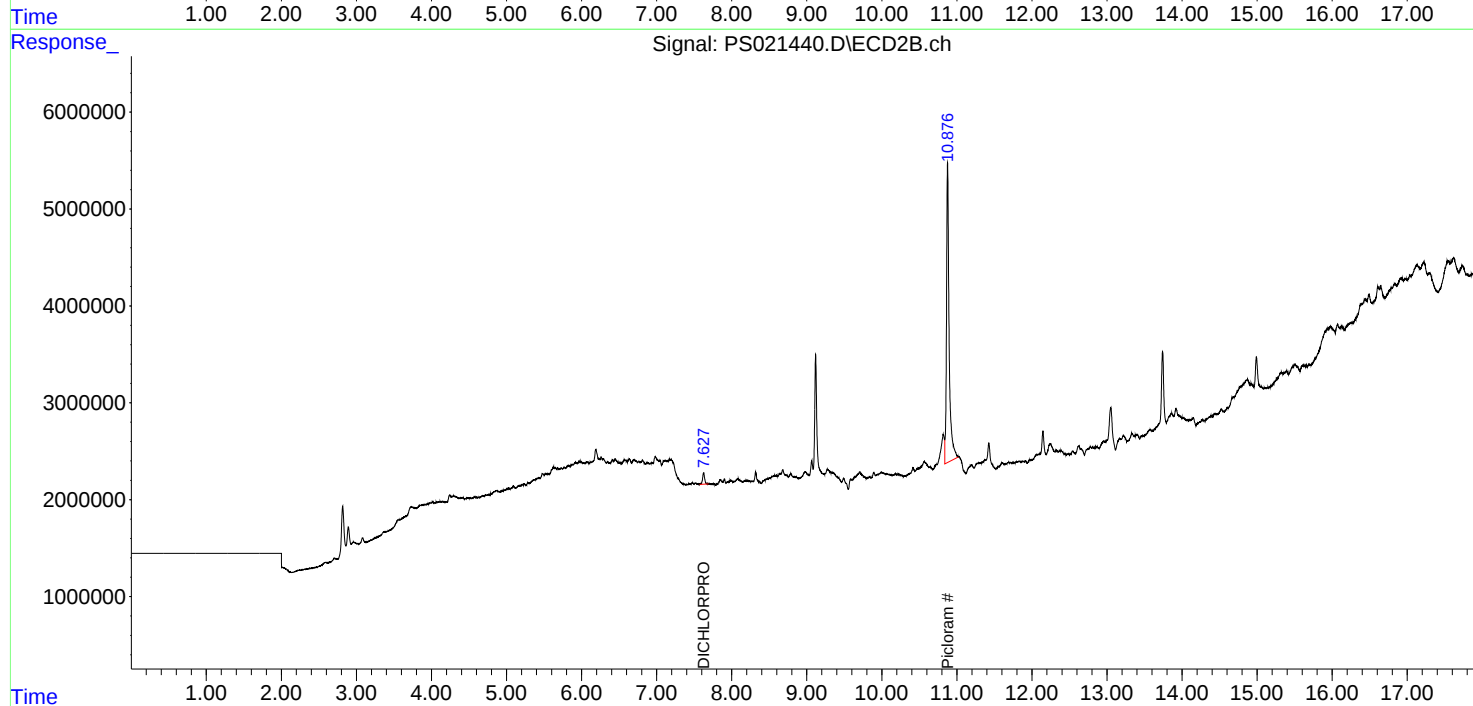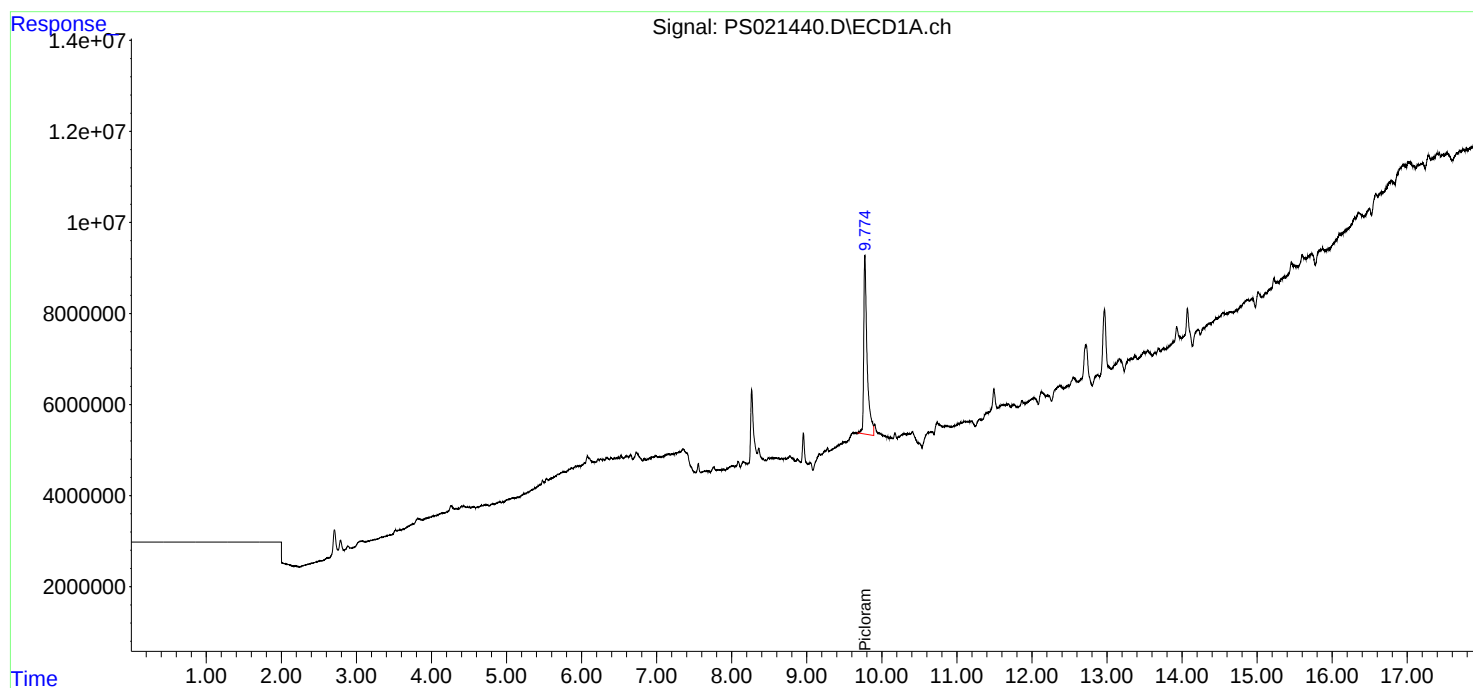


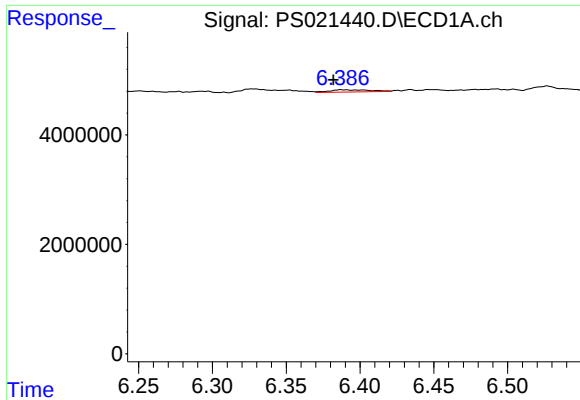

#4 2,4-DCAA


R.T.: 6.387 min
Delta R.T.: 0.005 min
Response: 809473
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

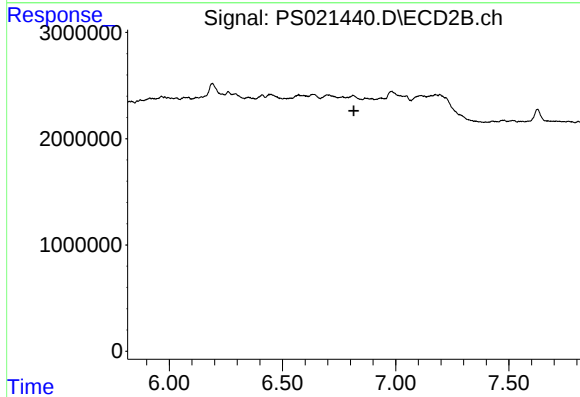


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

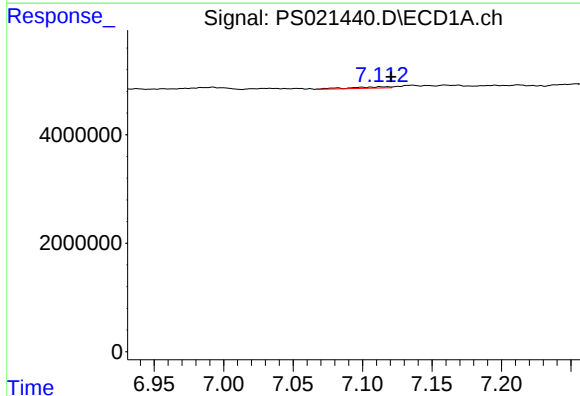


#8 DICHLORPROP

R.T.: 7.113 min
Delta R.T.: -0.007 min
Response: 485982
Conc: N.D.

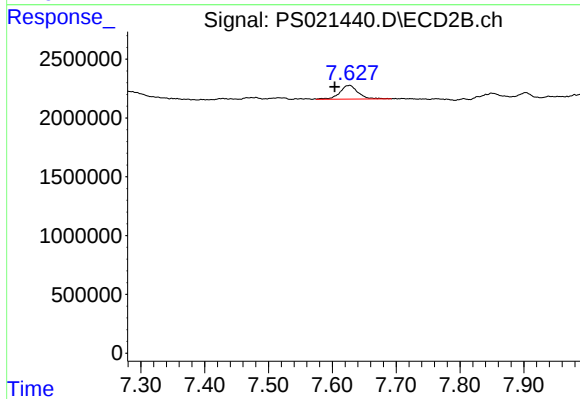

#8 DICHLORPROP


R.T.: 7.627 min
Delta R.T.: 0.023 min
Response: 2284036
Conc: 1.16 ng/ml

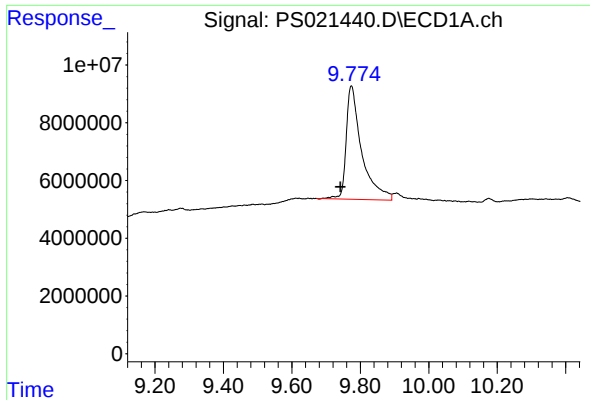

#15 Picloram

R.T.: 9.774 min
Delta R.T.: 0.032 min
Response: 123176867
Conc: 4.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

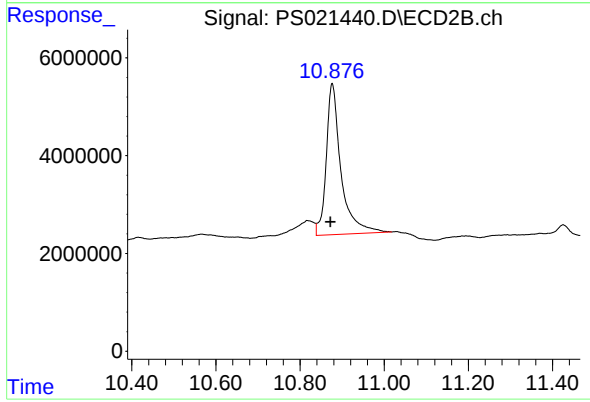

#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.004 min
Response: 75048132
Conc: 4.62 ng/ml