

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121322\
 Data File : PS021441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2022 08:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 20:41:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.380	6.811	1321.2E6	925.7E6	454.712	536.973
Target Compounds							
1) T	Dalapon	2.526f	0.000	693428	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.732	0.000	8799652	0	2.214	N.D. #
3) T	4-Nitroph...	6.228	0.000	5440916	0	3.026	N.D. #
6) T	MCP	0.000	7.124f	0	3660550	N.D.	<MDL
7) T	MCPA	6.763	7.216f	1206054	29205682	<MDL	3.303 #
8) T	DICHLORPROP	0.000	7.647f	0	2169249	N.D.	1.101
10) T	Pentachlo...	7.551	0.000	825062	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.089	0.000	9234959	0	<MDL	N.D. #
12) T	2,4,5-T	8.319	9.086	20554810	1863510	1.089	<MDL #
13) T	2,4-DB	8.844	9.505f	2898536	3114447	<MDL	2.167 #
15) T	Picloram	9.739	10.908	4037520	37150742	<MDL	2.285 #
16) T	DCPA	10.167	10.821	1352855	619451	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121322\
Data File : PS021441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2022 08:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 20:41:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

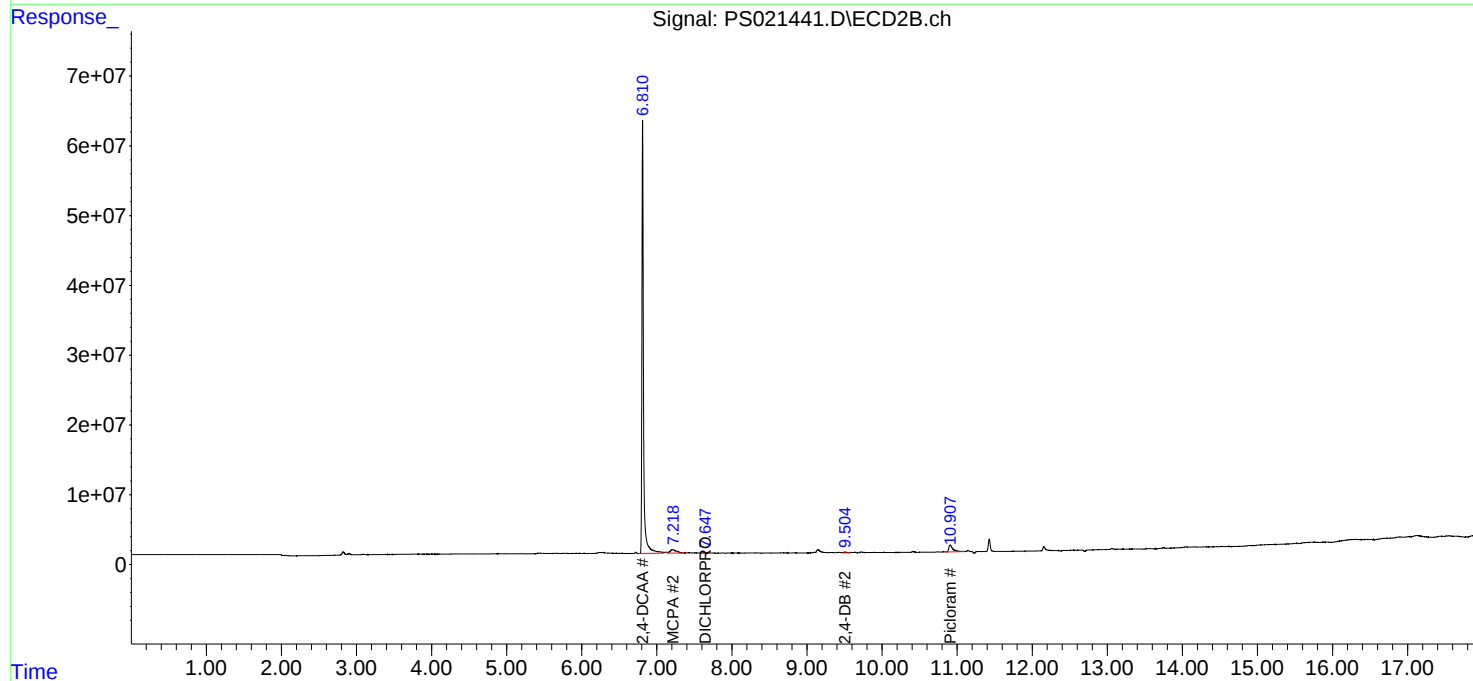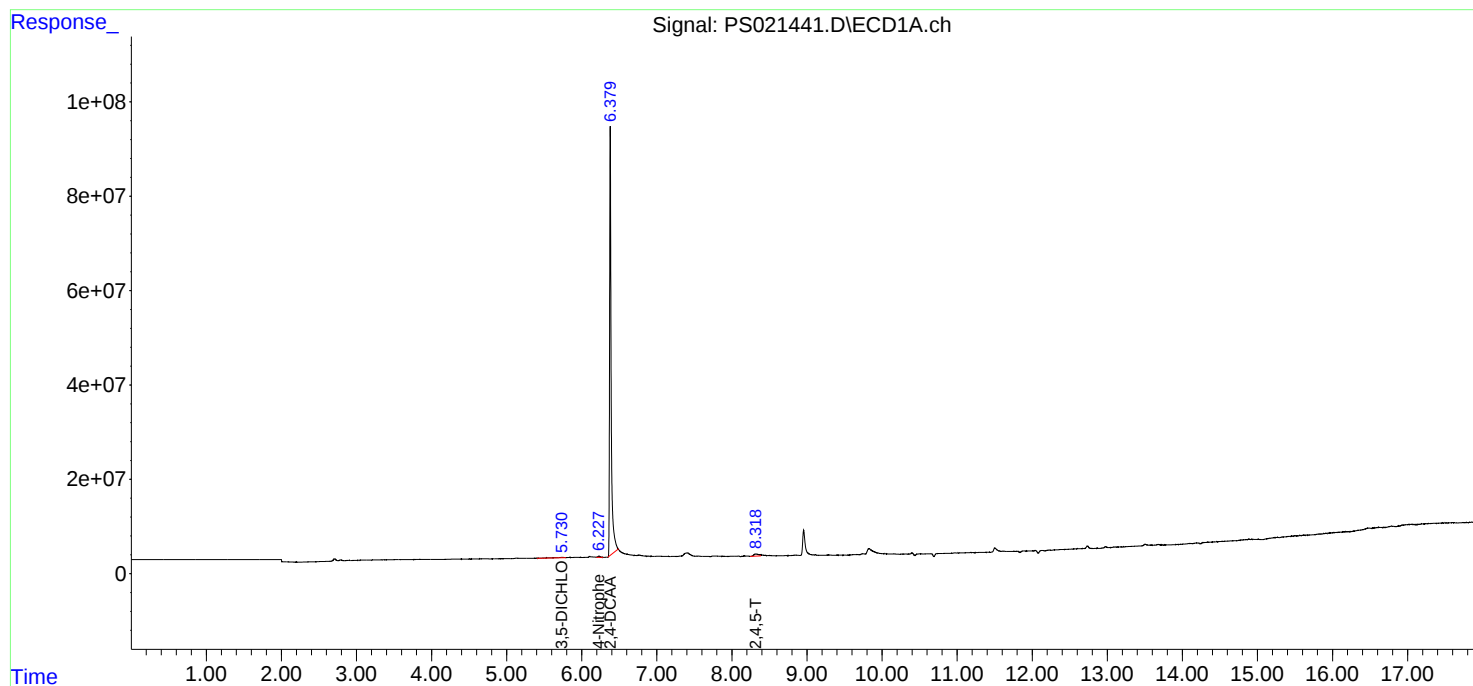


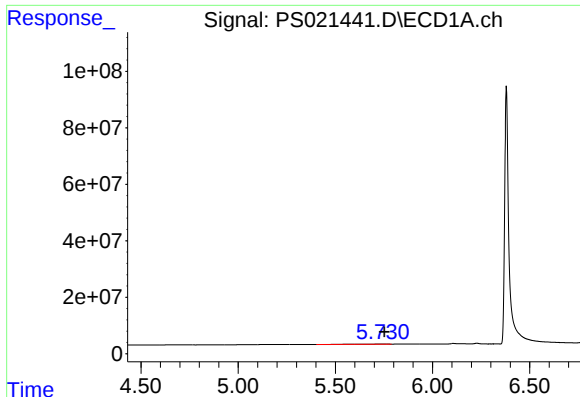

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.732 min
Delta R.T.: -0.021 min
Response: 8799652
Conc: 2.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

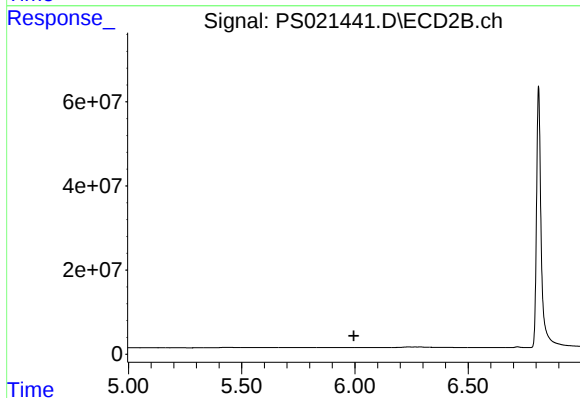


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

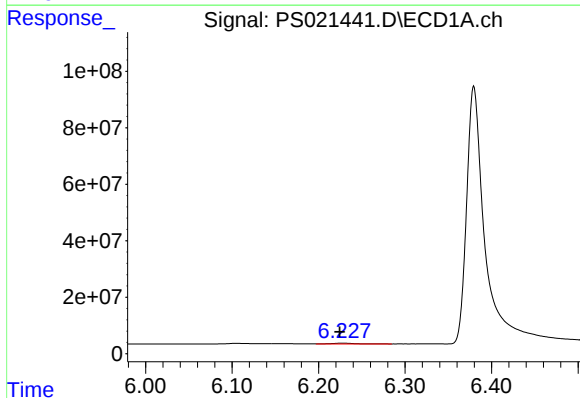


#3 4-Nitrophenol

R.T.: 6.228 min
Delta R.T.: 0.004 min
Response: 5440916
Conc: 3.03 ng/ml

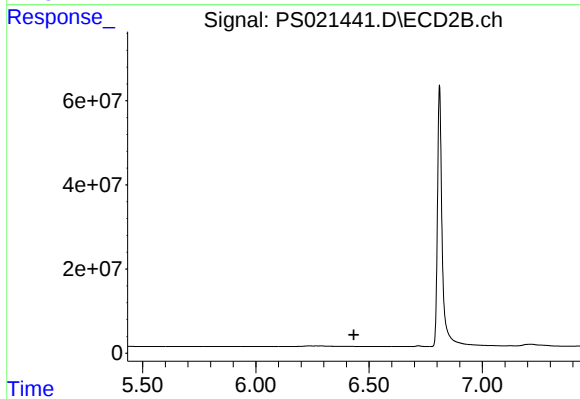

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

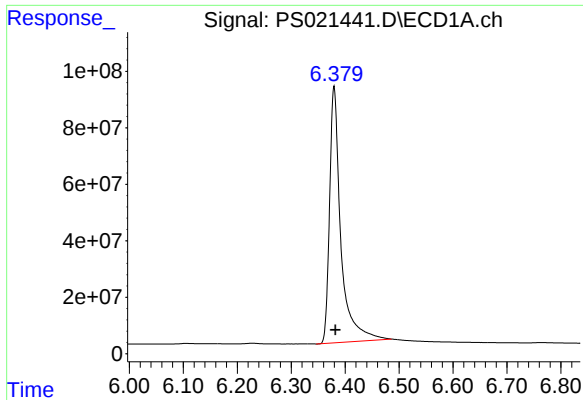

#4 2,4-DCAA


R.T.: 6.380 min
Delta R.T.: -0.002 min
Response: 1321162627
Conc: 454.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

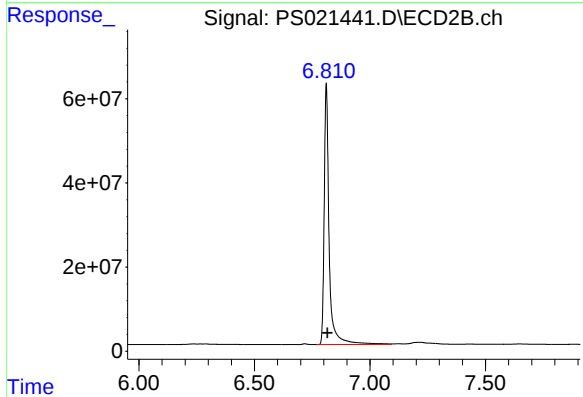


#4 2,4-DCAA

R.T.: 6.811 min
Delta R.T.: -0.005 min
Response: 925738347
Conc: 536.97 ng/ml

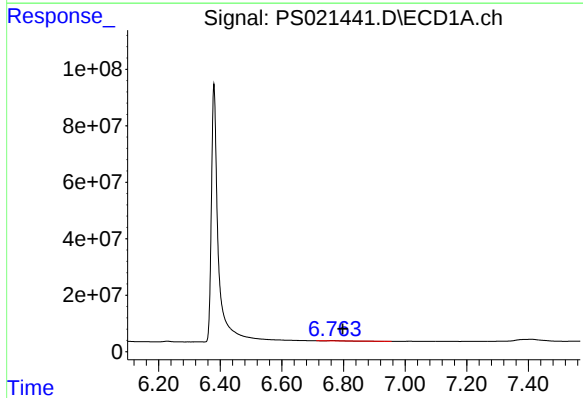


#7 MCPA

R.T.: 6.763 min
Delta R.T.: -0.035 min
Response: 1206054
Conc: N.D.

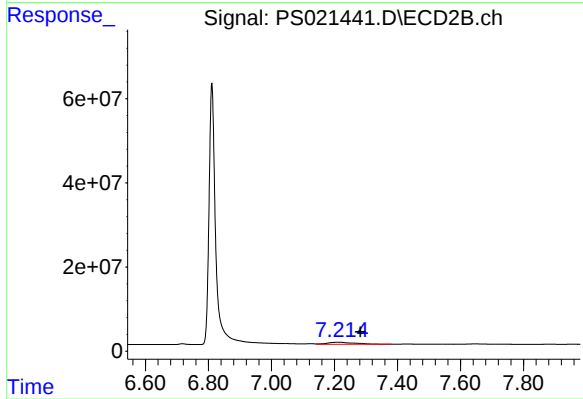

#7 MCPA


R.T.: 7.216 min
Delta R.T.: -0.066 min
Response: 29205682
Conc: 3.30 ug/ml

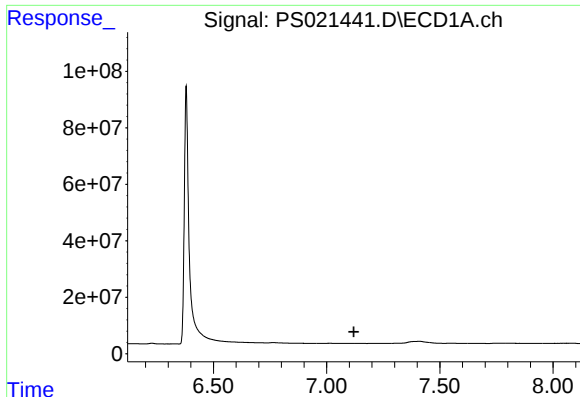

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

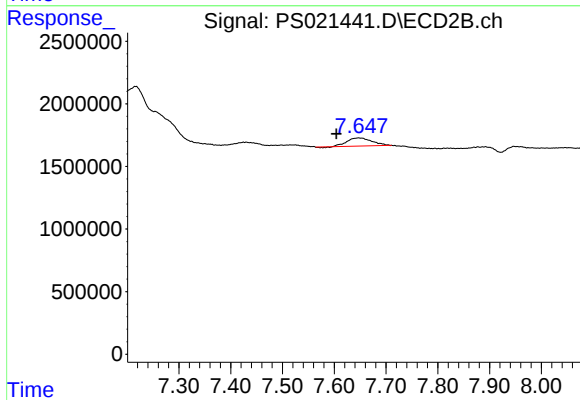


#8 DICHLORPROP

R.T.: 7.647 min
Delta R.T.: 0.043 min
Response: 2169249
Conc: 1.10 ng/ml

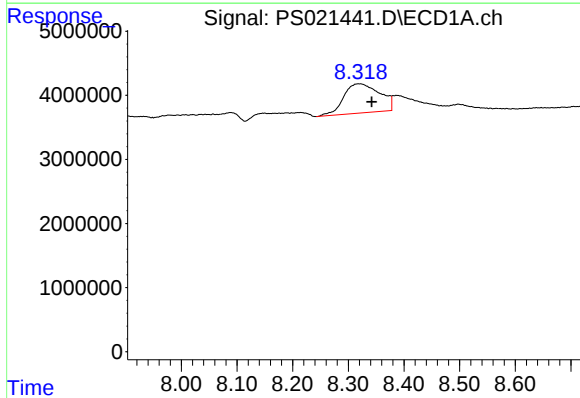


#12 2,4,5-T

R.T.: 8.319 min
Delta R.T.: -0.023 min
Response: 20554810
Conc: 1.09 ng/ml

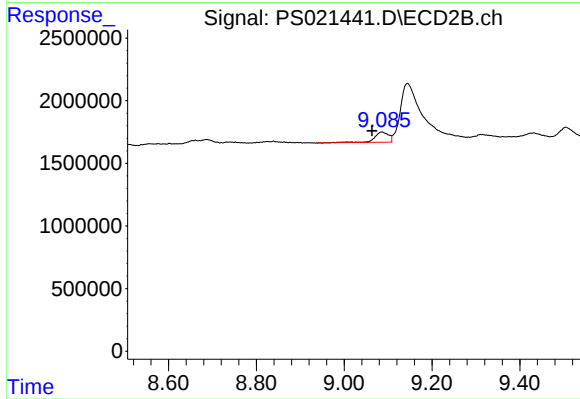

#12 2,4,5-T


R.T.: 9.086 min
Delta R.T.: 0.022 min
Response: 1863510
Conc: N.D.

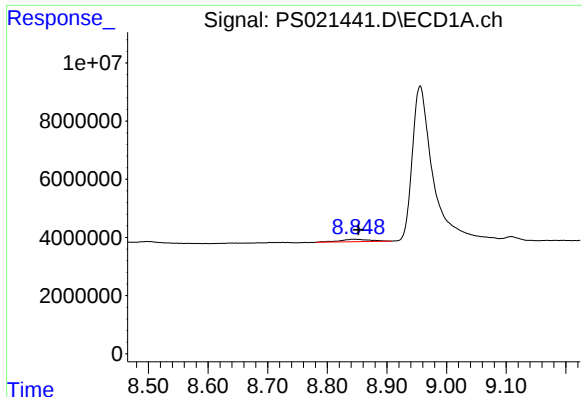

#13 2,4-DB


R.T.: 8.844 min
Delta R.T.: -0.008 min
Response: 2898536
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

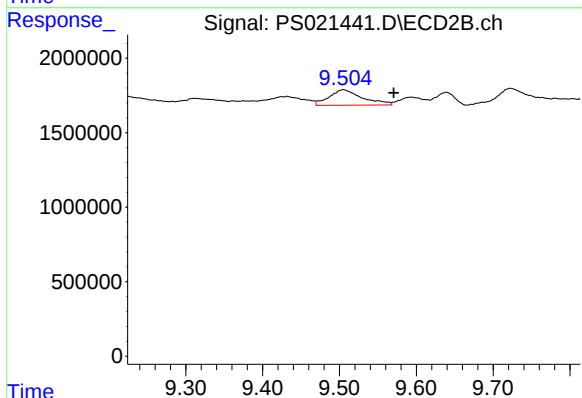


#13 2,4-DB

R.T.: 9.505 min
Delta R.T.: -0.066 min
Response: 3114447
Conc: 2.17 ng/ml

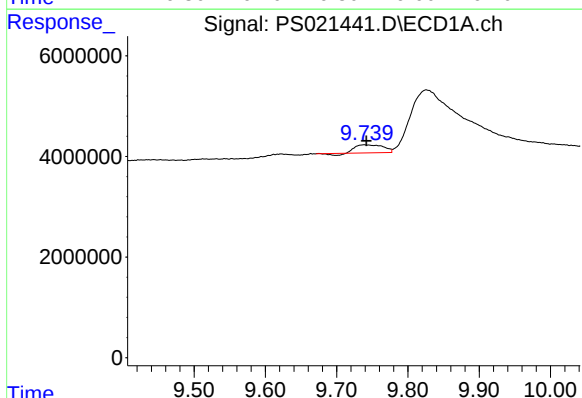

#15 Picloram

R.T.: 9.739 min
Delta R.T.: -0.003 min
Response: 4037520
Conc: N.D.

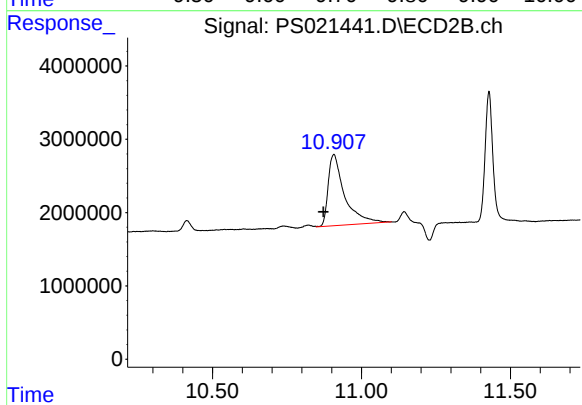

#15 Picloram

R.T.: 10.908 min
Delta R.T.: 0.036 min
Response: 37150742
Conc: 2.28 ng/ml