

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS121420\  
 Data File : PS013479.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Dec 2020 08:46  
 Operator : DD\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 14 10:41:53 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS120220.M  
 Quant Title : 8080.M  
 QLast Update : Thu Dec 03 02:59:27 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |       |         |           |        |
|------------------|--------------|--------|-------|---------|-----------|--------|
| 2) T             | 3,5-DICHL... | 6.470f | 0.000 | 304.5E6 | 0 237.551 | N.D. # |
| 15) T            | Picloram     | 10.971 | 0.000 | 106.5E6 | 0 15.462  | N.D. # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS121420\  
Data File : PS013479.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Dec 2020 08:46  
Operator : DD\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 14 10:41:53 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS120220.M  
Quant Title : 8080.M  
QLast Update : Thu Dec 03 02:59:27 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

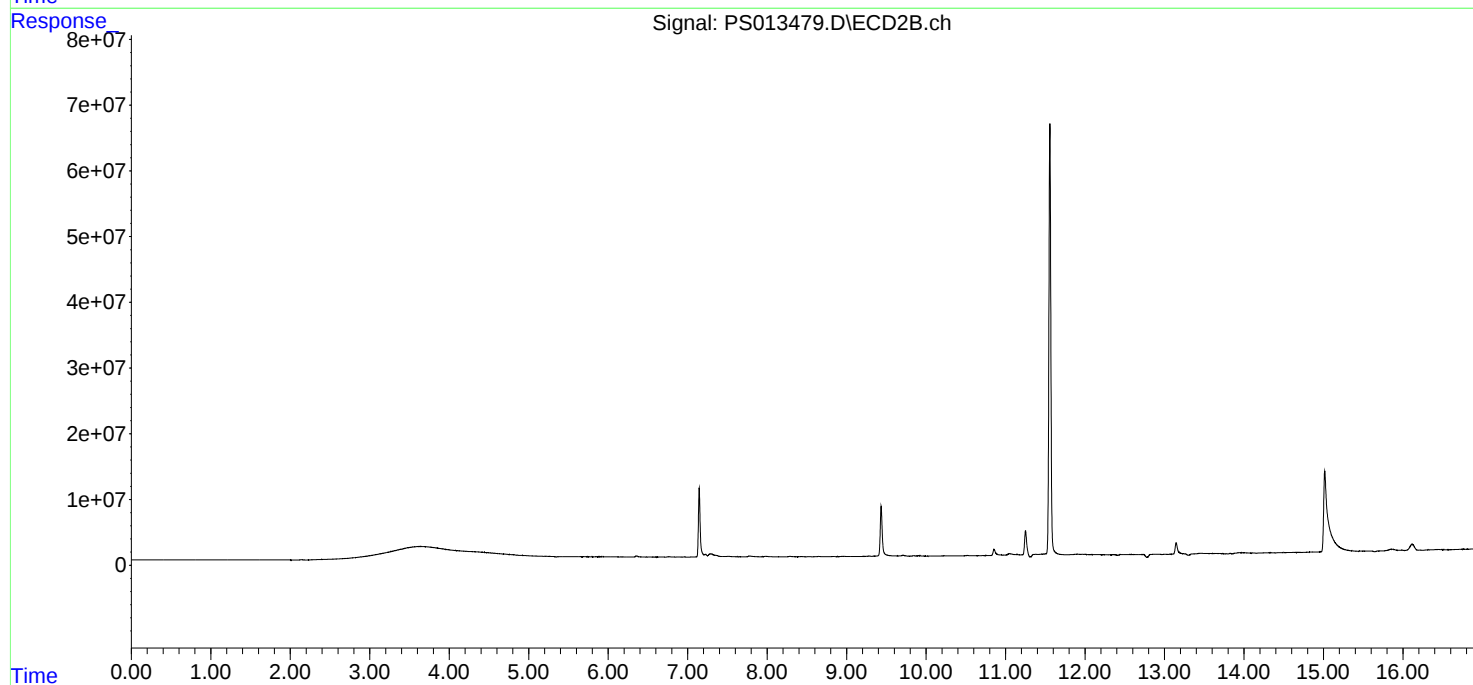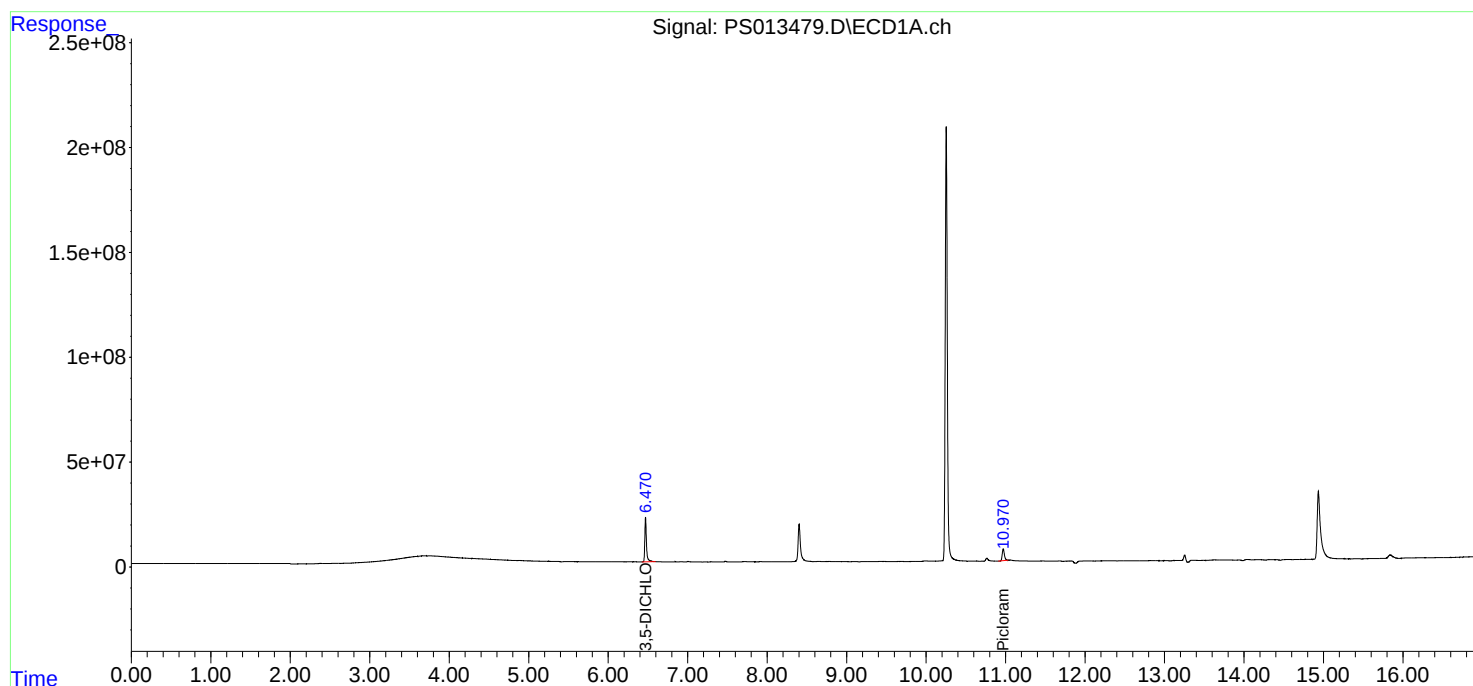


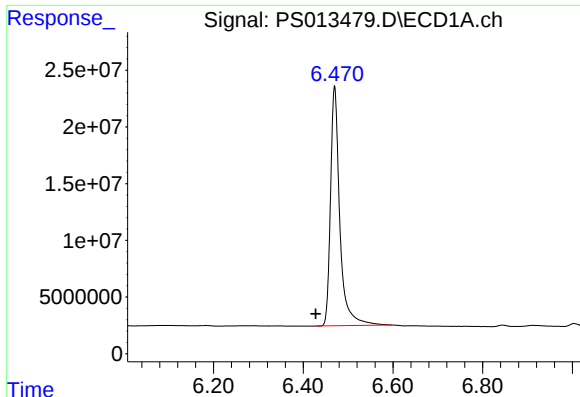

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.470 min  
Delta R.T.: 0.042 min  
Response: 304470762  
Conc: 237.55 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

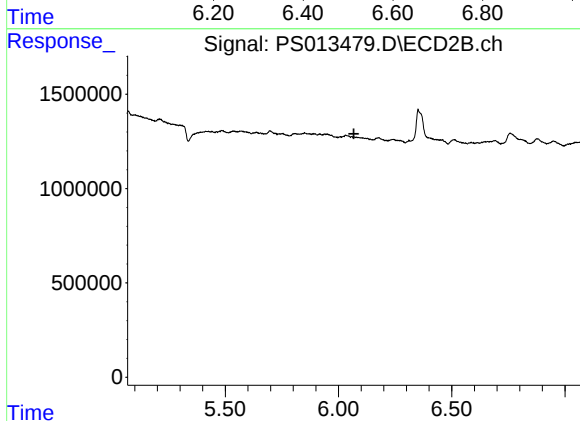


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 6.068 min  
Response: 0  
Conc: N.D.

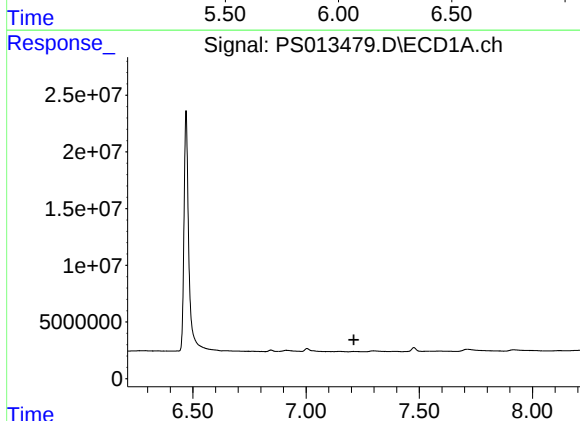


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 7.211 min  
Response: 0  
Conc: N.D.

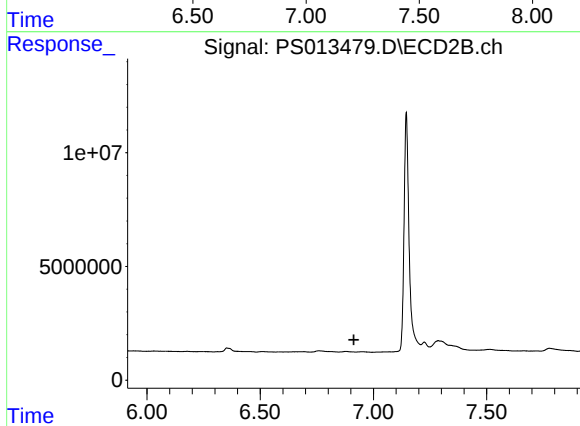

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T. : 6.914 min  
Response: 0  
Conc: N.D.

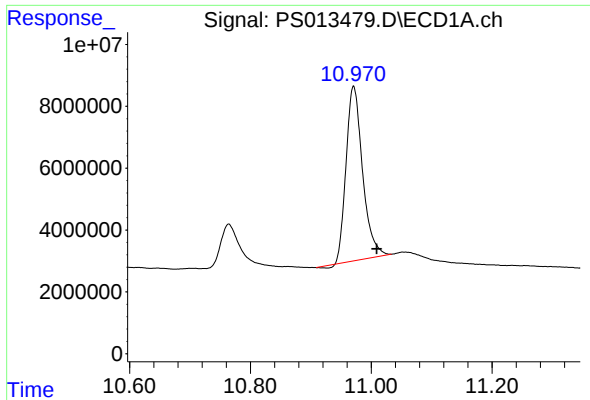

#15 Picloram

R.T.: 10.971 min  
Delta R.T.: -0.038 min  
Response: 106504530  
Conc: 15.46 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

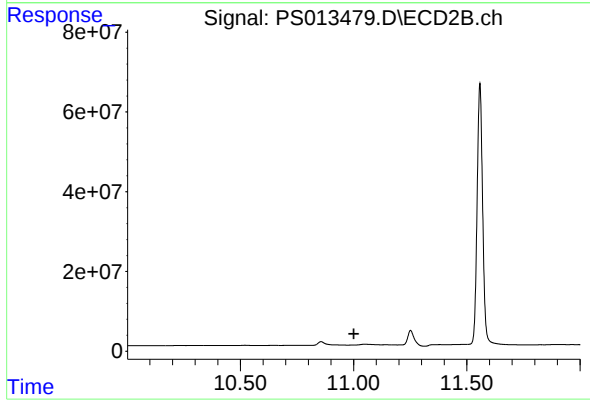

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 11.001 min  
Response: 0  
Conc: N.D.