

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121420\
 Data File : PS013501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2020 18:05
 Operator : DD\AJ
 Sample : L5043-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 KENS-SS2-121020-0-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:04:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	6.915	274.9E6	128.0E6	295.297	325.399
Target Compounds							
1) T	Dalapon	2.993	2.586	61246779	30409403	57.016	57.864
2) T	3,5-DICHL...	0.000	6.096	0	28689318	N.D.	46.171
3) T	4-Nitroph...	6.986f	6.541	14843223	3458699	32.943	14.511 #
5) T	DICAMBA	0.000	7.049	0	6274856	N.D.	3.734
6) T	MCP	7.563	0.000	7576480	0	2.790	N.D. #
7) T	MCPA	7.756	7.371	32110867	26601799	8.215	12.792 #
8) T	DICHLORPROP	0.000	7.744	0	5394847	N.D.	12.071
10) T	Pentachlo...	8.684f	0.000	21782403	0	1.625	N.D. #
11) T	2,4,5-TP ...	0.000	8.762	0	20126880	N.D.	8.573
12) T	2,4,5-T	9.401f	0.000	35138585	0	6.355	N.D. #
14) T	DINOSEB	11.150	0.000	18334038	0	4.326	N.D. #
16) T	DCPA	0.000	10.924	0	6659451	N.D.	2.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121420\
Data File : PS013501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2020 18:05
Operator : DD\AJ
Sample : L5043-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:04:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

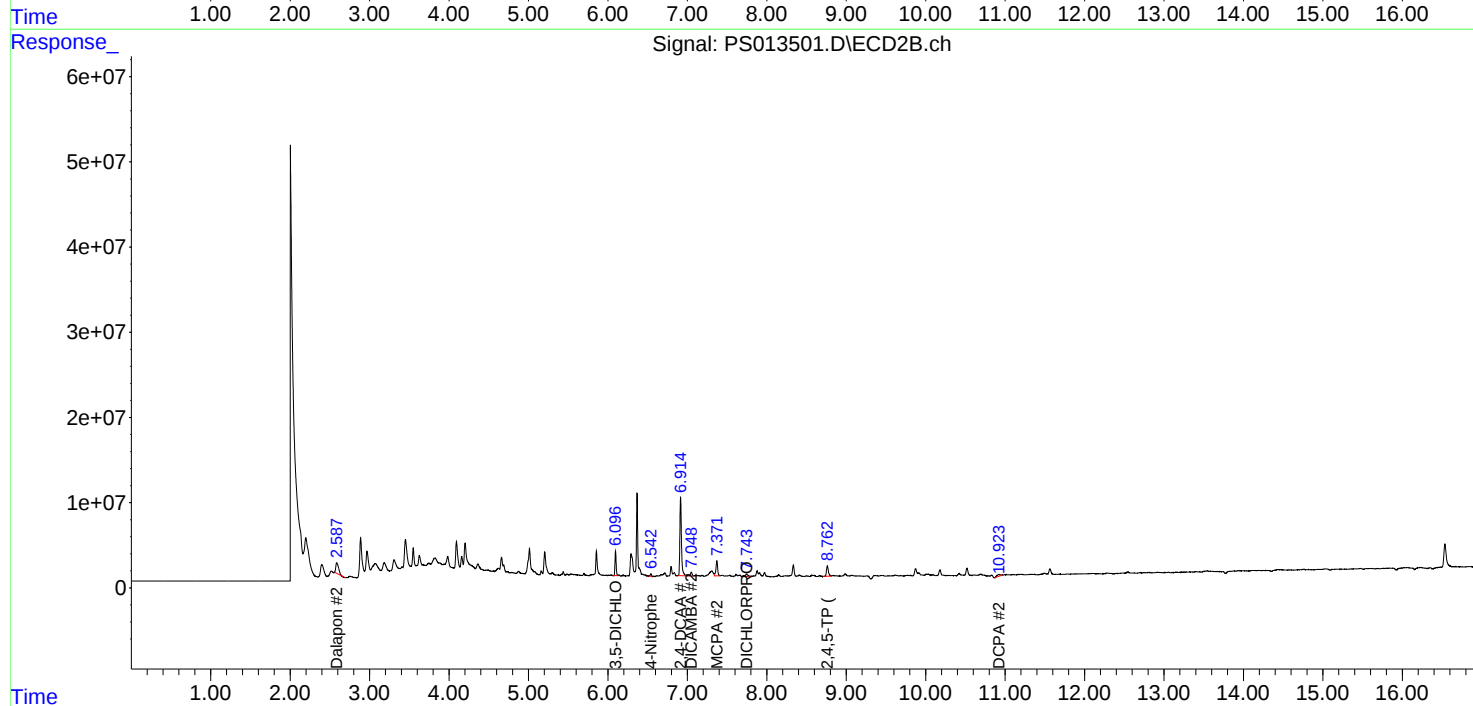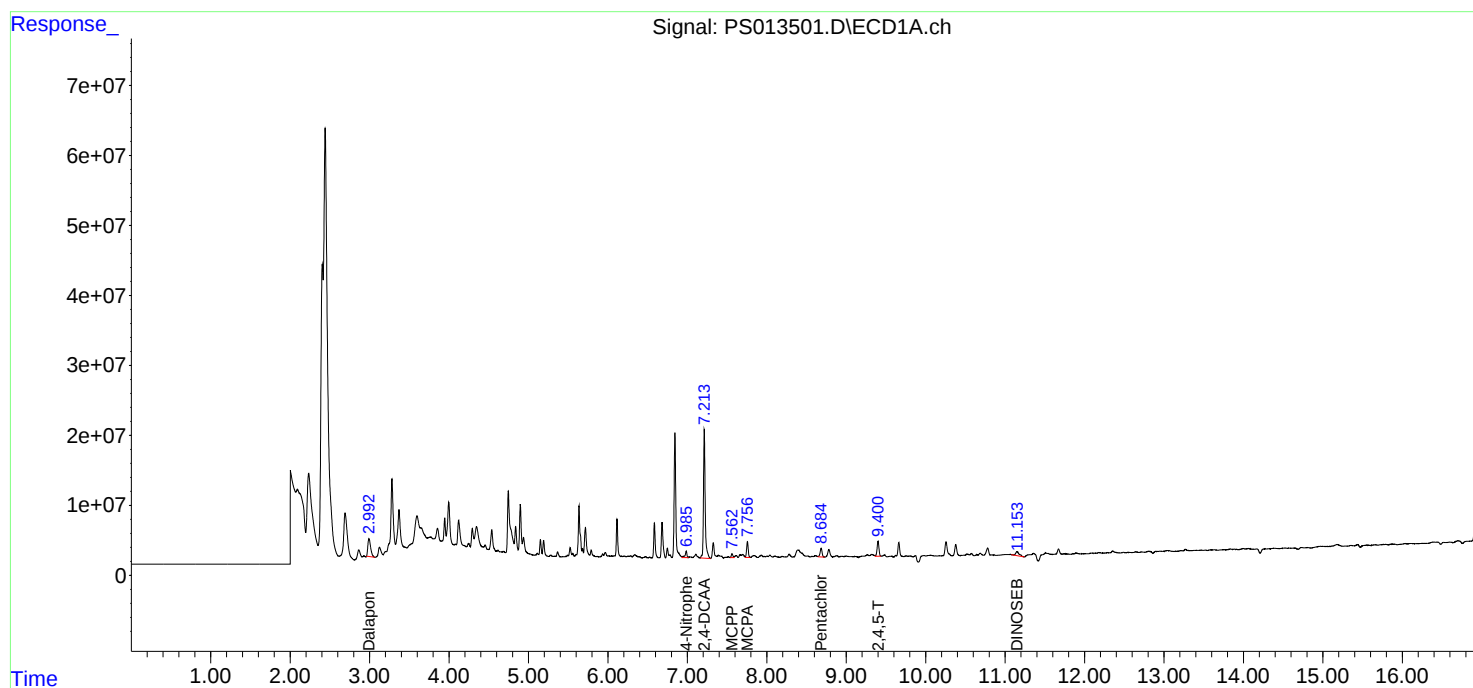


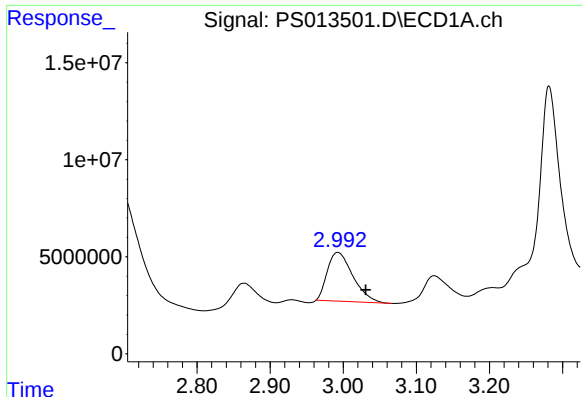

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.038 min
Response: 61246779
Conc: 57.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

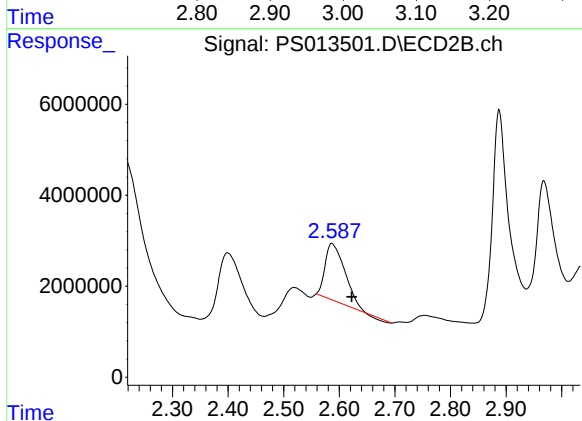


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 30409403
Conc: 57.86 ng/ml

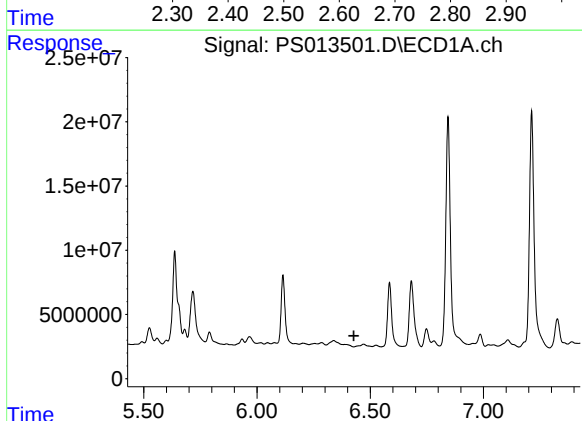


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

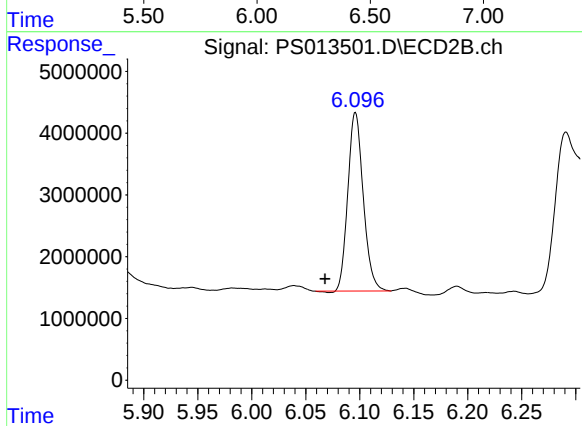

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.028 min
Response: 28689318
Conc: 46.17 ng/ml

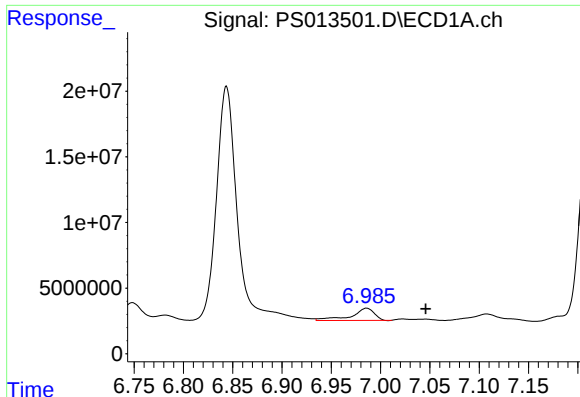

#3 4-Nitrophenol


R.T.: 6.986 min
Delta R.T.: -0.060 min
Response: 14843223
Conc: 32.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

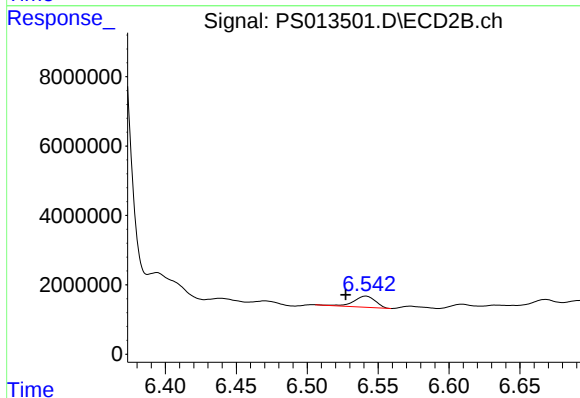


#3 4-Nitrophenol

R.T.: 6.541 min
Delta R.T.: 0.014 min
Response: 3458699
Conc: 14.51 ng/ml

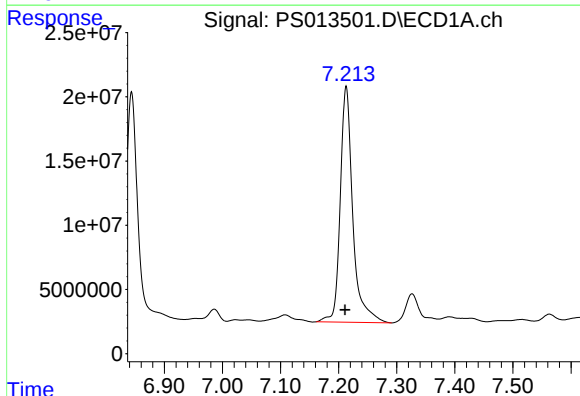


#4 2,4-DCAA

R.T.: 7.213 min
Delta R.T.: 0.002 min
Response: 274938632
Conc: 295.30 ng/ml

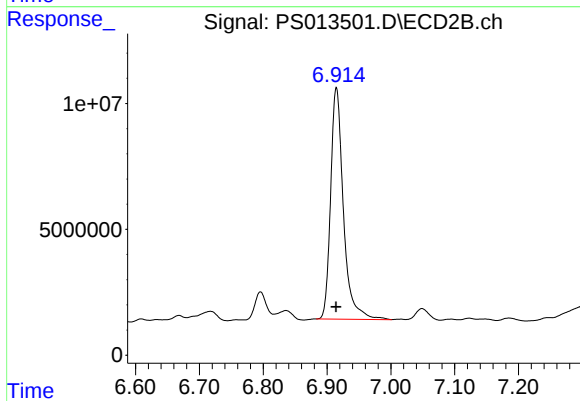

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 127999571
Conc: 325.40 ng/ml

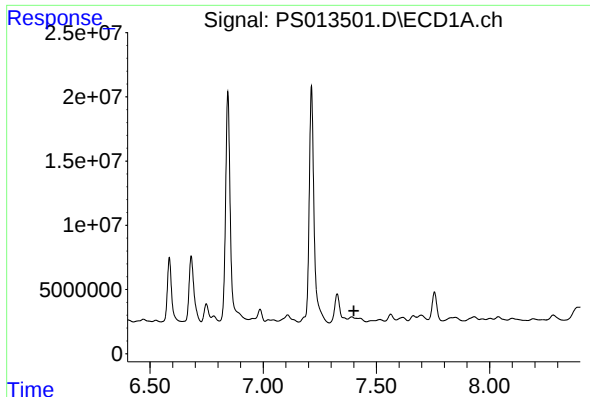

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.401 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

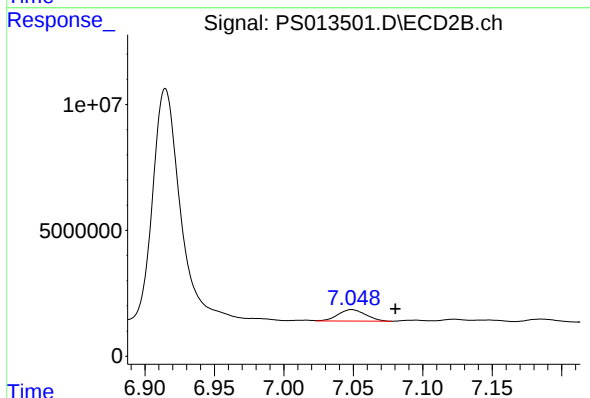


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.031 min
Response: 6274856
Conc: 3.73 ng/ml

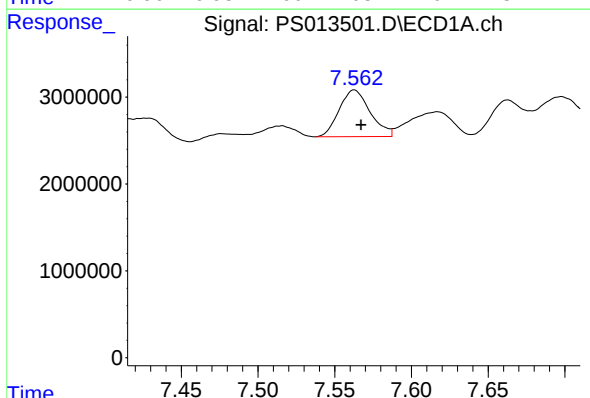


#6 MCP

R.T.: 7.563 min
Delta R.T.: -0.004 min
Response: 7576480
Conc: 2.79 ug/ml

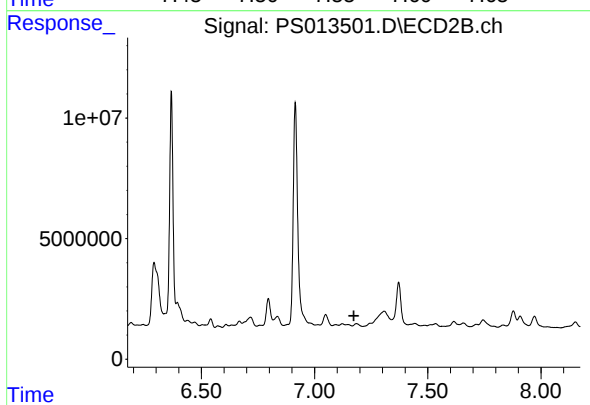

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.174 min
Response: 0
Conc: N.D.

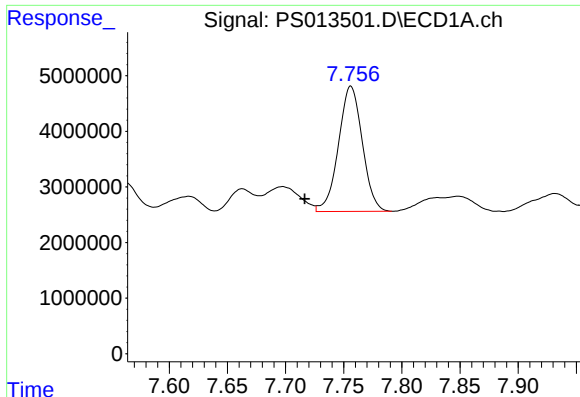

#7 MCPA


R.T.: 7.756 min
Delta R.T.: 0.040 min
Response: 32110867
Conc: 8.22 ug/ml

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

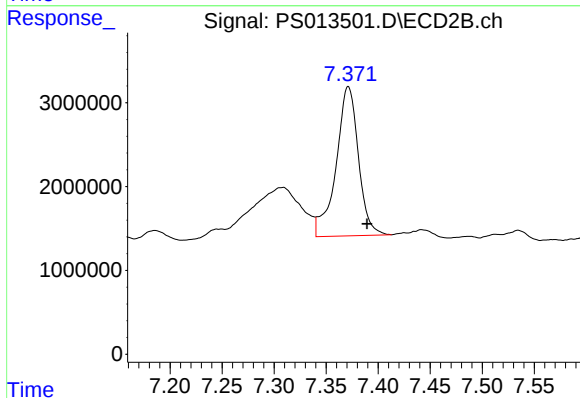


#7 MCPA

R.T.: 7.371 min
Delta R.T.: -0.018 min
Response: 26601799
Conc: 12.79 ug/ml

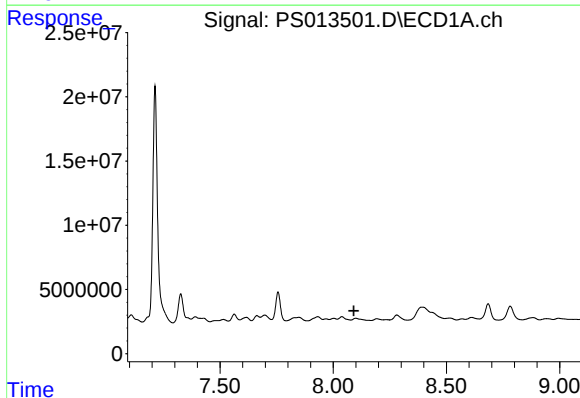


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

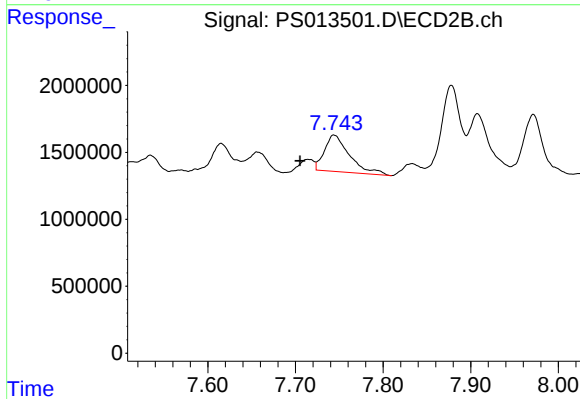

#8 DICHLORPROP


R.T.: 7.744 min
Delta R.T.: 0.039 min
Response: 5394847
Conc: 12.07 ng/ml

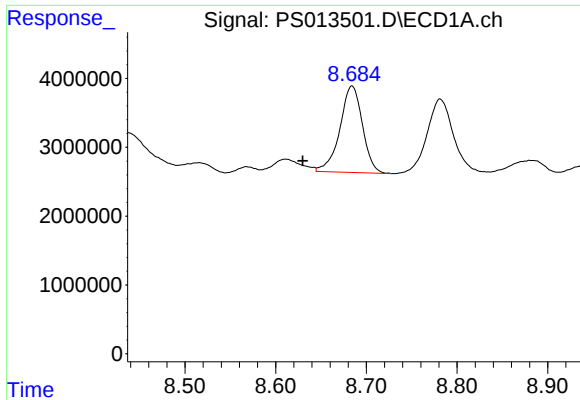

#10 Pentachlorophenol


R.T.: 8.684 min
Delta R.T.: 0.054 min
Response: 21782403
Conc: 1.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

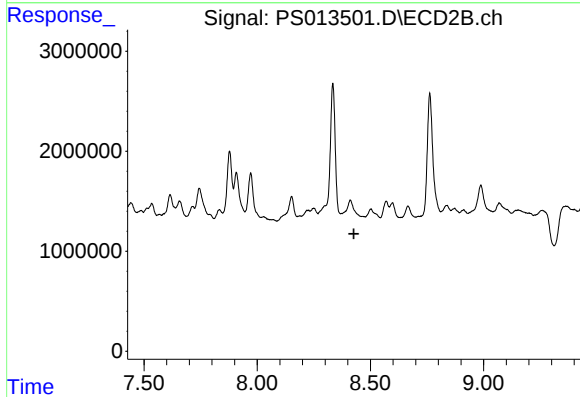


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.427 min
Response: 0
Conc: N.D.

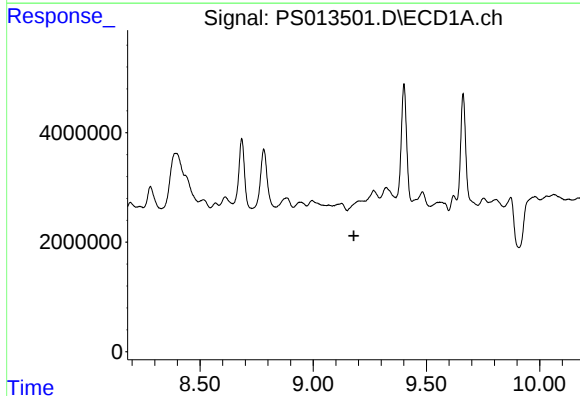


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

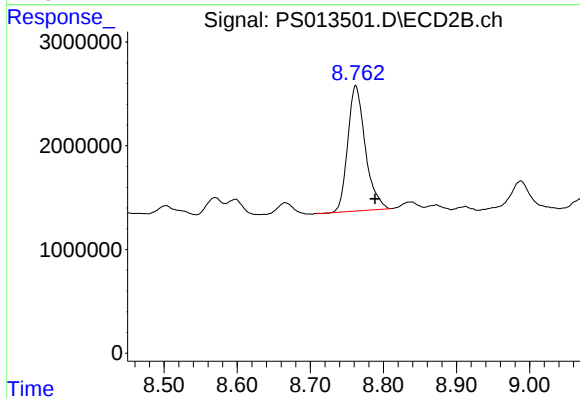

#11 2,4,5-TP (SILVEX)


R.T.: 8.762 min
Delta R.T.: -0.027 min
Response: 20126880
Conc: 8.57 ng/ml

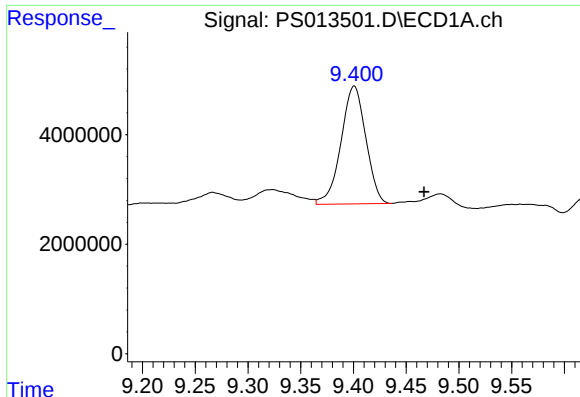

#12 2,4,5-T


R.T.: 9.401 min
Delta R.T.: -0.066 min
Response: 35138585
Conc: 6.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

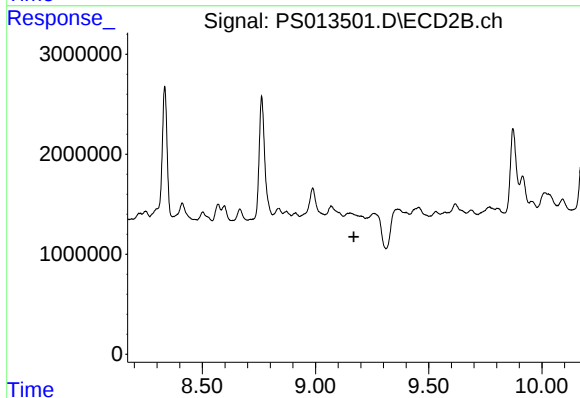


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

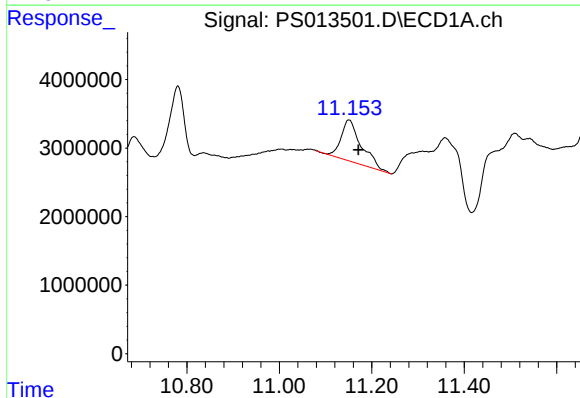


#14 DINOSEB

R.T.: 11.150 min
Delta R.T.: -0.021 min
Response: 18334038
Conc: 4.33 ng/ml

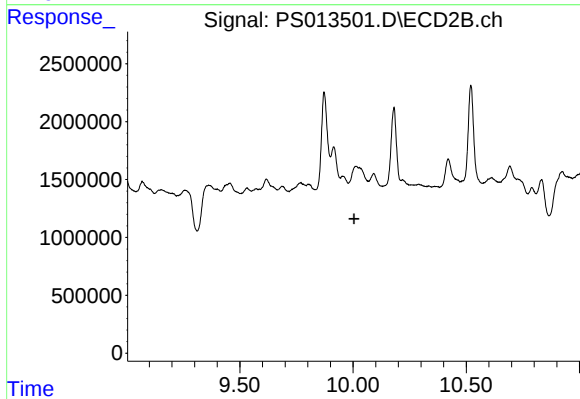

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 10.004 min
Response: 0
Conc: N.D.

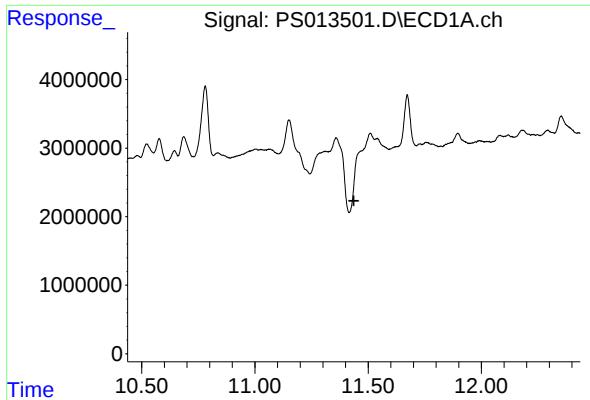

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
KENS-SS2-121020-0-7

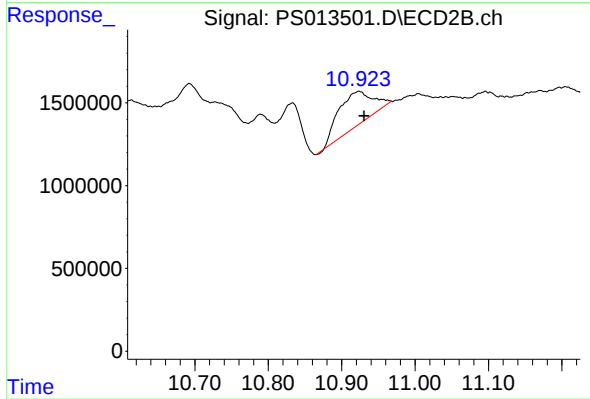

#16 DCPA

R.T.: 10.924 min
Delta R.T.: -0.007 min
Response: 6659451
Conc: 2.19 ng/ml