

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121421\
 Data File : PS017699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2021 23:12
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 01:14:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.129	6.716	672.6E6	285.5E6	430.311	478.981
Target Compounds							
2) T	3,5-DICHL...	6.395	0.000	5087467	0	2.277	N.D. #
9) T	2,4-D	8.305f	0.000	34559171	0	19.548	N.D. #
15) T	Picloram	10.874	0.000	4120051	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121421\
Data File : PS017699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2021 23:12
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 01:14:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

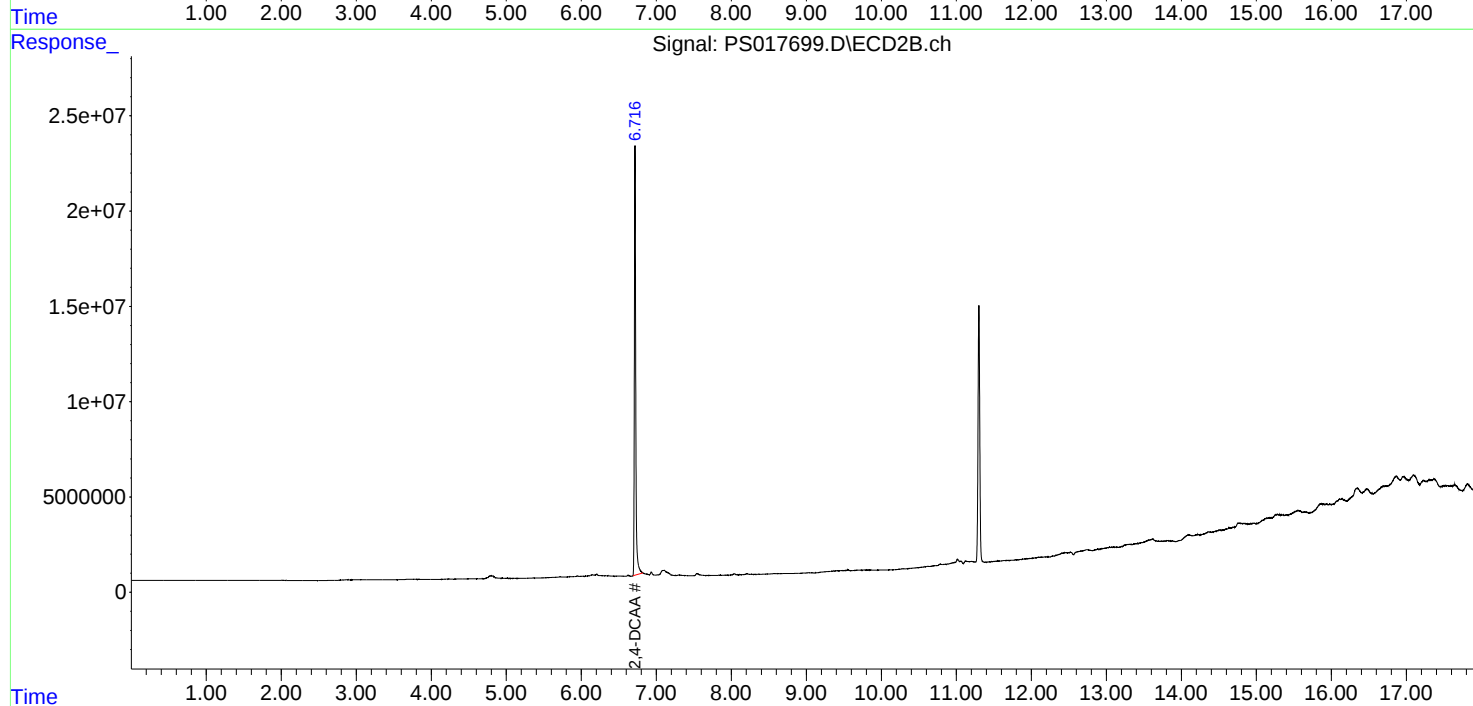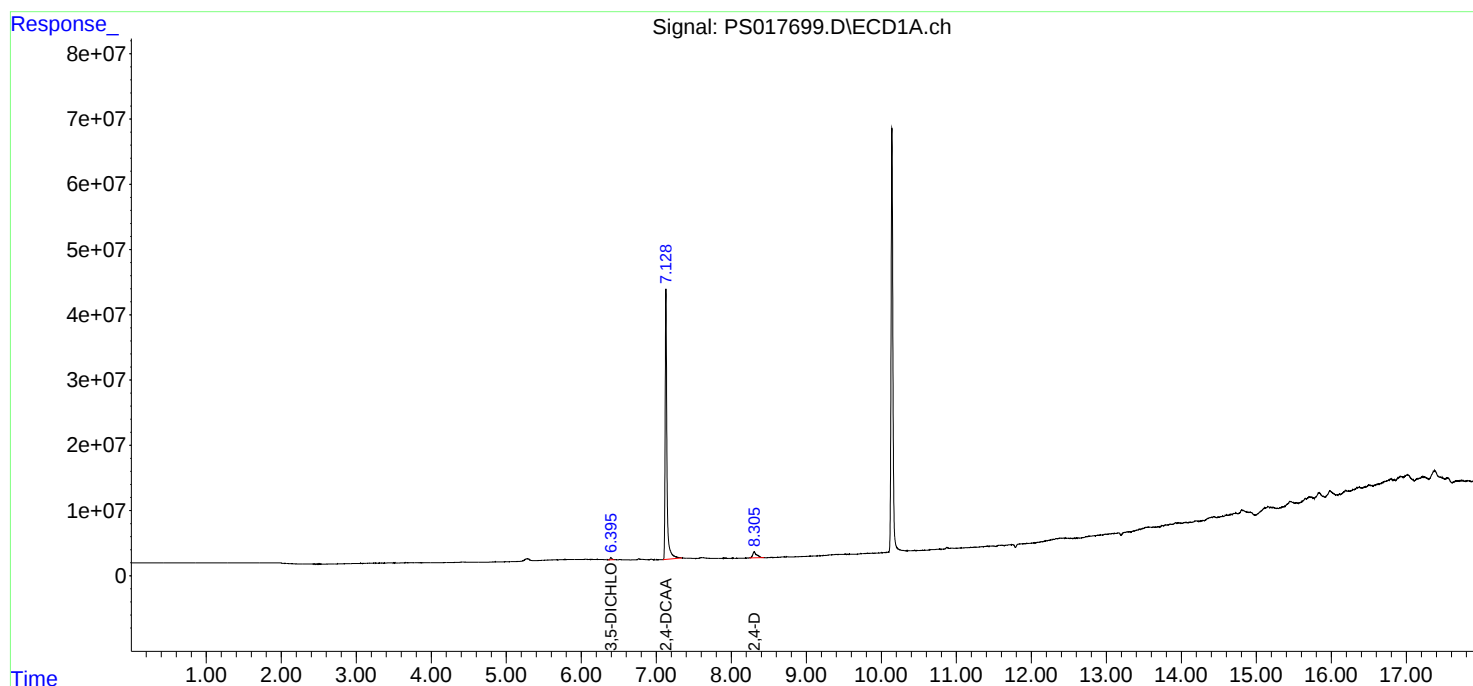


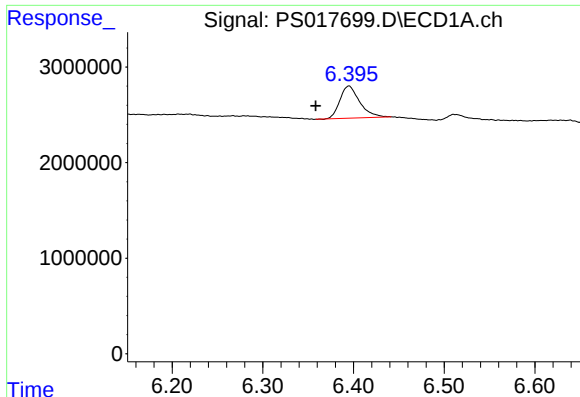

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.395 min
Delta R.T.: 0.037 min
Response: 5087467
Conc: 2.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

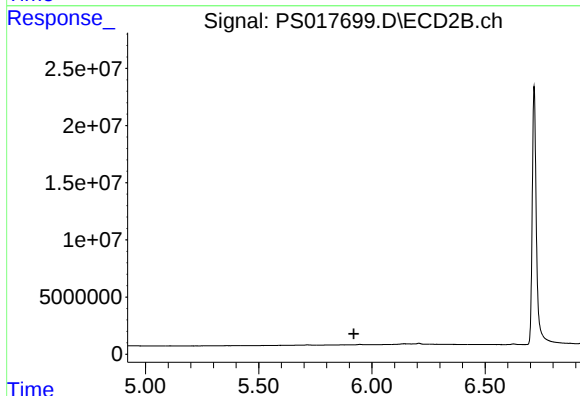


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

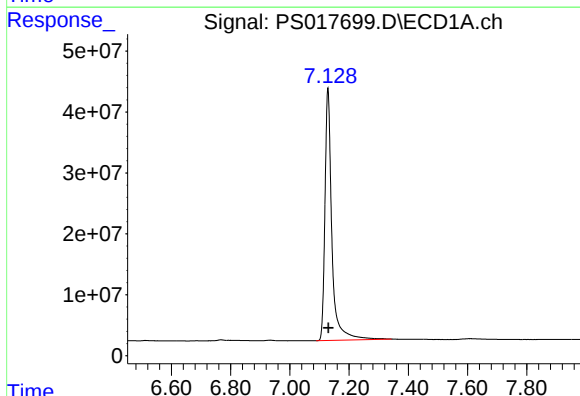


#4 2,4-DCAA

R.T.: 7.129 min
Delta R.T.: -0.001 min
Response: 672553301
Conc: 430.31 ng/ml

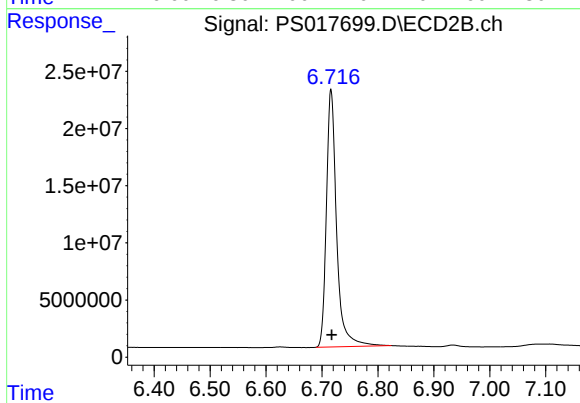

#4 2,4-DCAA


R.T.: 6.716 min
Delta R.T.: -0.001 min
Response: 285521570
Conc: 478.98 ng/ml

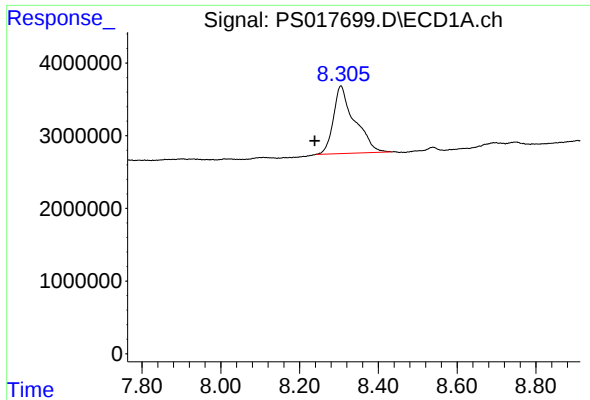

#9 2,4-D

R.T.: 8.305 min
Delta R.T.: 0.066 min
Response: 34559171
Conc: 19.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

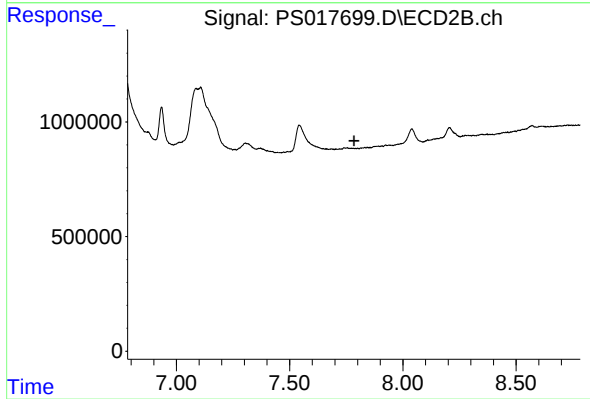

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.