

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121423\
 Data File : PS025076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 09:03
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 23:26:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.559	0	2982020	N.D.	2.600
2) T	3,5-DICHL...	5.697	0.000	6905134	0	2.043	N.D. #
3) T	4-Nitroph...	6.192	0.000	10761982	0	7.308	N.D. #
5) T	DICAMBA	0.000	6.967	0	5066092	N.D.	1.635
6) T	MCPPE	6.677	6.967f	3322184	5066092	<MDL	2.442 #
8) T	DICHLORPROP	0.000	7.551	0	2038684	N.D.	2.592
9) T	2,4-D	7.246	7.764f	52229037	583051	17.196	<MDL #
11) T	2,4,5-TP ...	0.000	8.642	0	3940655	N.D.	<MDL
12) T	2,4,5-T	0.000	8.974	0	538576	N.D.	<MDL
14) T	DINOSEB	0.000	9.786	0	490950	N.D.	<MDL
15) T	Picloram	9.679	10.756	23178635	15524522	1.190	2.372 #
16) T	DCPA	0.000	10.756	0	15524522	N.D.	2.864



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121423\
Data File : PS025076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 09:03
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 23:26:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

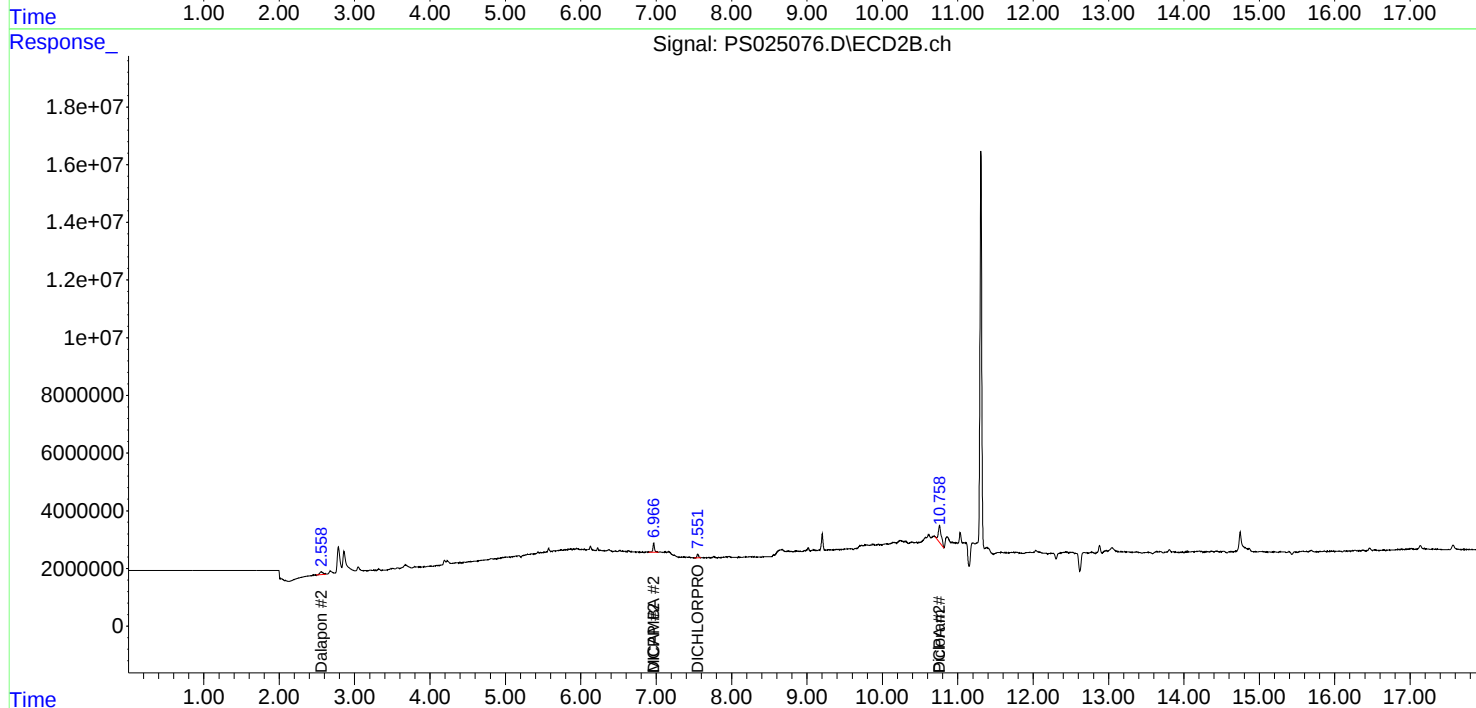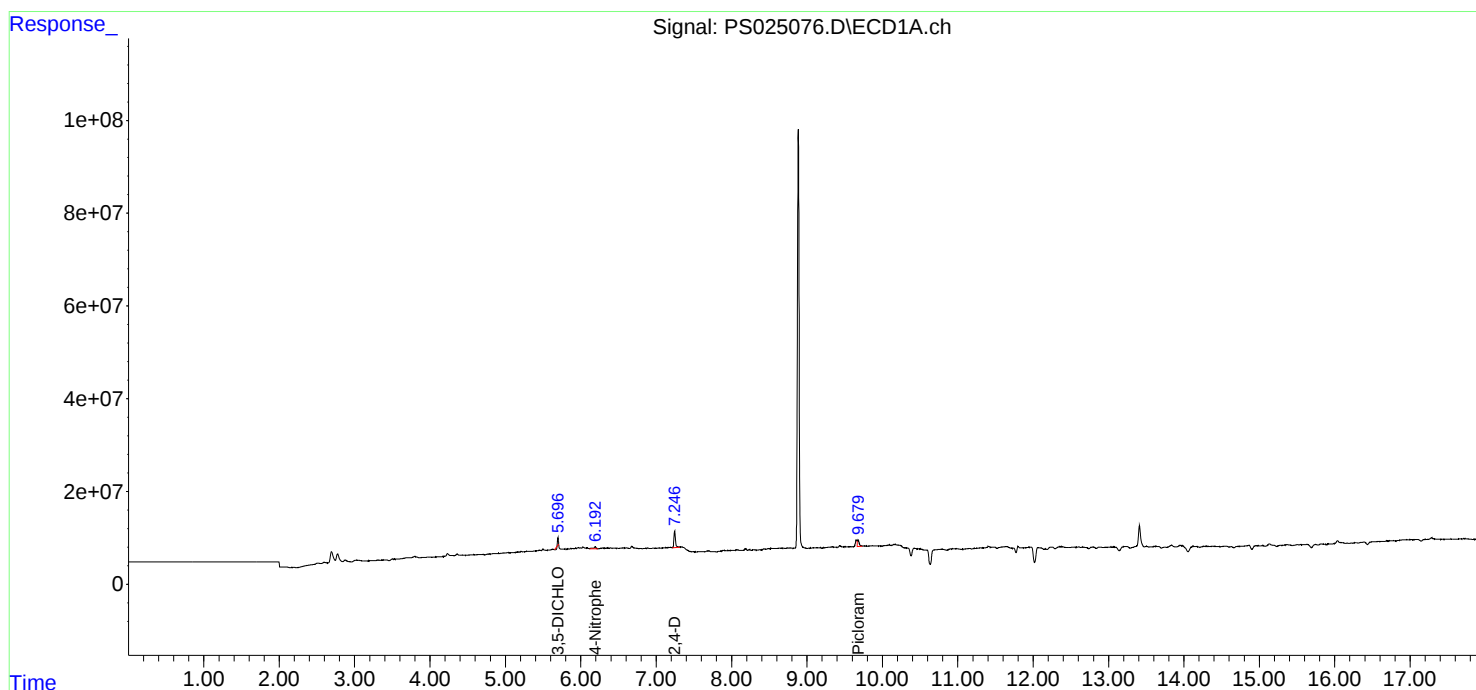


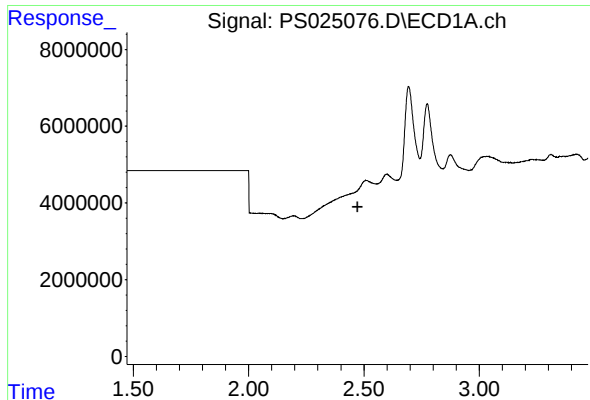

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

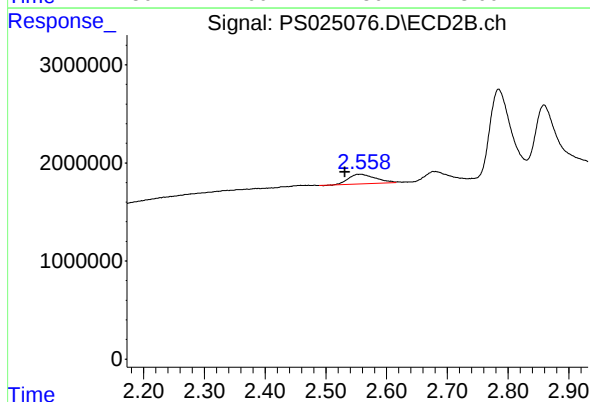


#1 Dalapon

R.T.: 2.559 min
Delta R.T.: 0.027 min
Response: 2982020
Conc: 2.60 ng/ml

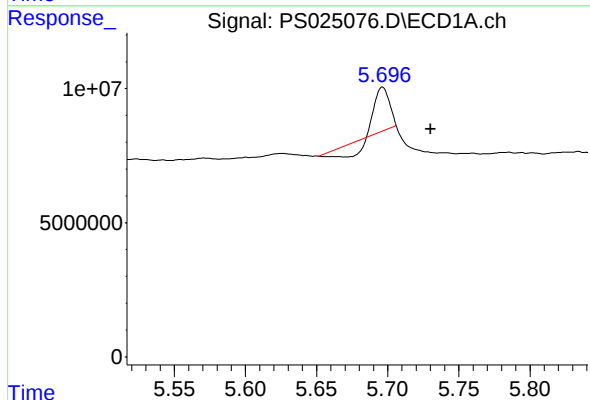


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.697 min
Delta R.T.: -0.034 min
Response: 6905134
Conc: 2.04 ng/ml

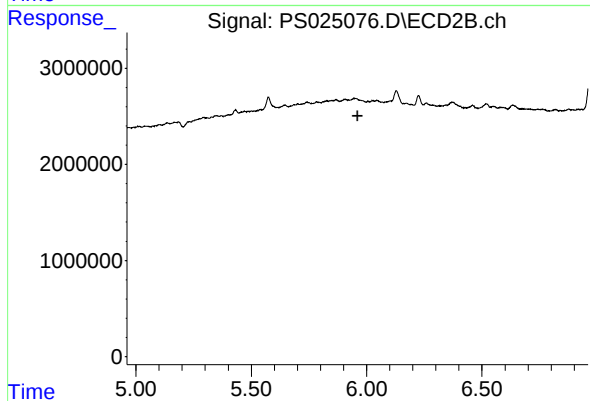

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

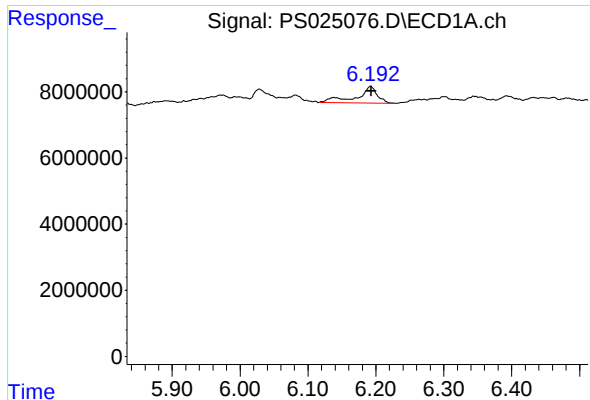

#3 4-Nitrophenol


R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 10761982
Conc: 7.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

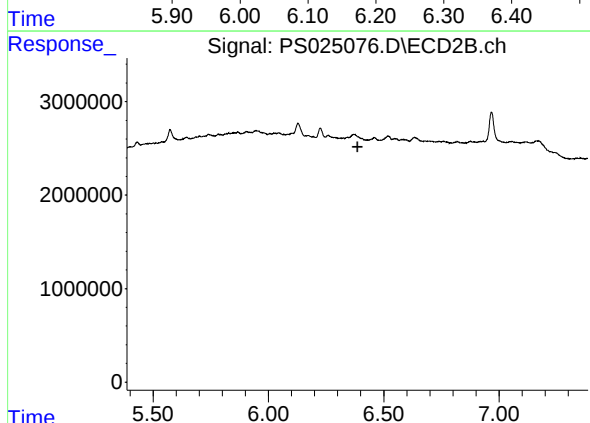


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

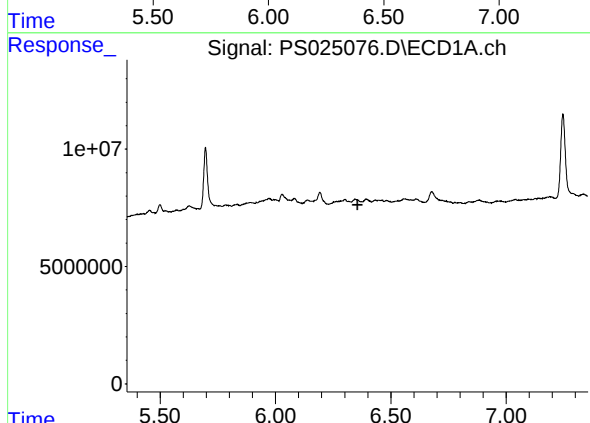


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

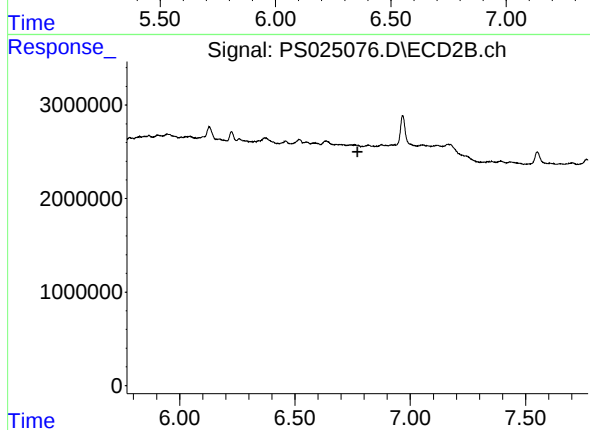

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

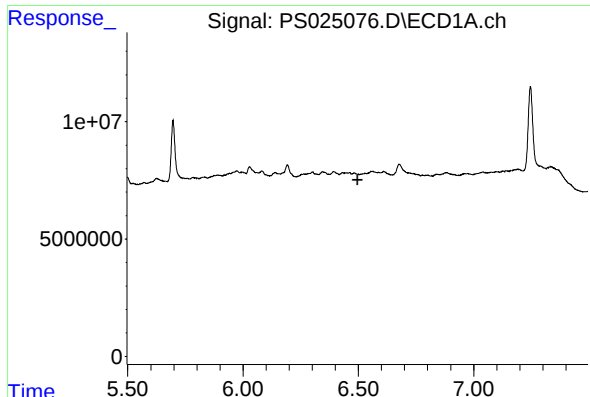

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

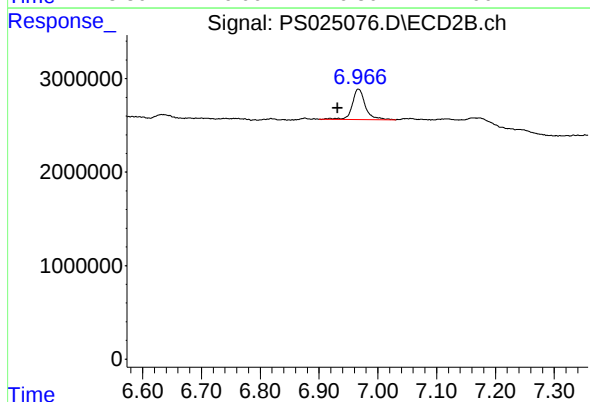


#5 DICAMBA

R.T.: 6.967 min
Delta R.T.: 0.035 min
Response: 5066092
Conc: 1.64 ng/ml

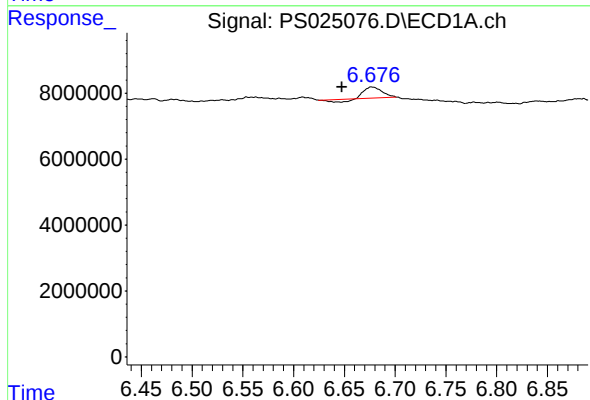


#6 MCPP

R.T.: 6.677 min
Delta R.T.: 0.030 min
Response: 3322184
Conc: N.D.

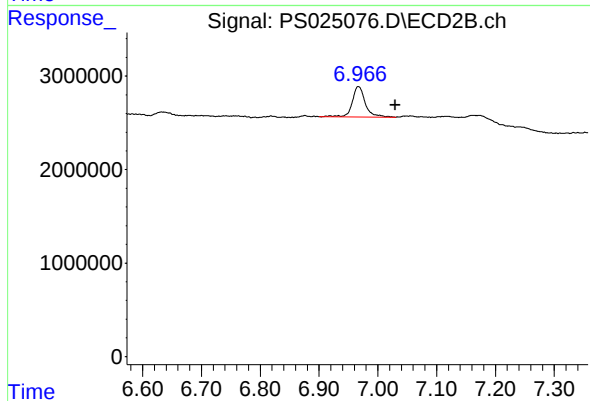

#6 MCPP


R.T.: 6.967 min
Delta R.T.: -0.062 min
Response: 5066092
Conc: 2.44 ug/ml

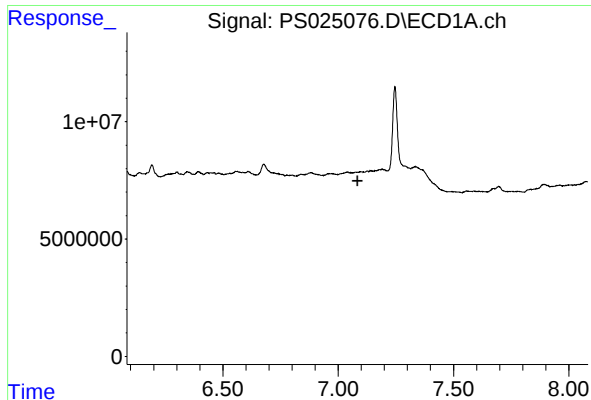

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

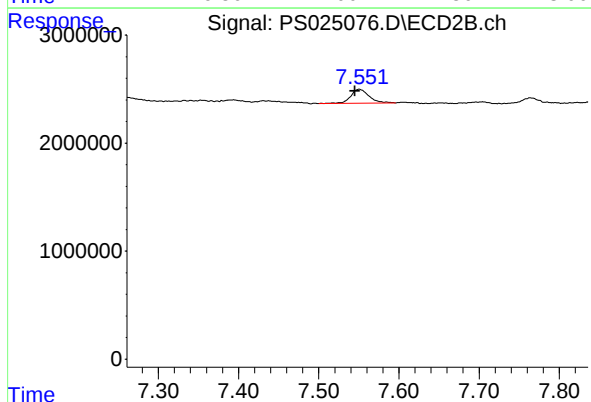


#8 DICHLORPROP

R.T.: 7.551 min
Delta R.T.: 0.006 min
Response: 2038684
Conc: 2.59 ng/ml

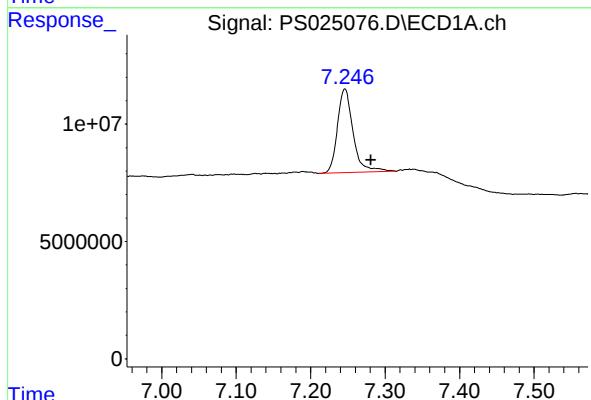


#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.035 min
Response: 52229037
Conc: 17.20 ng/ml

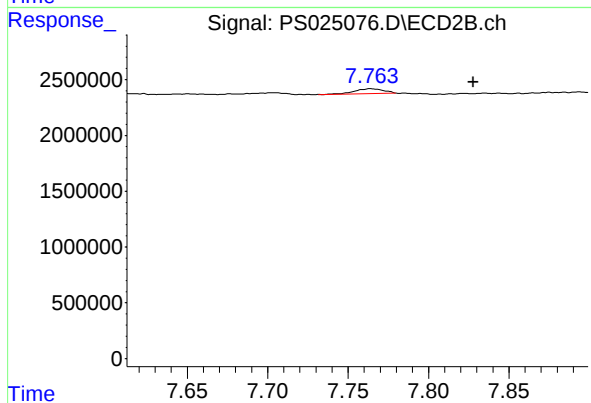

#9 2,4-D


R.T.: 7.764 min
Delta R.T.: -0.064 min
Response: 583051
Conc: N.D.

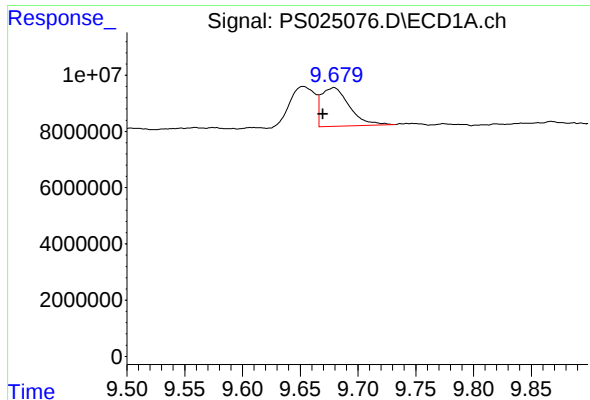

#15 Picloram


R.T.: 9.679 min
Delta R.T.: 0.009 min
Response: 23178635
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

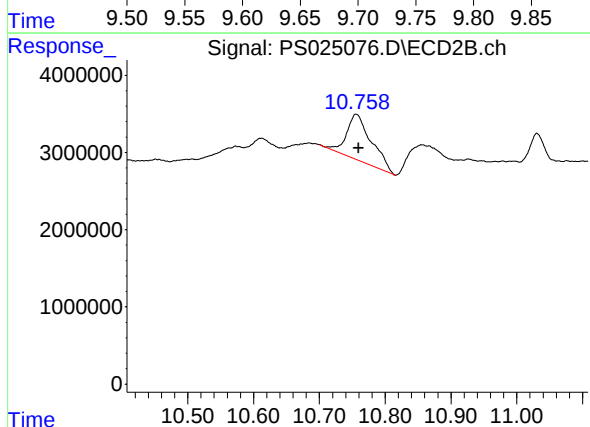


#15 Picloram

R.T.: 10.756 min
Delta R.T.: -0.004 min
Response: 15524522
Conc: 2.37 ng/ml

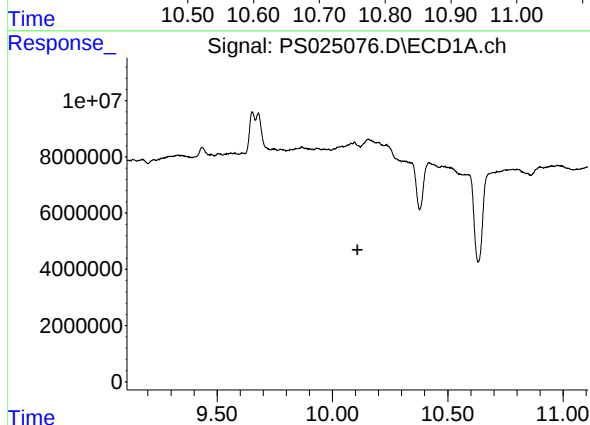

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

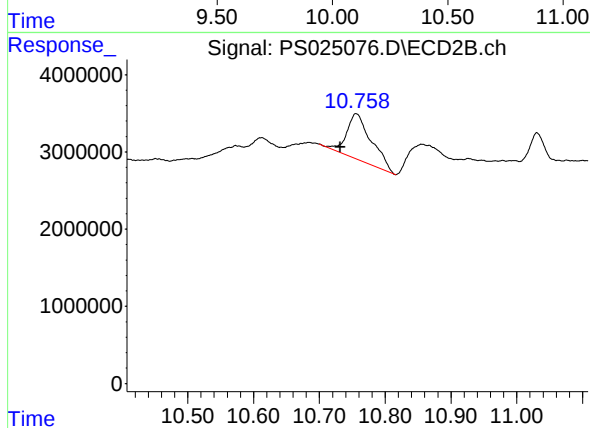

#16 DCPA

R.T.: 10.756 min
Delta R.T.: 0.024 min
Response: 15524522
Conc: 2.86 ng/ml