

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121423\
 Data File : PS025077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 09:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 23:26:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.355	6.769	1140.5E6	363.0E6	509.628	500.979
Target Compounds						
1) T Dalapon	2.507	2.560	7336384	1573731	2.544	1.372 #
7) T MCPA	0.000	7.227	0	3742712	N.D.	1.138
8) T DICHLORPROP	0.000	7.561	0	1337414	N.D.	1.700
9) T 2,4-D	0.000	7.768f	0	392855	N.D.	<MDL
12) T 2,4,5-T	0.000	9.020f	0	1506477	N.D.	<MDL
15) T Picloram	9.687	10.761	22303197	6670492	1.145	1.019
16) T DCPA	0.000	10.761	0	6670492	N.D.	1.231



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121423\
Data File : PS025077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 09:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 23:26:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

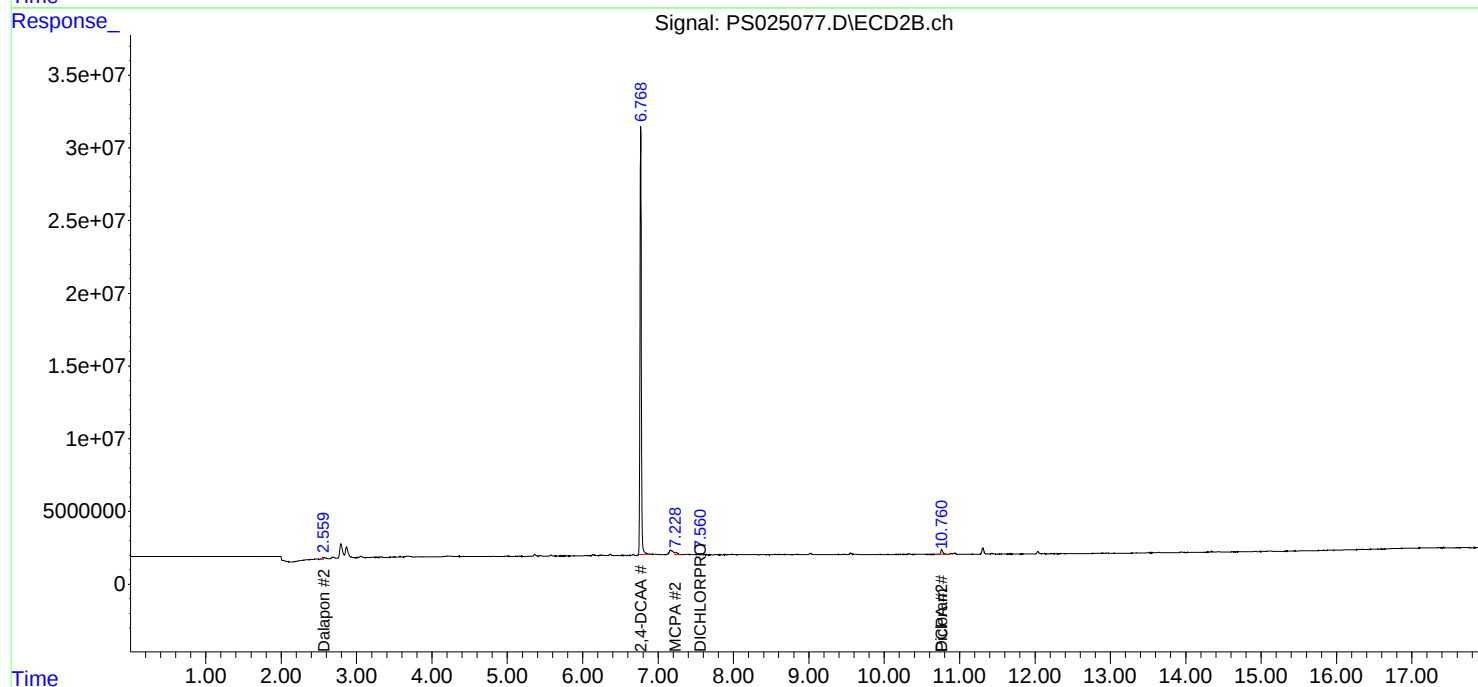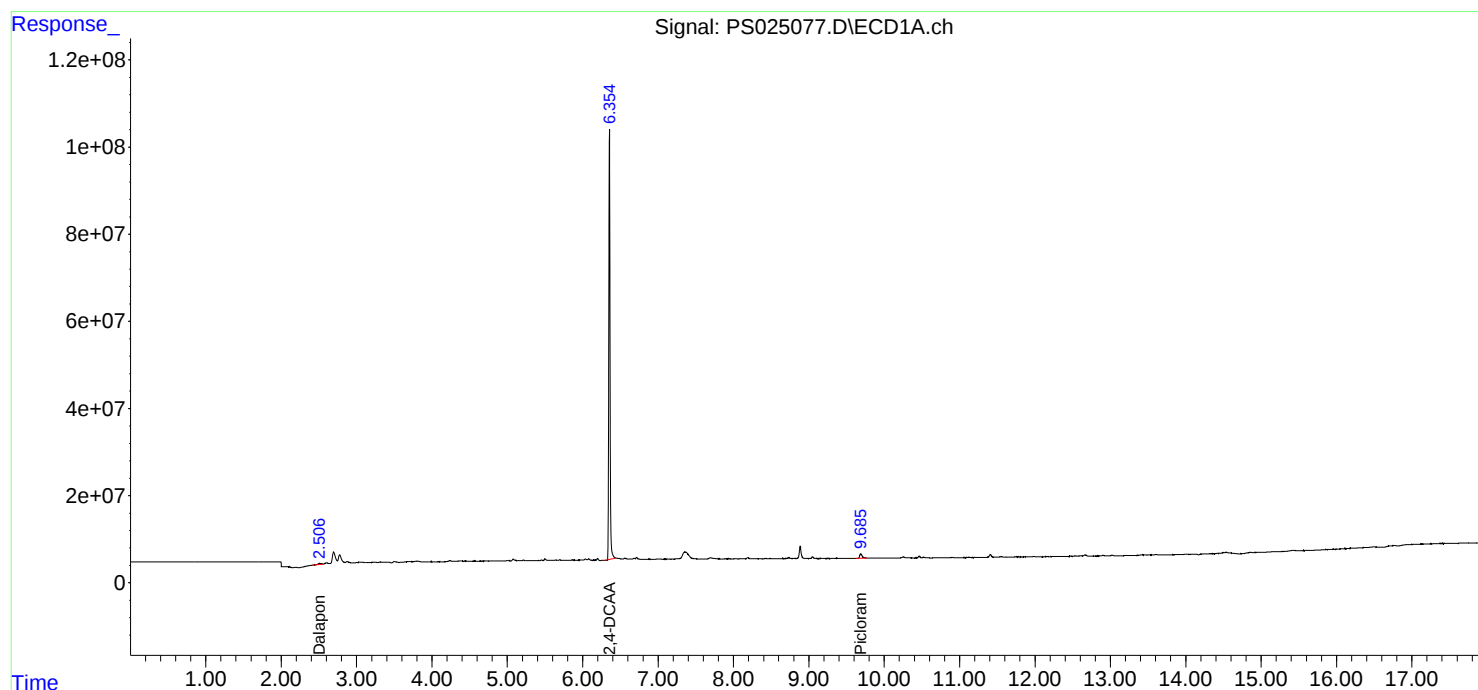


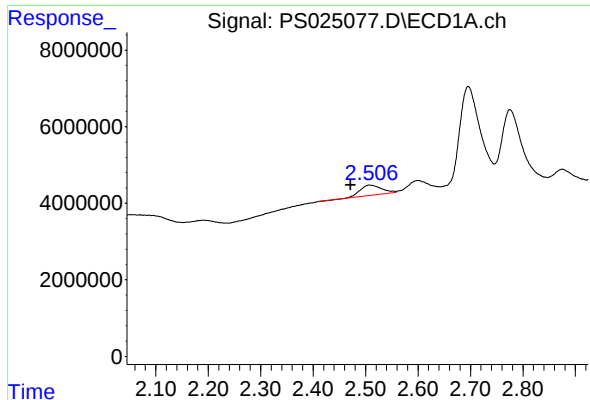

#1 Dalapon


R.T.: 2.507 min
Delta R.T.: 0.035 min
Response: 7336384
Conc: 2.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

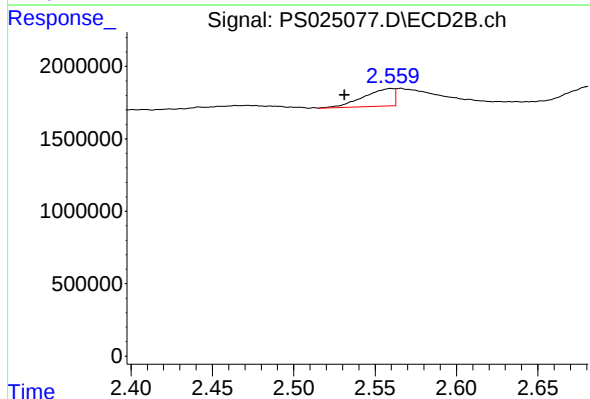


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.028 min
Response: 1573731
Conc: 1.37 ng/ml

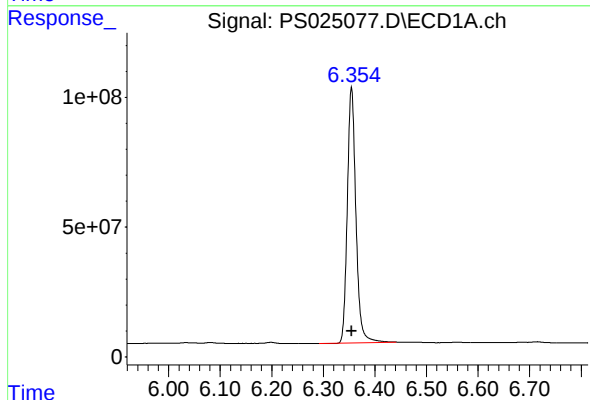


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1140468635
Conc: 509.63 ng/ml

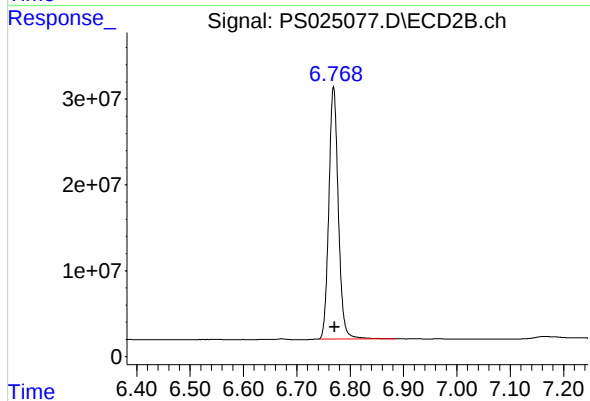

#4 2,4-DCAA


R.T.: 6.769 min
Delta R.T.: -0.002 min
Response: 362986480
Conc: 500.98 ng/ml

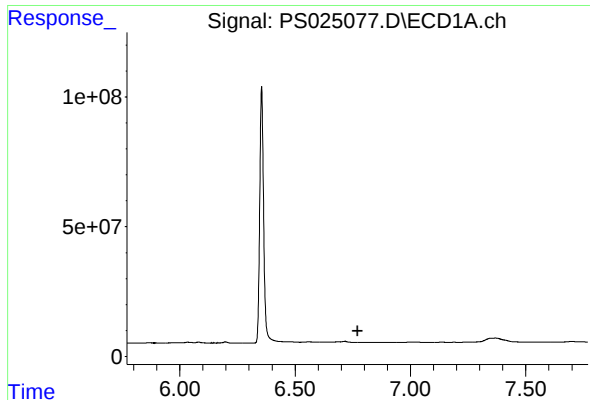

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

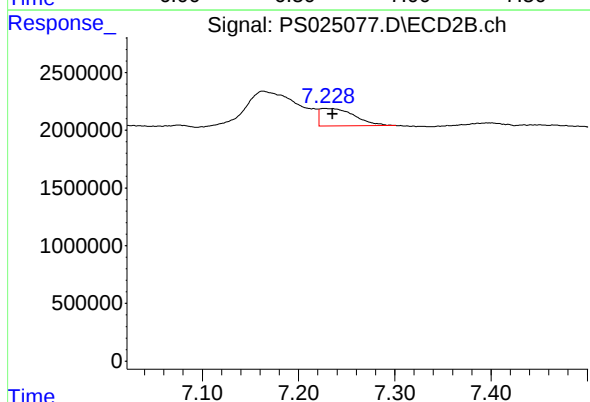


#7 MCPA

R.T.: 7.227 min
Delta R.T.: -0.008 min
Response: 3742712
Conc: 1.14 ug/ml

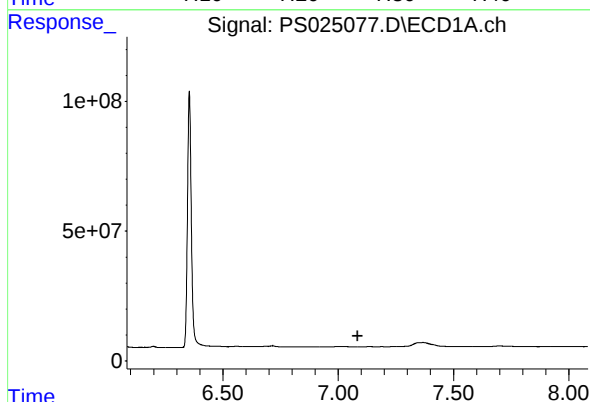


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

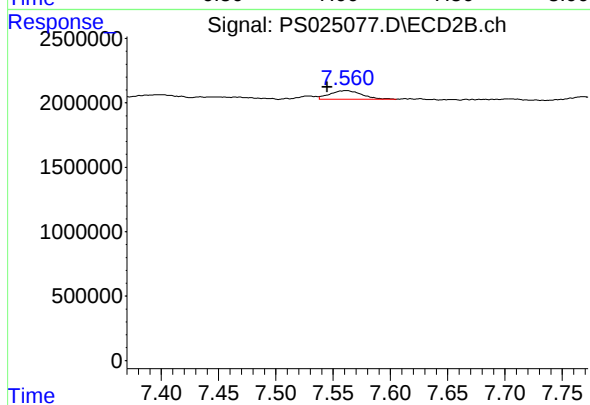

#8 DICHLORPROP


R.T.: 7.561 min
Delta R.T.: 0.016 min
Response: 1337414
Conc: 1.70 ng/ml

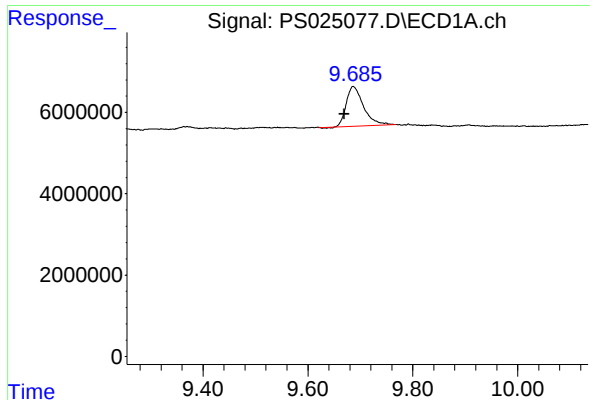

#15 Picloram


R.T.: 9.687 min
Delta R.T.: 0.017 min
Response: 22303197
Conc: 1.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

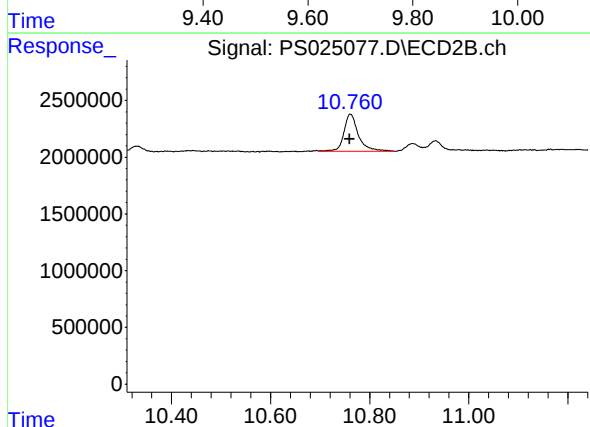


#15 Picloram

R.T.: 10.761 min
Delta R.T.: 0.000 min
Response: 6670492
Conc: 1.02 ng/ml

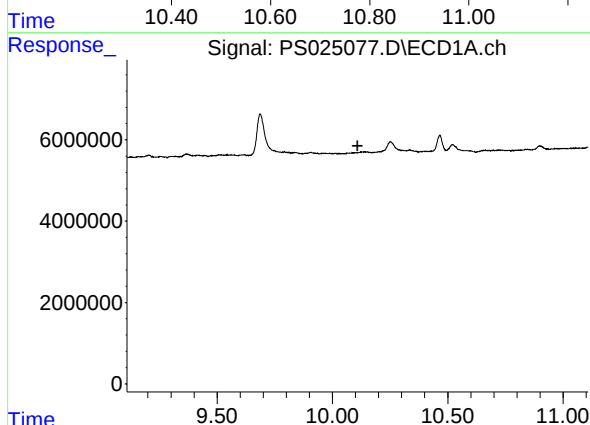

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

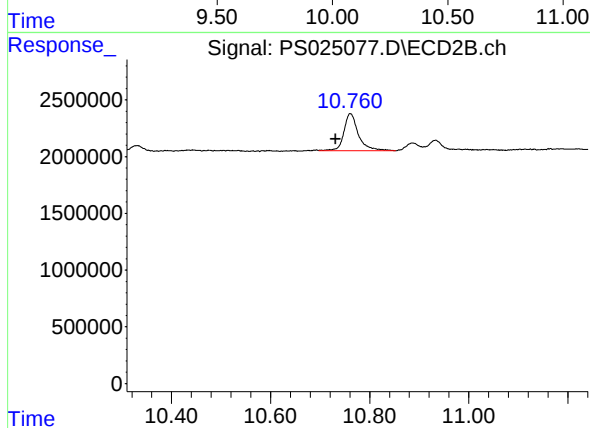

#16 DCPA

R.T.: 10.761 min
Delta R.T.: 0.029 min
Response: 6670492
Conc: 1.23 ng/ml