

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121520\
 Data File : PS013534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2020 08:13
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 10:35:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.469f	0.000	401.6E6	0	313.331	N.D. #
7) T	MCPA	7.693	0.000	17996603	0	4.604	N.D. #
8) T	DICHLORPROP	0.000	7.762f	0	12469924	N.D.	27.902
12) T	2,4,5-T	9.407f	0.000	17061987	0	3.086	N.D. #
15) T	Picloram	11.037	11.028	125.8E6	65960755	18.266	18.945
16) T	DCPA	0.000	10.931	0	4748863	N.D.	1.561



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121520\
Data File : PS013534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2020 08:13
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 10:35:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

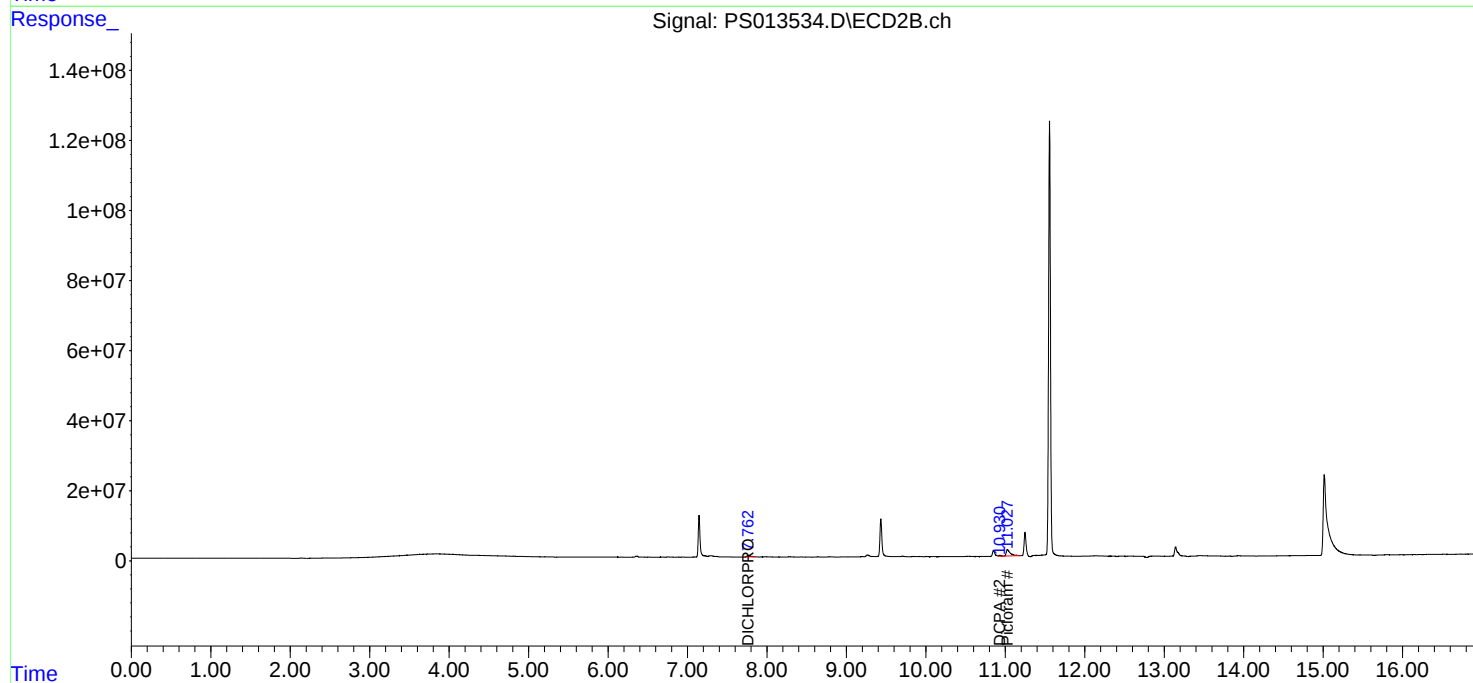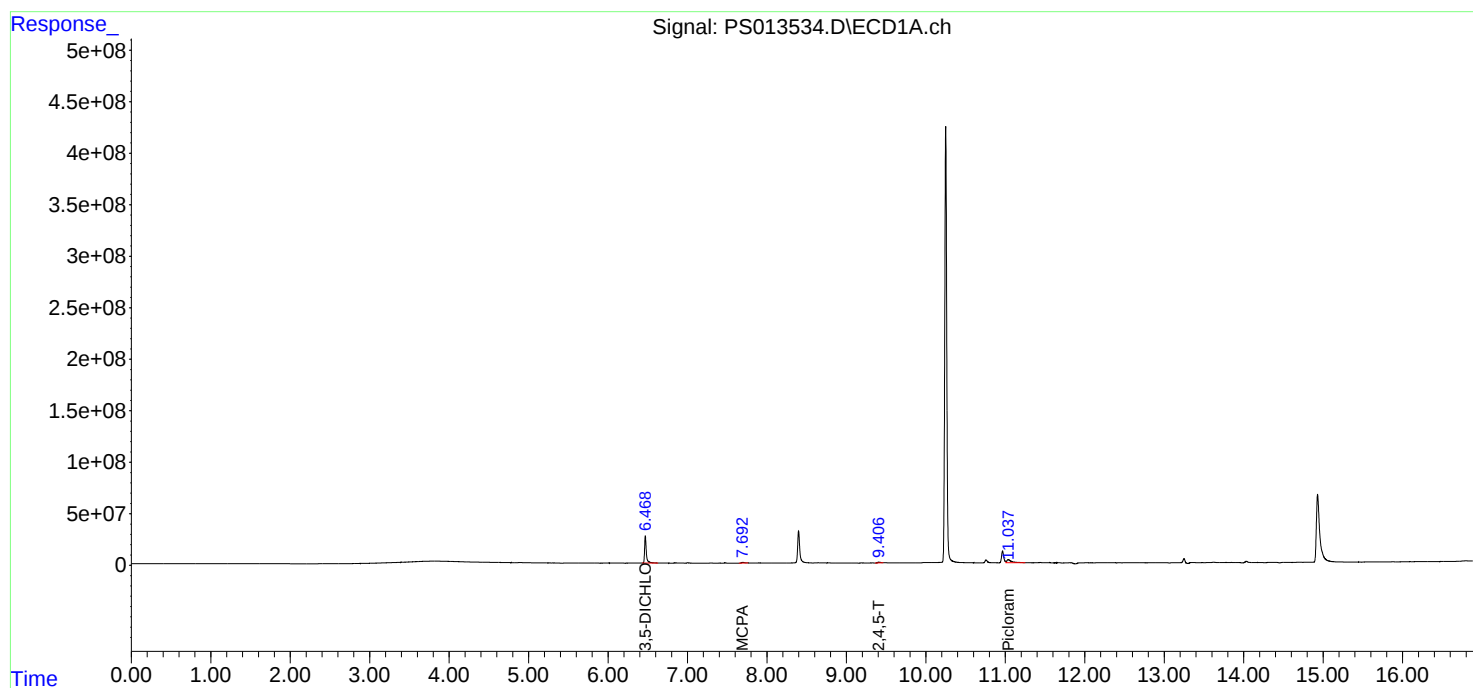


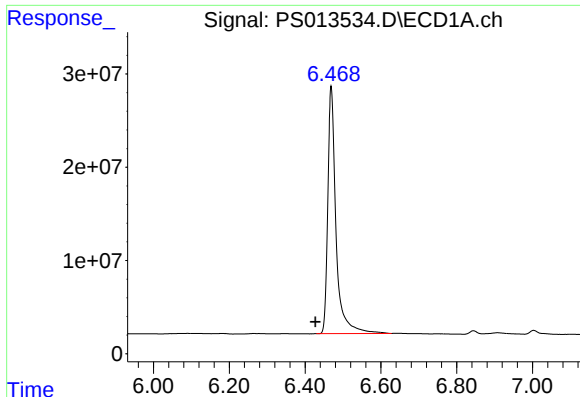

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.469 min
Delta R.T.: 0.041 min
Response: 401598229
Conc: 313.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

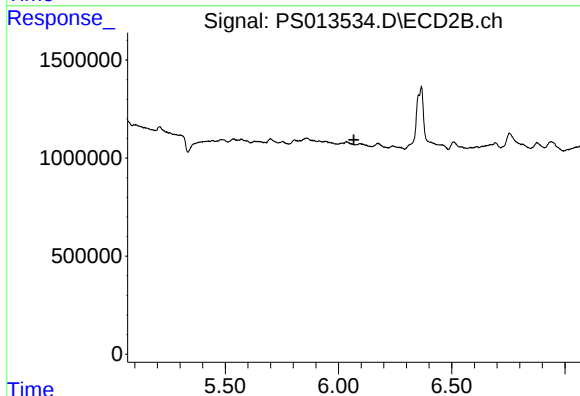


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.068 min
Response: 0
Conc: N.D.

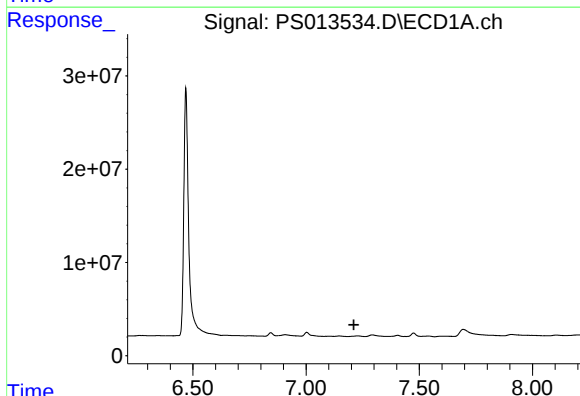


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.211 min
Response: 0
Conc: N.D.

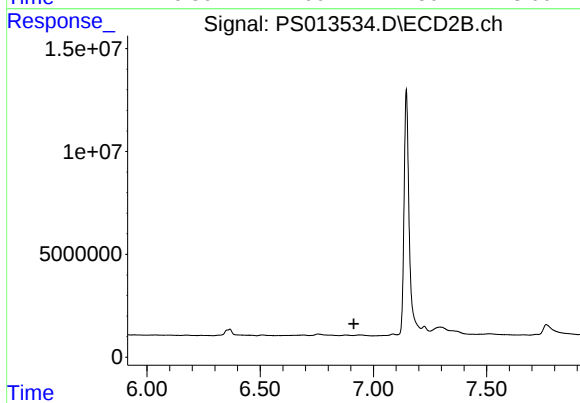

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.914 min
Response: 0
Conc: N.D.

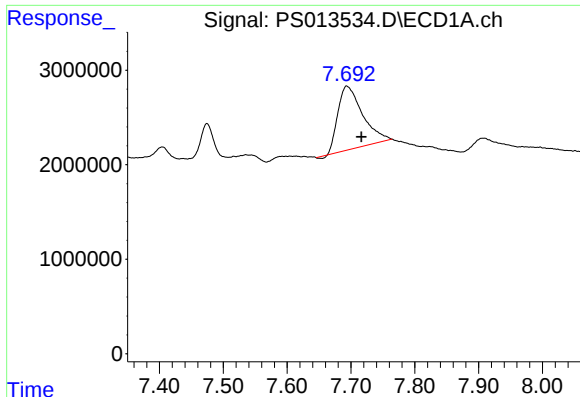

#7 MCPA


R.T.: 7.693 min
Delta R.T.: -0.024 min
Response: 17996603
Conc: 4.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

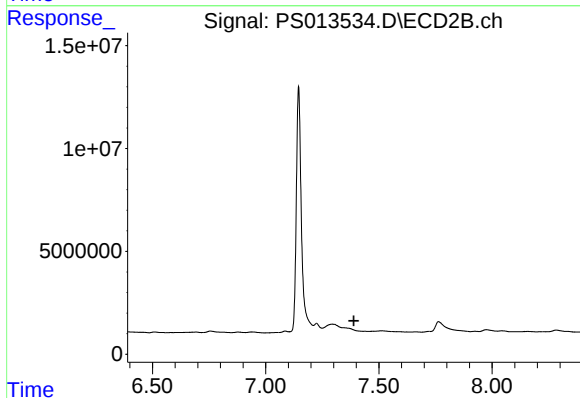


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

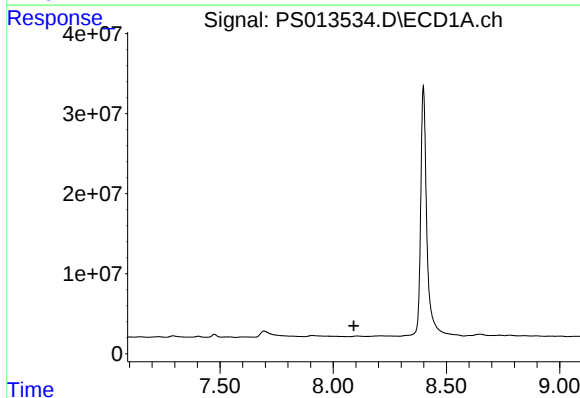


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

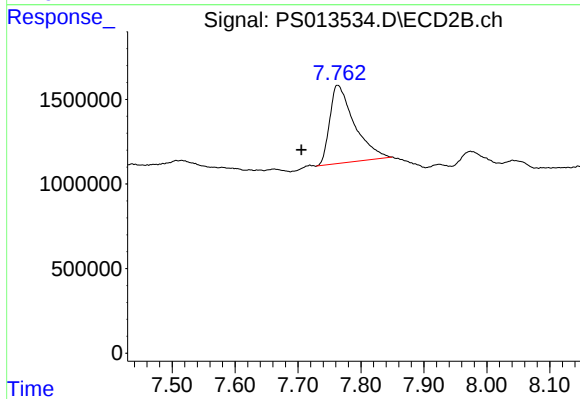

#8 DICHLORPROP


R.T.: 7.762 min
Delta R.T.: 0.057 min
Response: 12469924
Conc: 27.90 ng/ml

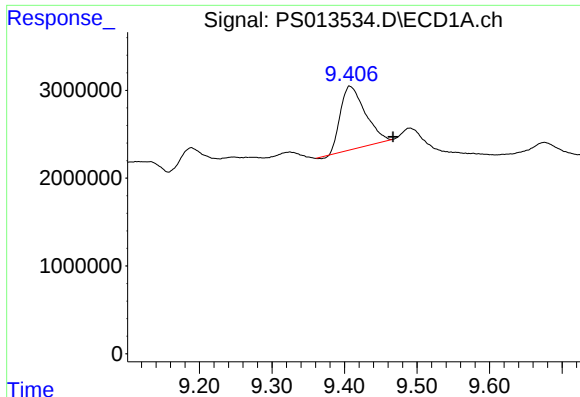

#12 2,4,5-T


R.T.: 9.407 min
Delta R.T.: -0.060 min
Response: 17061987
Conc: 3.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

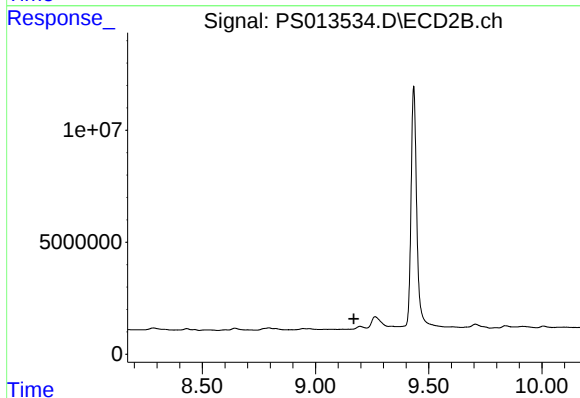


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

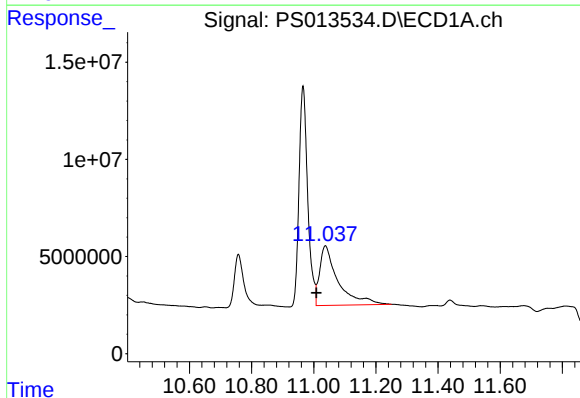


#15 Picloram

R.T.: 11.037 min
Delta R.T.: 0.029 min
Response: 125814108
Conc: 18.27 ng/ml

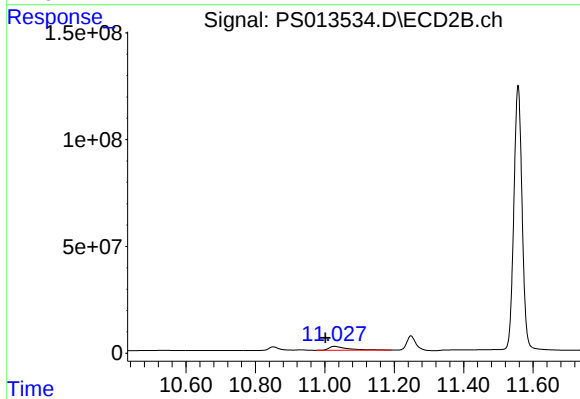

#15 Picloram


R.T.: 11.028 min
Delta R.T.: 0.027 min
Response: 65960755
Conc: 18.94 ng/ml

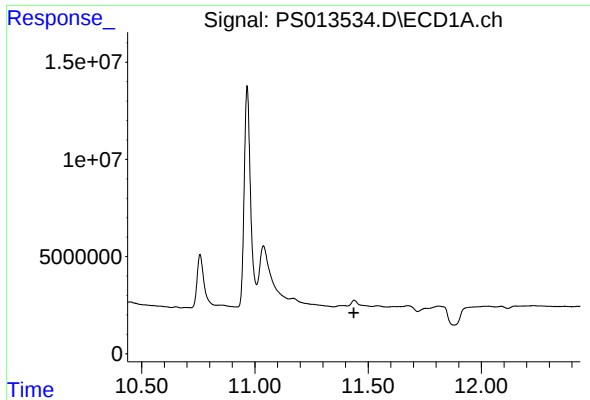

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

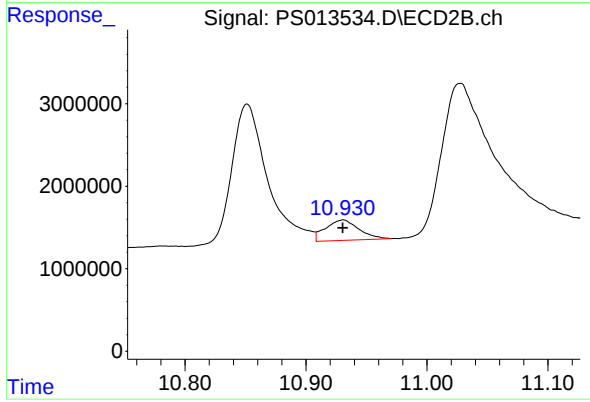

#16 DCPA

R.T.: 10.931 min
Delta R.T.: 0.000 min
Response: 4748863
Conc: 1.56 ng/ml