

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121521\
 Data File : PS017702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2021 11:04
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 15:24:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.128	6.714	674.8E6	285.7E6	431.740	479.347
Target Compounds							
2) T	3,5-DICHL...	6.396	0.000	8455398	0	3.785	N.D. #
5) T	DICAMBA	7.315	0.000	6855145	0	1.084	N.D. #
9) T	2,4-D	8.304f	0.000	32428909	0	18.343	N.D. #
12) T	2,4,5-T	9.404	0.000	19562176	0	2.249	N.D. #
14) T	DINOSEB	11.065	0.000	13172431	0	1.926	N.D. #
15) T	Picloram	10.927	10.766	114.2E6	49088710	10.524	9.995
16) T	DCPA	11.333	0.000	5179084	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121521\
Data File : PS017702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2021 11:04
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 15:24:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

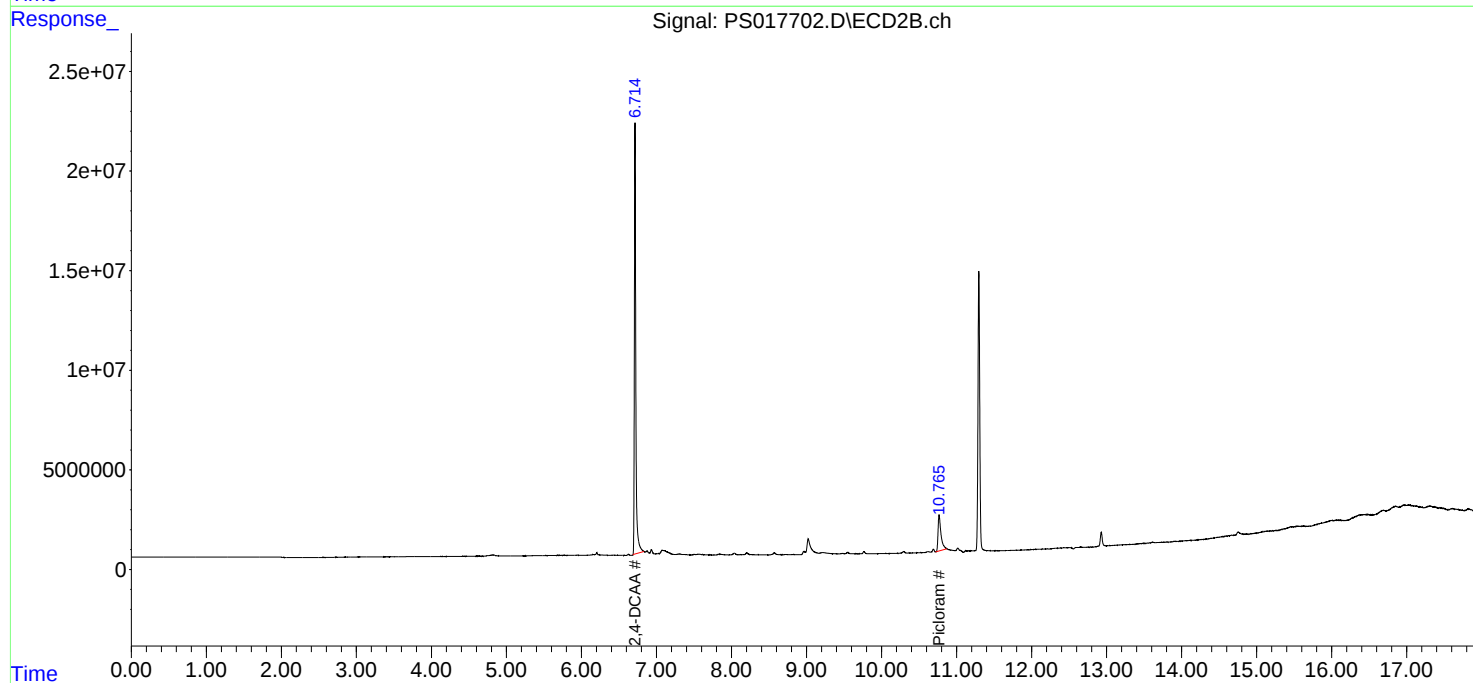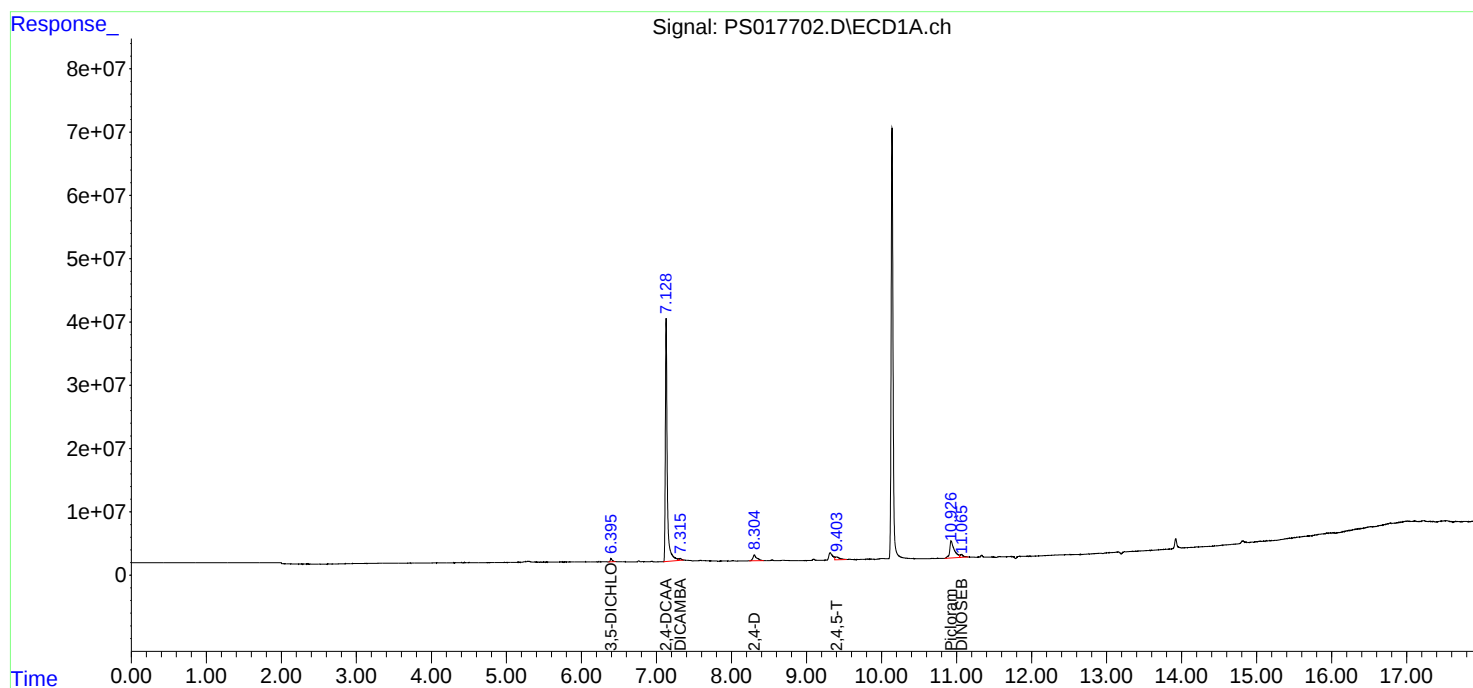


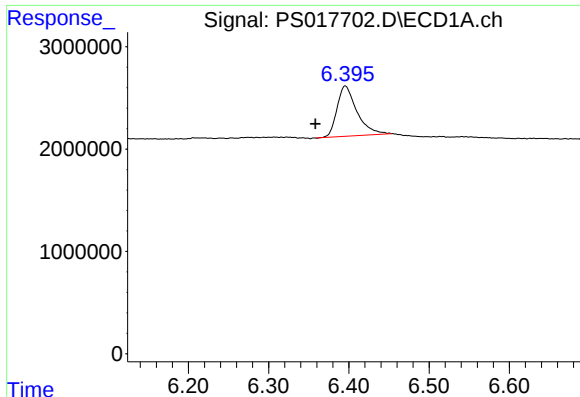

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.396 min
Delta R.T.: 0.037 min
Response: 8455398
Conc: 3.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

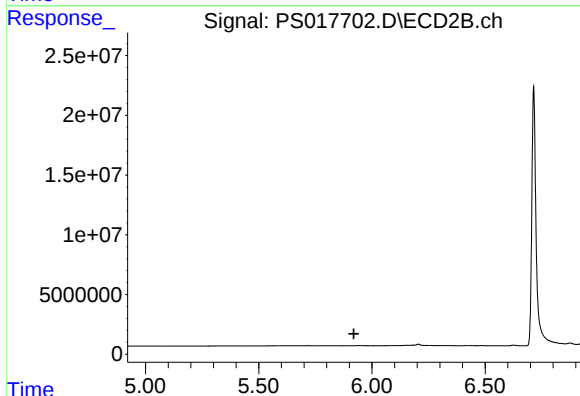


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

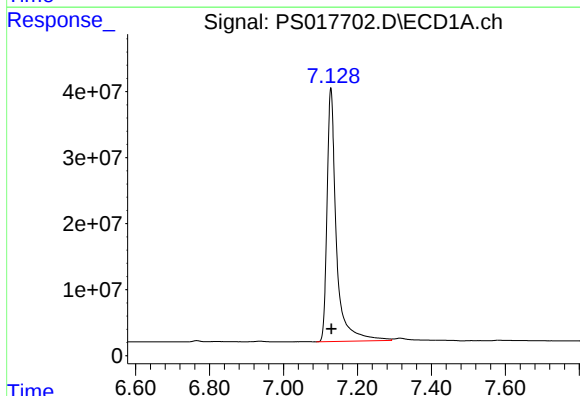


#4 2,4-DCAA

R.T.: 7.128 min
Delta R.T.: -0.002 min
Response: 674786819
Conc: 431.74 ng/ml

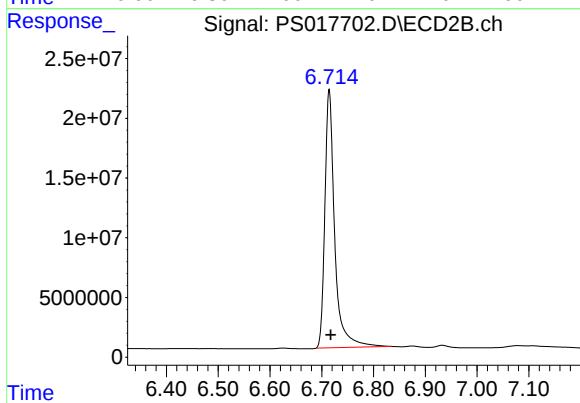

#4 2,4-DCAA


R.T.: 6.714 min
Delta R.T.: -0.003 min
Response: 285739275
Conc: 479.35 ng/ml

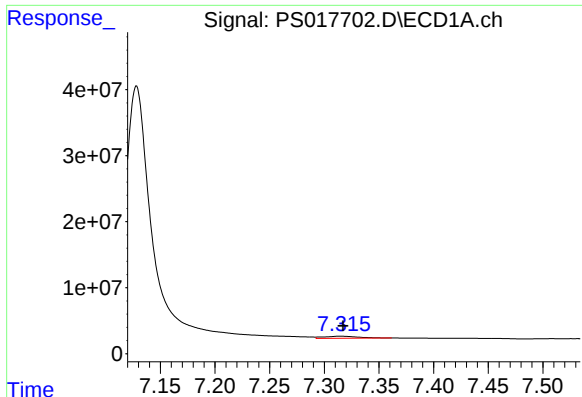

#5 DICAMBA


R.T.: 7.315 min
Delta R.T.: -0.002 min
Response: 6855145
Conc: 1.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

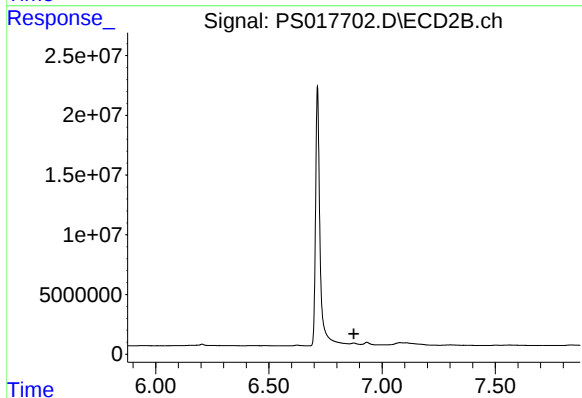


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

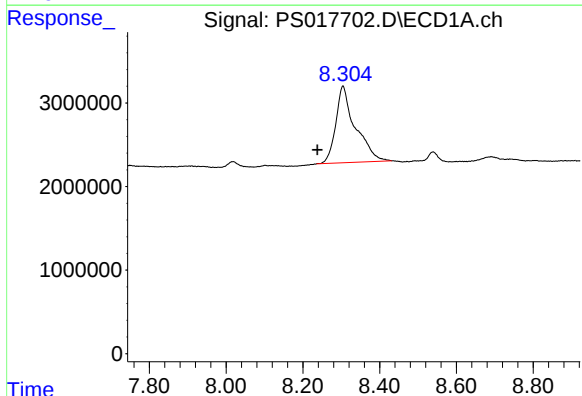


#9 2,4-D

R.T.: 8.304 min
Delta R.T.: 0.066 min
Response: 32428909
Conc: 18.34 ng/ml

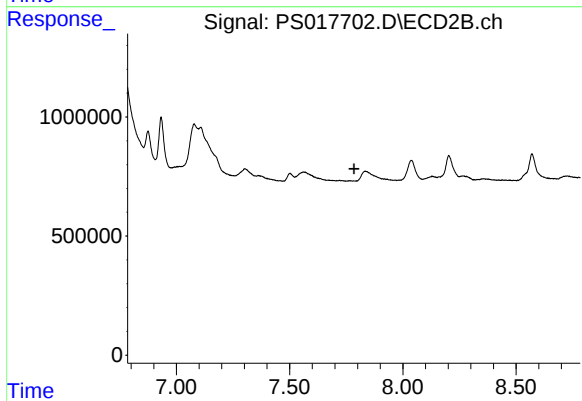

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

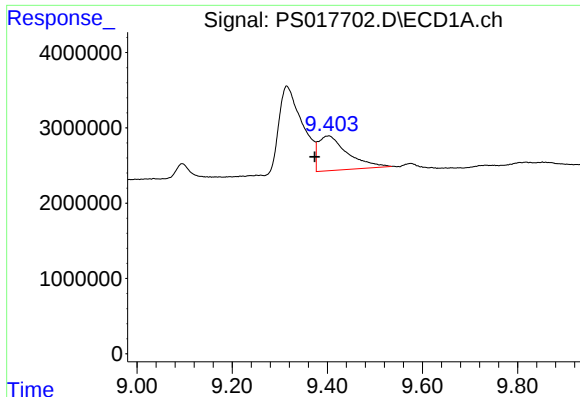

#12 2,4,5-T


R.T.: 9.404 min
Delta R.T.: 0.030 min
Response: 19562176
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

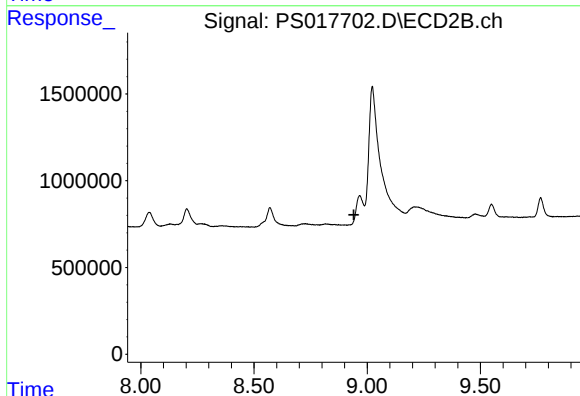


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

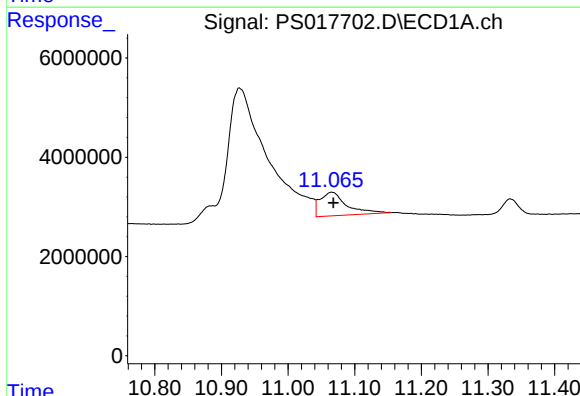


#14 DINOSEB

R.T.: 11.065 min
Delta R.T.: -0.002 min
Response: 13172431
Conc: 1.93 ng/ml

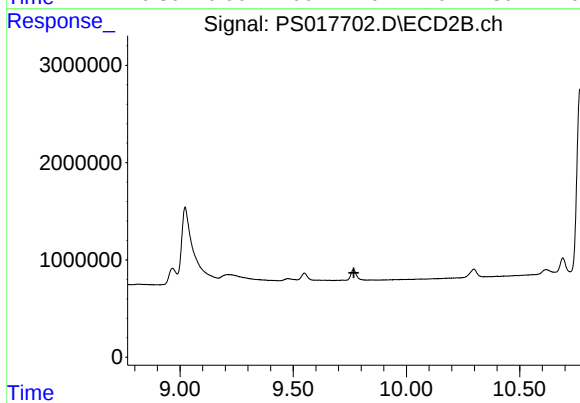

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

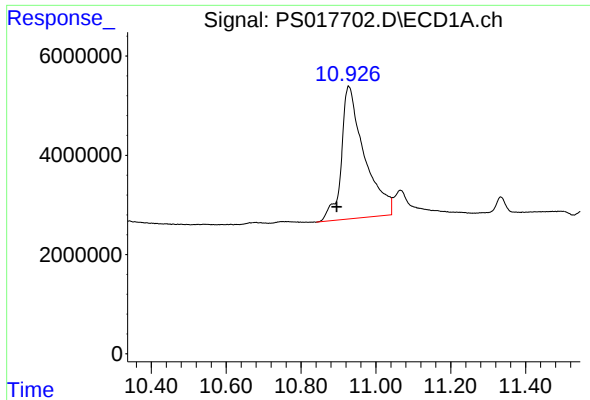

#15 Picloram

R.T.: 10.927 min
Delta R.T.: 0.032 min
Response: 114193805
Conc: 10.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

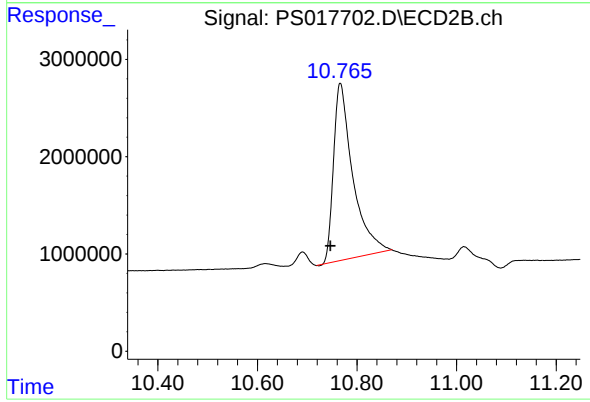

#15 Picloram

R.T.: 10.766 min
Delta R.T.: 0.020 min
Response: 49088710
Conc: 9.99 ng/ml