

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121523\
 Data File : PS025113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 12:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 15:41:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.768	1183.5E6	378.7E6	528.849	522.726
Target Compounds							
1) T	Dalapon	0.000	2.560	0	3174967	N.D.	2.768
2) T	3,5-DICHL...	5.696	0.000	2064238	0	<MDL	N.D. #
3) T	4-Nitroph...	6.197	0.000	8705261	0	5.911	N.D. #
5) T	DICAMBA	0.000	6.968	0	2174239	N.D.	<MDL
6) T	MCP	0.000	6.968f	0	2174239	N.D.	1.048
8) T	DICHLORPROP	0.000	7.555	0	2828535	N.D.	3.596
9) T	2,4-D	7.246	7.767f	16441505	112707	5.413	<MDL #
11) T	2,4,5-TP ...	0.000	8.605	0	519417	N.D.	<MDL
12) T	2,4,5-T	0.000	8.977	0	1020953	N.D.	<MDL
13) T	2,4-DB	0.000	9.476	0	771019	N.D.	1.393
15) T	Picloram	9.682	10.759	80229994	21268027	4.117	3.249
16) T	DCPA	0.000	10.759	0	21268027	N.D.	3.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121523\
Data File : PS025113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 12:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 15:41:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

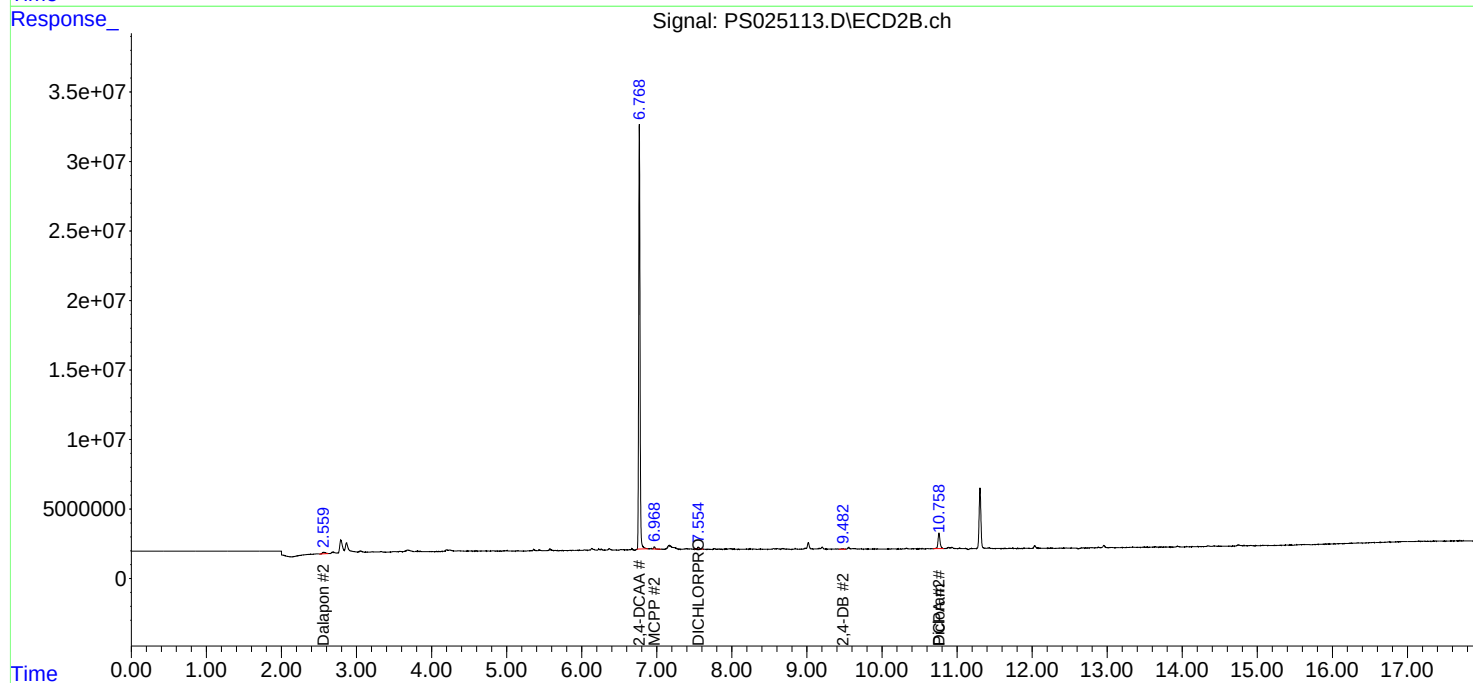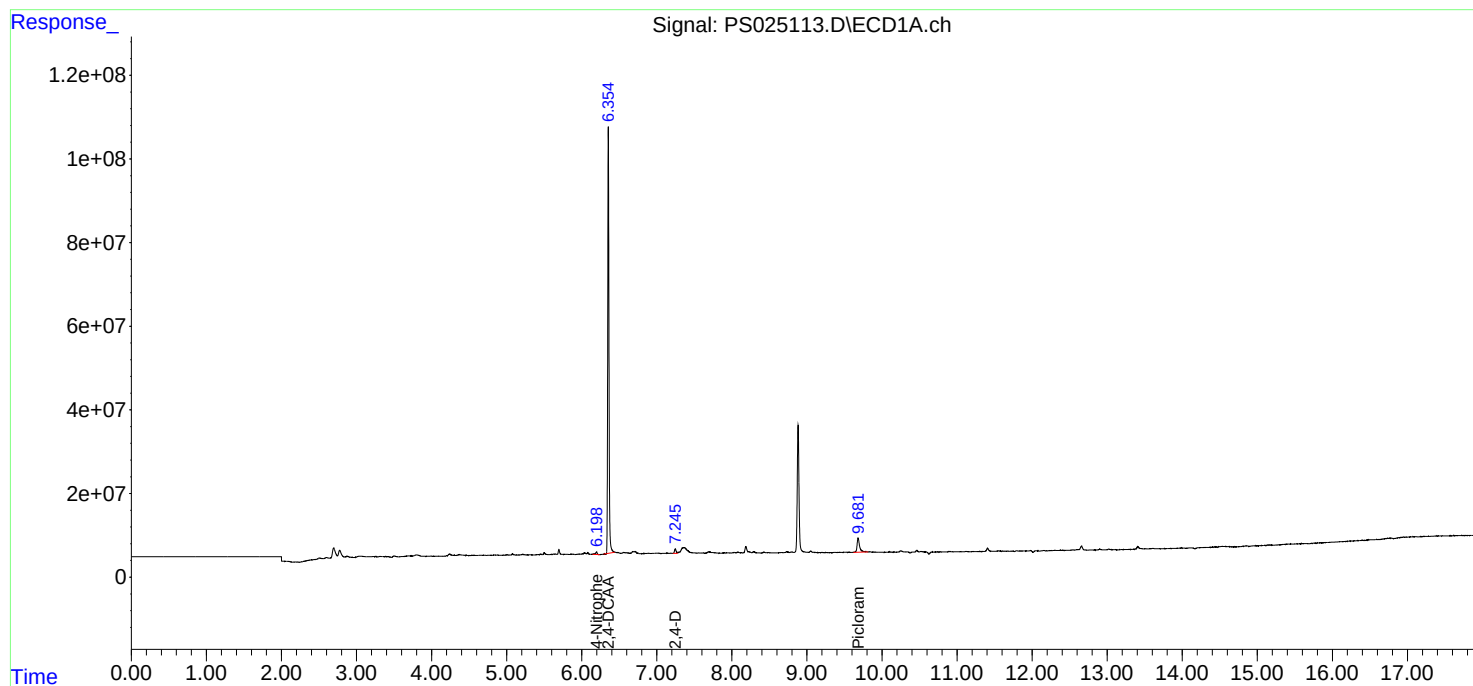


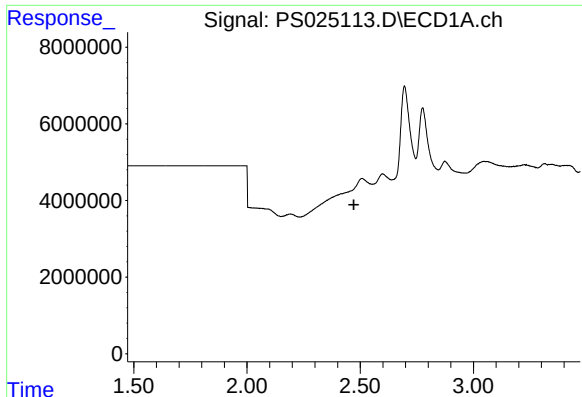

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

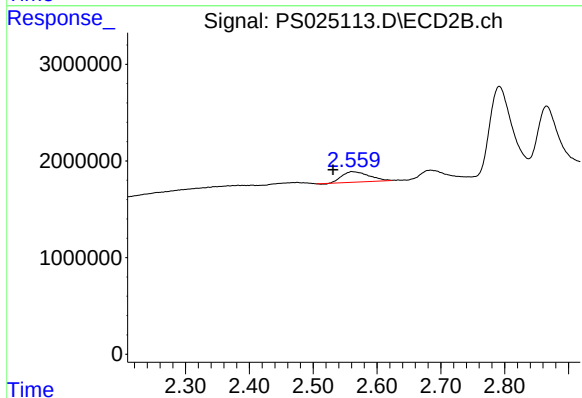


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.028 min
Response: 3174967
Conc: 2.77 ng/ml

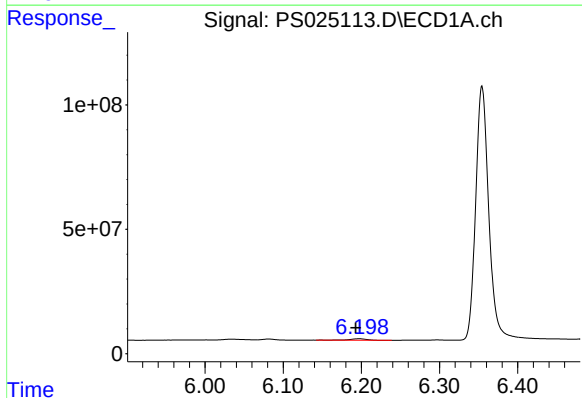


#3 4-Nitrophenol

R.T.: 6.197 min
Delta R.T.: 0.004 min
Response: 8705261
Conc: 5.91 ng/ml

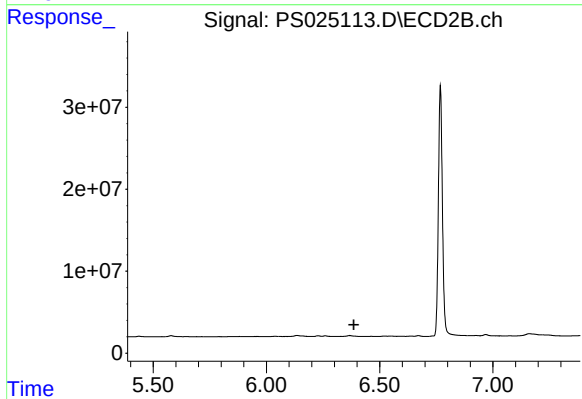

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

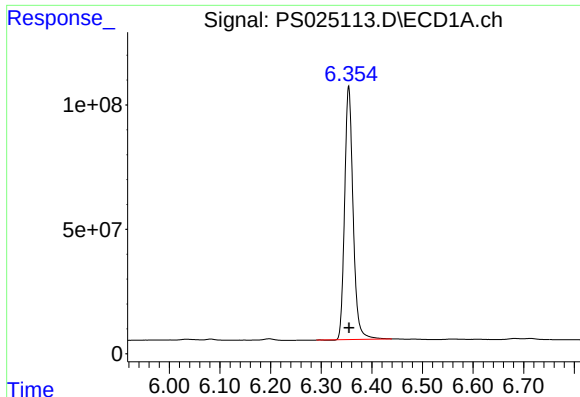

#4 2,4-DCAA


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 1183482353
Conc: 528.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

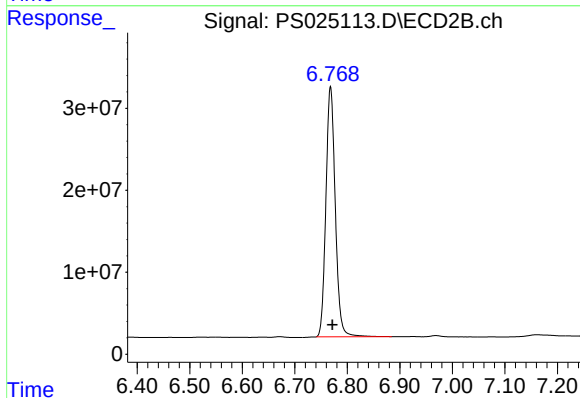


#4 2,4-DCAA

R.T.: 6.768 min
Delta R.T.: -0.003 min
Response: 378743639
Conc: 522.73 ng/ml

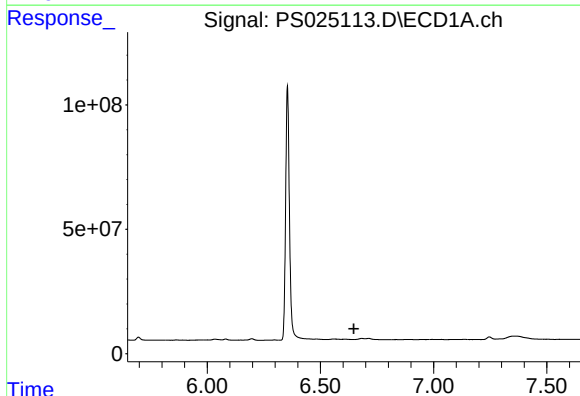


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

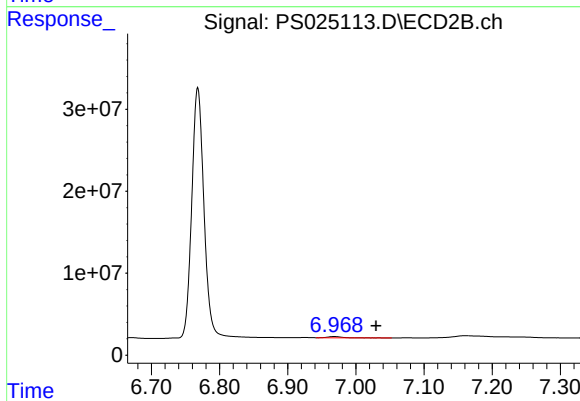

#6 MCP


R.T.: 6.968 min
Delta R.T.: -0.061 min
Response: 2174239
Conc: 1.05 ug/ml

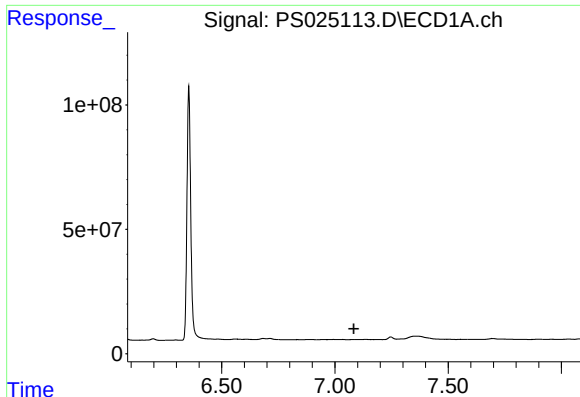

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

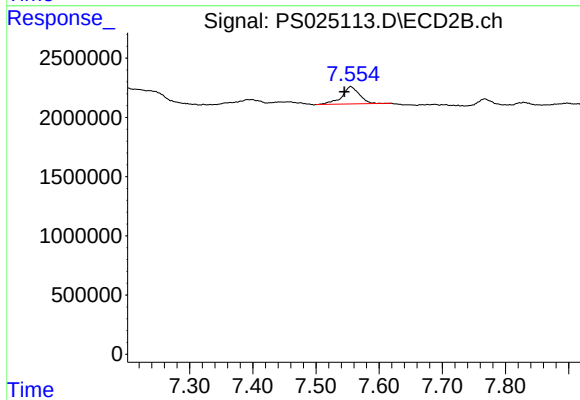


#8 DICHLORPROP

R.T.: 7.555 min
Delta R.T.: 0.010 min
Response: 2828535
Conc: 3.60 ng/ml

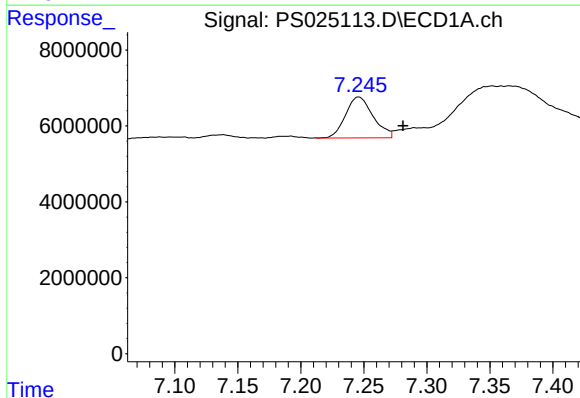


#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.035 min
Response: 16441505
Conc: 5.41 ng/ml

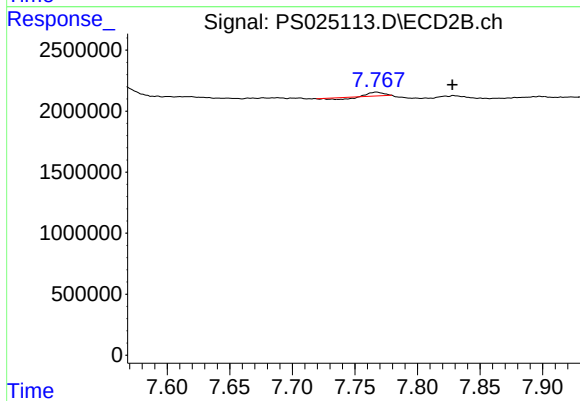

#9 2,4-D


R.T.: 7.767 min
Delta R.T.: -0.061 min
Response: 112707
Conc: N.D.

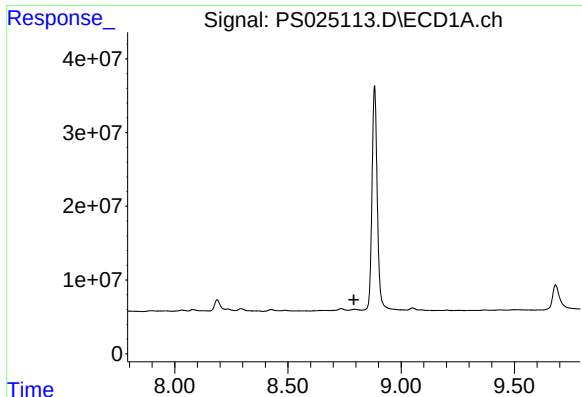

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

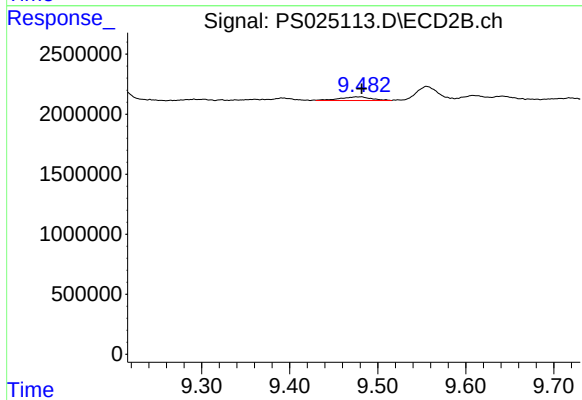


#13 2,4-DB

R.T.: 9.476 min
Delta R.T.: -0.006 min
Response: 771019
Conc: 1.39 ng/ml

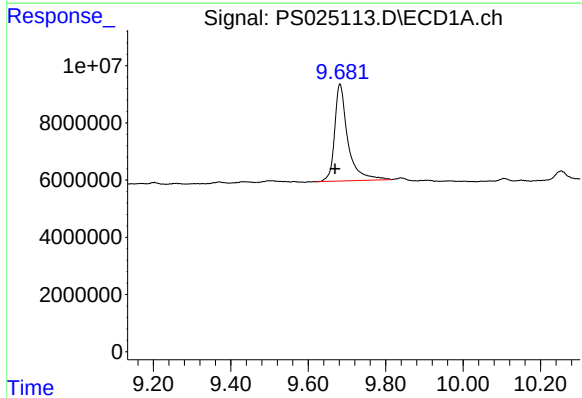


#15 Picloram

R.T.: 9.682 min
Delta R.T.: 0.012 min
Response: 80229994
Conc: 4.12 ng/ml

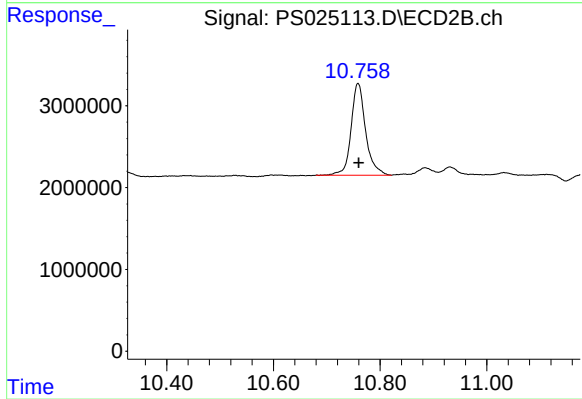

#15 Picloram


R.T.: 10.759 min
Delta R.T.: -0.001 min
Response: 21268027
Conc: 3.25 ng/ml

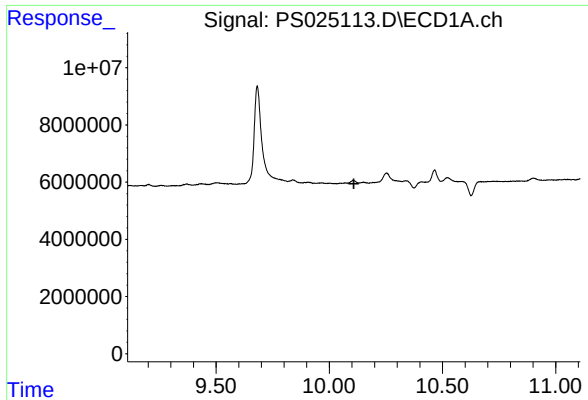

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

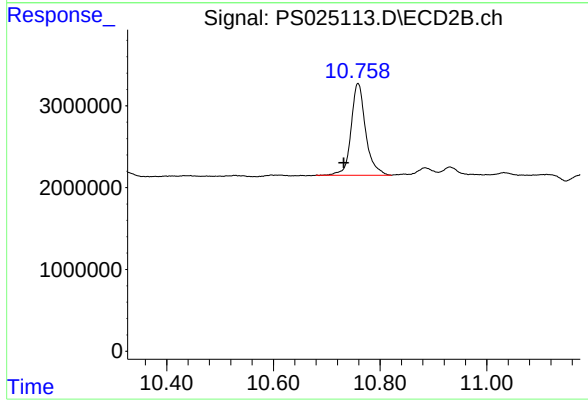

#16 DCPA

R.T.: 10.759 min
Delta R.T.: 0.027 min
Response: 21268027
Conc: 3.92 ng/ml