

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121523\
 Data File : PS025117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 14:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 15:43:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.769	1203.9E6	387.5E6	537.980	534.779
Target Compounds							
1) T	Dalapon	2.508	2.563	9300454	4371216	3.225	3.811
2) T	3,5-DICHL...	5.696	0.000	3827208	0	1.132	N.D. #
3) T	4-Nitroph...	6.196	0.000	8035155	0	5.456	N.D. #
5) T	DICAMBA	0.000	6.969	0	3816592	N.D.	1.232
6) T	MCPD	6.682	6.969f	2522468	3816592	<MDL	1.840 #
7) T	MCPA	0.000	7.219	0	5033346	N.D.	1.530
8) T	DICHLORPROP	0.000	7.557	0	3833790	N.D.	4.874
9) T	2,4-D	7.245	7.769f	30296061	659093	9.975	<MDL #
11) T	2,4,5-TP ...	0.000	8.604	0	246758	N.D.	<MDL
12) T	2,4,5-T	0.000	8.978	0	744890	N.D.	<MDL
15) T	Picloram	9.686	10.760	18828955	6357471	<MDL	<MDL #
16) T	DCPA	0.000	10.760	0	6357471	N.D.	1.173


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121523\
Data File : PS025117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 14:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 15:43:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

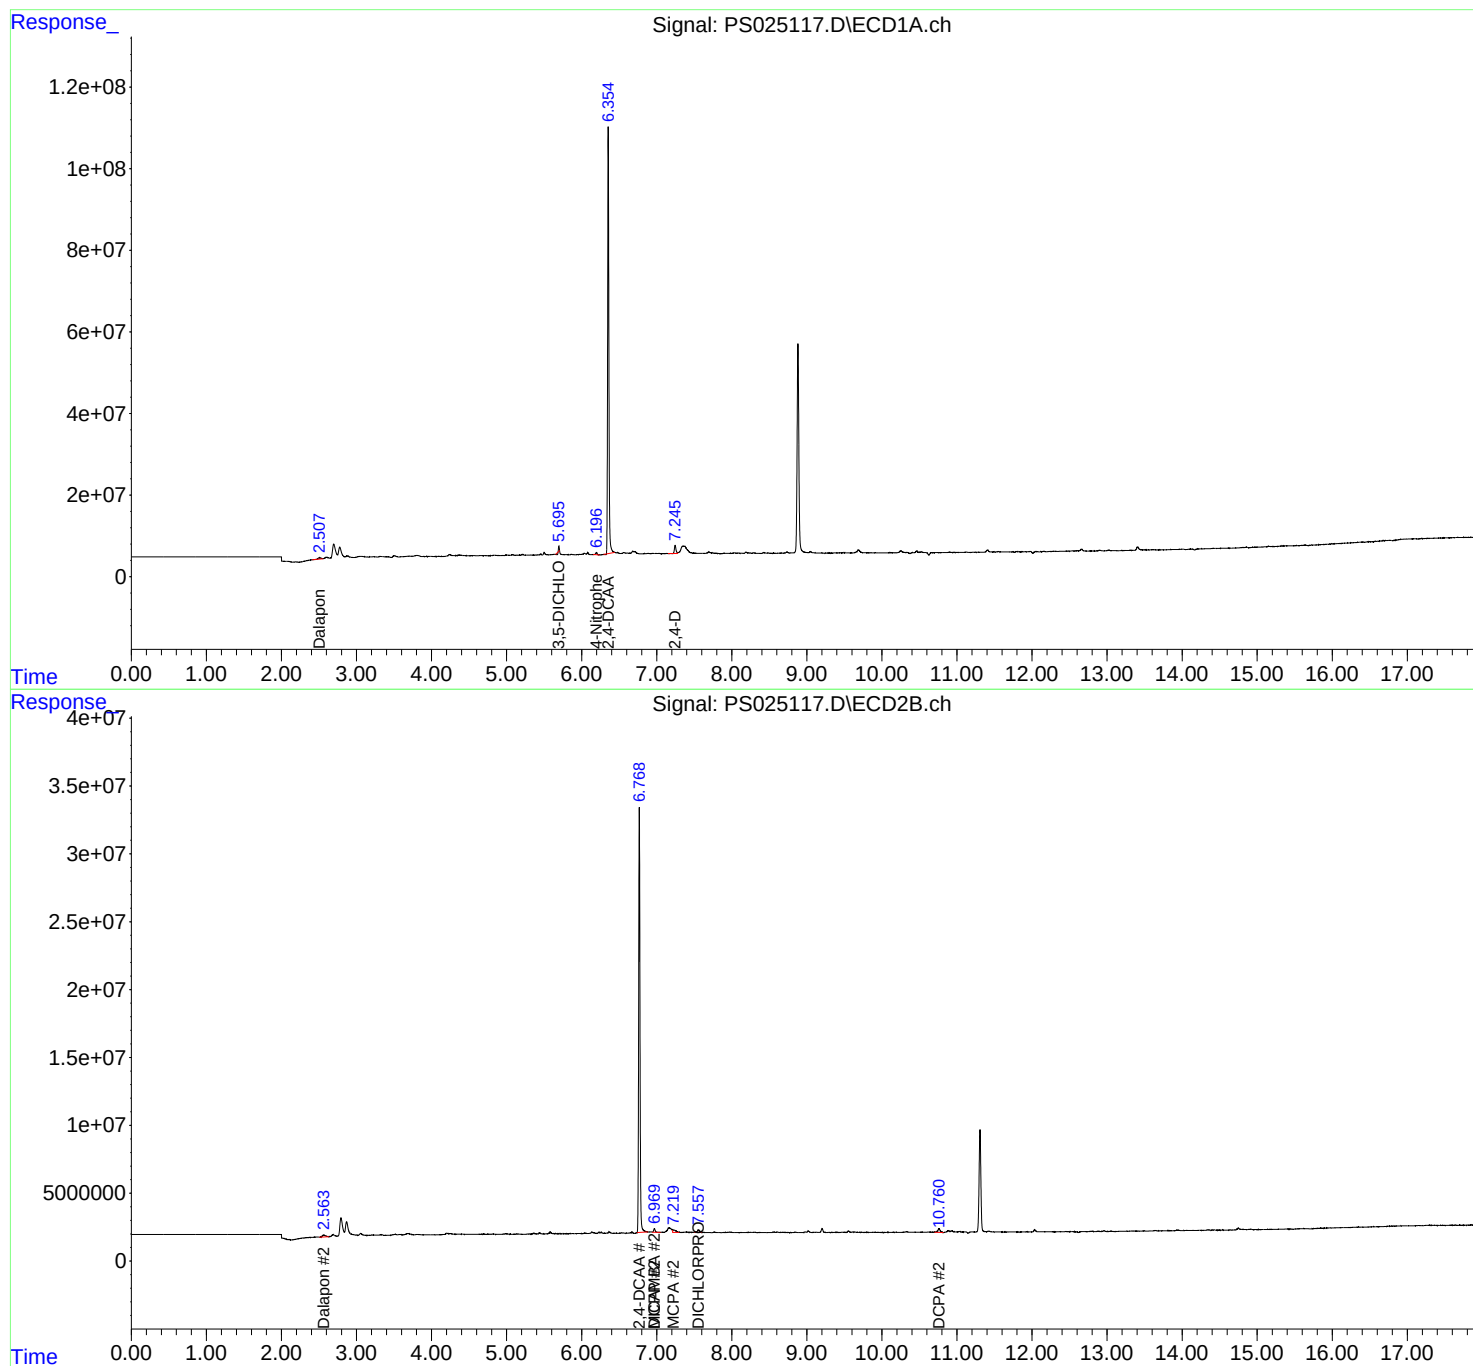


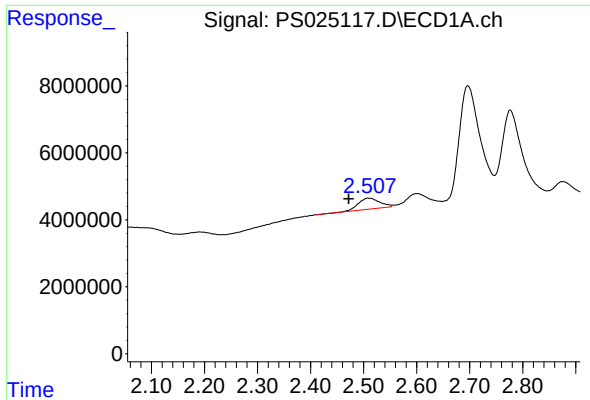

#1 Dalapon


R.T.: 2.508 min
Delta R.T.: 0.036 min
Response: 9300454
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

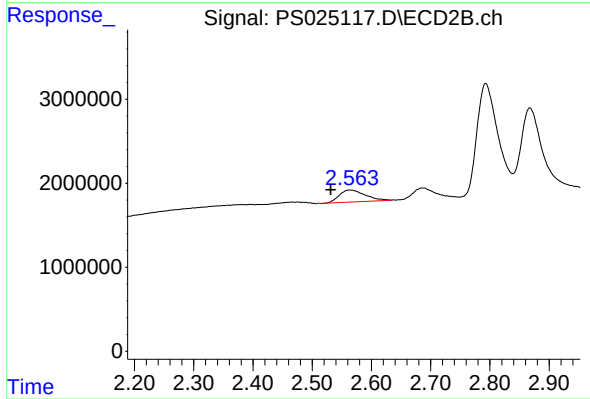


#1 Dalapon

R.T.: 2.563 min
Delta R.T.: 0.032 min
Response: 4371216
Conc: 3.81 ng/ml

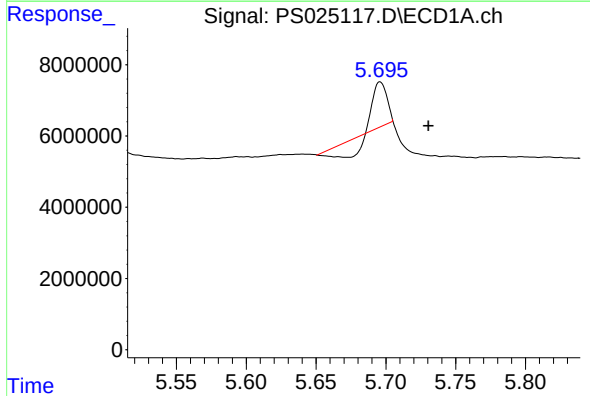


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.696 min
Delta R.T.: -0.034 min
Response: 3827208
Conc: 1.13 ng/ml

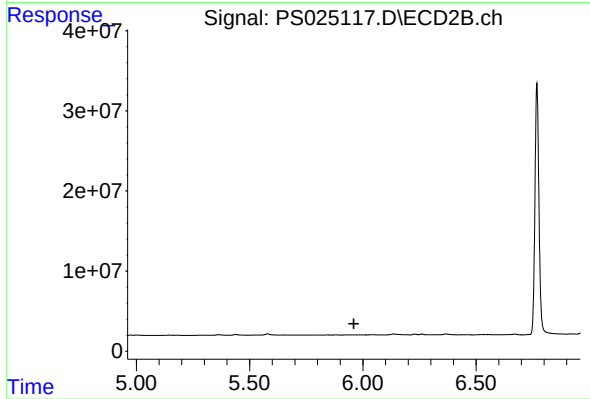

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

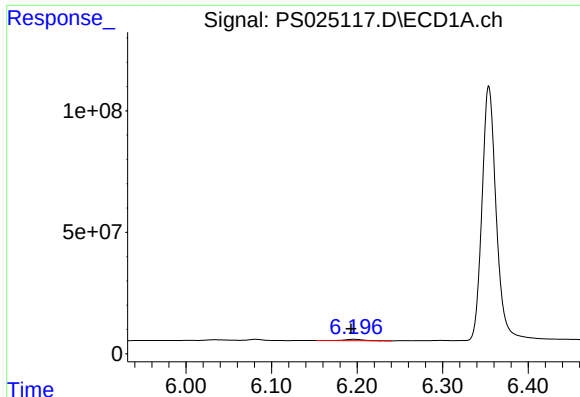

#3 4-Nitrophenol


R.T.: 6.196 min
Delta R.T.: 0.003 min
Response: 8035155
Conc: 5.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

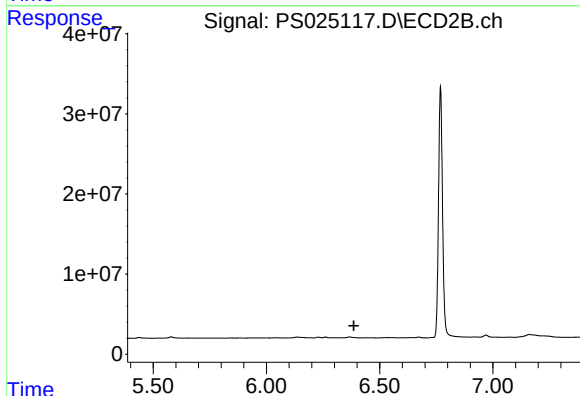


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

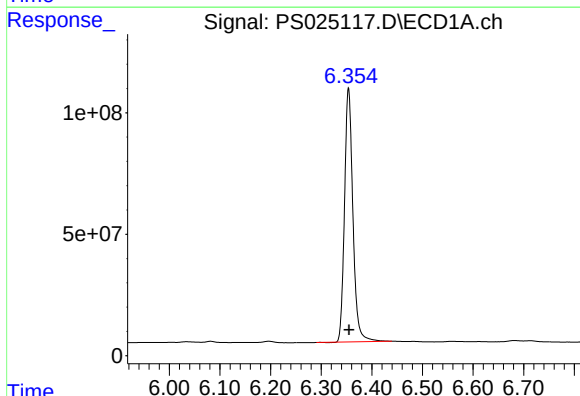


#4 2,4-DCAA

R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 1203916236
Conc: 537.98 ng/ml

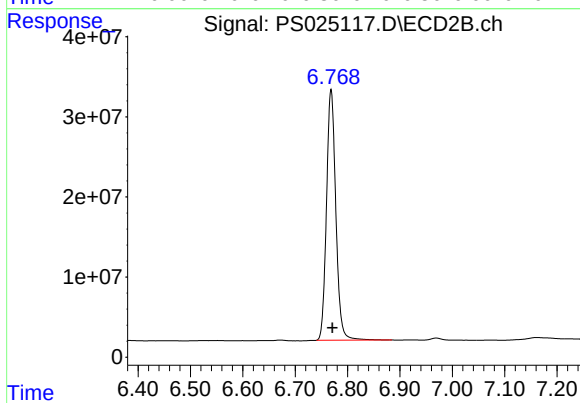

#4 2,4-DCAA


R.T.: 6.769 min
Delta R.T.: -0.003 min
Response: 387476510
Conc: 534.78 ng/ml

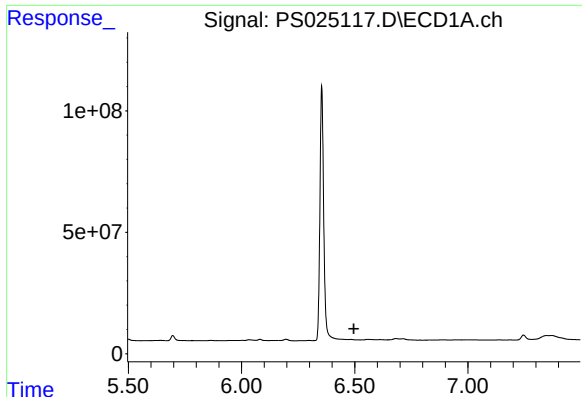

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

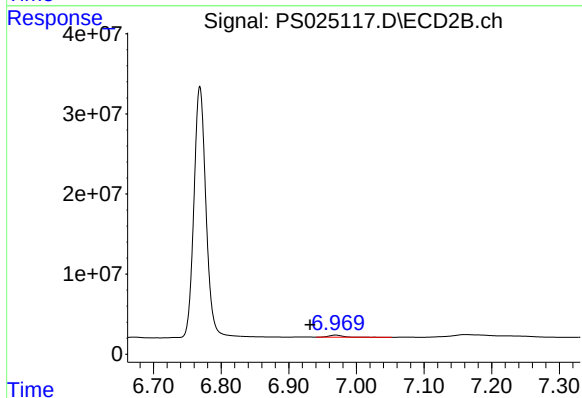


#5 DICAMBA

R.T.: 6.969 min
Delta R.T.: 0.037 min
Response: 3816592
Conc: 1.23 ng/ml

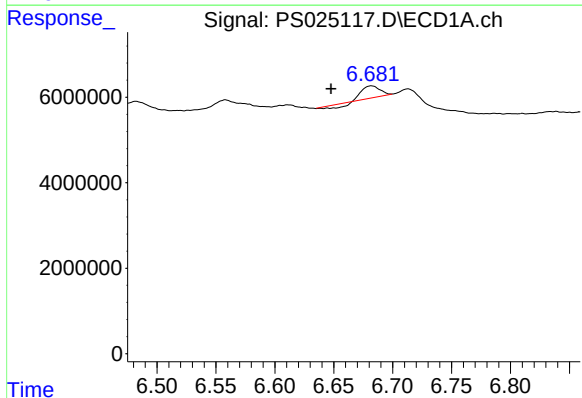


#6 MCP

R.T.: 6.682 min
Delta R.T.: 0.034 min
Response: 2522468
Conc: N.D.

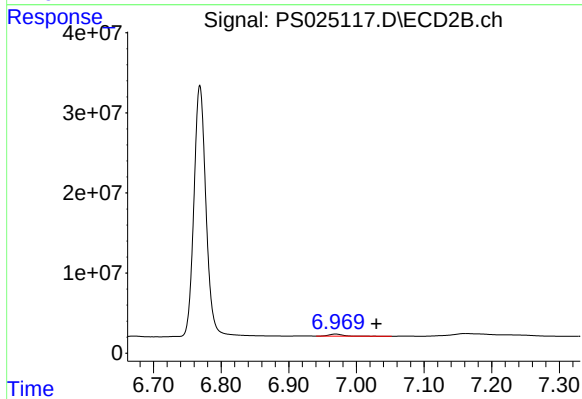

#6 MCP


R.T.: 6.969 min
Delta R.T.: -0.060 min
Response: 3816592
Conc: 1.84 ug/ml

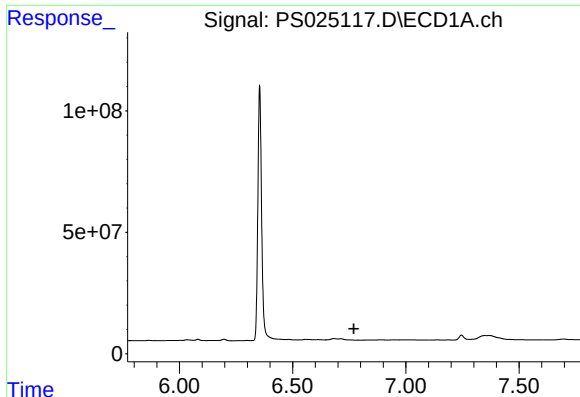

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

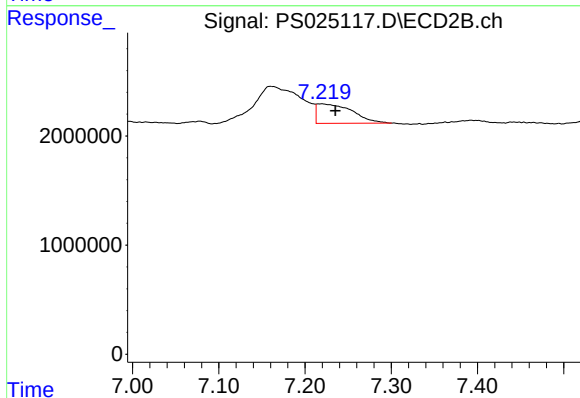


#7 MCPA

R.T.: 7.219 min
Delta R.T.: -0.016 min
Response: 5033346
Conc: 1.53 ug/ml

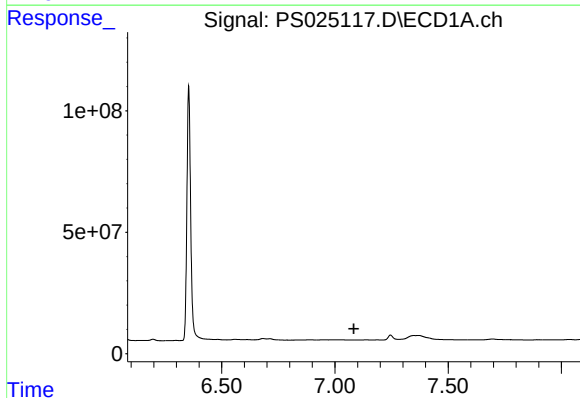


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

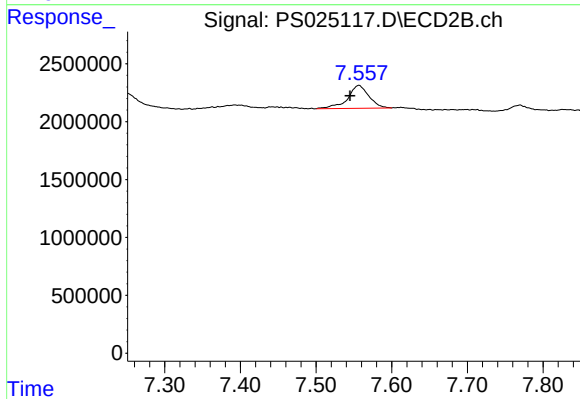

#8 DICHLORPROP


R.T.: 7.557 min
Delta R.T.: 0.012 min
Response: 3833790
Conc: 4.87 ng/ml

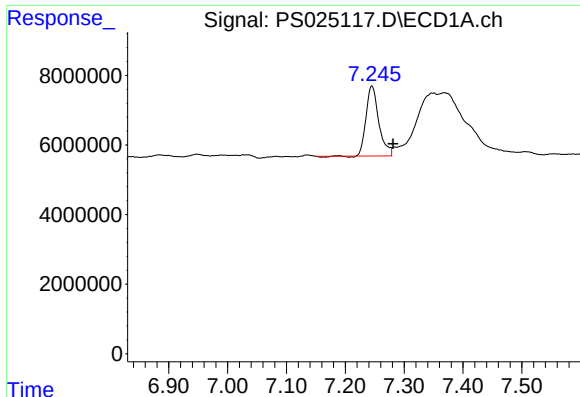

#9 2,4-D


R.T.: 7.245 min
Delta R.T.: -0.036 min
Response: 30296061
Conc: 9.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

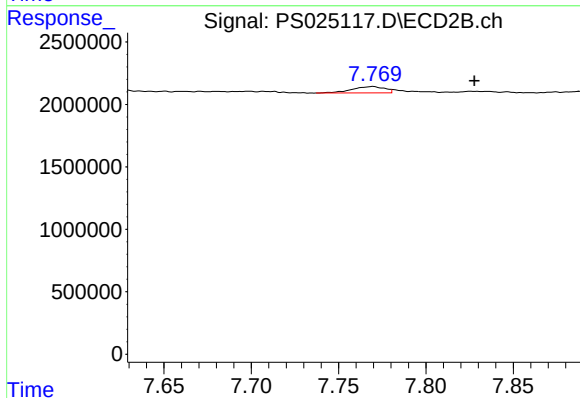


#9 2,4-D

R.T.: 7.769 min
Delta R.T.: -0.058 min
Response: 659093
Conc: N.D.

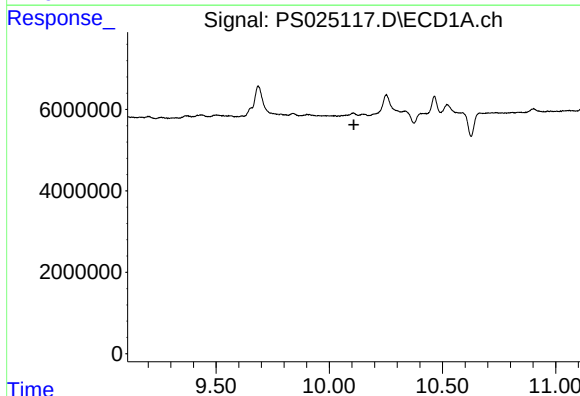

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.109 min
Response: 0
Conc: N.D.

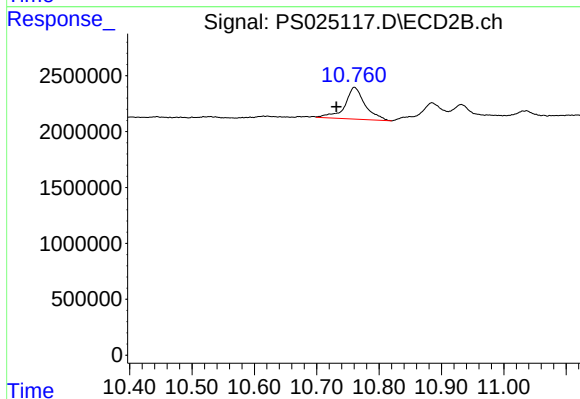

#16 DCPA

R.T.: 10.760 min
Delta R.T.: 0.029 min
Response: 6357471
Conc: 1.17 ng/ml