

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121523\
 Data File : PS025130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 22:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 02:33:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.353	6.768	1215.1E6	386.6E6	542.979	533.567
Target Compounds							
1) T	Dalapon	2.507	2.561	7956192	3637428	2.759	3.171
2) T	3,5-DICHL...	5.695	0.000	10230358	0	3.027	N.D. #
3) T	4-Nitroph...	6.195	0.000	12368760	0	8.399	N.D. #
5) T	DICAMBA	0.000	6.968	0	4272289	N.D.	1.379
6) T	MCP	6.679	7.074f	6622080	1164401	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.553	0	5714884	N.D.	7.265
9) T	2,4-D	7.244	7.766f	29212910	973306	9.618	<MDL #
10) T	Pentachlo...	0.000	8.249	0	657489	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.606	0	873118	N.D.	<MDL
12) T	2,4,5-T	0.000	8.976	0	970404	N.D.	<MDL
15) T	Picloram	9.679	10.758	16586073	6924500	<MDL	1.058 #
16) T	DCPA	10.132	10.758	9190896	6924500	<MDL	1.278 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121523\
Data File : PS025130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 22:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 02:33:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

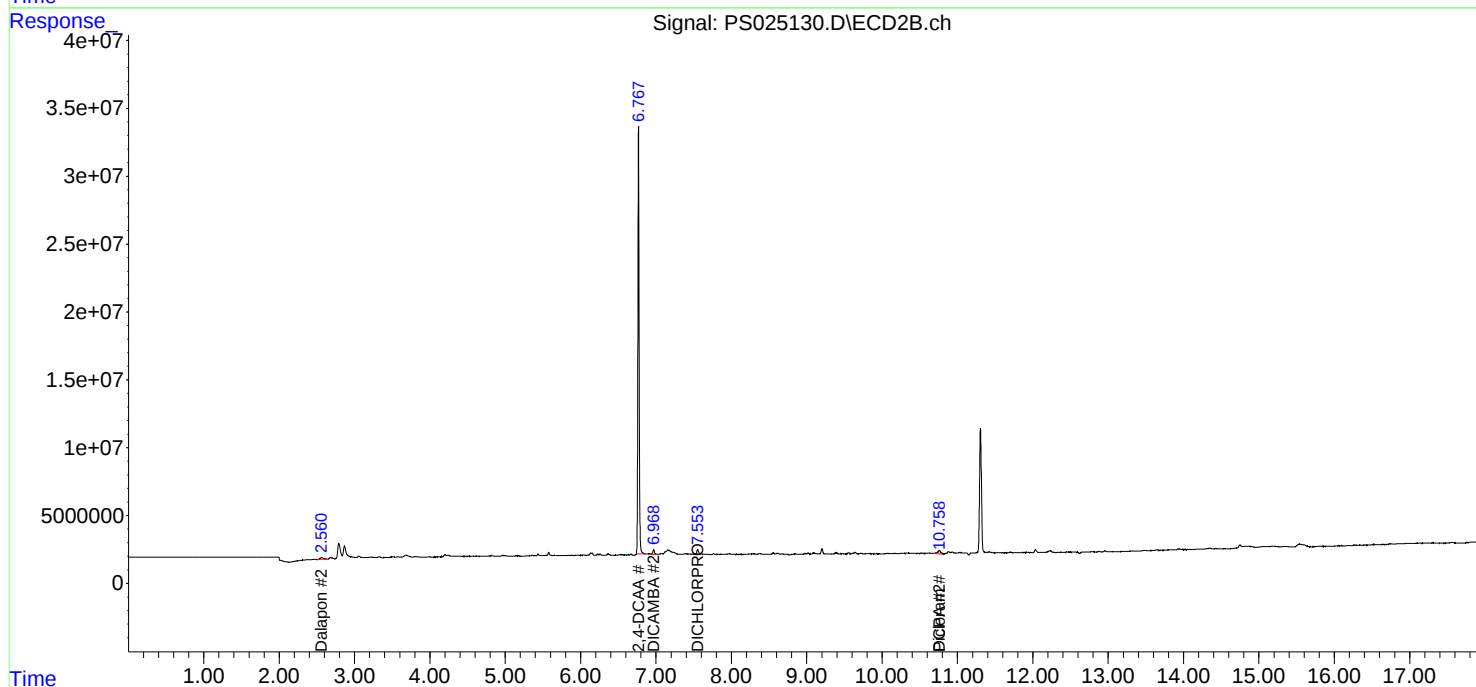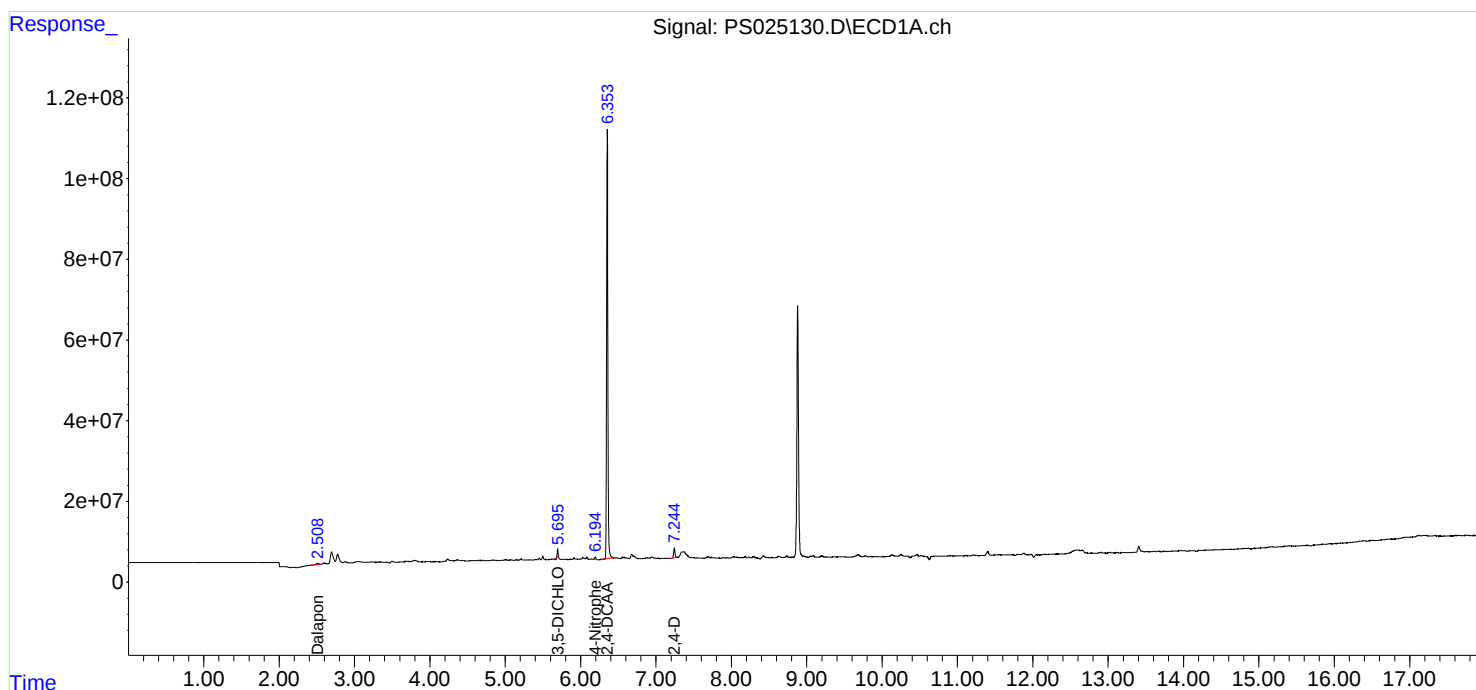


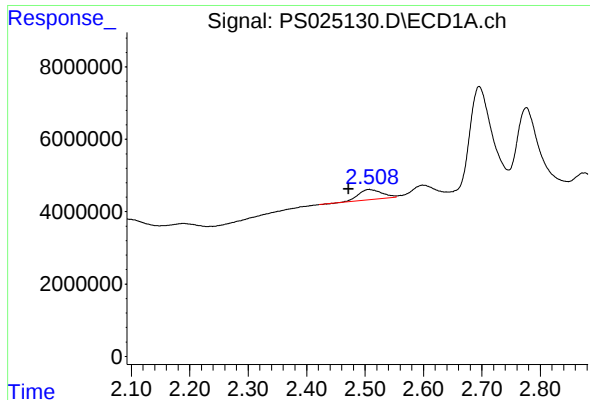

#1 Dalapon


R.T.: 2.507 min
Delta R.T.: 0.035 min
Response: 7956192
Conc: 2.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

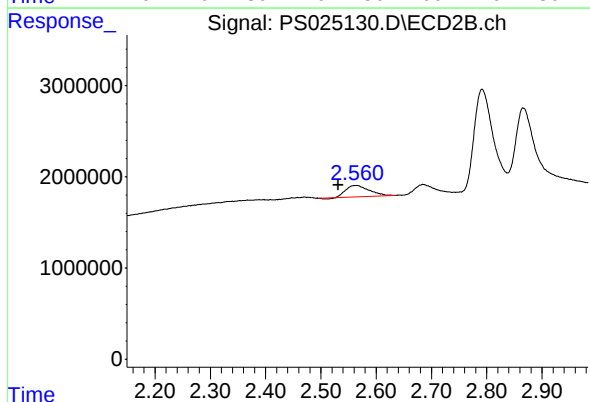


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.030 min
Response: 3637428
Conc: 3.17 ng/ml

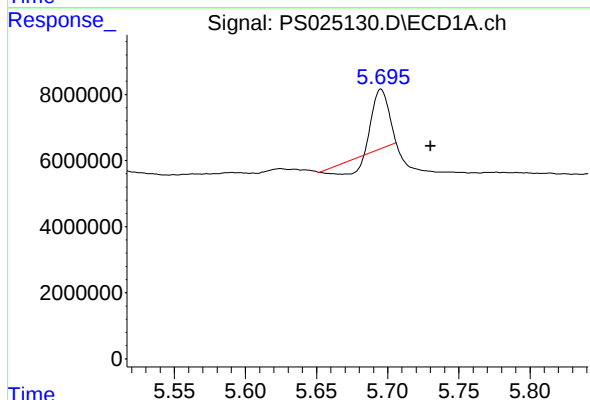


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.695 min
Delta R.T.: -0.035 min
Response: 10230358
Conc: 3.03 ng/ml

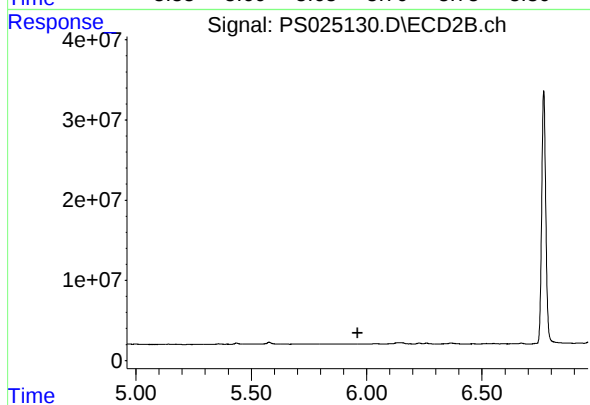

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

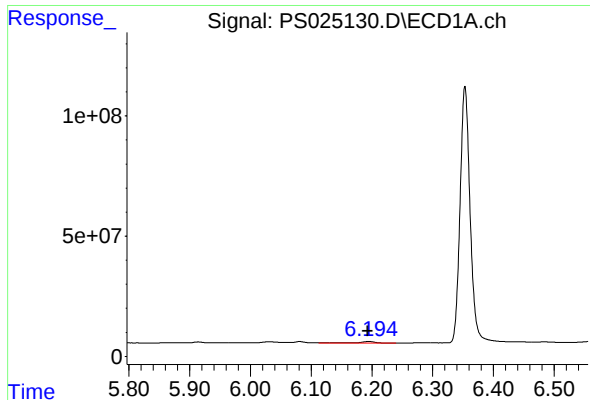

#3 4-Nitrophenol


R.T.: 6.195 min
Delta R.T.: 0.002 min
Response: 12368760
Conc: 8.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

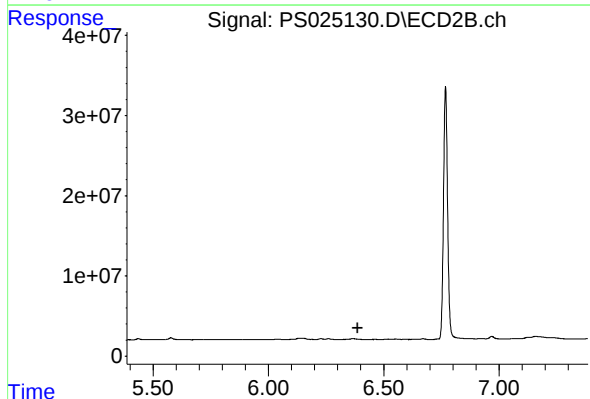


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

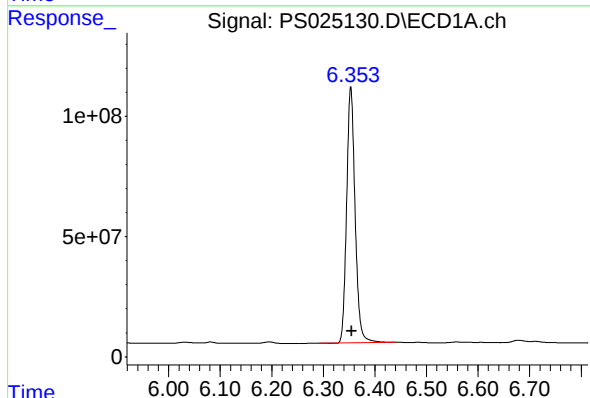


#4 2,4-DCAA

R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 1215102470
Conc: 542.98 ng/ml

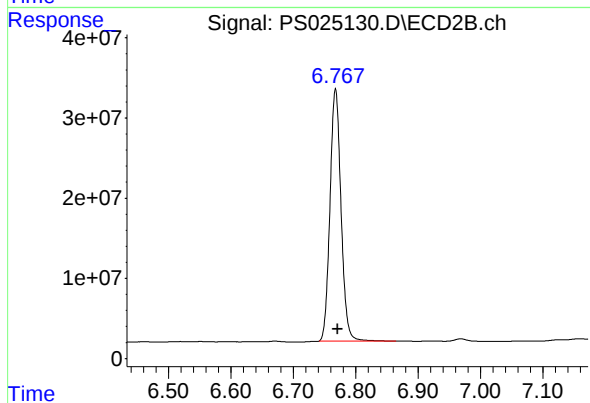

#4 2,4-DCAA


R.T.: 6.768 min
Delta R.T.: -0.003 min
Response: 386598331
Conc: 533.57 ng/ml

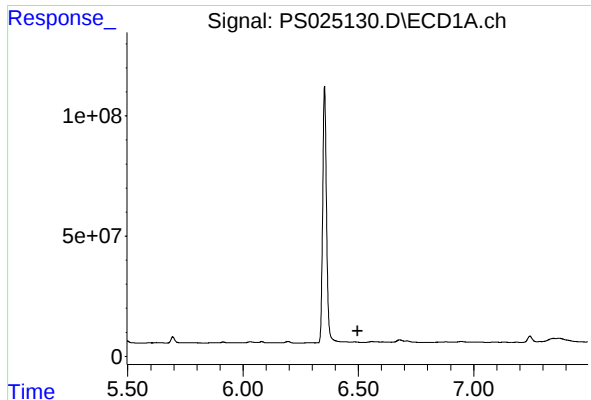

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

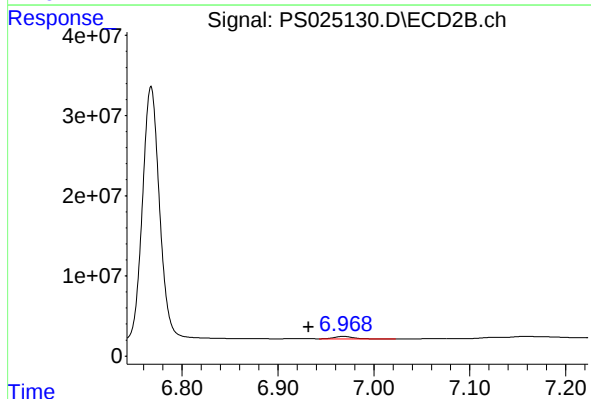


#5 DICAMBA

R.T.: 6.968 min
Delta R.T.: 0.037 min
Response: 4272289
Conc: 1.38 ng/ml

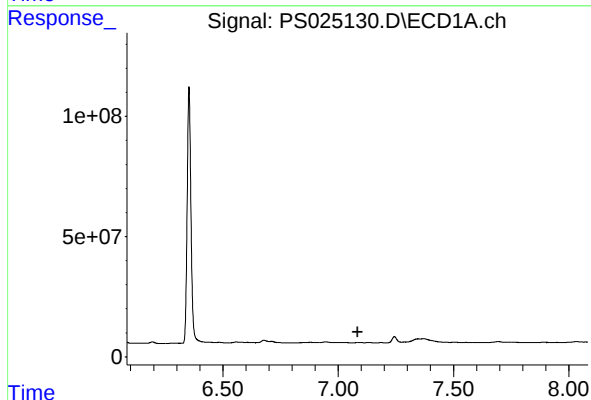


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

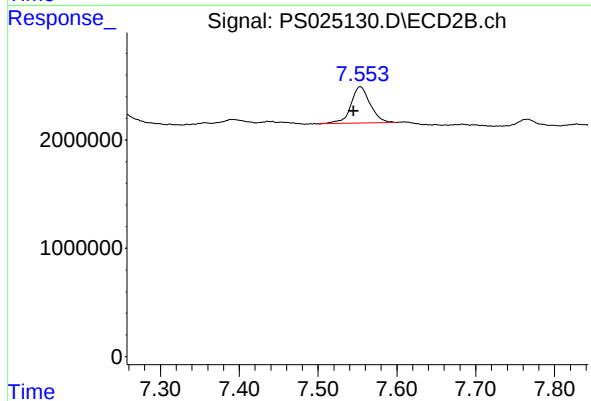

#8 DICHLORPROP


R.T.: 7.553 min
Delta R.T.: 0.008 min
Response: 5714884
Conc: 7.26 ng/ml

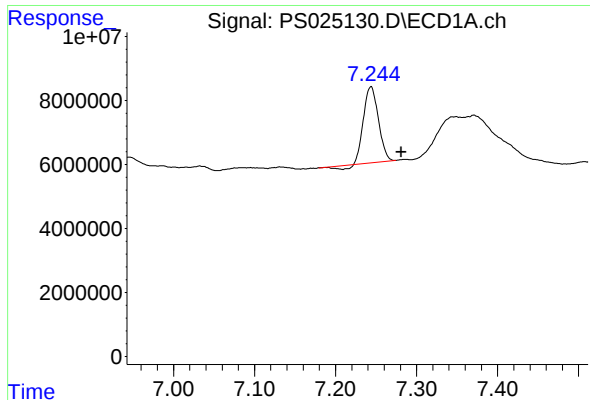

#9 2,4-D


R.T.: 7.244 min
Delta R.T.: -0.037 min
Response: 29212910
Conc: 9.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

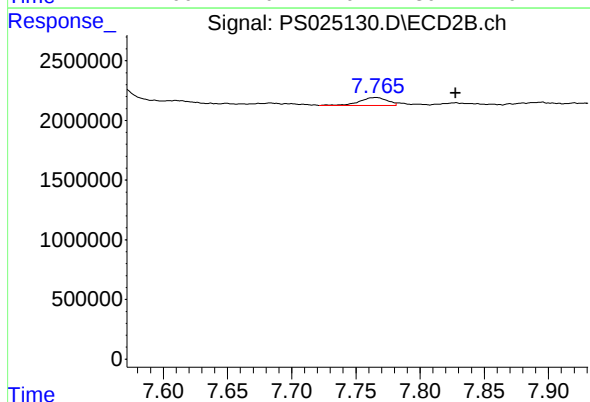


#9 2,4-D

R.T.: 7.766 min
Delta R.T.: -0.062 min
Response: 973306
Conc: N.D.

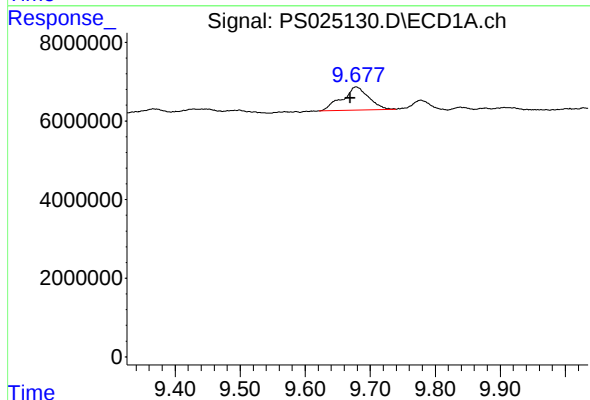


#15 Picloram

R.T.: 9.679 min
Delta R.T.: 0.009 min
Response: 16586073
Conc: N.D.

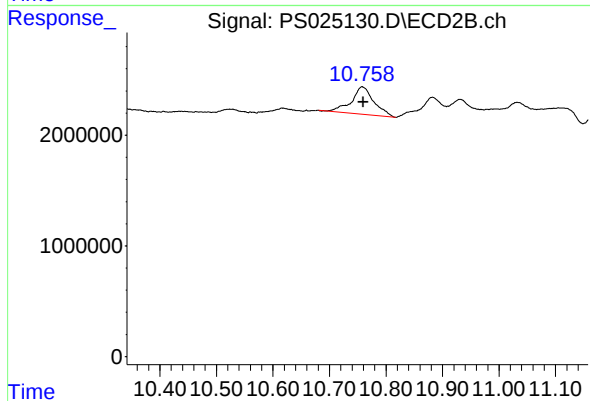

#15 Picloram


R.T.: 10.758 min
Delta R.T.: -0.002 min
Response: 6924500
Conc: 1.06 ng/ml

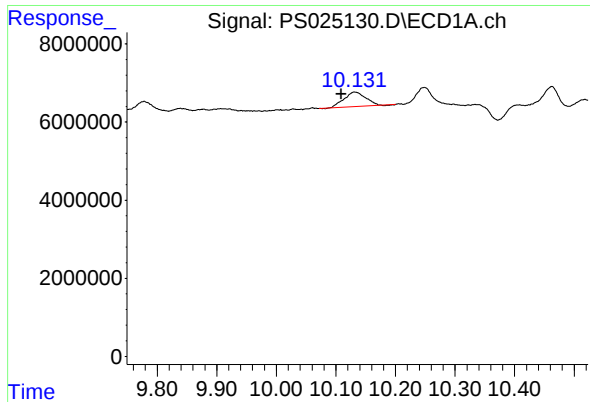

#16 DCPA

R.T.: 10.132 min
Delta R.T.: 0.023 min
Response: 9190896
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

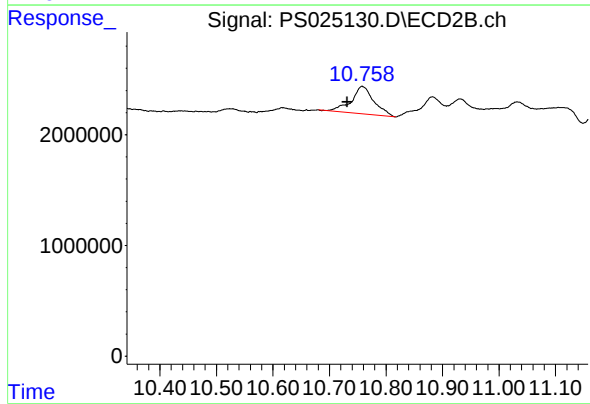

#16 DCPA

R.T.: 10.758 min
Delta R.T.: 0.026 min
Response: 6924500
Conc: 1.28 ng/ml