

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121525\
 Data File : PS032750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2025 22:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 01:17:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.310	7.984	2381.9E6	1135.8E6	333.784	405.592
Target Compounds							
1) T	Dalapon	2.736f	0.000	323.4E6	0	30.168	N.D. #
2) T	3,5-DICHL...	6.465	0.000	7086966	0	<MDL	N.D. #
3) T	4-Nitroph...	7.088	7.461f	11625318	1472287	2.582	<MDL #
5) T	DICAMBA	0.000	8.192	0	3246648	N.D.	<MDL
6) T	MCPD	0.000	8.292	0	2728550	N.D.	<MDL
7) T	MCPA	0.000	8.578f	0	4204373	N.D.	<MDL
8) T	DICHLORPROP	8.197f	0.000	8724652	0	1.361	N.D. #
10) T	Pentachlo...	8.796	0.000	26856392	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.358	10.162f	10825541	7671975	<MDL	<MDL #
12) T	2,4,5-T	9.659	10.619	8145328	12167232	<MDL	<MDL #
13) T	2,4-DB	10.211f	0.000	14194951	0	2.244	N.D. #
14) T	DINOSEB	11.421f	11.579	151.4E6	68871920	5.579	5.463
15) T	Picloram	11.260	12.702	76373138	29636317	1.599	1.187 #
16) T	DCPA	11.745	12.644	250.4E6	15105280	5.204	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121525\
Data File : PS032750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2025 22:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 01:17:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

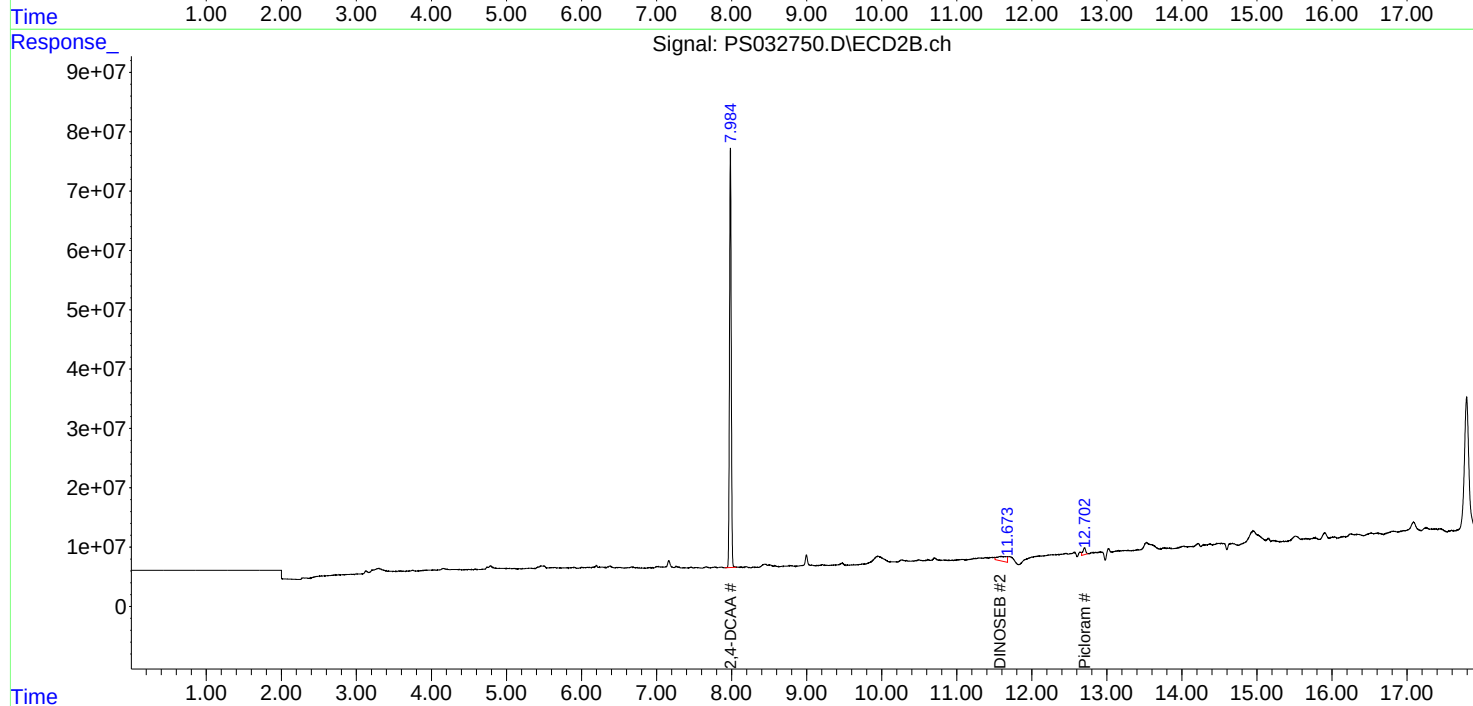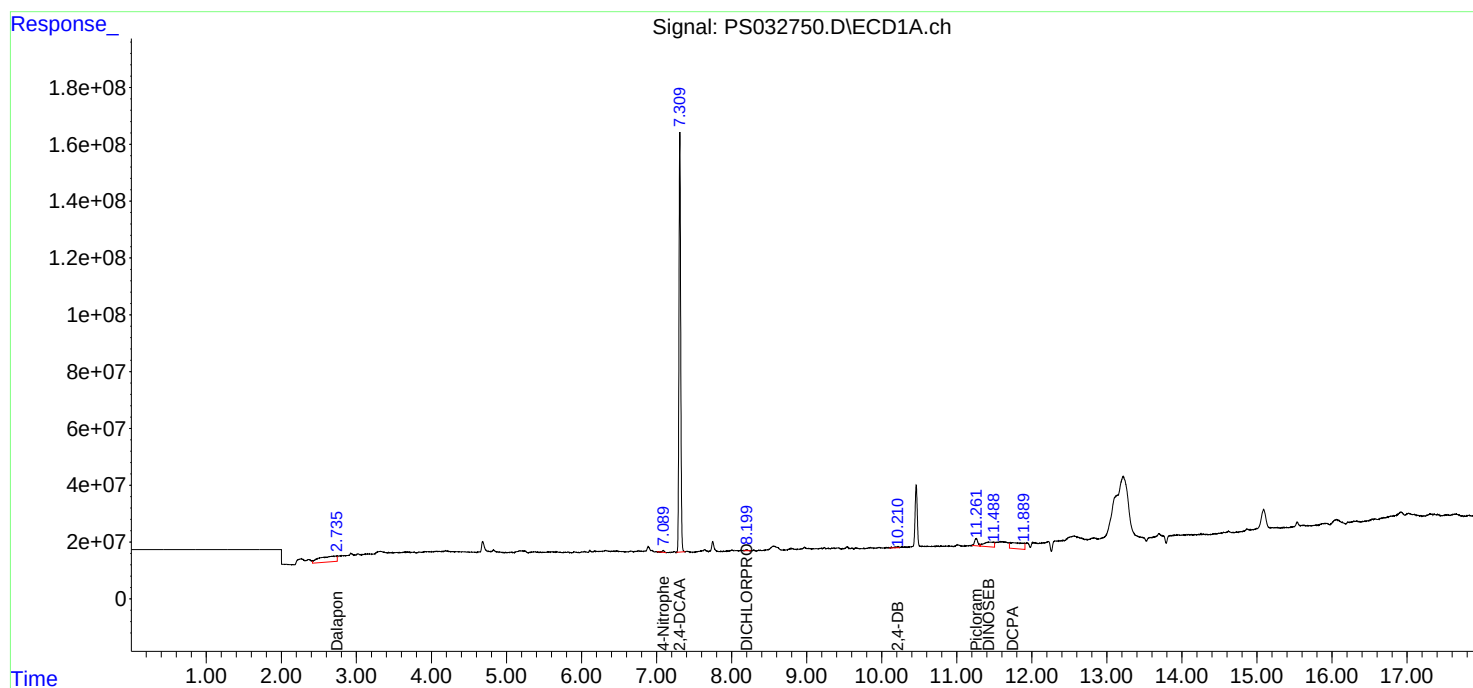


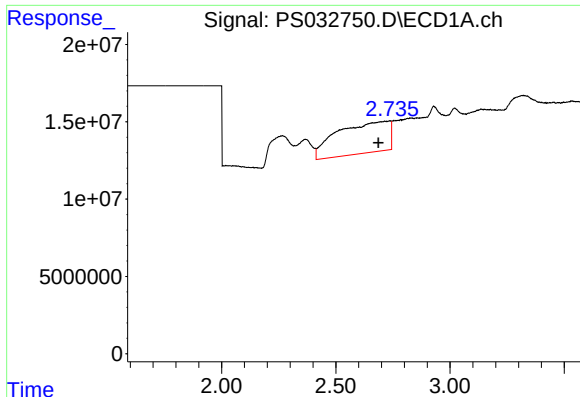

#1 Dalapon


R.T.: 2.736 min
Delta R.T.: 0.050 min
Response: 323385180
Conc: 30.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

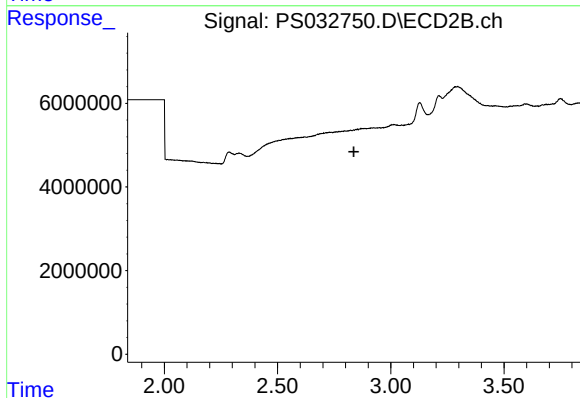


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.837 min
Response: 0
Conc: N.D.

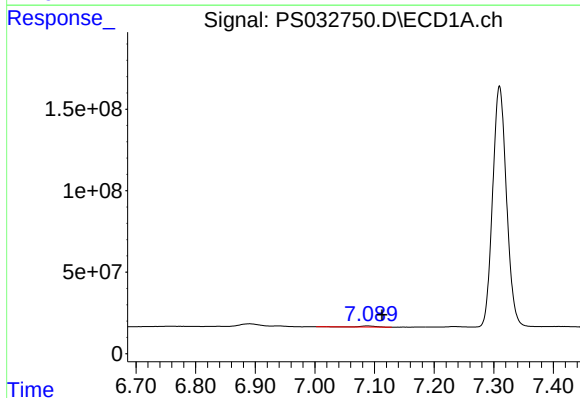


#3 4-Nitrophenol

R.T.: 7.088 min
Delta R.T.: -0.024 min
Response: 11625318
Conc: 2.58 ng/ml

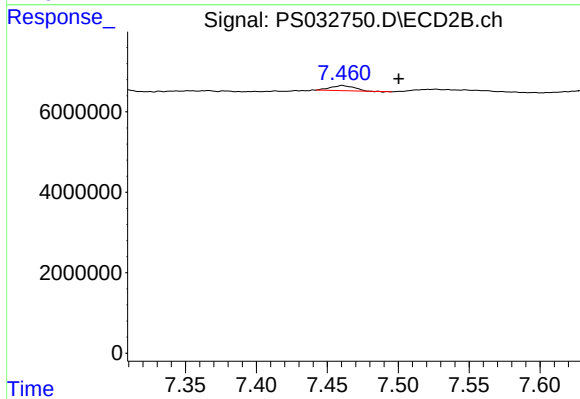

#3 4-Nitrophenol


R.T.: 7.461 min
Delta R.T.: -0.040 min
Response: 1472287
Conc: N.D.

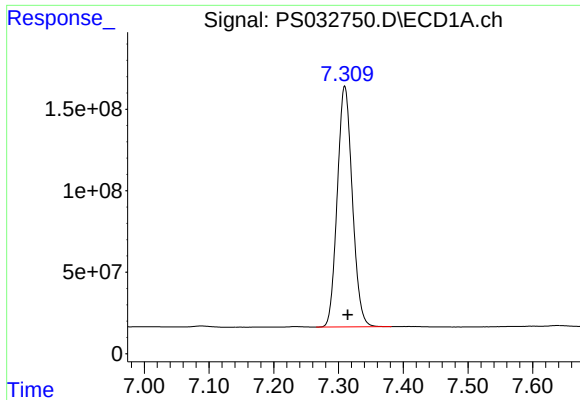

#4 2,4-DCAA


R.T.: 7.310 min
Delta R.T.: -0.005 min
Response: 2381864003
Conc: 333.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

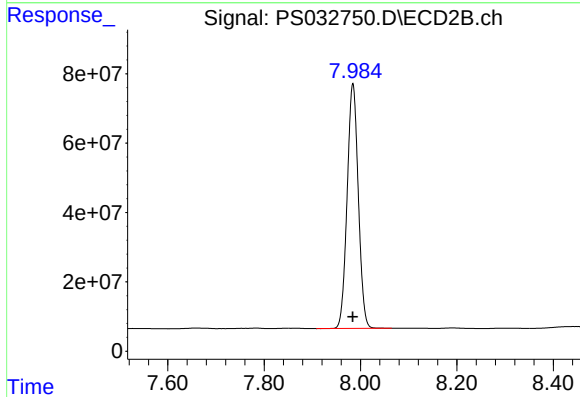


#4 2,4-DCAA

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 1135789447
Conc: 405.59 ng/ml

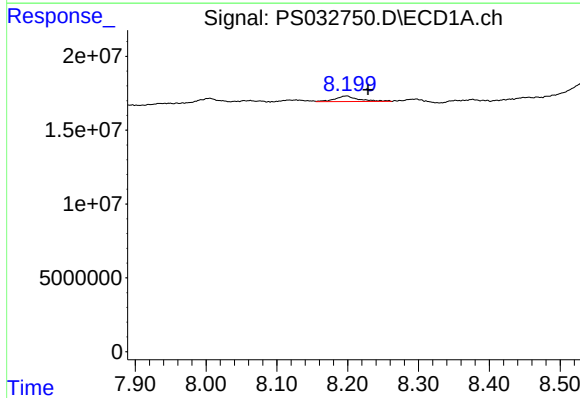


#8 DICHLORPROP

R.T.: 8.197 min
Delta R.T.: -0.031 min
Response: 8724652
Conc: 1.36 ng/ml

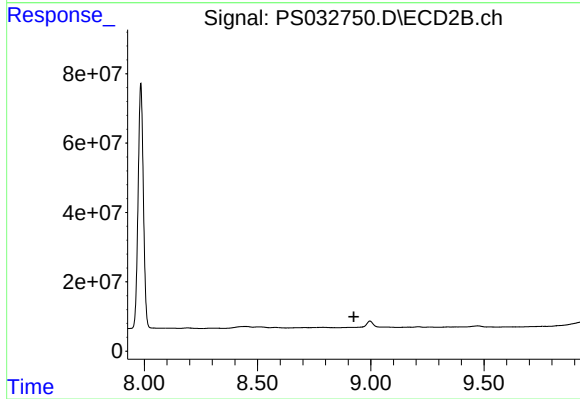

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.925 min
Response: 0
Conc: N.D.

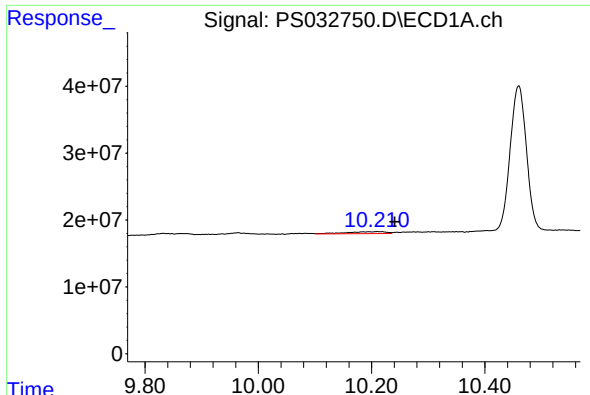

#13 2,4-DB


R.T.: 10.211 min
Delta R.T.: -0.030 min
Response: 14194951
Conc: 2.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

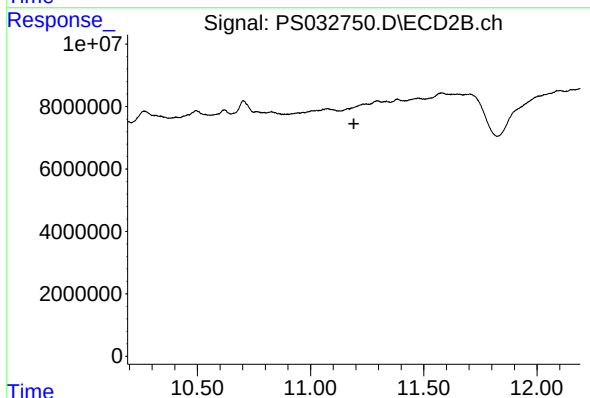


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 11.191 min
Response: 0
Conc: N.D.

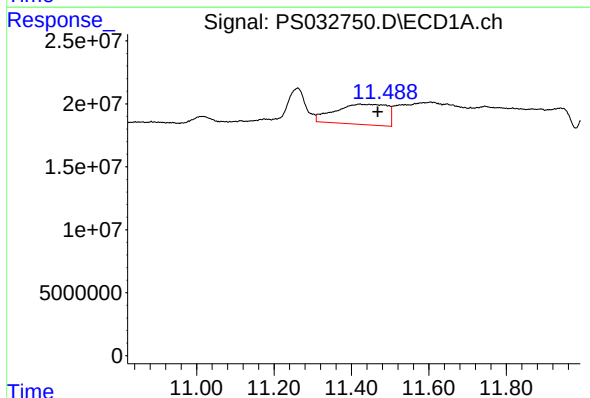


#14 DINOSEB

R.T.: 11.421 min
Delta R.T.: -0.046 min
Response: 151364150
Conc: 5.58 ng/ml

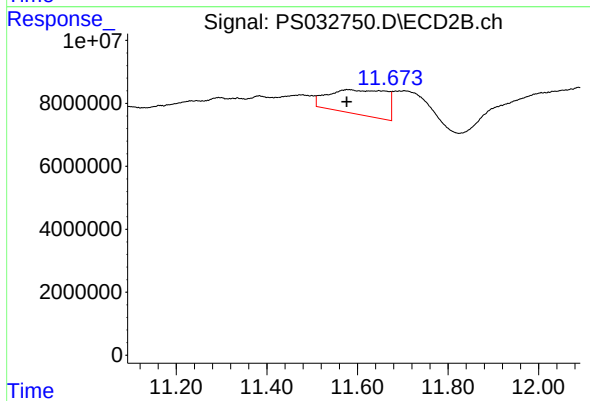

#14 DINOSEB


R.T.: 11.579 min
Delta R.T.: 0.003 min
Response: 68871920
Conc: 5.46 ng/ml

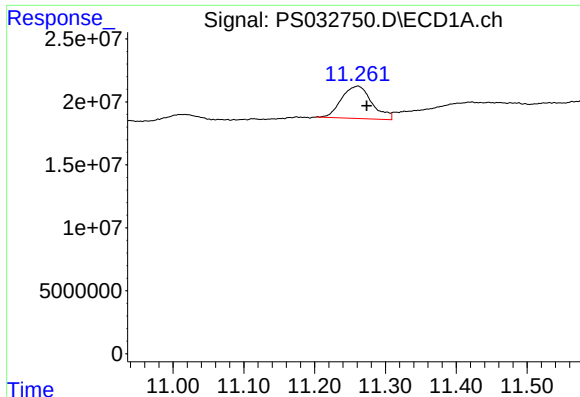

#15 Picloram


R.T.: 11.260 min
Delta R.T.: -0.014 min
Response: 76373138
Conc: 1.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

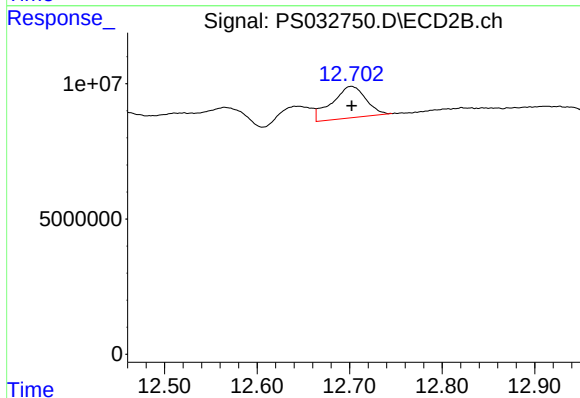


#15 Picloram

R.T.: 12.702 min
Delta R.T.: 0.000 min
Response: 29636317
Conc: 1.19 ng/ml

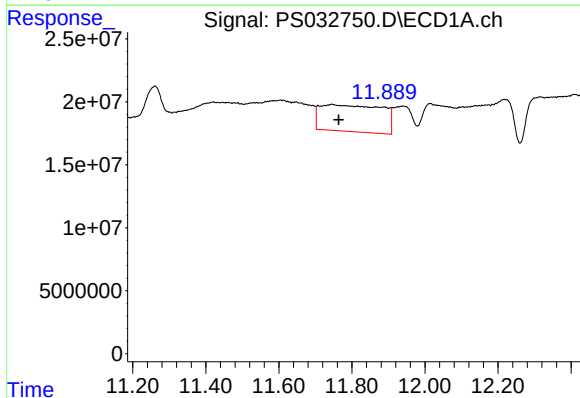

#16 DCPA

R.T.: 11.745 min
Delta R.T.: -0.019 min
Response: 250350690
Conc: 5.20 ng/ml

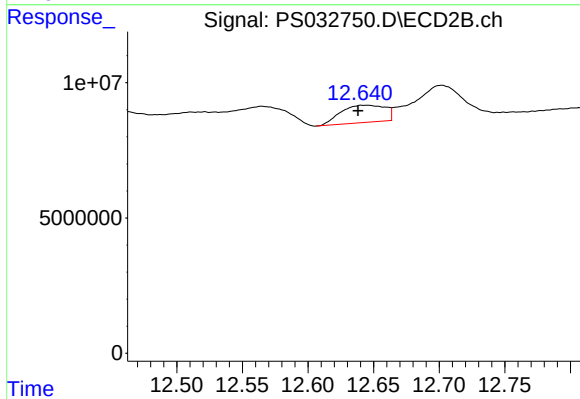

#16 DCPA

R.T.: 12.644 min
Delta R.T.: 0.006 min
Response: 15105280
Conc: N.D.