

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121525\
 Data File : PS032741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2025 19:05
 Operator : AR\AJ
 Sample : Q3854-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ETGI-360

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/16/2025
 Supervised By :Yogesh Patel 12/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 01:16:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.307	7.983	2688.9E6	542.4E6	376.817m	193.690 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121525\
Data File : PS032741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2025 19:05
Operator : AR\AJ
Sample : Q3854-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
ETGI-360


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/16/2025
Supervised By : Yogesh Patel 12/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 01:16:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

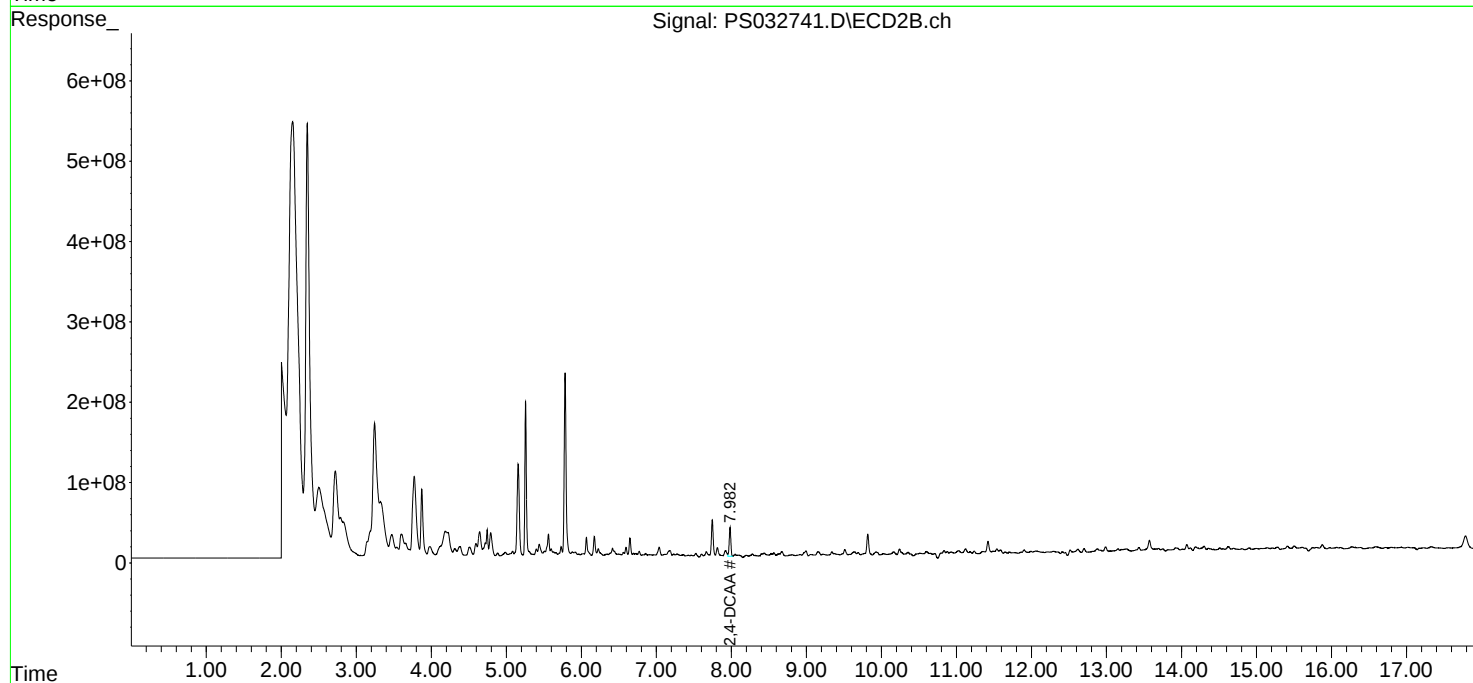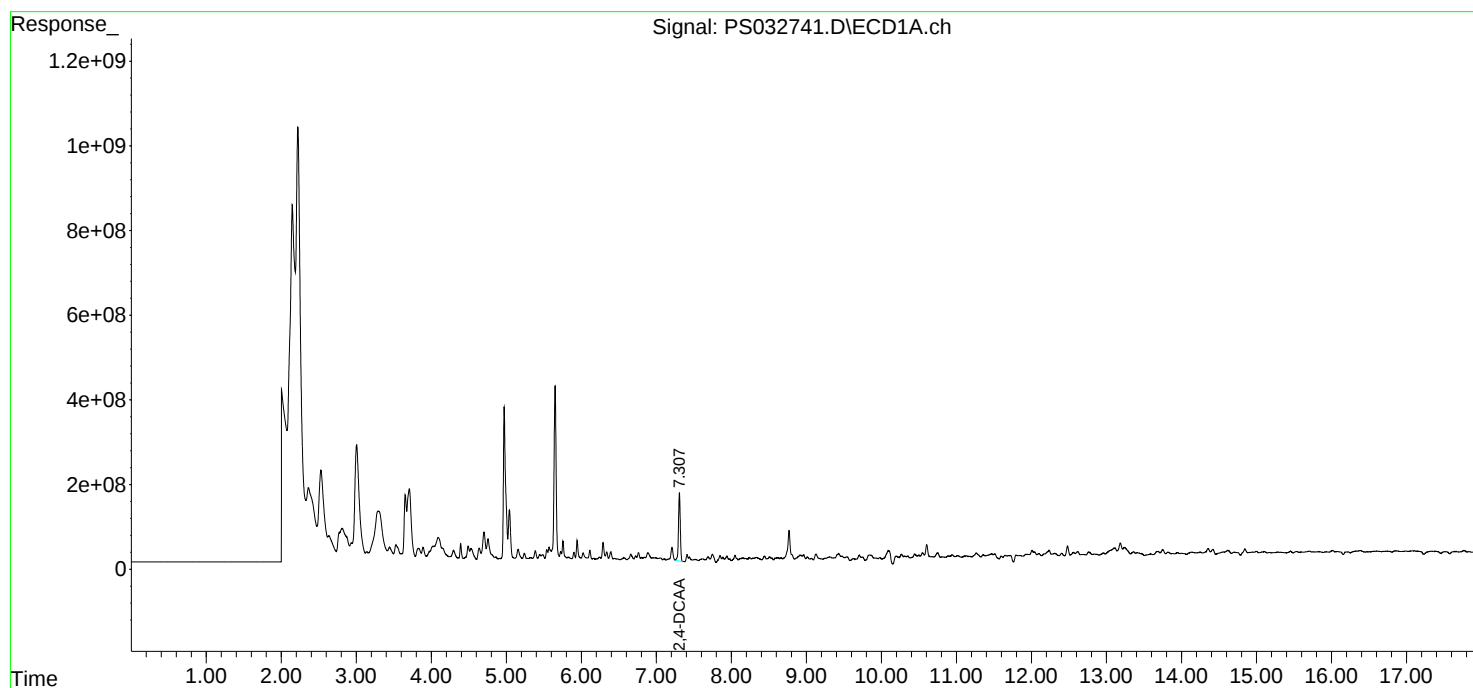

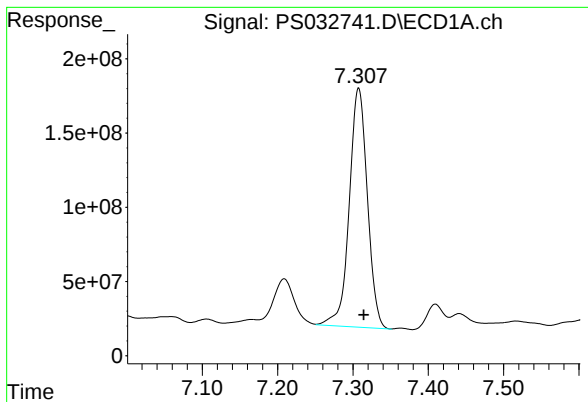

#4 2,4-DCAA

R.T.: 7.307 min
Delta R.T.: -0.007 min
Response: 2688946574
Conc: 376.82 ng/ml

Instrument :

ECD_S

ClientSampleId :


ETGI-360

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 12/16/2025

Supervised By :Yogesh Patel 12/16/2025

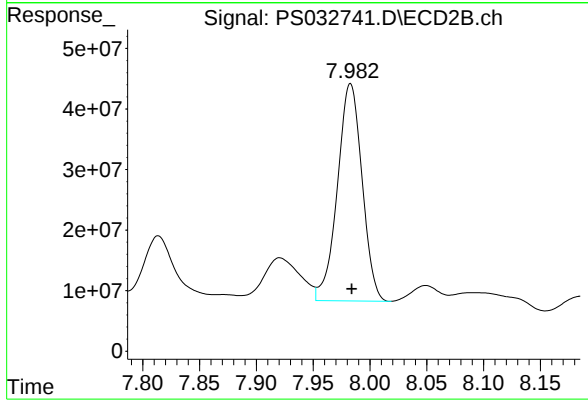

#4 2,4-DCAA

R.T.: 7.983 min
Delta R.T.: -0.001 min
Response: 542394798
Conc: 193.69 ng/ml