

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121620\
 Data File : PS013543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2020 08:50
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 13:49:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.469f	0.000	500.6E6	0	390.579	N.D. #
3) T	4-Nitroph...	7.001f	0.000	897886	0	1.993	N.D. #
7) T	MCPA	7.689	0.000	12674475	0	3.243	N.D. #
8) T	DICHLORPROP	0.000	7.761f	0	9126251	N.D.	20.421
12) T	2,4,5-T	9.405f	0.000	9323611	0	1.686	N.D. #
15) T	Picloram	11.033	11.028	64970870	32414007	9.433	9.310



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121620\
Data File : PS013543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2020 08:50
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 13:49:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

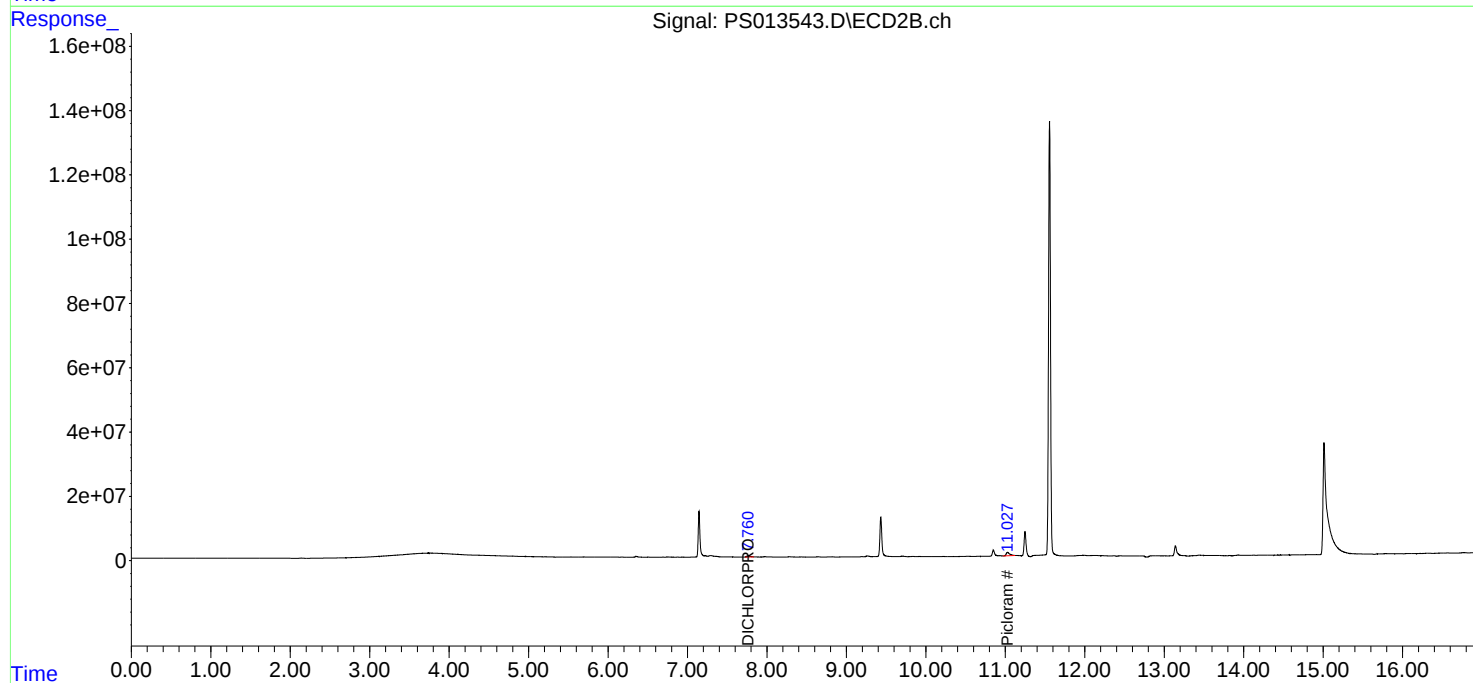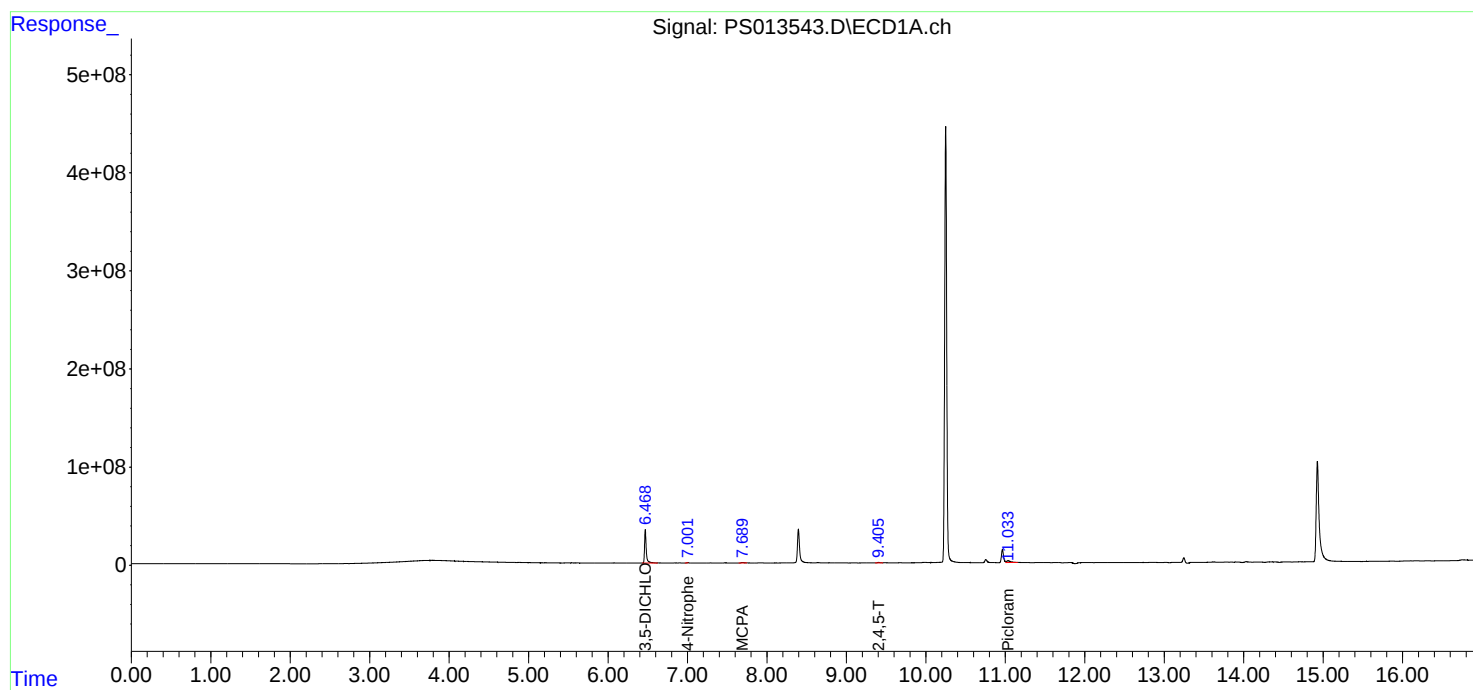


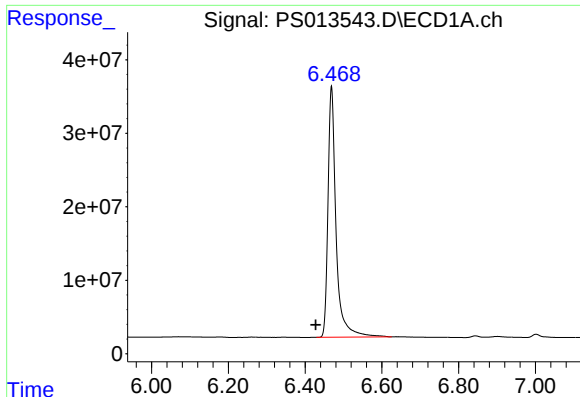

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.469 min
Delta R.T.: 0.041 min
Response: 500608101
Conc: 390.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

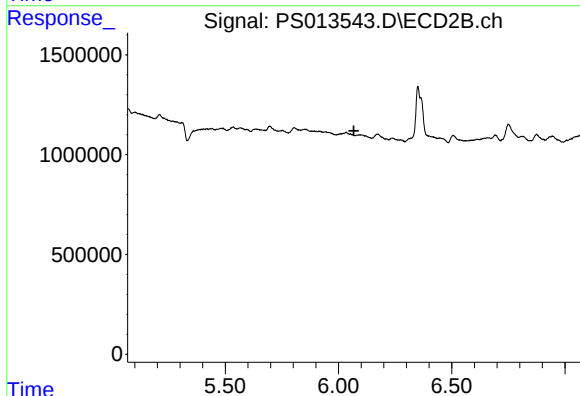


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.068 min
Response: 0
Conc: N.D.

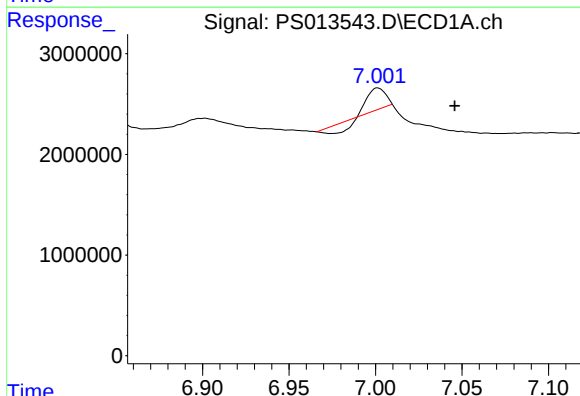


#3 4-Nitrophenol

R.T.: 7.001 min
Delta R.T.: -0.045 min
Response: 897886
Conc: 1.99 ng/ml

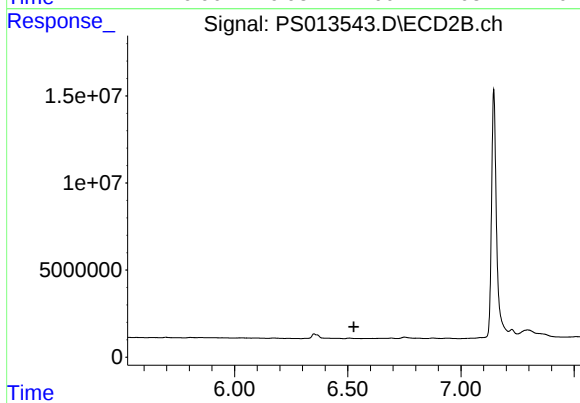

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

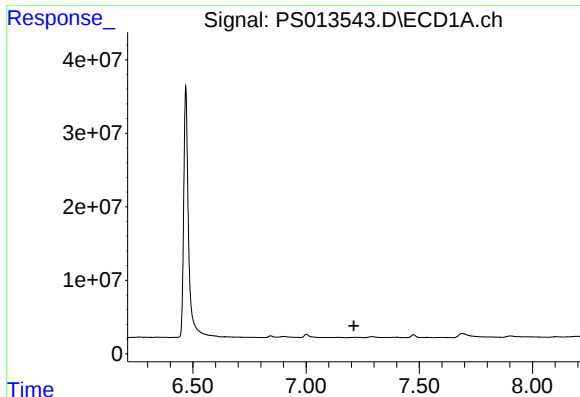

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

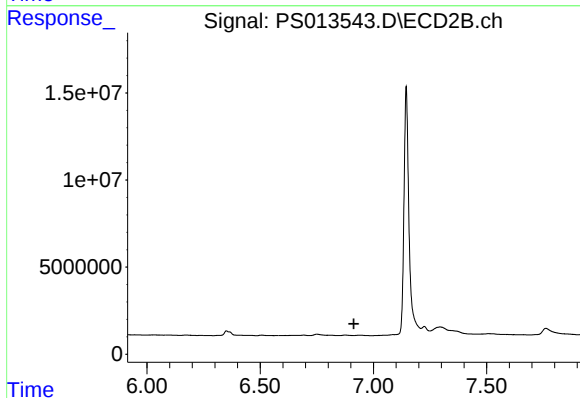


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.914 min
Response: 0
Conc: N.D.

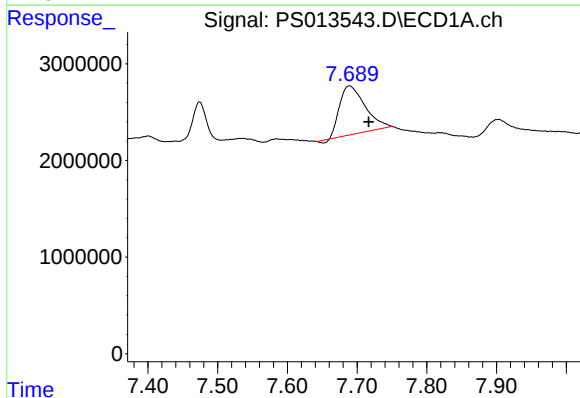


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.027 min
Response: 12674475
Conc: 3.24 ug/ml

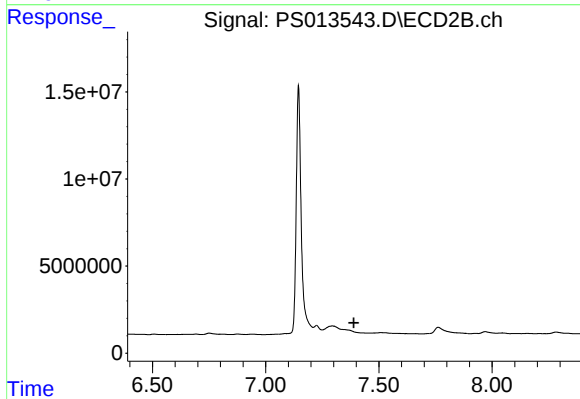

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

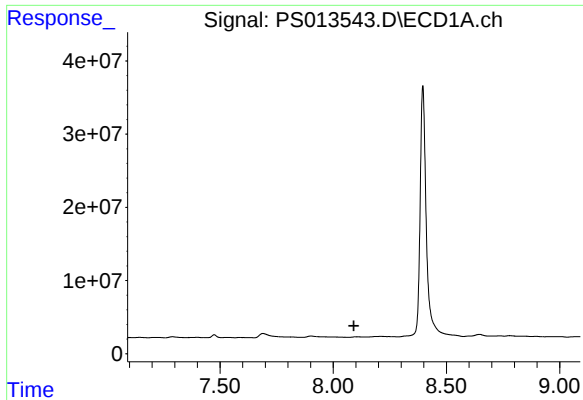

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

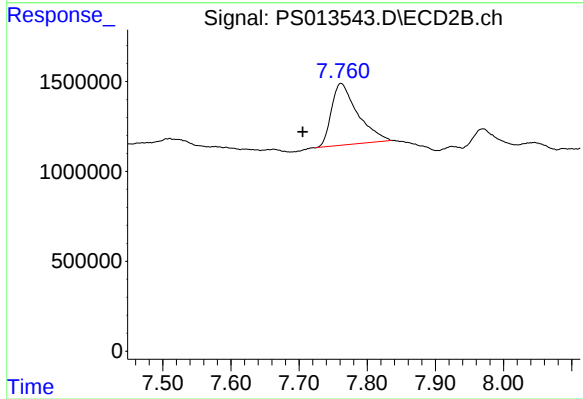


#8 DICHLORPROP

R.T.: 7.761 min
Delta R.T.: 0.056 min
Response: 9126251
Conc: 20.42 ng/ml

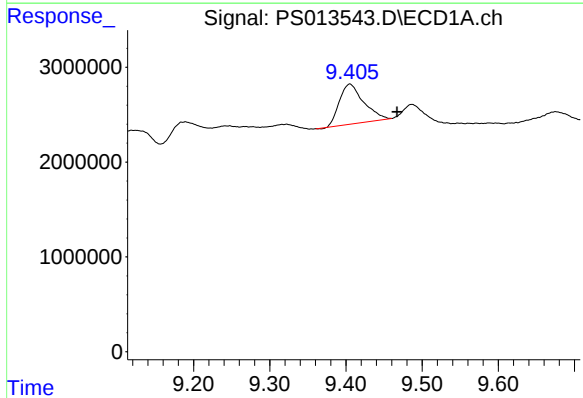


#12 2,4,5-T

R.T.: 9.405 min
Delta R.T.: -0.062 min
Response: 9323611
Conc: 1.69 ng/ml

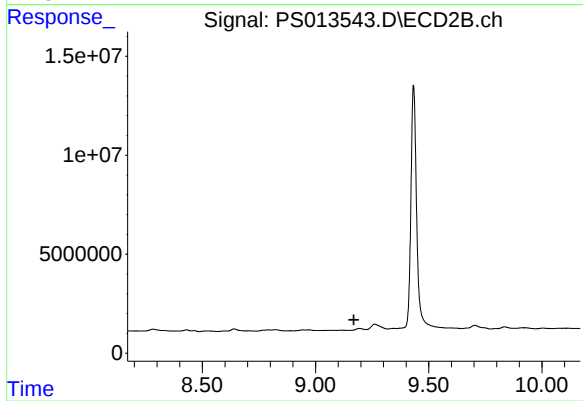

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

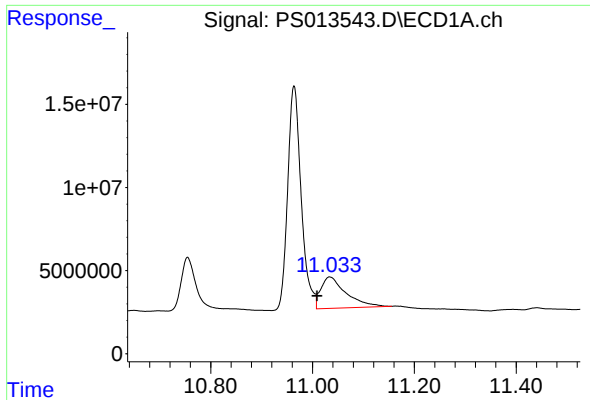

#15 Picloram

R.T.: 11.033 min
Delta R.T.: 0.024 min
Response: 64970870
Conc: 9.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

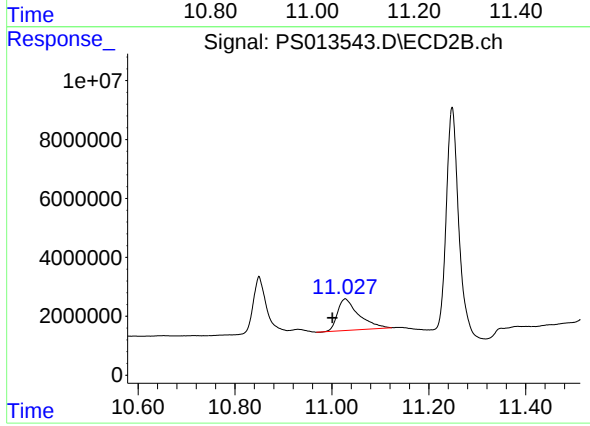

#15 Picloram

R.T.: 11.028 min
Delta R.T.: 0.027 min
Response: 32414007
Conc: 9.31 ng/ml