

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121620\
 Data File : PS013553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2020 20:35
 Operator : DD\AJ
 Sample : L5115-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SOIL-CUTTINGS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:40:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) T	MCPA	7.704	0.000	154.6E6	0	39.555	N.D.	#
9) T	2,4-D	0.000	8.066f	0	4990794	N.D.	9.249	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121620\
Data File : PS013553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2020 20:35
Operator : DD\AJ
Sample : L5115-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SOIL-CUTTINGS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:40:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

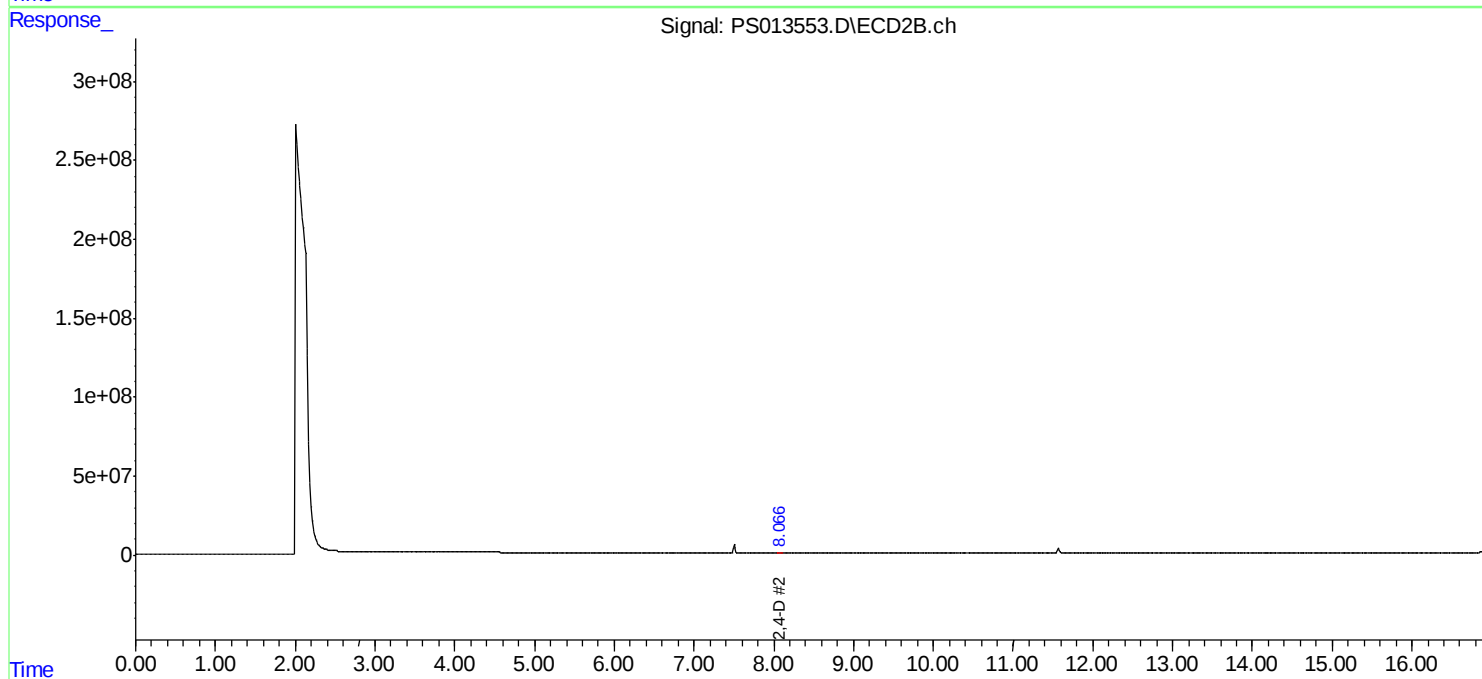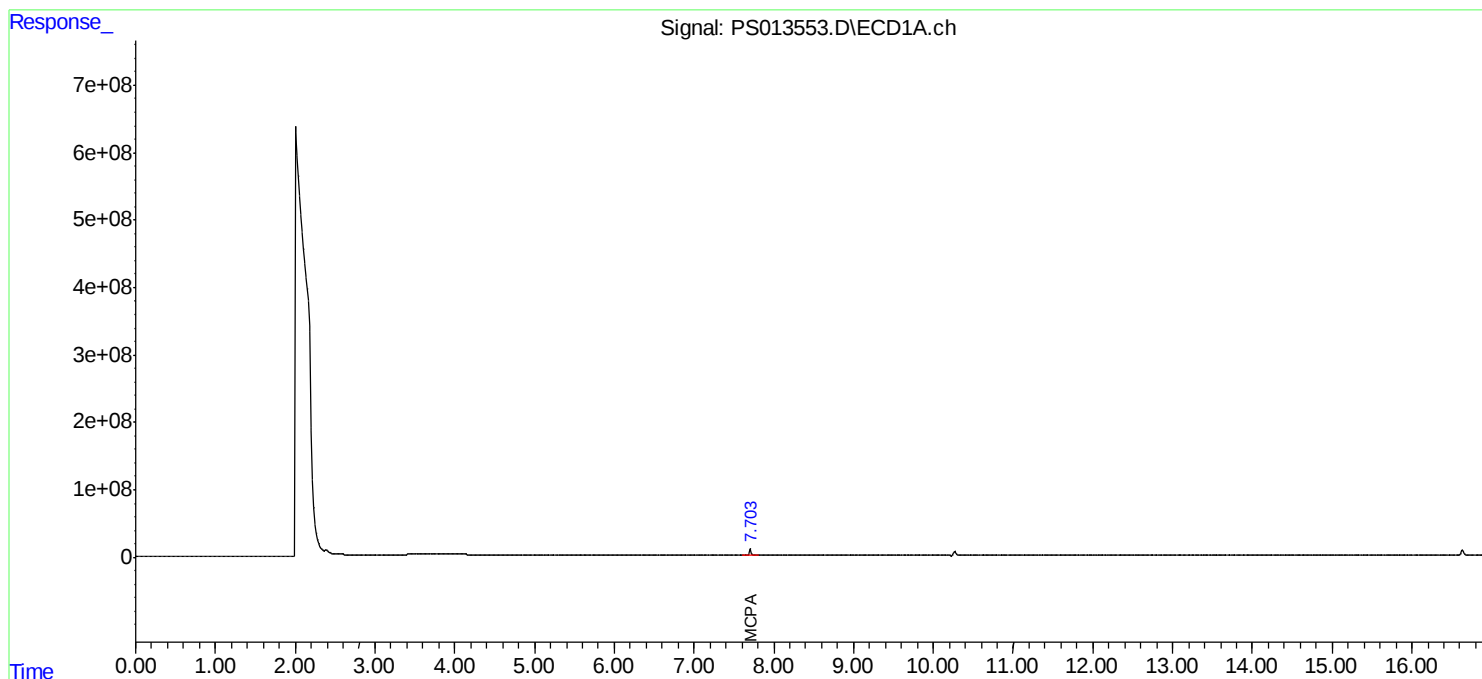


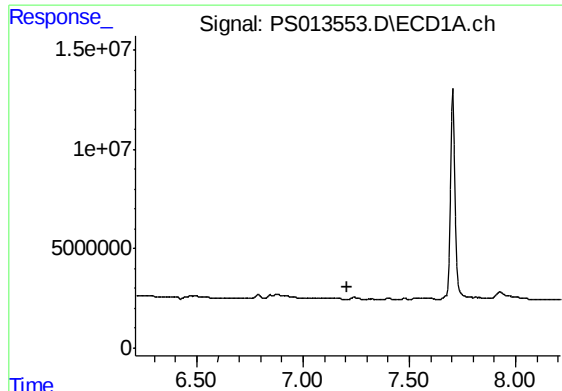

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SOIL-CUTTINGS

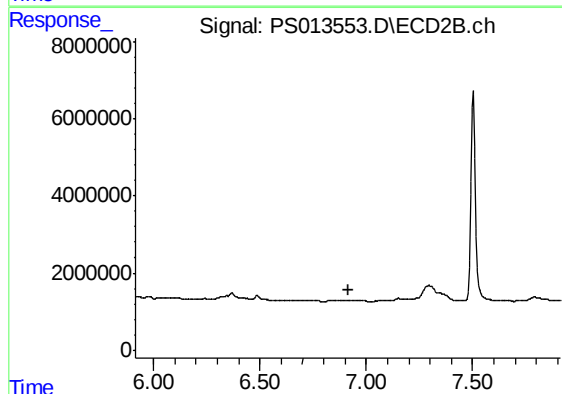


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.914 min
Response: 0
Conc: N.D.

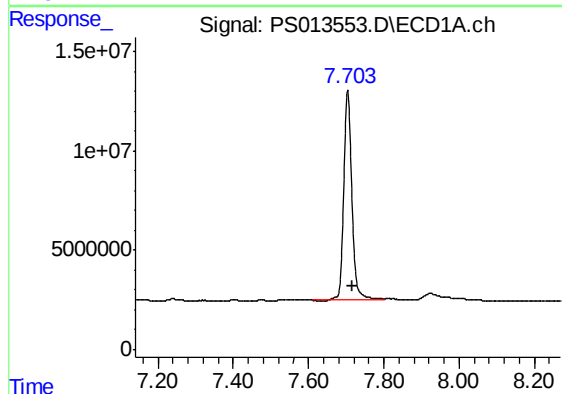


#7 MCPA

R.T.: 7.704 min
Delta R.T.: -0.013 min
Response: 154605591
Conc: 39.56 ug/ml

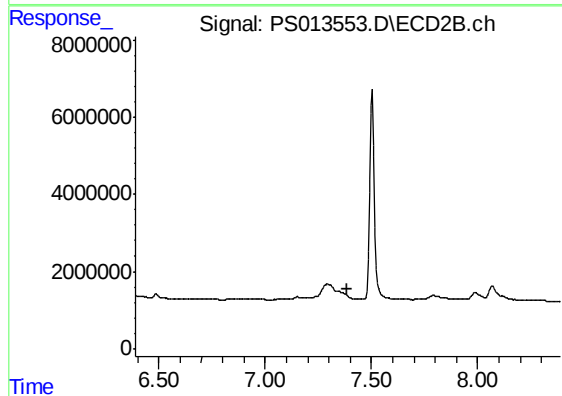

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

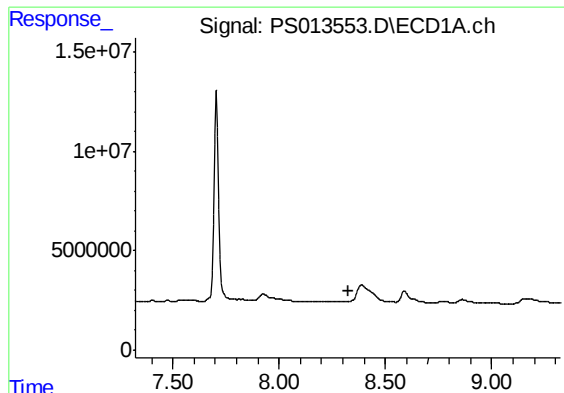

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SOIL-CUTTINGS

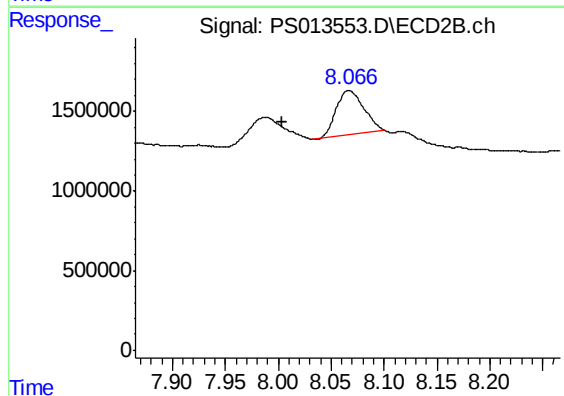

#9 2,4-D

R.T.: 8.066 min
Delta R.T.: 0.063 min
Response: 4990794
Conc: 9.25 ng/ml