

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121621\
 Data File : PS017725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2021 09:50
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 15:06:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.131	0.000	3246198	0	2.077	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.390	0.000	9507687	0	4.256	N.D. #
5) T	DICAMBA	7.316	0.000	10154831	0	1.606	N.D. #
7) T	MCPA	7.681f	0.000	1388213	0	<MDL	N.D. #
8) T	DICHLORPROP	8.007	0.000	3880235	0	2.483	N.D. #
9) T	2,4-D	8.246	0.000	11736811	0	6.639	N.D. #
10) T	Pentachlo...	8.536	8.193	19215144	8122981	<MDL	<MDL #
11) T	2,4,5-TP ...	9.087	8.555	17258065	6540138	2.029	1.799
12) T	2,4,5-T	9.378	8.937	34879024	11161854	4.009	3.264
13) T	2,4-DB	9.932	0.000	10206691	0	6.912	N.D. #
14) T	DINOSEB	11.067	0.000	21614133	0	3.161	N.D. #
15) T	Picloram	10.902	10.743	247.2E6	102.7E6	22.785	20.910
16) T	DCPA	11.334	10.684	22423429	9838564	2.065	2.197



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121621\
Data File : PS017725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2021 09:50
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 15:06:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

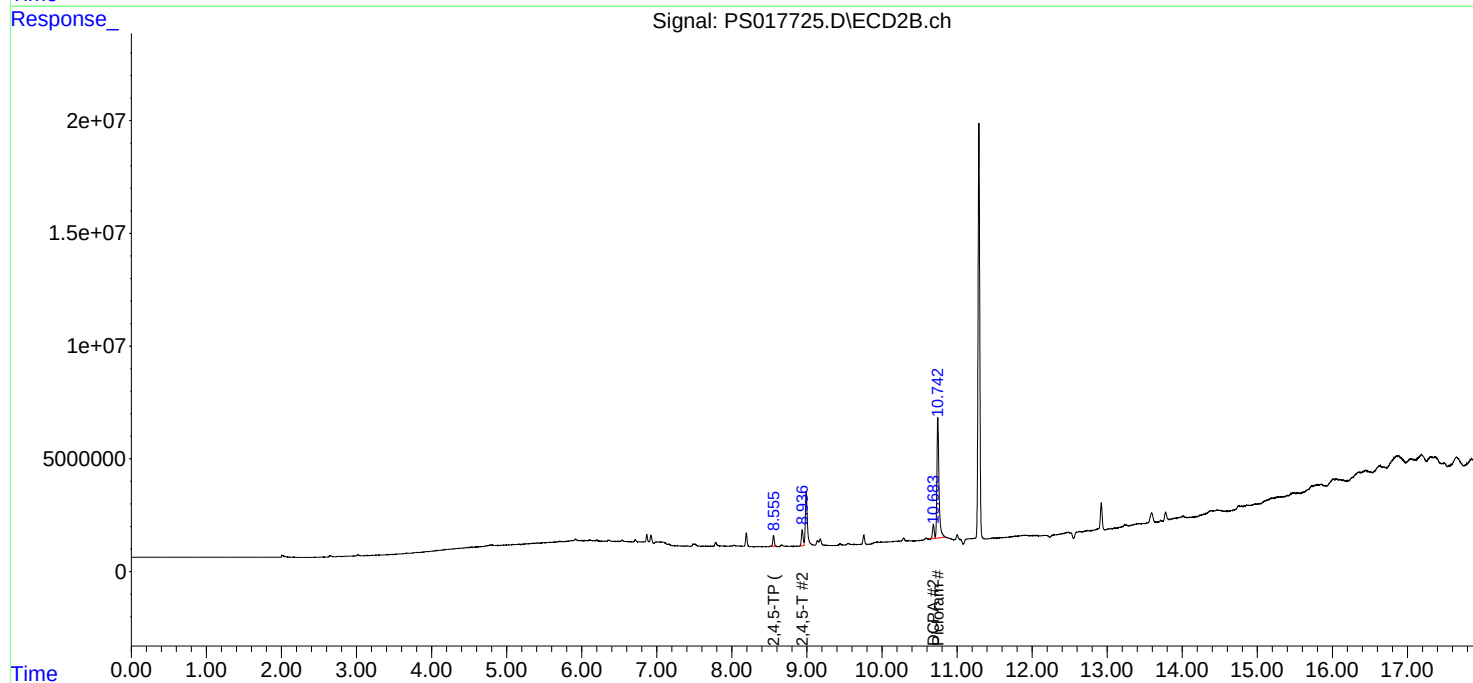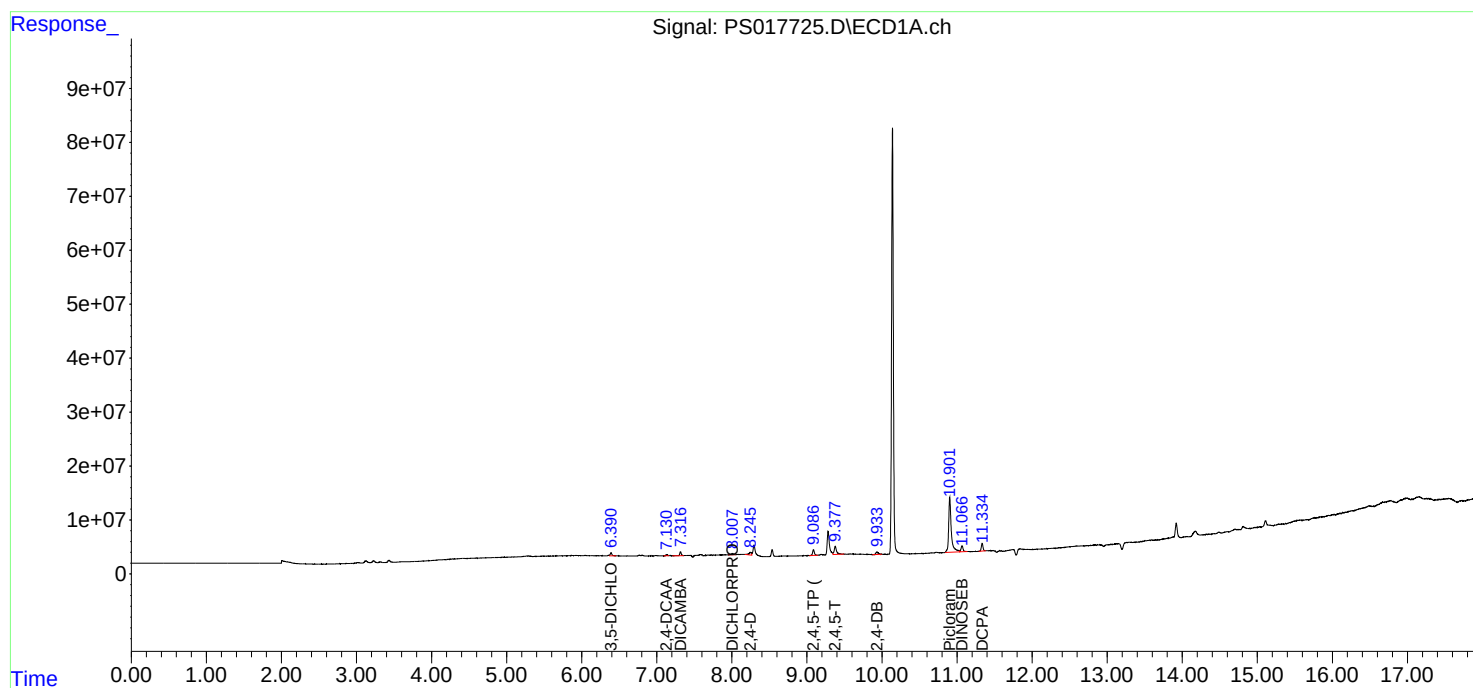


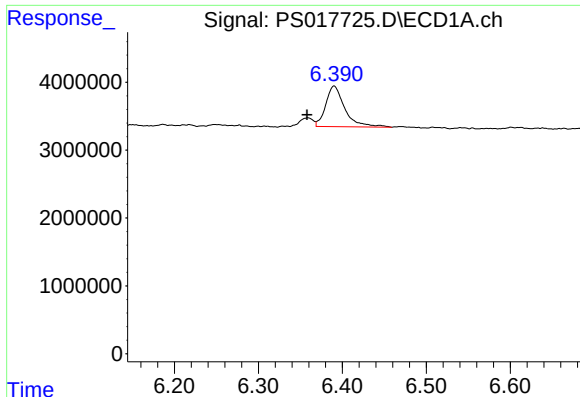

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.390 min
Delta R.T.: 0.032 min
Response: 9507687
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

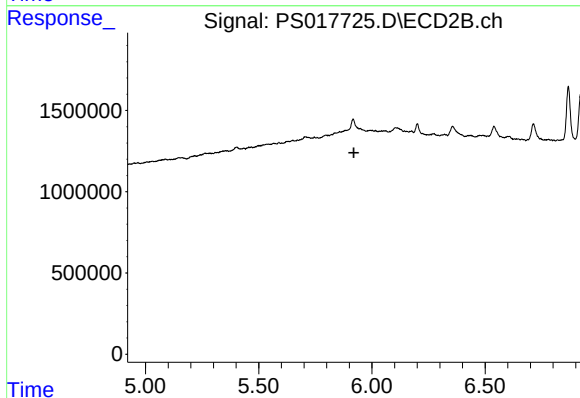


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

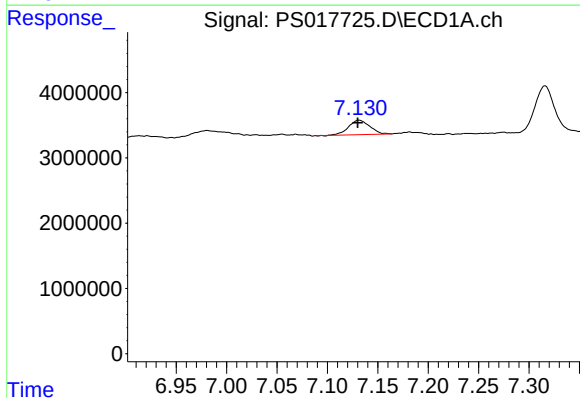


#4 2,4-DCAA

R.T.: 7.131 min
Delta R.T.: 0.001 min
Response: 3246198
Conc: 2.08 ng/ml

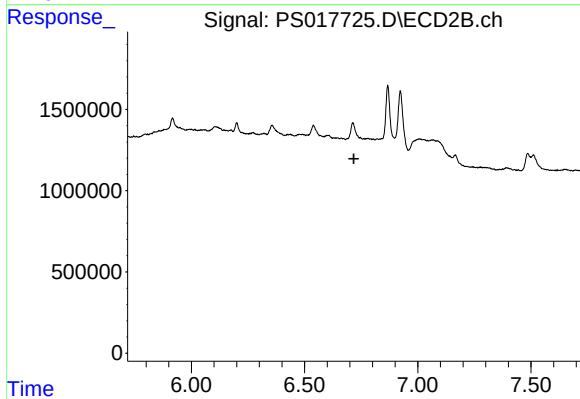

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.718 min
Response: 0
Conc: N.D.

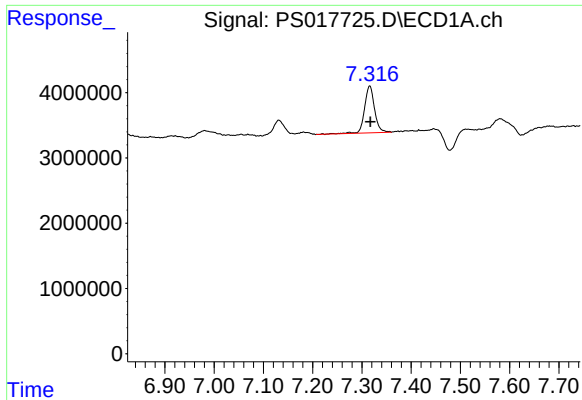

#5 DICAMBA


R.T.: 7.316 min
Delta R.T.: -0.001 min
Response: 10154831
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

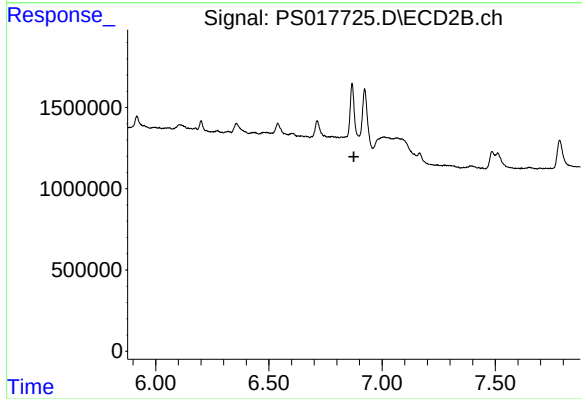


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

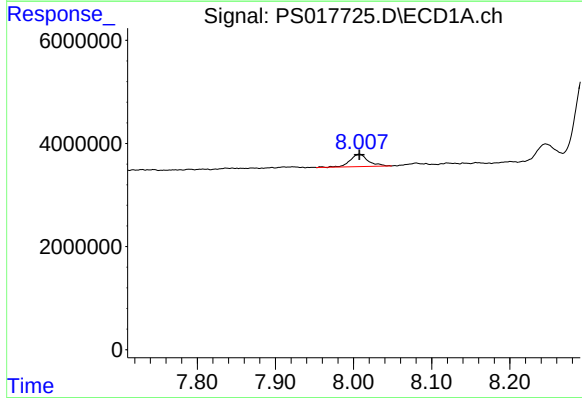


#8 DICHLORPROP

R.T.: 8.007 min
Delta R.T.: 0.000 min
Response: 3880235
Conc: 2.48 ng/ml

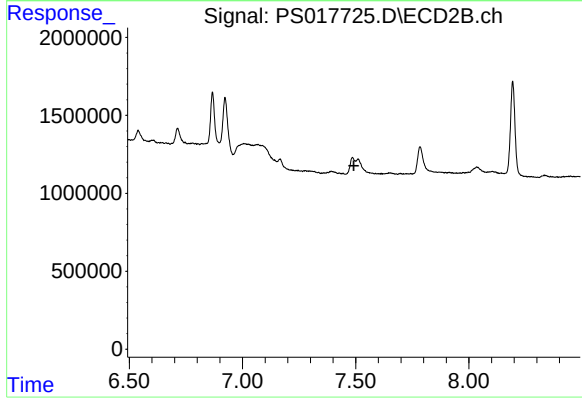

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.492 min
Response: 0
Conc: N.D.

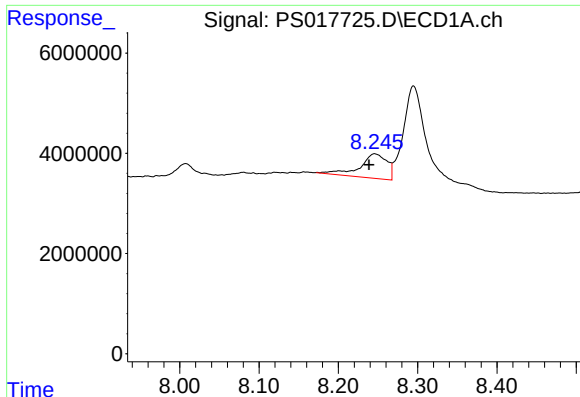

#9 2,4-D


R.T.: 8.246 min
Delta R.T.: 0.007 min
Response: 11736811
Conc: 6.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

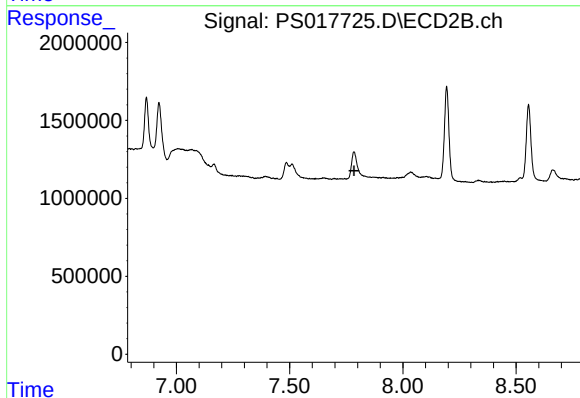


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

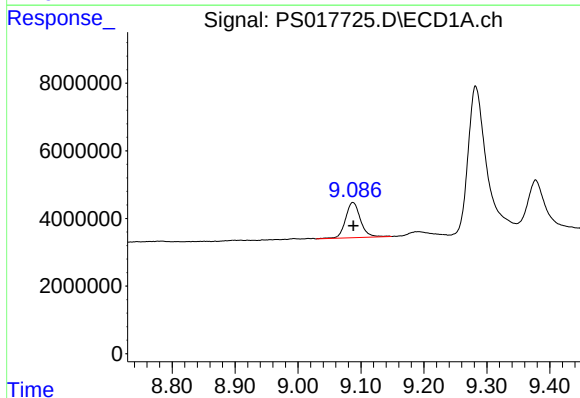


#11 2,4,5-TP (SILVEX)

R.T.: 9.087 min
Delta R.T.: -0.001 min
Response: 17258065
Conc: 2.03 ng/ml

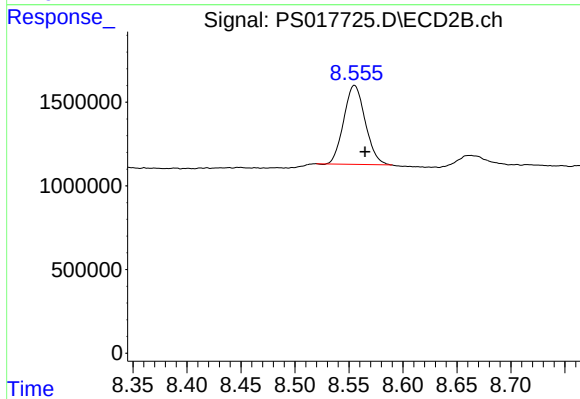

#11 2,4,5-TP (SILVEX)


R.T.: 8.555 min
Delta R.T.: -0.010 min
Response: 6540138
Conc: 1.80 ng/ml

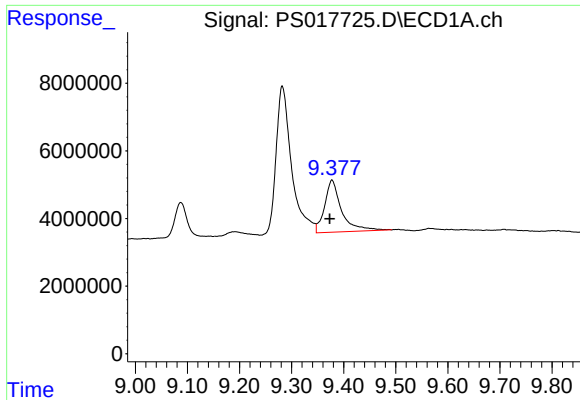

#12 2,4,5-T


R.T.: 9.378 min
Delta R.T.: 0.004 min
Response: 34879024
Conc: 4.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

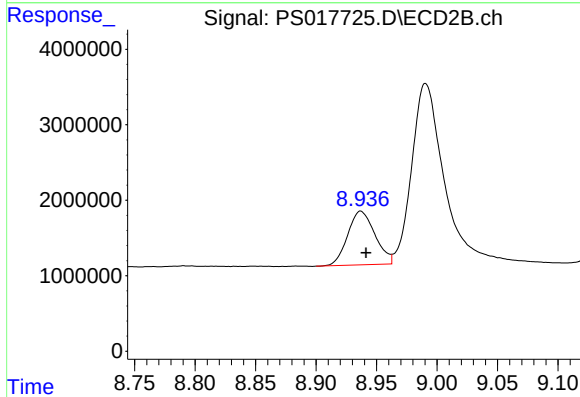


#12 2,4,5-T

R.T.: 8.937 min
Delta R.T.: -0.005 min
Response: 11161854
Conc: 3.26 ng/ml

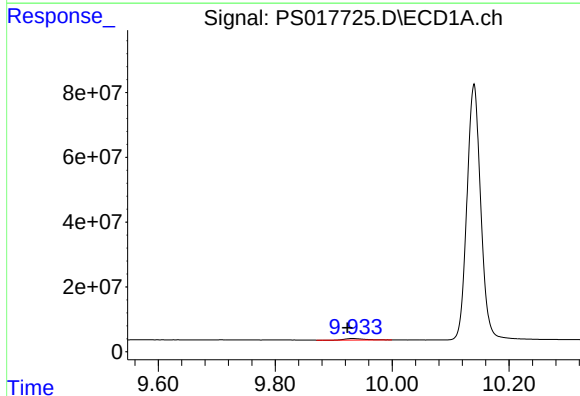


#13 2,4-DB

R.T.: 9.932 min
Delta R.T.: 0.008 min
Response: 10206691
Conc: 6.91 ng/ml

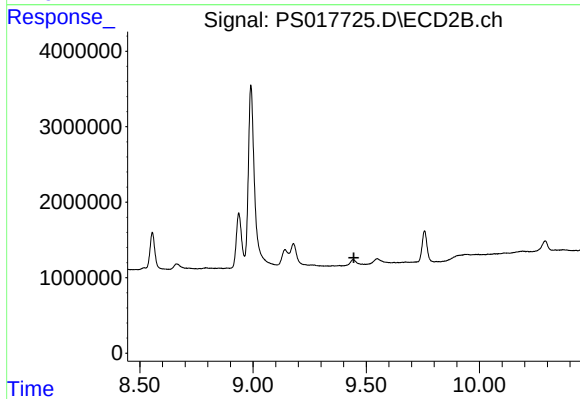

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.445 min
Response: 0
Conc: N.D.

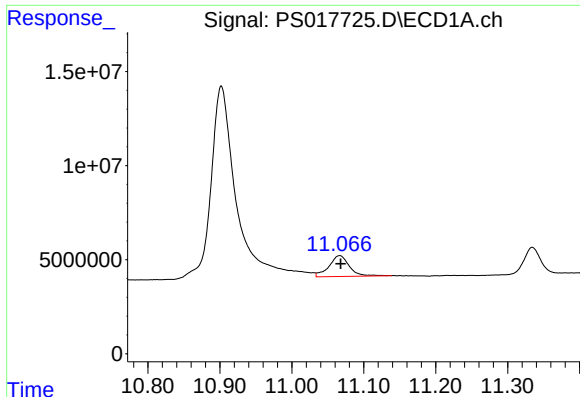

#14 DINOSEB


R.T.: 11.067 min
Delta R.T.: -0.001 min
Response: 21614133
Conc: 3.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

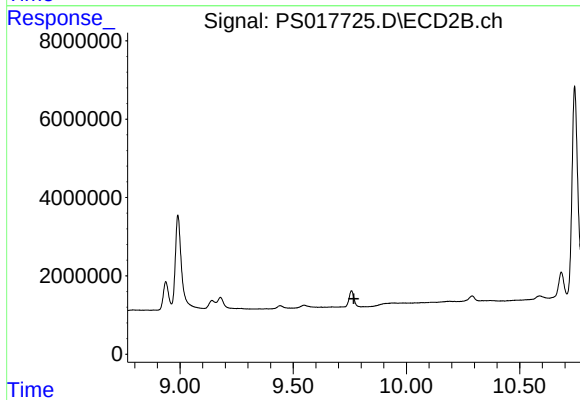


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

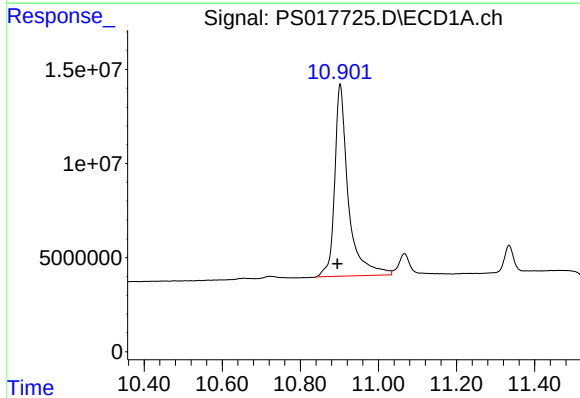


#15 Picloram

R.T.: 10.902 min
Delta R.T.: 0.007 min
Response: 247242016
Conc: 22.78 ng/ml

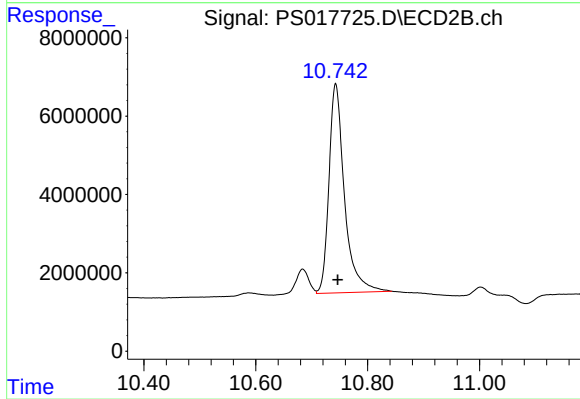

#15 Picloram


R.T.: 10.743 min
Delta R.T.: -0.004 min
Response: 102700459
Conc: 20.91 ng/ml

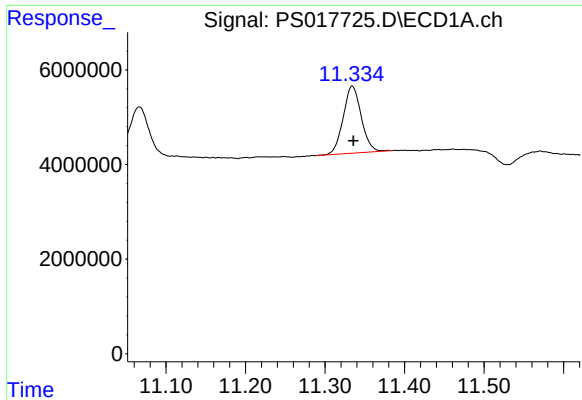

#16 DCPA

R.T.: 11.334 min
Delta R.T.: -0.002 min
Response: 22423429
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

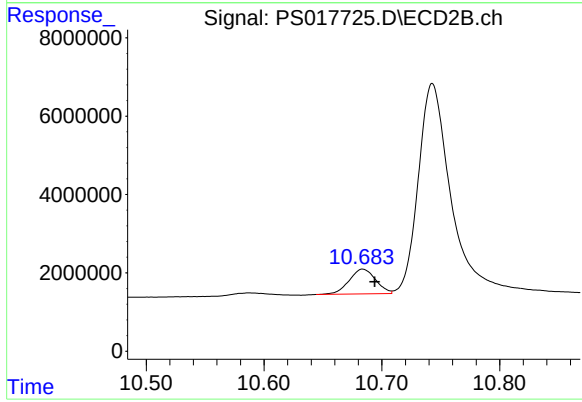

#16 DCPA

R.T.: 10.684 min
Delta R.T.: -0.010 min
Response: 9838564
Conc: 2.20 ng/ml