

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121621\
 Data File : PS017726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2021 10:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 15:06:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.127	6.713	710.9E6	304.4E6	454.843	510.616
Target Compounds							
2) T	3,5-DICHL...	6.395	0.000	16950363	0	7.587	N.D. #
5) T	DICAMBA	7.314	0.000	4408956	0	<MDL	N.D. #
9) T	2,4-D	8.303f	0.000	58601381	0	33.148	N.D. #
12) T	2,4,5-T	9.395	0.000	10875004	0	1.250	N.D. #
14) T	DINOSEB	11.066	0.000	11227146	0	1.642	N.D. #
15) T	Picloram	10.922	10.764	143.7E6	59260640	13.245	12.066
16) T	DCPA	11.333	10.764f	3715297	59260640	<MDL	13.231 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121621\
Data File : PS017726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2021 10:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 15:06:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

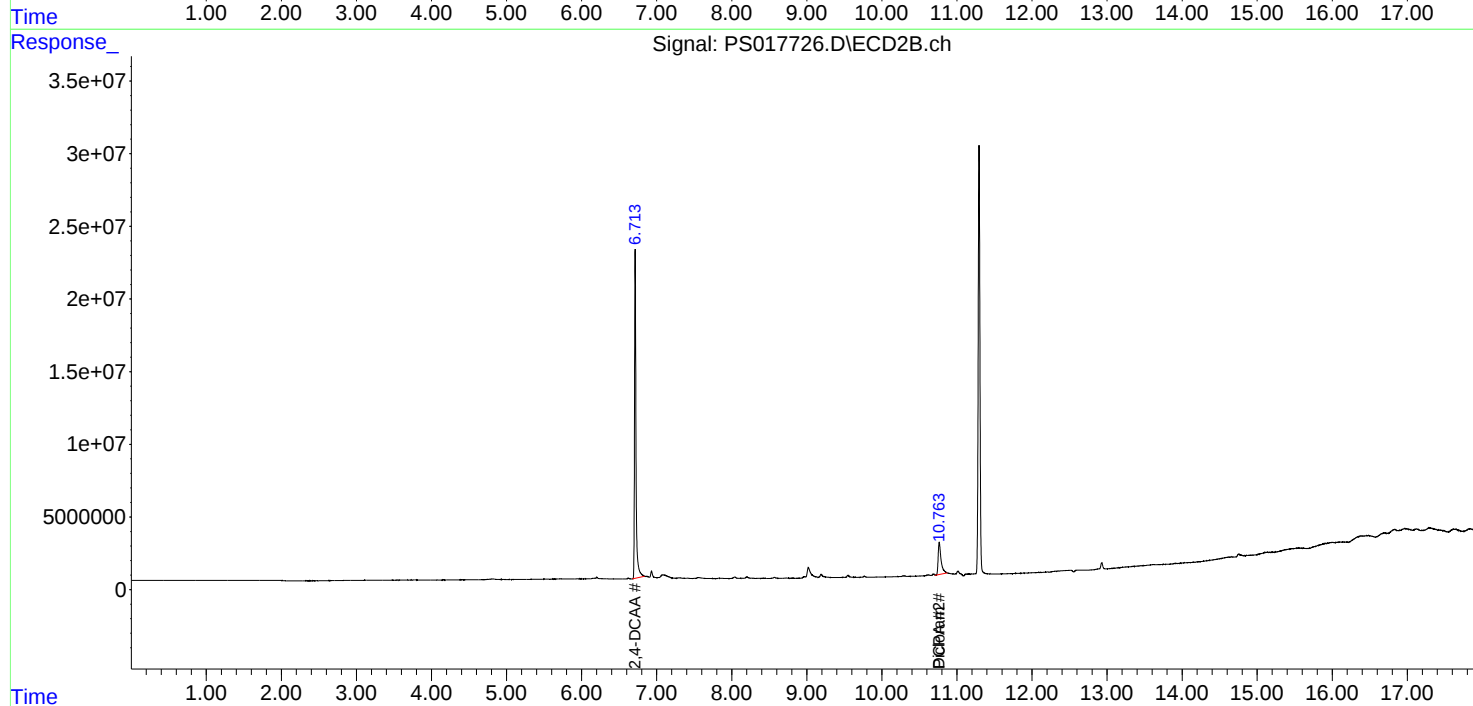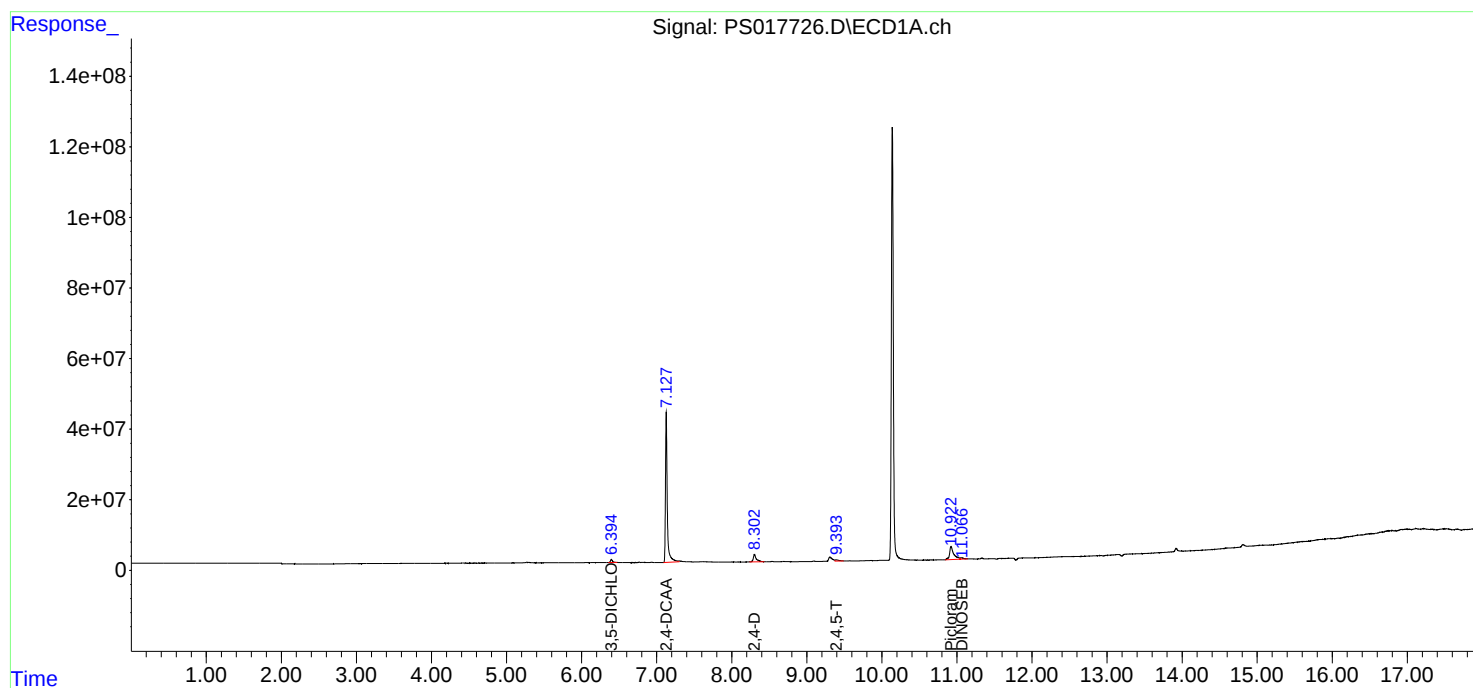


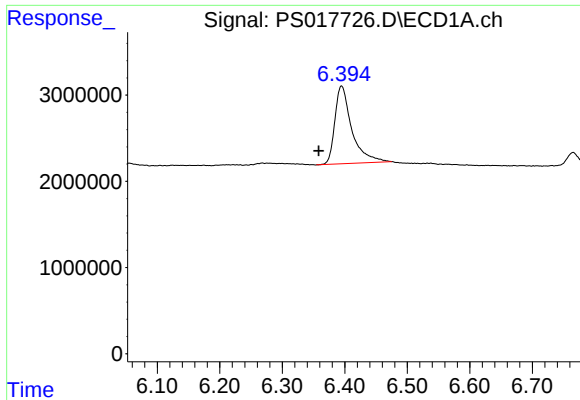

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.395 min
Delta R.T.: 0.037 min
Response: 16950363
Conc: 7.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

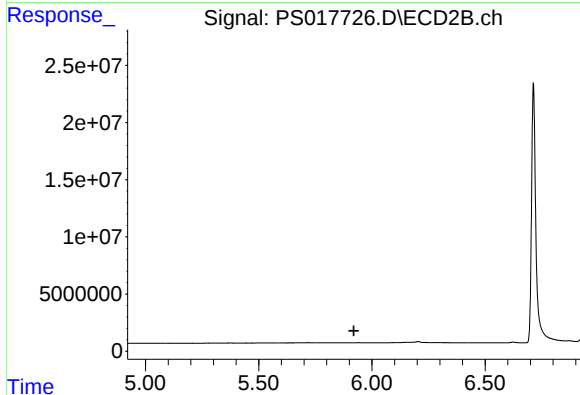


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

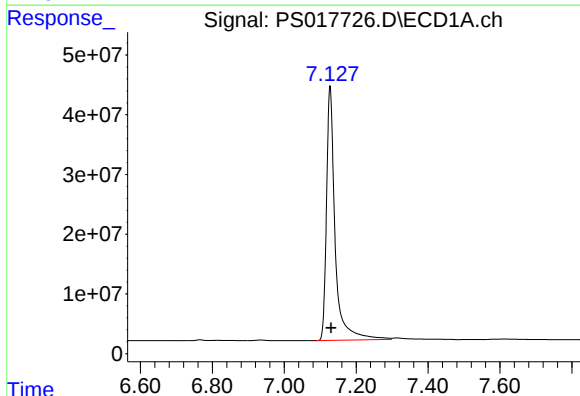


#4 2,4-DCAA

R.T.: 7.127 min
Delta R.T.: -0.003 min
Response: 710894874
Conc: 454.84 ng/ml

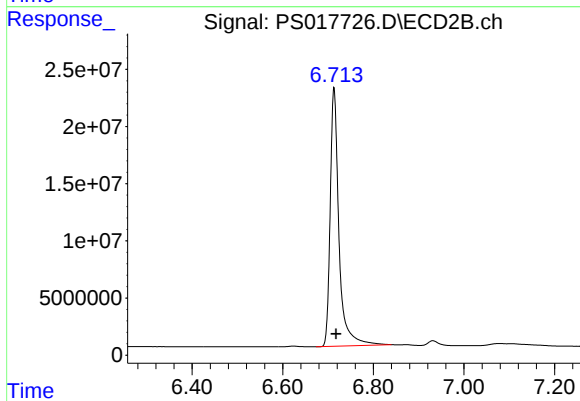

#4 2,4-DCAA


R.T.: 6.713 min
Delta R.T.: -0.004 min
Response: 304379274
Conc: 510.62 ng/ml

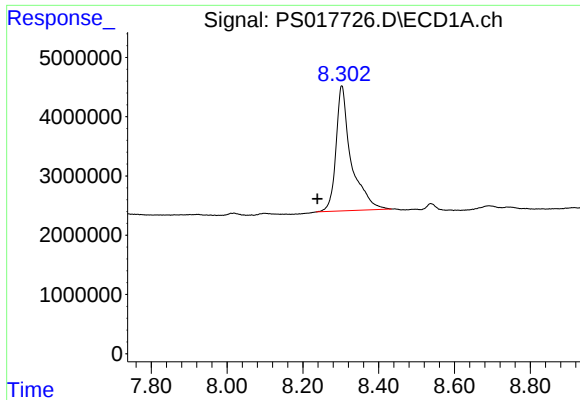

#9 2,4-D


R.T.: 8.303 min
Delta R.T.: 0.064 min
Response: 58601381
Conc: 33.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

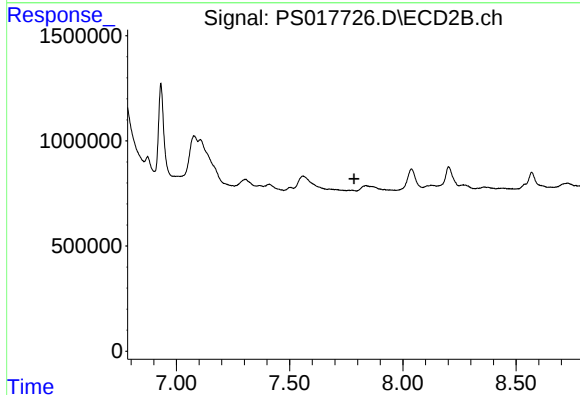


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

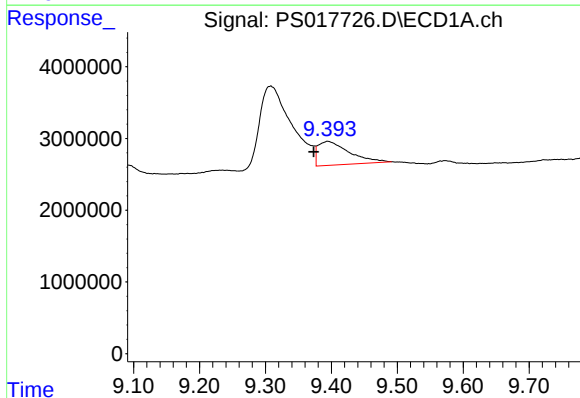


#12 2,4,5-T

R.T.: 9.395 min
Delta R.T.: 0.021 min
Response: 10875004
Conc: 1.25 ng/ml

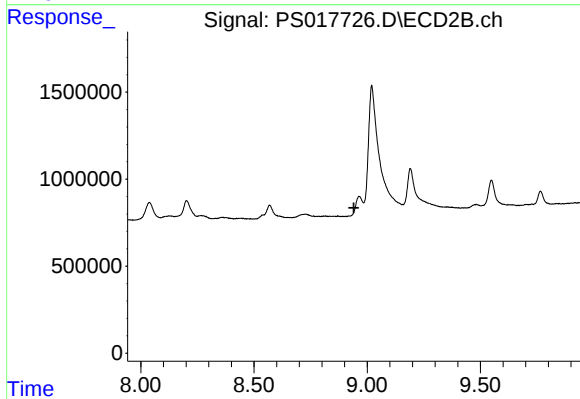

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

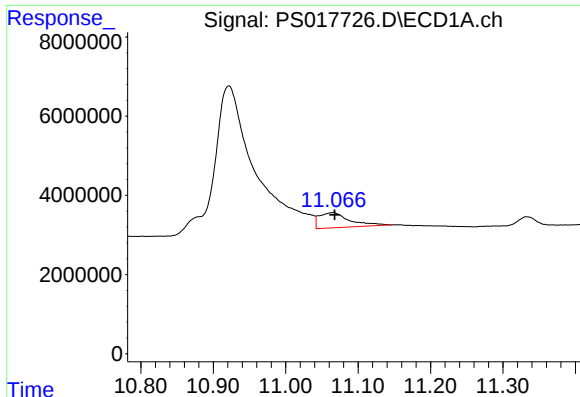

#14 DINOSEB


R.T.: 11.066 min
Delta R.T.: -0.002 min
Response: 11227146
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

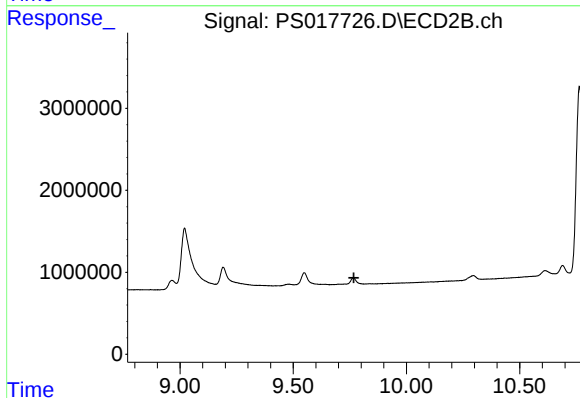


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

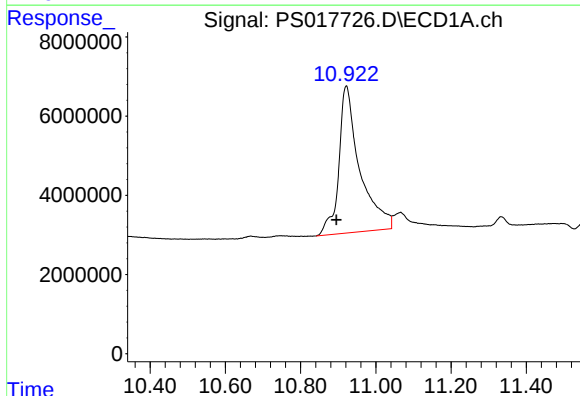


#15 Picloram

R.T.: 10.922 min
Delta R.T.: 0.027 min
Response: 143729077
Conc: 13.25 ng/ml

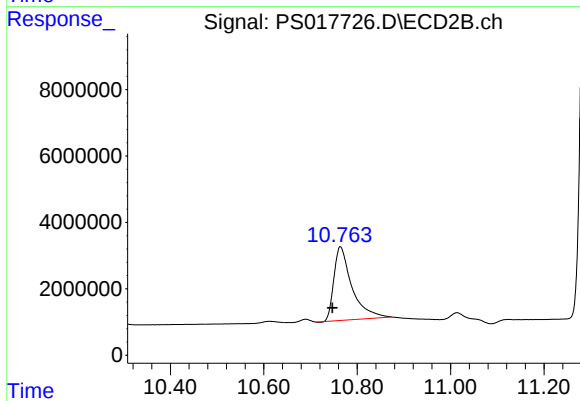

#15 Picloram


R.T.: 10.764 min
Delta R.T.: 0.017 min
Response: 59260640
Conc: 12.07 ng/ml

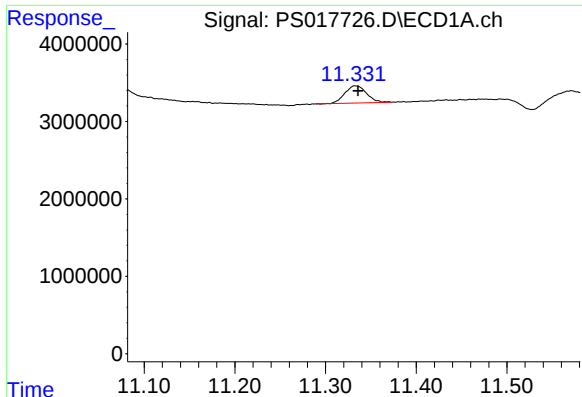

#16 DCPA

R.T.: 11.333 min
Delta R.T.: -0.003 min
Response: 3715297
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

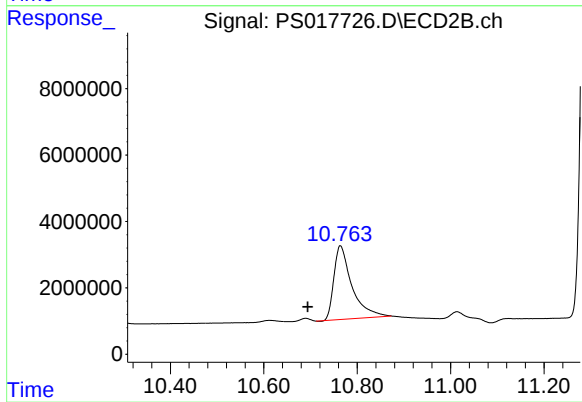

#16 DCPA

R.T.: 10.764 min
Delta R.T.: 0.070 min
Response: 59260640
Conc: 13.23 ng/ml