

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121718\
 Data File : PS002629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2018 18:37
 Operator : EI\SJ
 Sample : J6340-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 02:18:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.404	10.901	158.5E6	169.0E6	499.321	437.082
Target Compounds							
1) T	Dalapon	2.889	0.000	3176458	0	6.901	N.D. #
3) T	4-Nitroph...	11.053	10.058	3226860	3978281	20.367	22.258
5) T	DICAMBA	0.000	11.198	0	1242839	N.D.	0.872 #
6) T	MCP	12.085	0.000	26613423	0	26.673	N.D. #
7) T	MCPA	0.000	11.796	0	3762478	N.D.	2.617 #
8) T	DICHLORPROP	0.000	12.318	0	2089038	N.D.	5.841 #
12) T	2,4,5-T	0.000	14.499	0	13468091	N.D.	7.872 #
13) T	2,4-DB	15.683	0.000	2531739	0	11.194	N.D. #
14) T	DINOSEB	0.000	15.611	0	4259253	N.D.	2.791 #
16) T	DCPA	0.000	16.849	0	6806750	N.D.	2.343 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121718\
Data File : PS002629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2018 18:37
Operator : EI\SJ
Sample : J6340-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 02:18:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

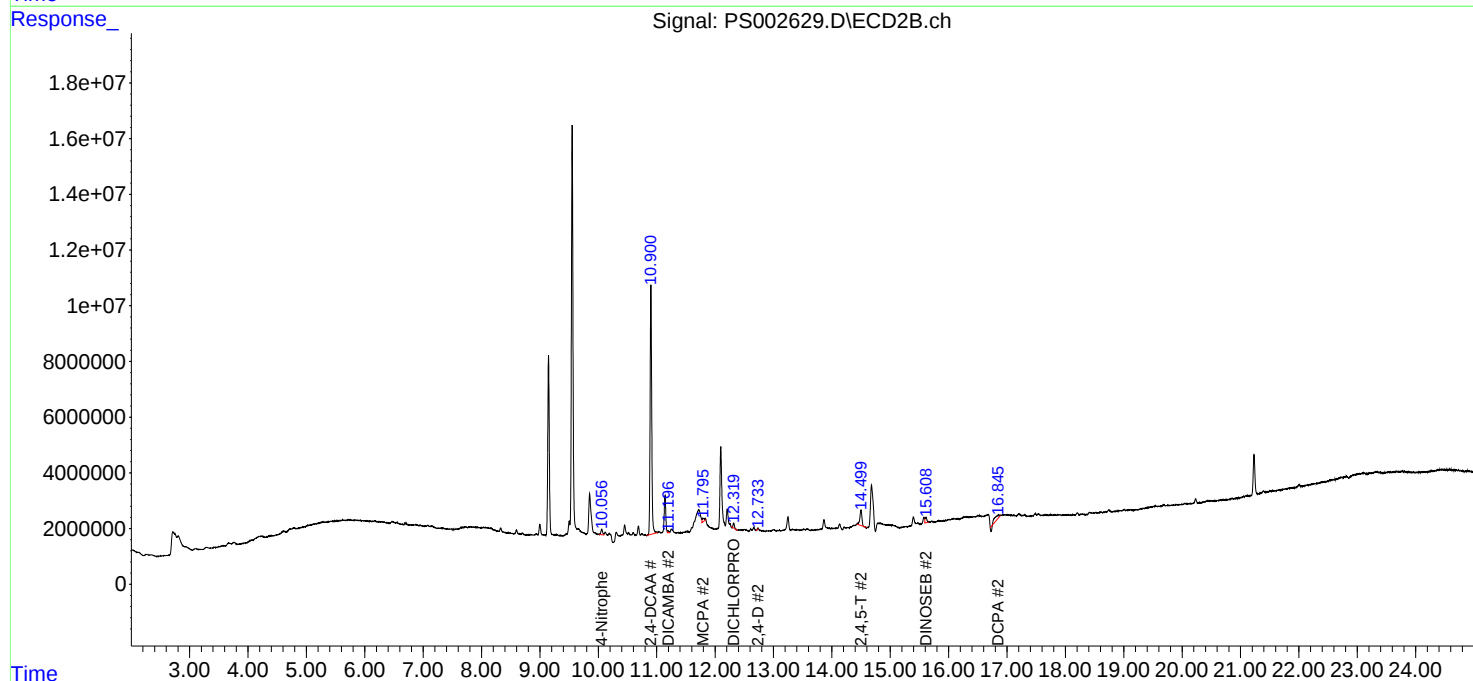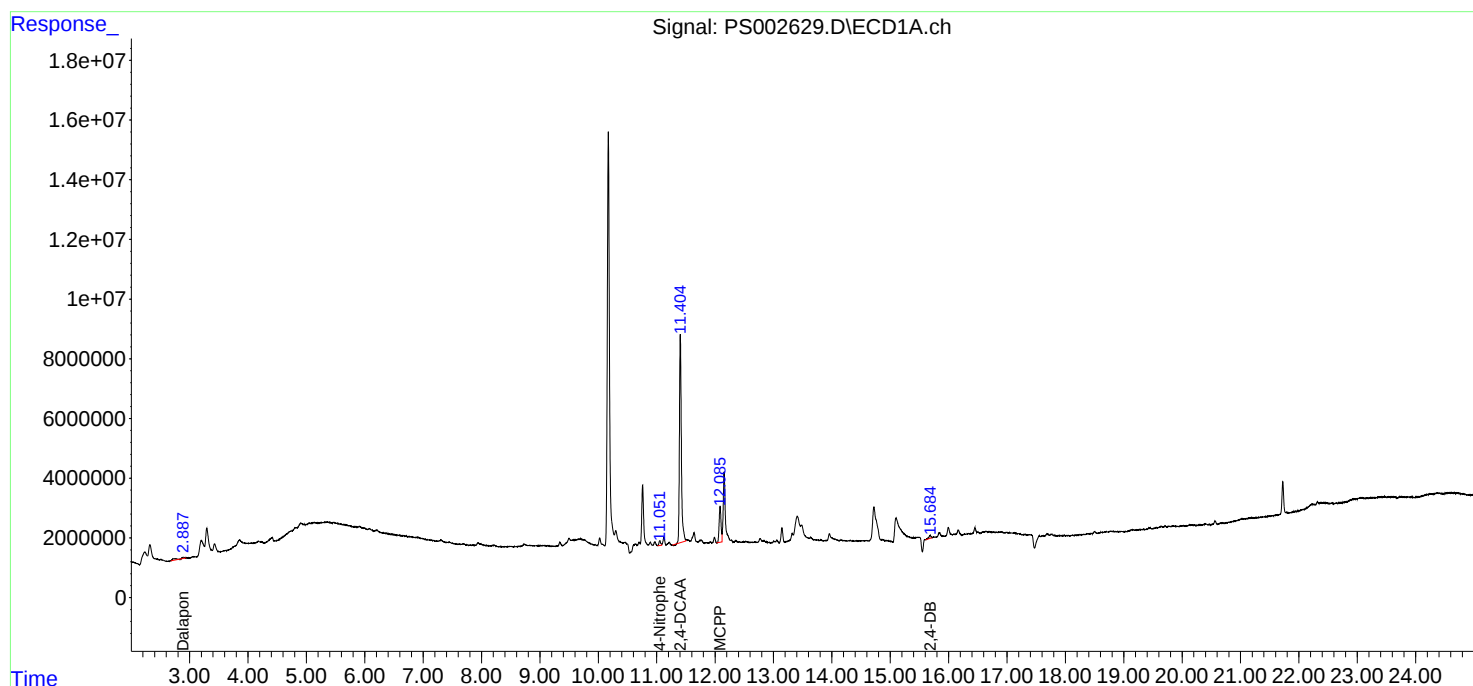


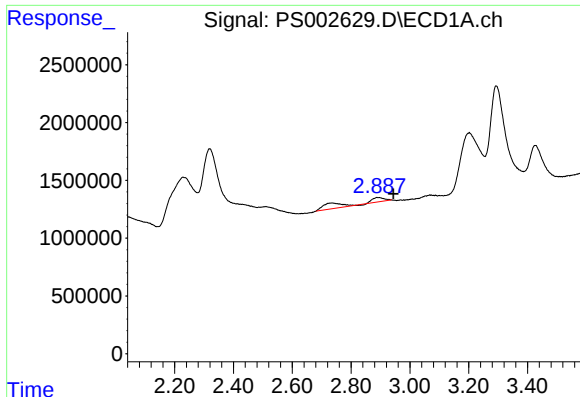

#1 Dalapon


R.T.: 2.889 min
Delta R.T.: -0.055 min
Response: 3176458
Conc: 6.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

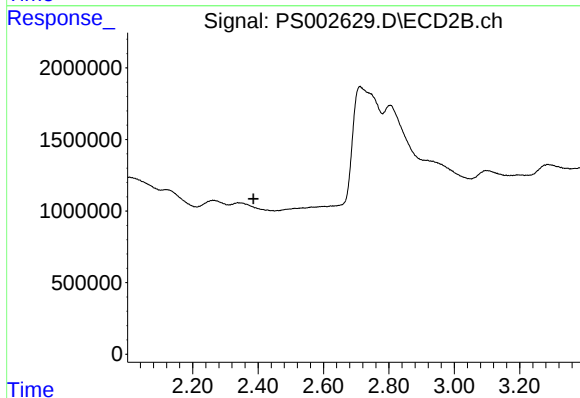


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.385 min
Response: 0
Conc: N.D.

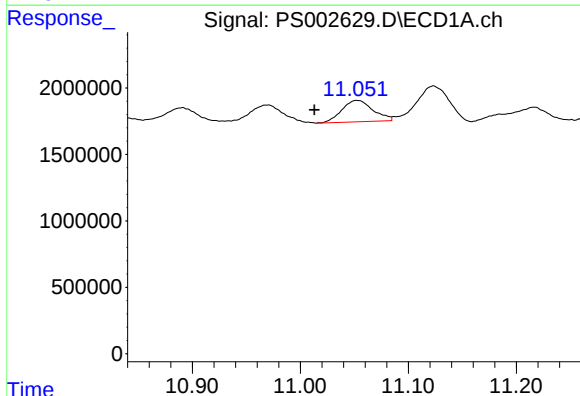


#3 4-Nitrophenol

R.T.: 11.053 min
Delta R.T.: 0.040 min
Response: 3226860
Conc: 20.37 ng/ml

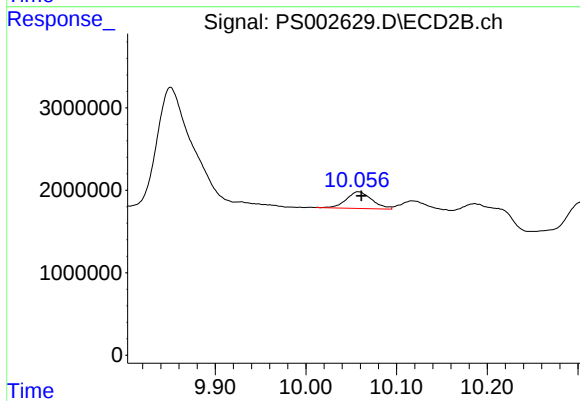

#3 4-Nitrophenol


R.T.: 10.058 min
Delta R.T.: -0.003 min
Response: 3978281
Conc: 22.26 ng/ml

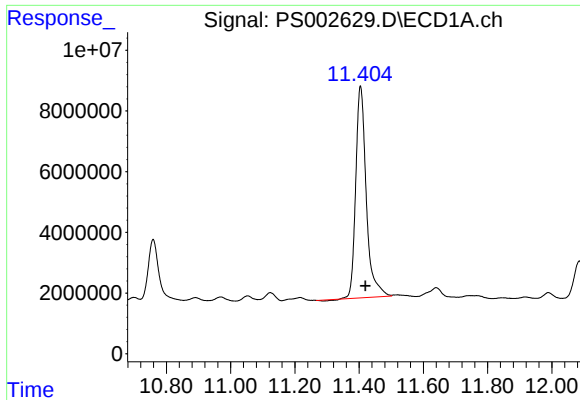

#4 2,4-DCAA


R.T.: 11.404 min
Delta R.T.: -0.016 min
Response: 158494468
Conc: 499.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

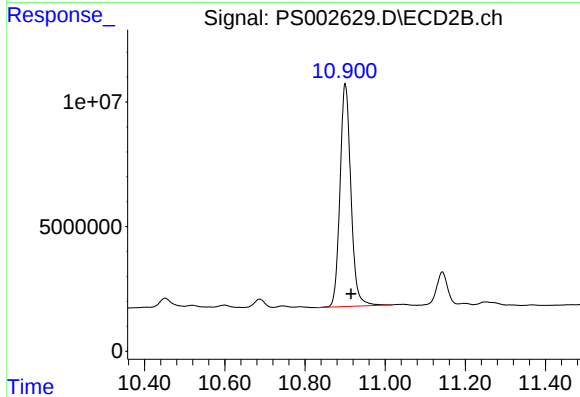


#4 2,4-DCAA

R.T.: 10.901 min
Delta R.T.: -0.014 min
Response: 169049936
Conc: 437.08 ng/ml

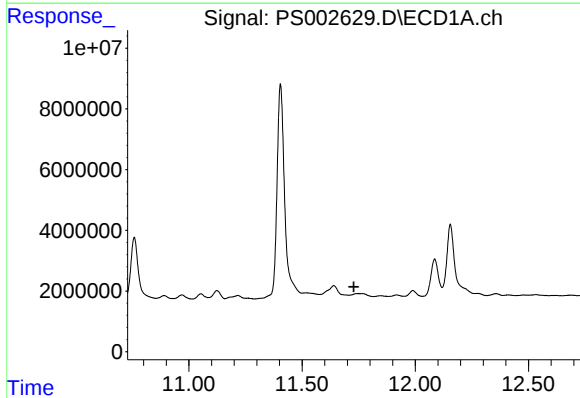


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.729 min
Response: 0
Conc: N.D.

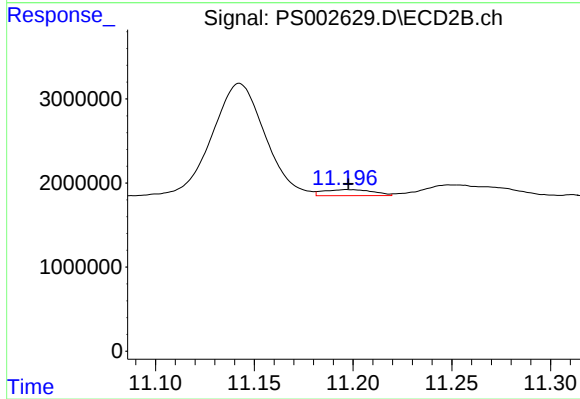

#5 DICAMBA


R.T.: 11.198 min
Delta R.T.: 0.000 min
Response: 1242839
Conc: 0.87 ng/ml

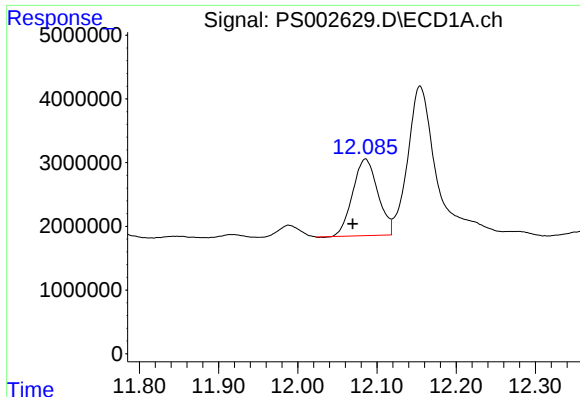

#6 MCPP


R.T.: 12.085 min
Delta R.T.: 0.016 min
Response: 26613423
Conc: 26.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

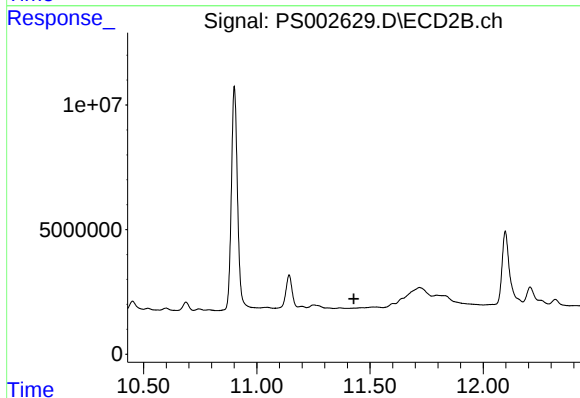


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.429 min
Response: 0
Conc: N.D.

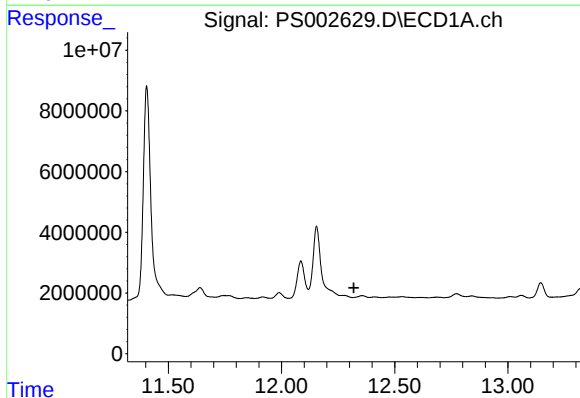


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.319 min
Response: 0
Conc: N.D.

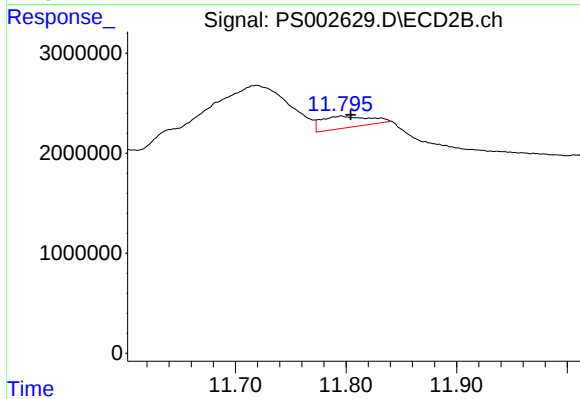

#7 MCPA


R.T.: 11.796 min
Delta R.T.: -0.009 min
Response: 3762478
Conc: 2.62 ug/ml

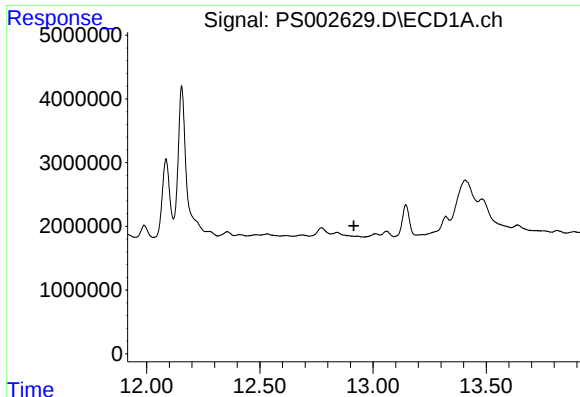

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

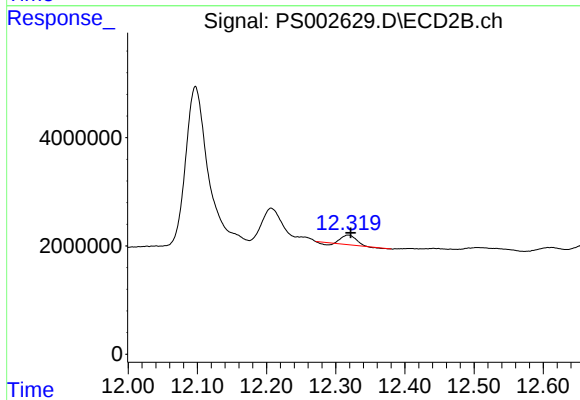


#8 DICHLORPROP

R.T.: 12.318 min
Delta R.T.: -0.003 min
Response: 2089038
Conc: 5.84 ng/ml

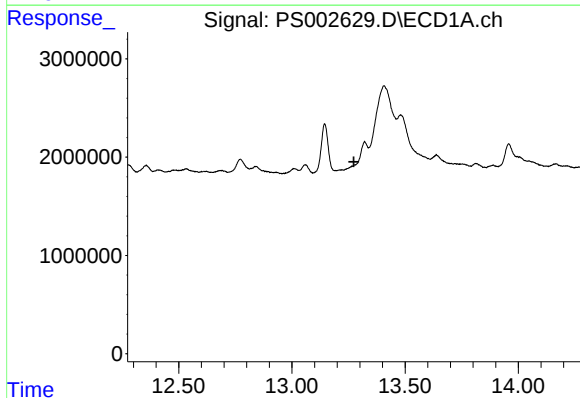


#9 2,4-D

R.T.: 13.321 min
Delta R.T.: 0.047 min
Response: -1441801
Conc: N.D.

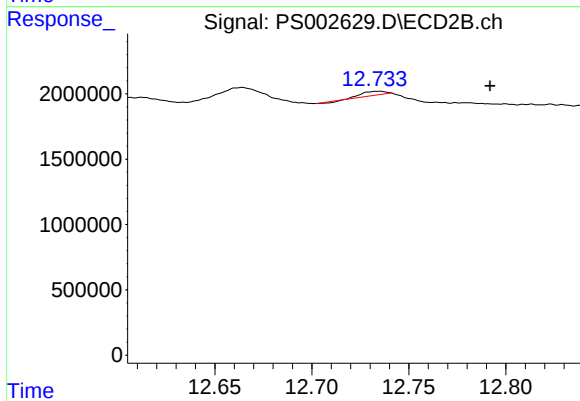

#9 2,4-D


R.T.: 12.734 min
Delta R.T.: -0.058 min
Response: 243877
Conc: 0.58 ng/ml

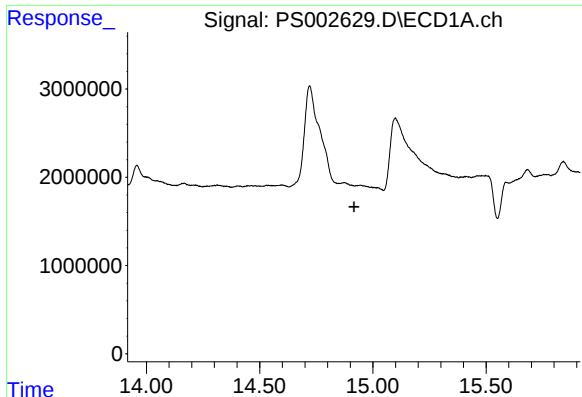

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

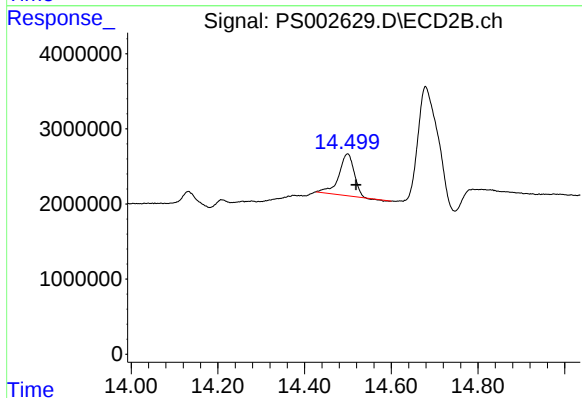


#12 2,4,5-T

R.T.: 14.499 min
Delta R.T.: -0.019 min
Response: 13468091
Conc: 7.87 ng/ml

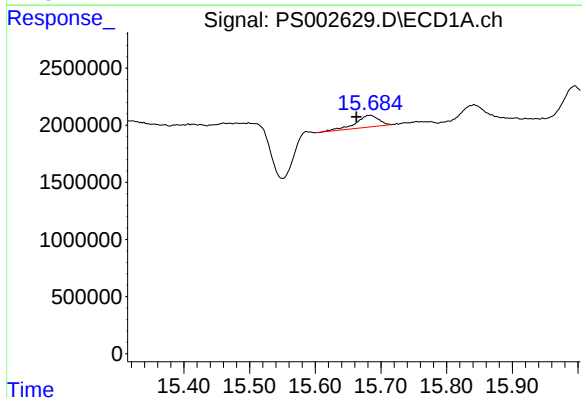


#13 2,4-DB

R.T.: 15.683 min
Delta R.T.: 0.020 min
Response: 2531739
Conc: 11.19 ng/ml

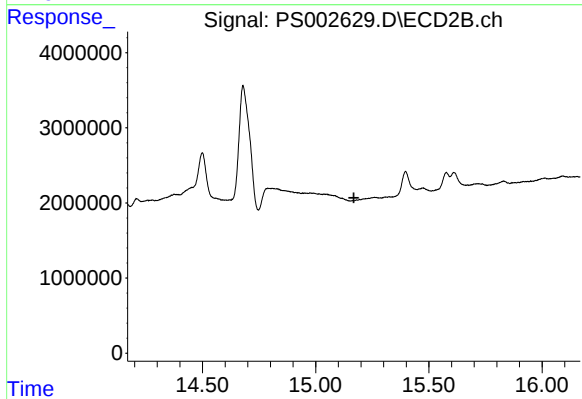

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.169 min
Response: 0
Conc: N.D.

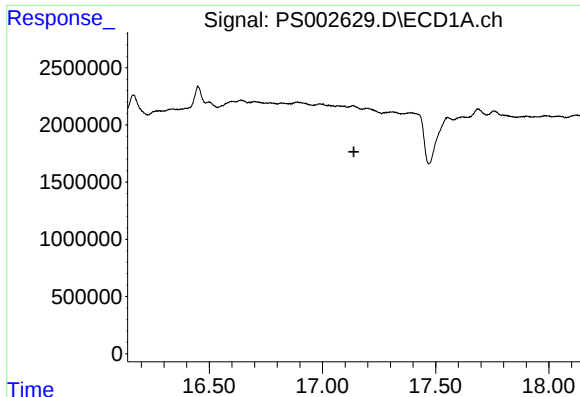

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

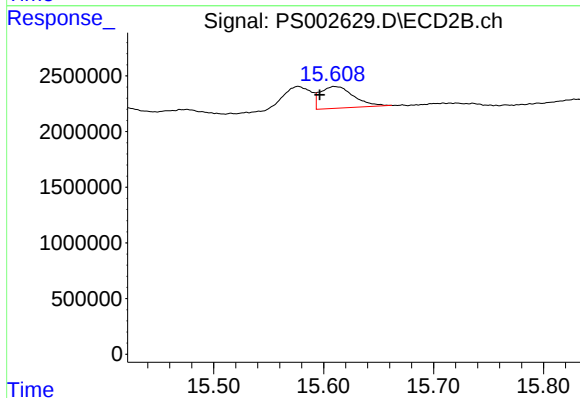


#14 DINOSEB

R.T.: 15.611 min
Delta R.T.: 0.014 min
Response: 4259253
Conc: 2.79 ng/ml

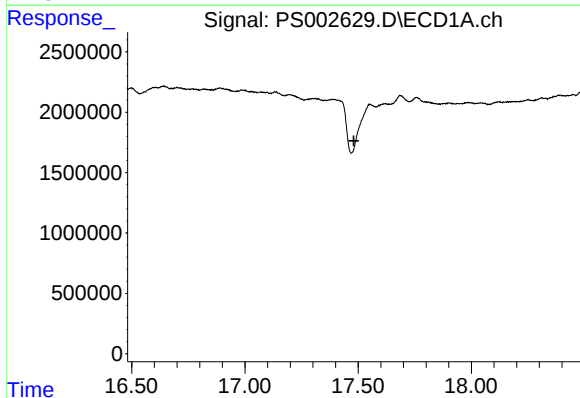

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.481 min
Response: 0
Conc: N.D.

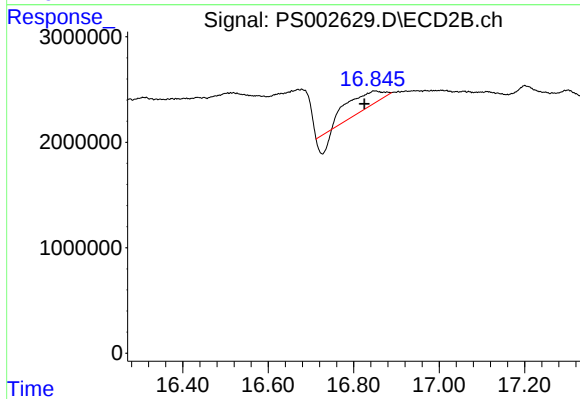

#16 DCPA

R.T.: 16.849 min
Delta R.T.: 0.024 min
Response: 6806750
Conc: 2.34 ng/ml