

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121718\
 Data File : PS002640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2018 00:20
 Operator : EI\SJ
 Sample : J6429-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 02:22:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.395	10.892	119.4E6	130.7E6	376.031	337.891
Target Compounds							
1) T	Dalapon	2.874	2.338	24059496	42674417	52.267	93.763 #
2) T	3,5-DICHL...	0.000	9.137	0	96506682	N.D.	200.826 #
3) T	4-Nitroph...	11.042	10.049	1933466	3327848	12.203	18.619 #
5) T	DICAMBA	0.000	11.134	0	29370936	N.D.	20.602 #
6) T	MCP	12.075	0.000	29742789	0	29.810	N.D. #
7) T	MCPA	0.000	11.821	0	2358396	N.D.	1.641 #
12) T	2,4,5-T	0.000	14.562	0	1289950	N.D.	0.754 #
14) T	DINOSEB	0.000	15.630	0	760364	N.D.	0.498 #
16) T	DCPA	0.000	16.854	0	3434168	N.D.	1.182 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121718\
Data File : PS002640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2018 00:20
Operator : EI\SJ
Sample : J6429-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 02:22:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

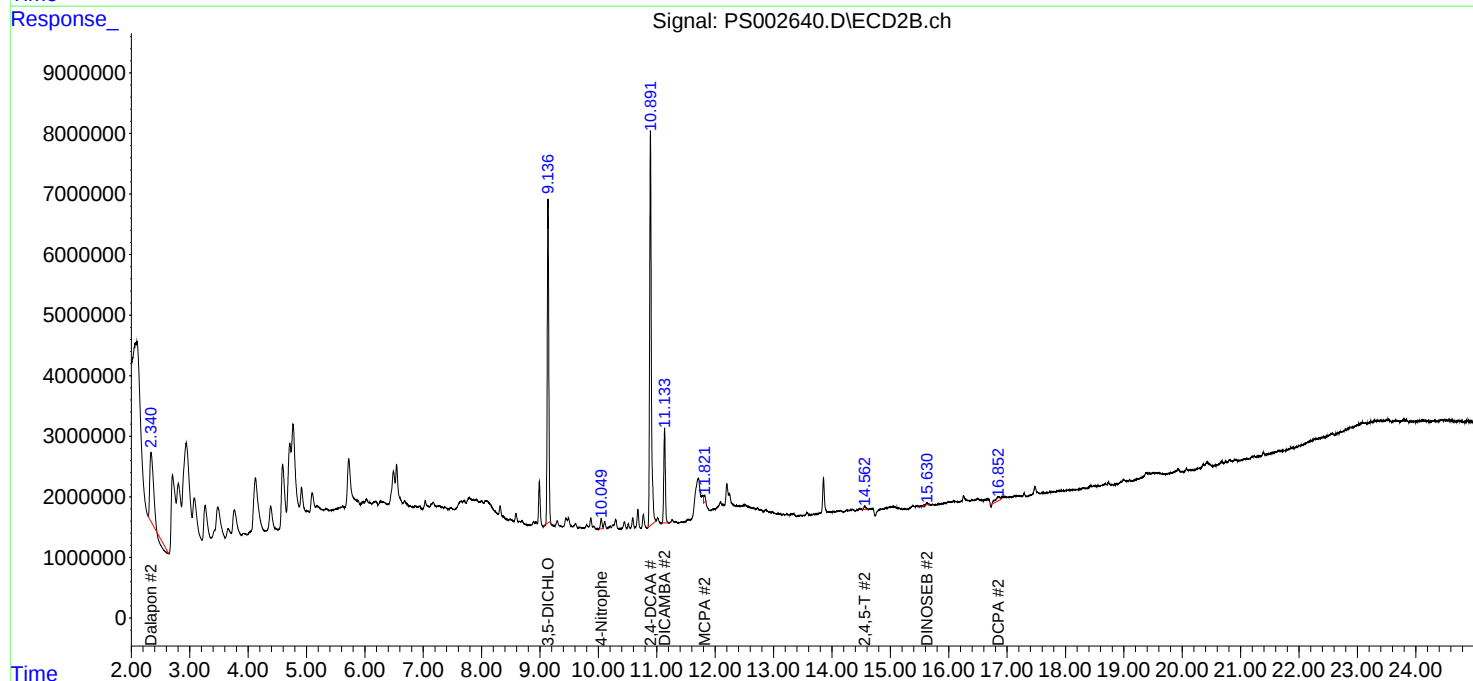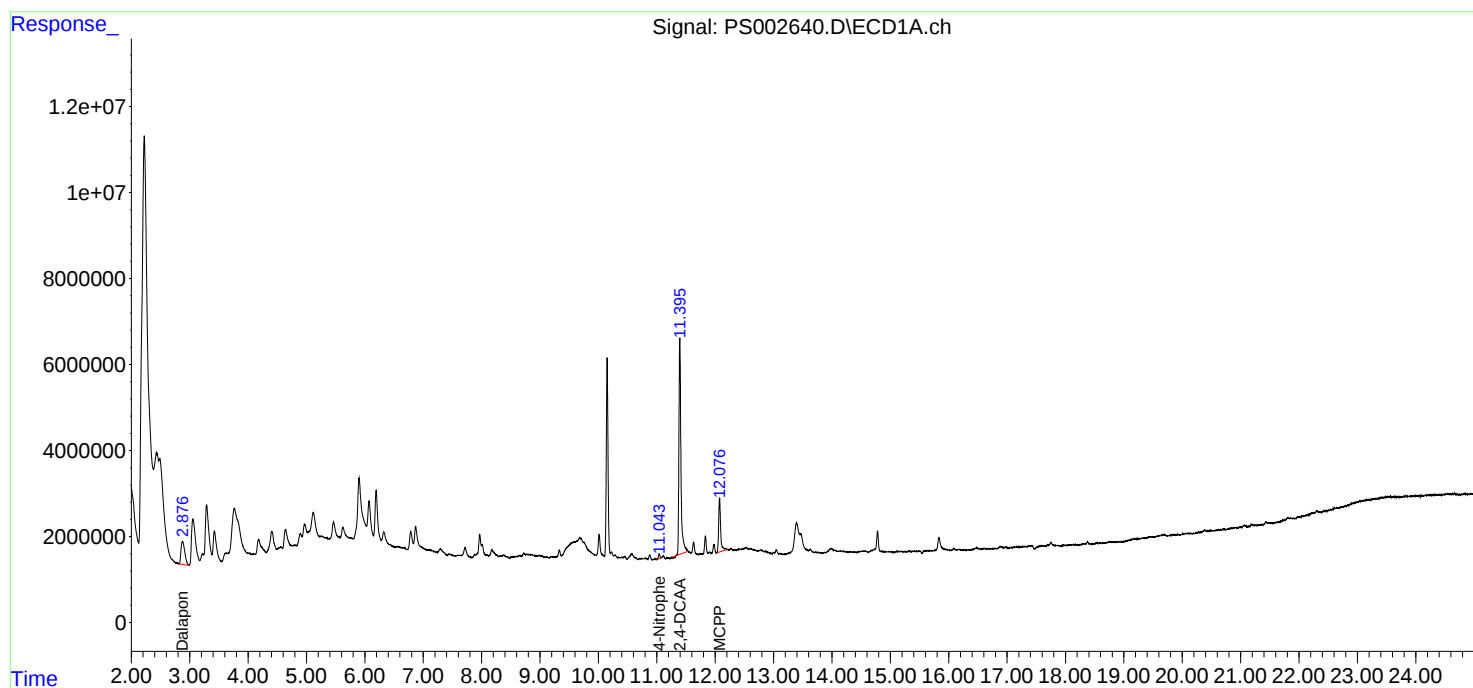


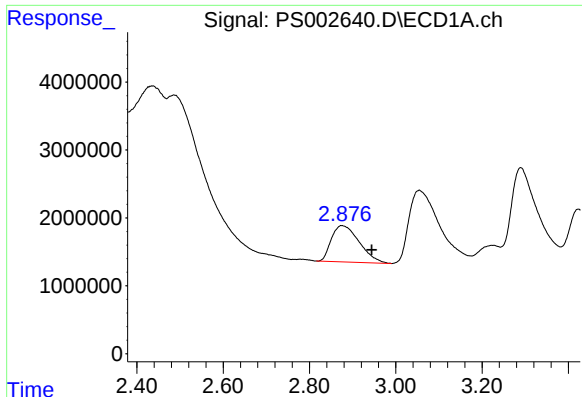

#1 Dalapon


R.T.: 2.874 min
Delta R.T.: -0.070 min
Response: 24059496
Conc: 52.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

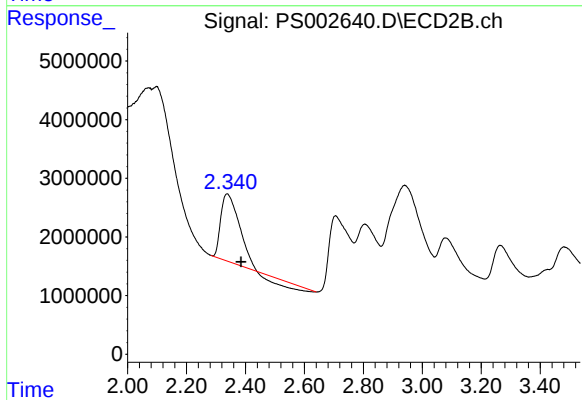


#1 Dalapon

R.T.: 2.338 min
Delta R.T.: -0.047 min
Response: 42674417
Conc: 93.76 ng/ml

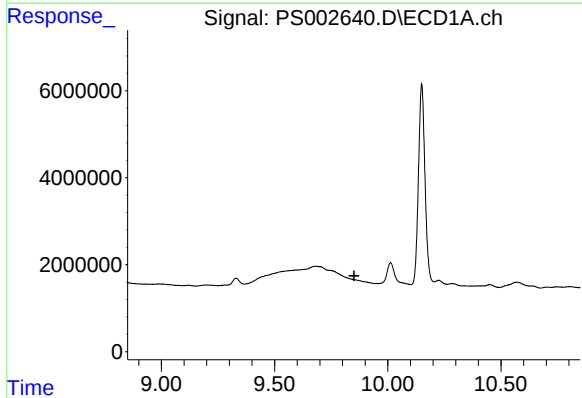


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.851 min
Response: 0
Conc: N.D.

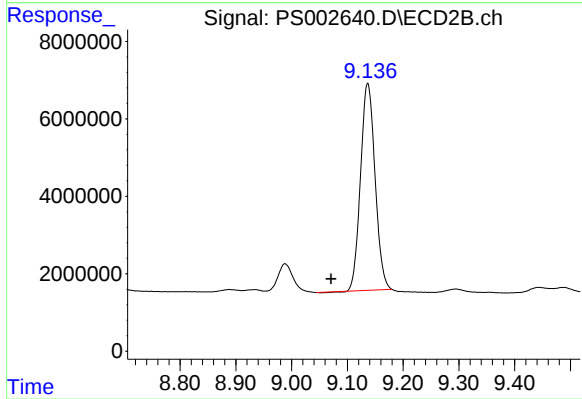

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.137 min
Delta R.T.: 0.066 min
Response: 96506682
Conc: 200.83 ng/ml

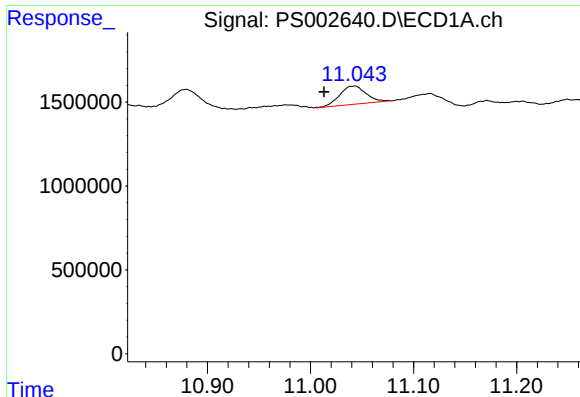

#3 4-Nitrophenol


R.T.: 11.042 min
Delta R.T.: 0.029 min
Response: 1933466
Conc: 12.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

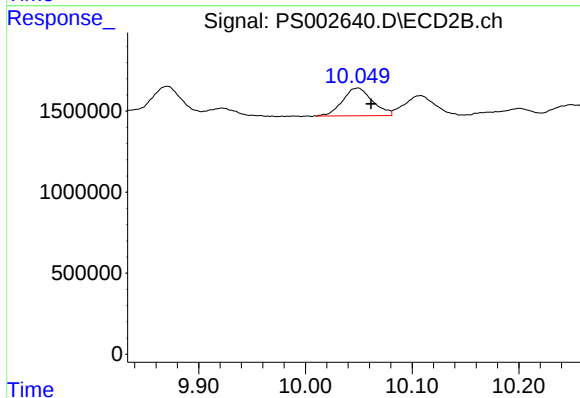


#3 4-Nitrophenol

R.T.: 10.049 min
Delta R.T.: -0.012 min
Response: 3327848
Conc: 18.62 ng/ml

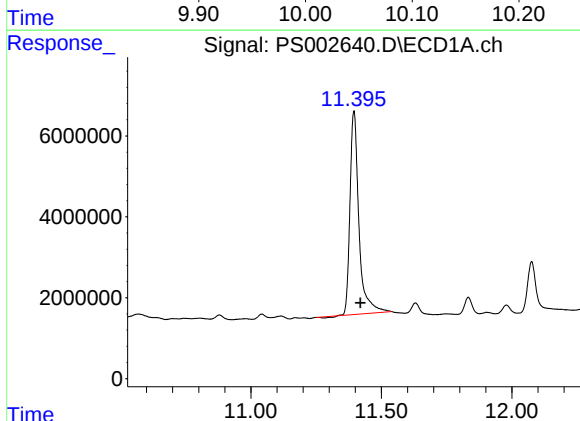


#4 2,4-DCAA

R.T.: 11.395 min
Delta R.T.: -0.025 min
Response: 119359525
Conc: 376.03 ng/ml

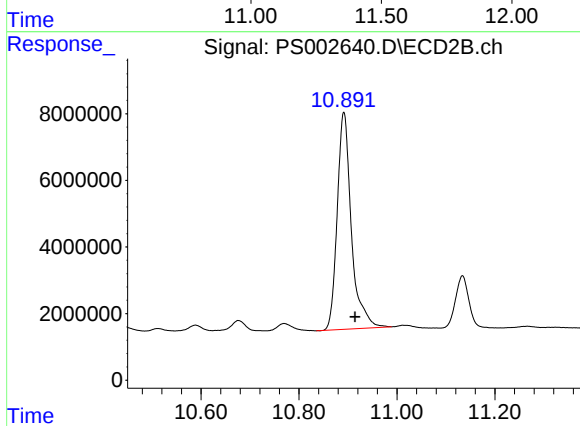

#4 2,4-DCAA


R.T.: 10.892 min
Delta R.T.: -0.023 min
Response: 130685833
Conc: 337.89 ng/ml

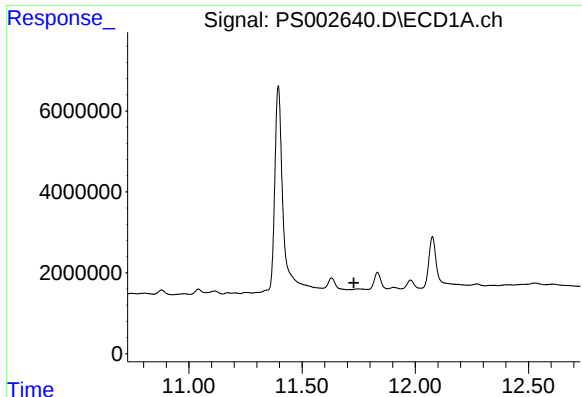

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

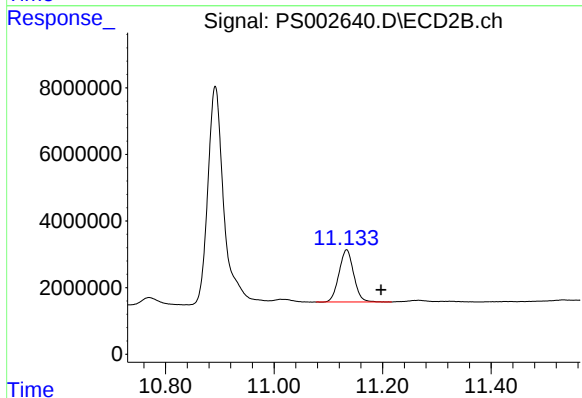


#5 DICAMBA

R.T.: 11.134 min
Delta R.T.: -0.064 min
Response: 29370936
Conc: 20.60 ng/ml

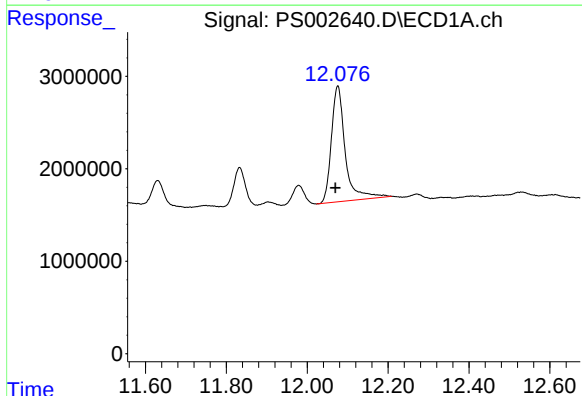


#6 MCP

R.T.: 12.075 min
Delta R.T.: 0.006 min
Response: 29742789
Conc: 29.81 ug/ml

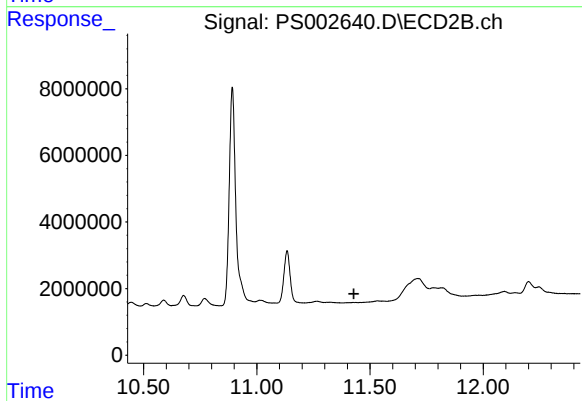

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.429 min
Response: 0
Conc: N.D.

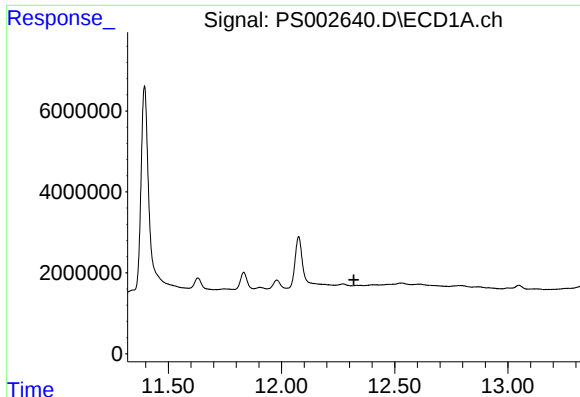

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

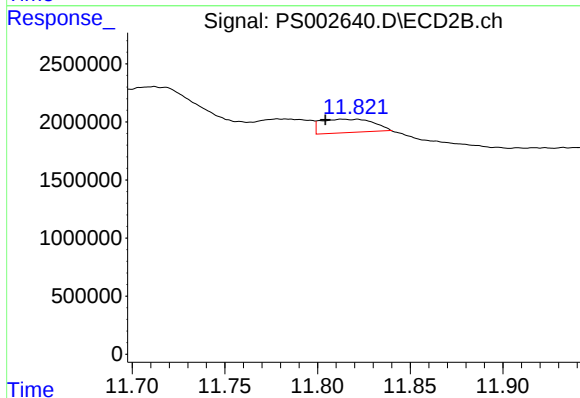


#7 MCPA

R.T.: 11.821 min
Delta R.T.: 0.017 min
Response: 2358396
Conc: 1.64 ug/ml

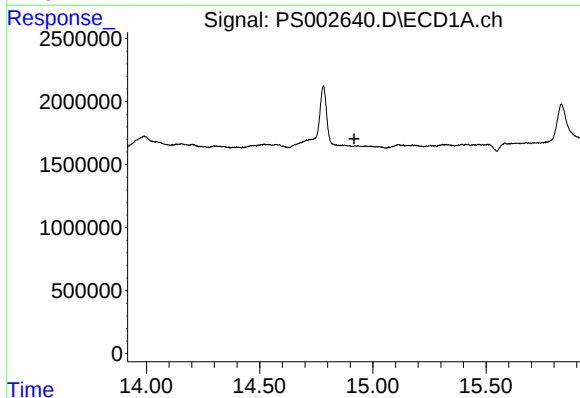


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.917 min
Response: 0
Conc: N.D.

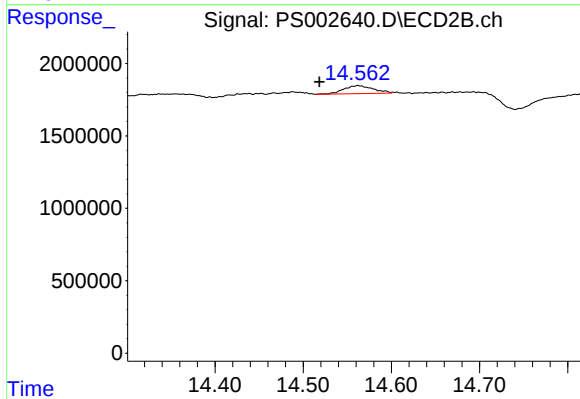

#12 2,4,5-T


R.T.: 14.562 min
Delta R.T.: 0.044 min
Response: 1289950
Conc: 0.75 ng/ml

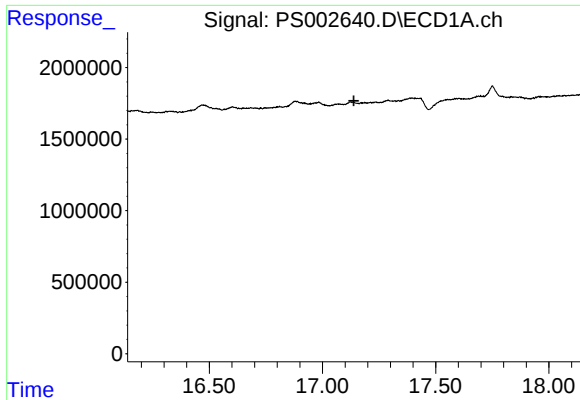

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

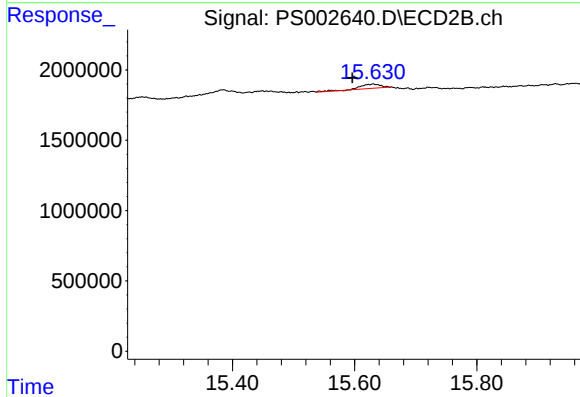


#14 DINOSEB

R.T.: 15.630 min
Delta R.T.: 0.034 min
Response: 760364
Conc: 0.50 ng/ml

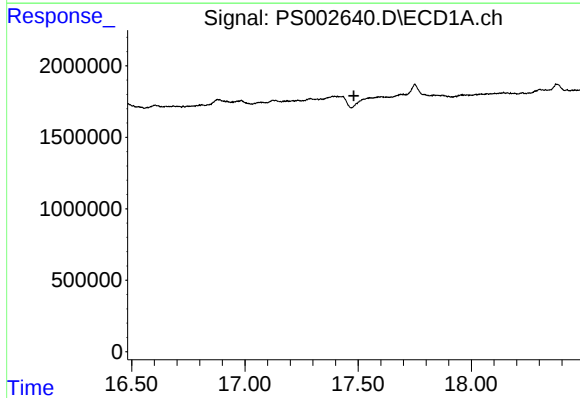

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.481 min
Response: 0
Conc: N.D.

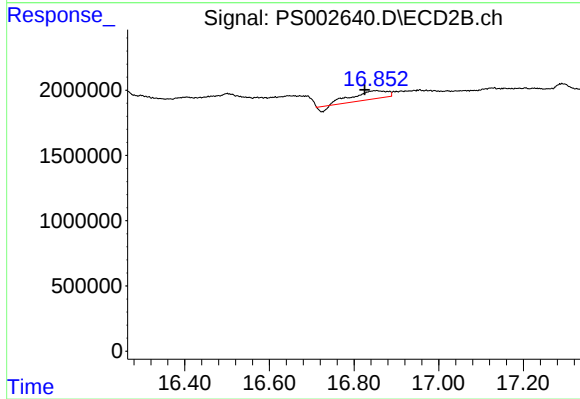

#16 DCPA

R.T.: 16.854 min
Delta R.T.: 0.028 min
Response: 3434168
Conc: 1.18 ng/ml