

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
 Data File : PS008045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 07:57
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 11:10:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10) T	Pentachlo...	0.000	6.454	0	8810632	N.D. <MDL
12) T	2,4,5-T	7.444	0.000	51179070	0	5.530 N.D. #
15) T	Picloram	0.000	8.854	0	8930258	N.D. 1.446
16) T	DCPA	0.000	8.854	0	8930258	N.D. 1.556



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
Data File : PS008045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 07:57
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 11:10:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

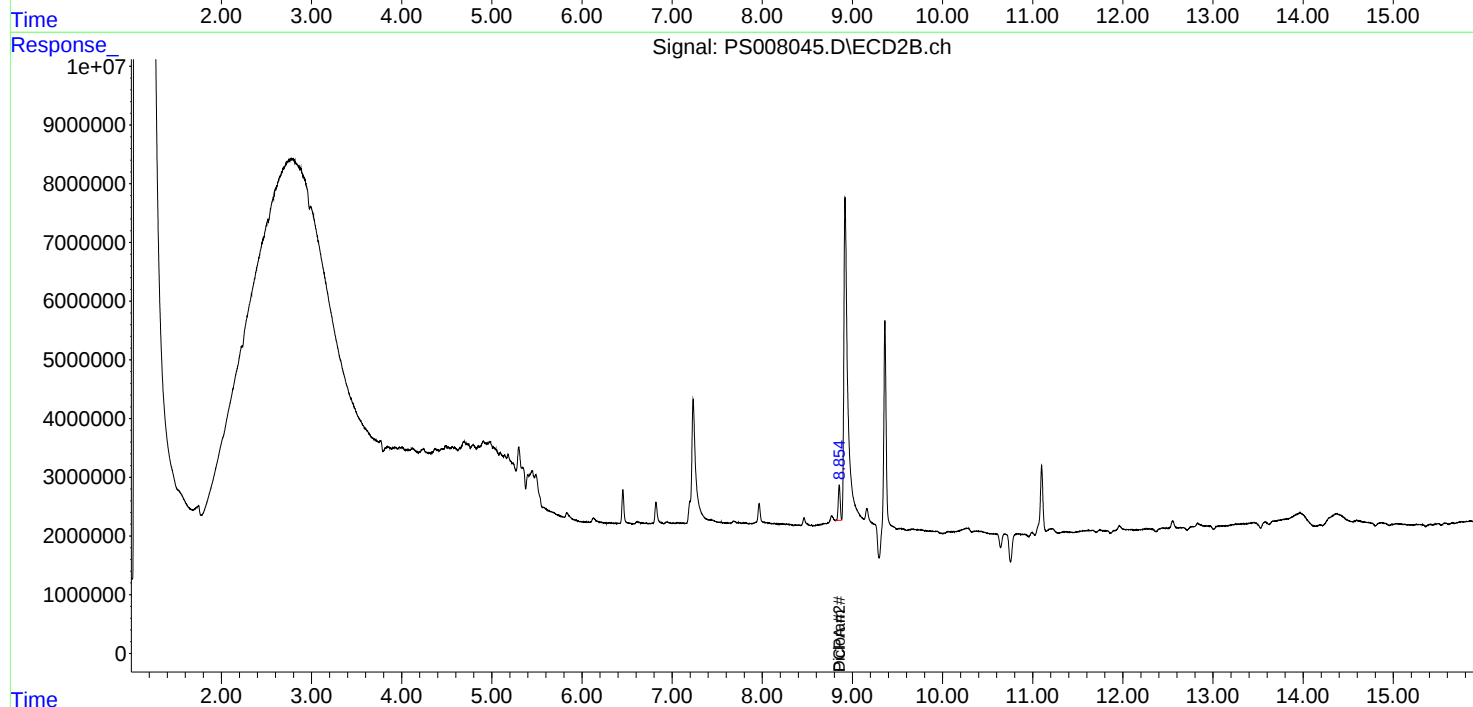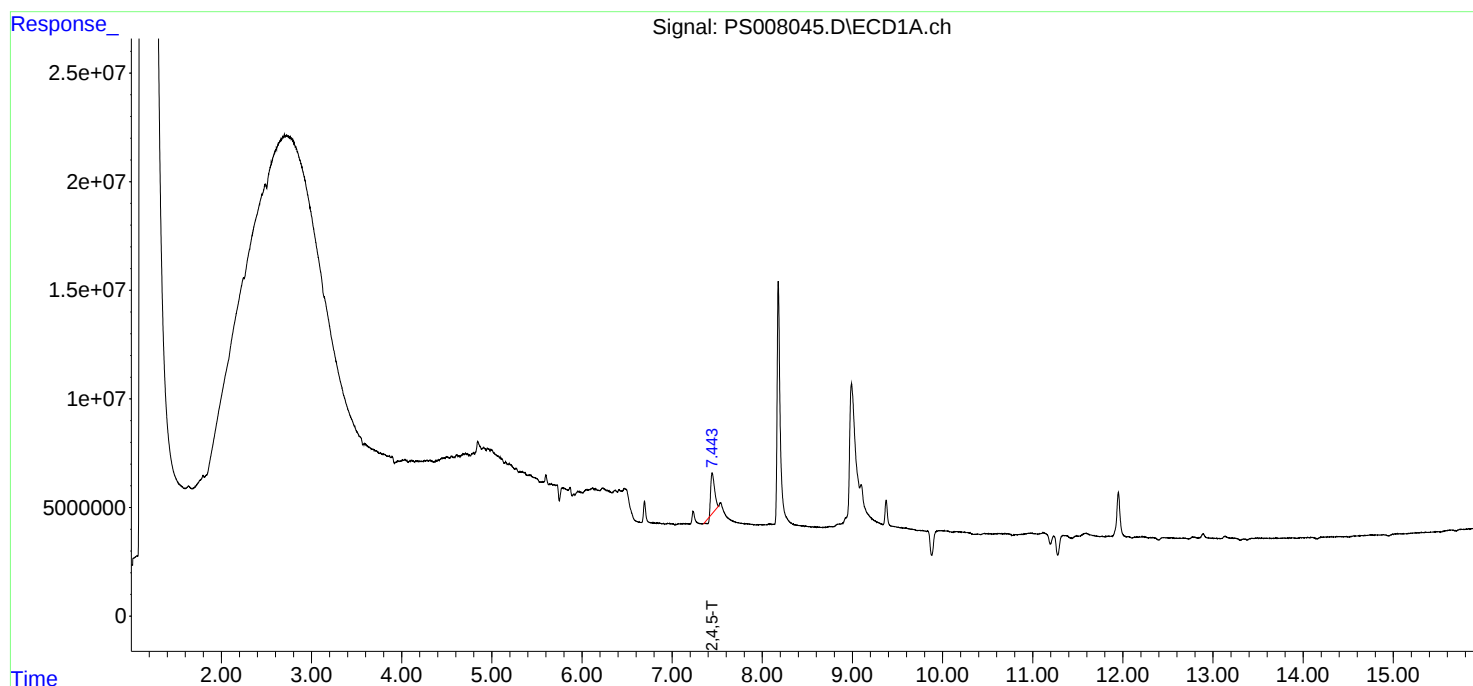


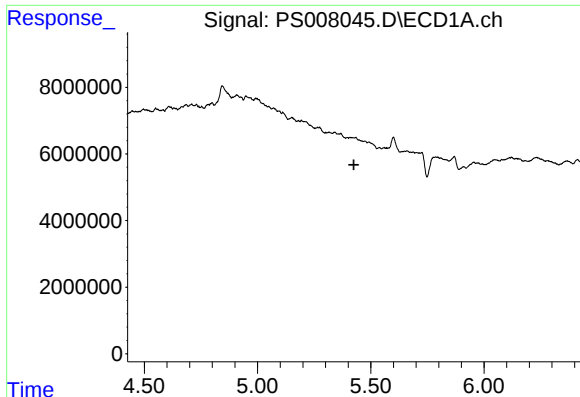

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.425 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

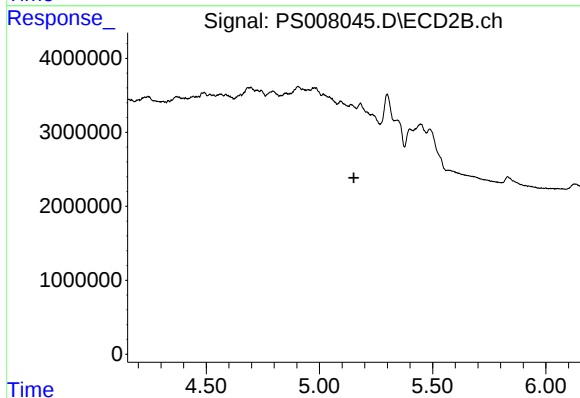


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.152 min
Response: 0
Conc: N.D.

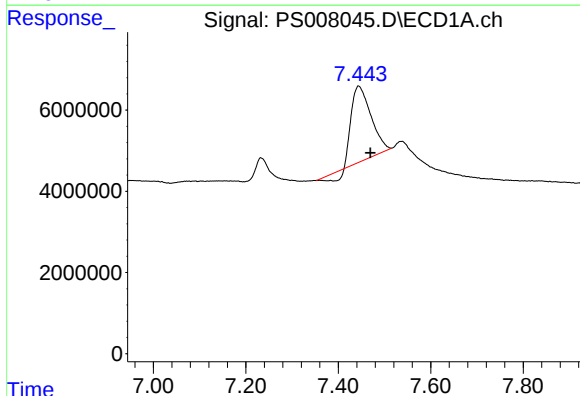


#12 2,4,5-T

R.T.: 7.444 min
Delta R.T.: -0.025 min
Response: 51179070
Conc: 5.53 ng/ml

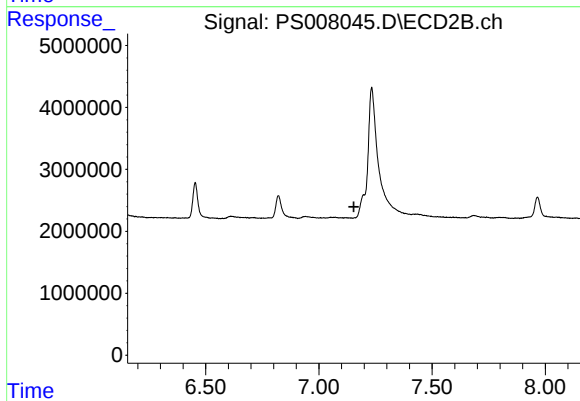

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

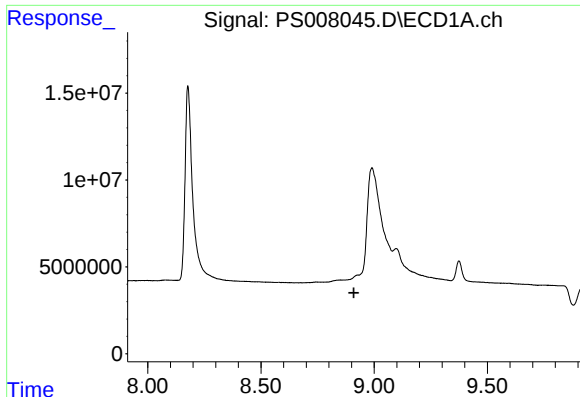

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 8.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

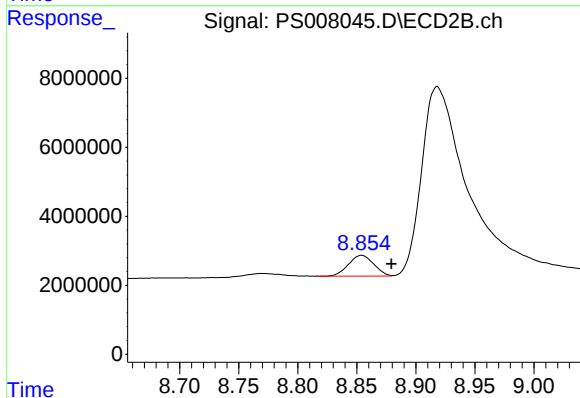


#15 Picloram

R.T.: 8.854 min
Delta R.T.: -0.025 min
Response: 8930258
Conc: 1.45 ng/ml

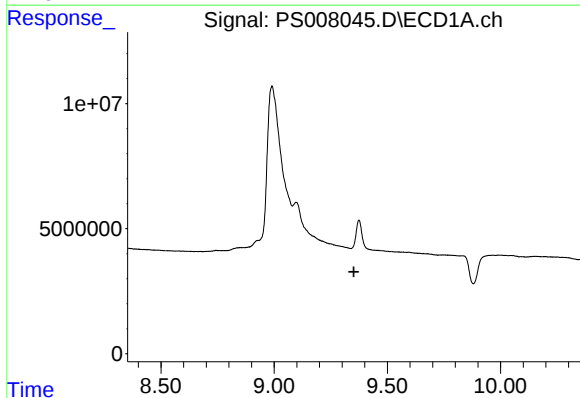

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.352 min
Response: 0
Conc: N.D.

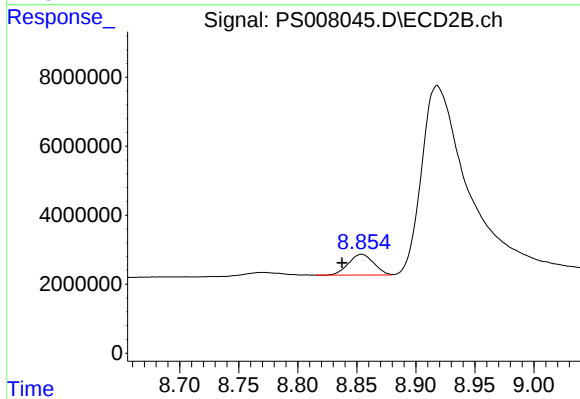

#16 DCPA

R.T.: 8.854 min
Delta R.T.: 0.017 min
Response: 8930258
Conc: 1.56 ng/ml