

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
 Data File : PS008057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 13:49
 Operator : SM\AJ
 Sample : K6113-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 15:14:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.430	5.156	418.9E6	224.3E6	267.768	289.098
Target Compounds							
1) T	Dalapon	1.988	1.708	58145166	169.8E6	28.512	142.924 #
2) T	3,5-DICHL...	0.000	4.446	0	5087233	N.D.	4.916
3) T	4-Nitroph...	0.000	4.776	0	9188358	N.D.	20.290
5) T	DICAMBA	5.516	0.000	55012874	0	9.669	N.D. #
8) T	DICHLORPROP	0.000	5.829	0	10866691	N.D.	15.159
9) T	2,4-D	6.476	6.057	77265748	6848646	48.027	7.751 #
10) T	Pentachlo...	0.000	6.366	0	25072698	N.D.	2.297
11) T	2,4,5-TP ...	0.000	6.754	0	36124492	N.D.	8.423



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
Data File : PS008057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 13:49
Operator : SM\AJ
Sample : K6113-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 15:14:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

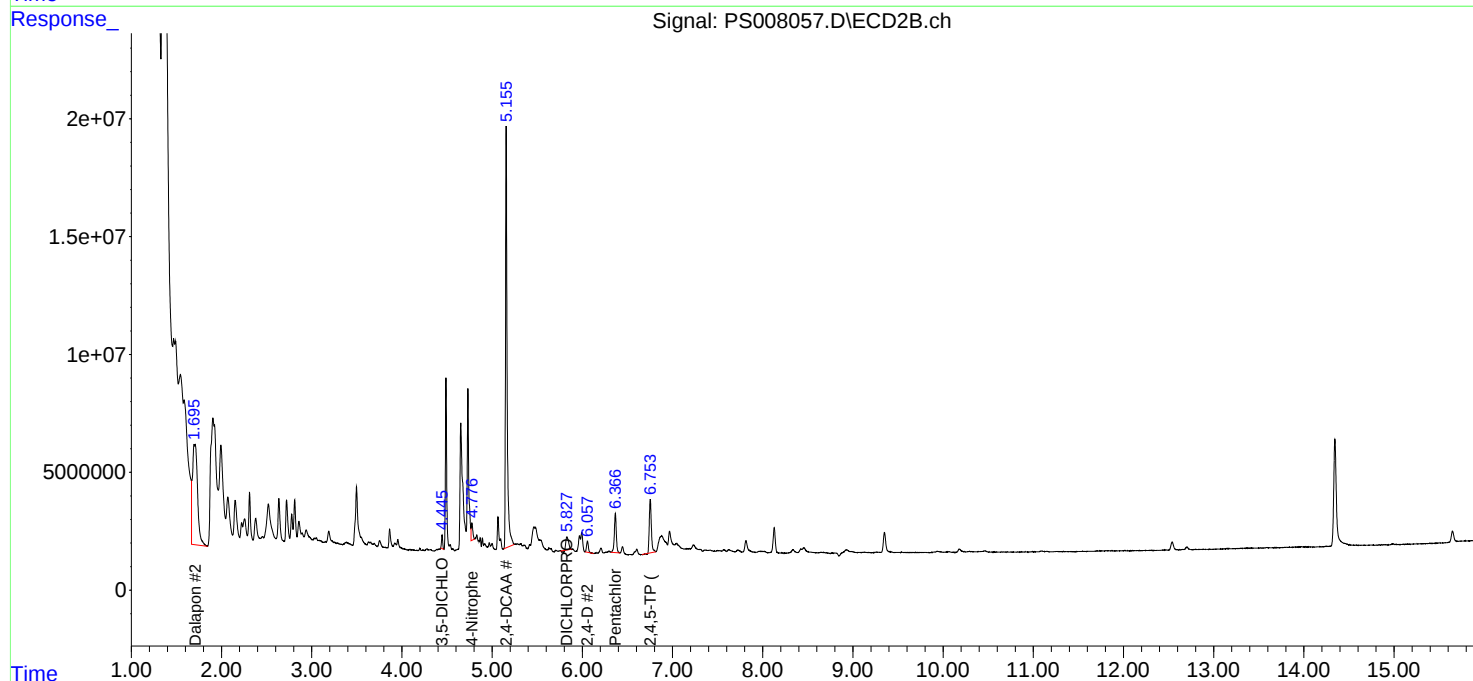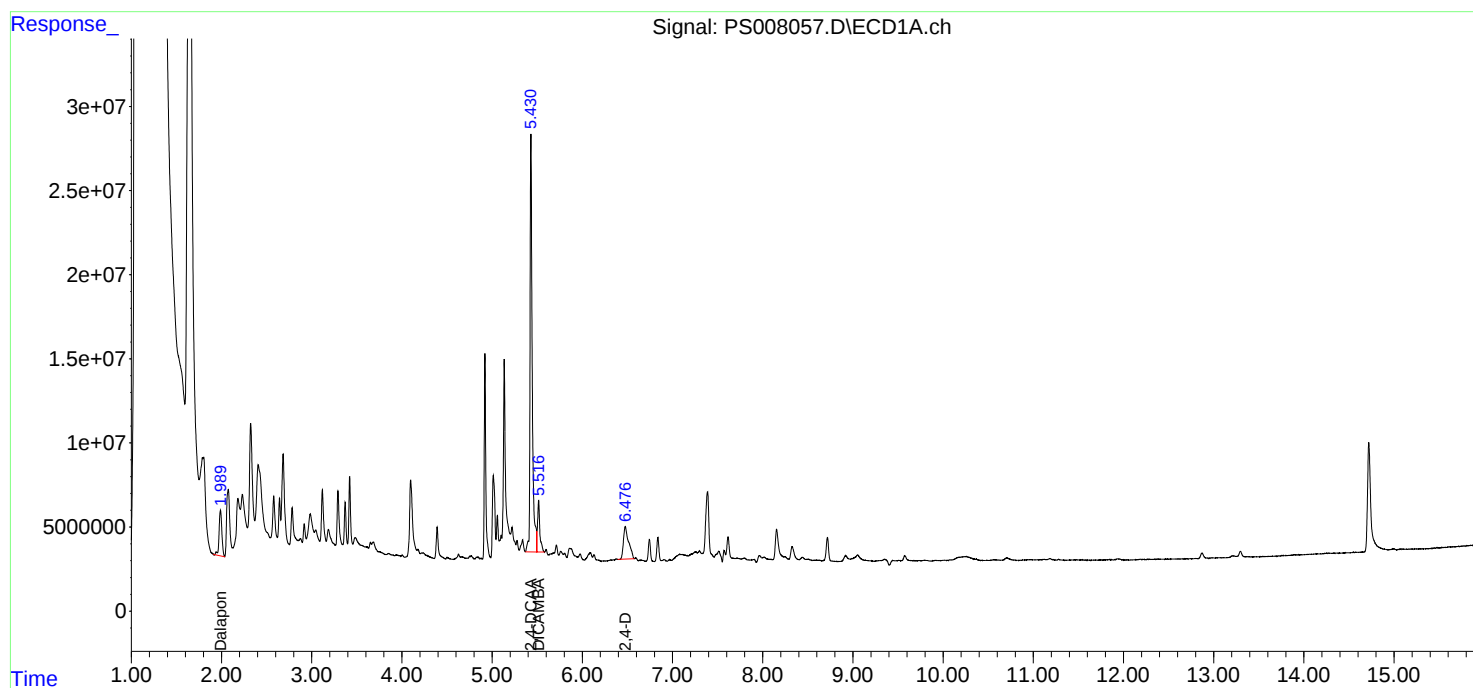


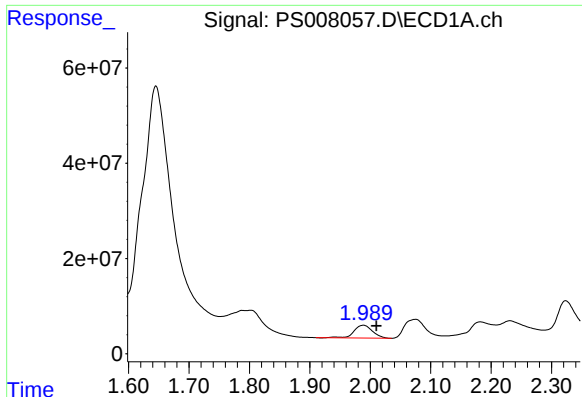

#1 Dalapon


R.T.: 1.988 min
Delta R.T.: -0.022 min
Response: 58145166
Conc: 28.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

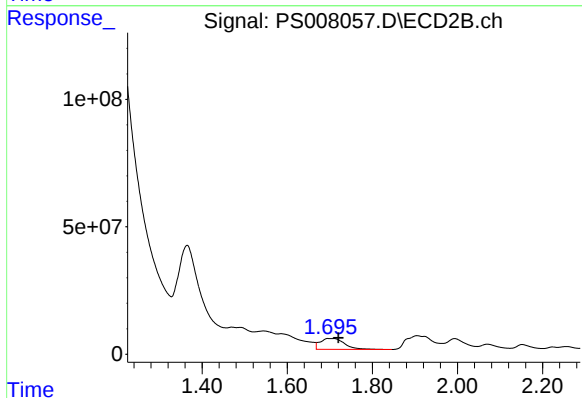


#1 Dalapon

R.T.: 1.708 min
Delta R.T.: -0.013 min
Response: 169763464
Conc: 142.92 ng/ml

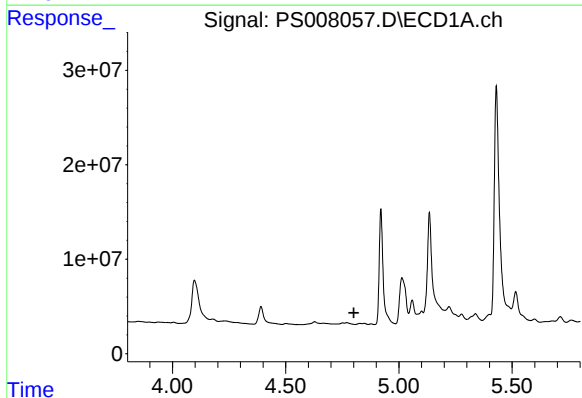


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

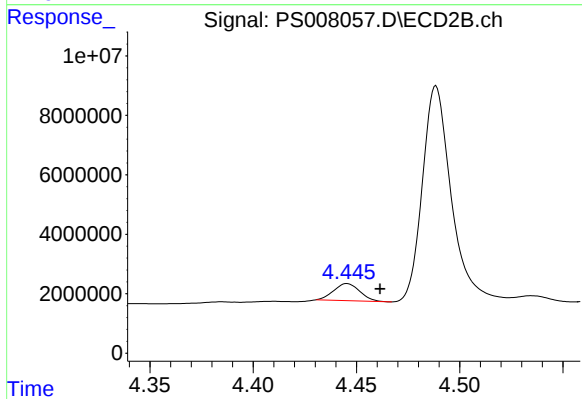

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.446 min
Delta R.T.: -0.016 min
Response: 5087233
Conc: 4.92 ng/ml

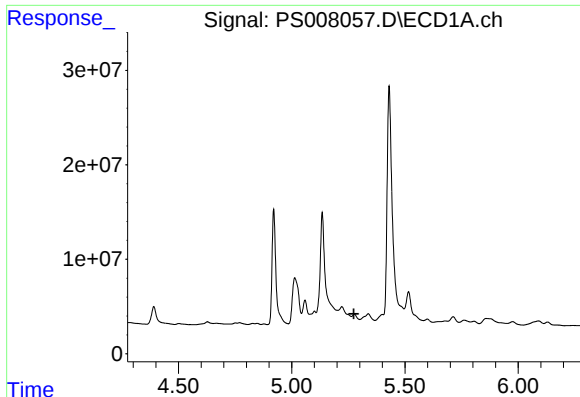

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

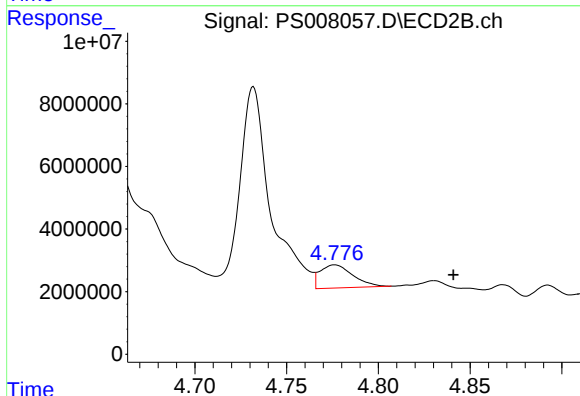


#3 4-Nitrophenol

R.T.: 4.776 min
Delta R.T.: -0.065 min
Response: 9188358
Conc: 20.29 ng/ml

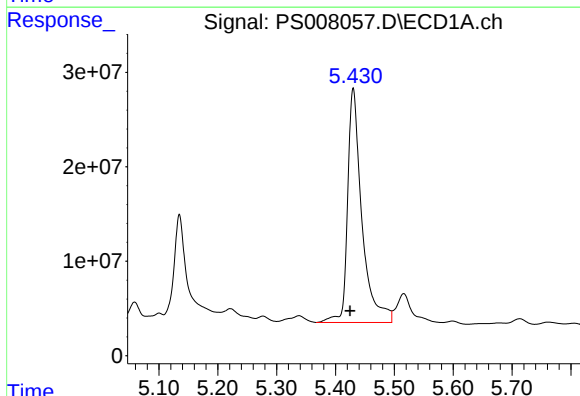


#4 2,4-DCAA

R.T.: 5.430 min
Delta R.T.: 0.005 min
Response: 418878075
Conc: 267.77 ng/ml

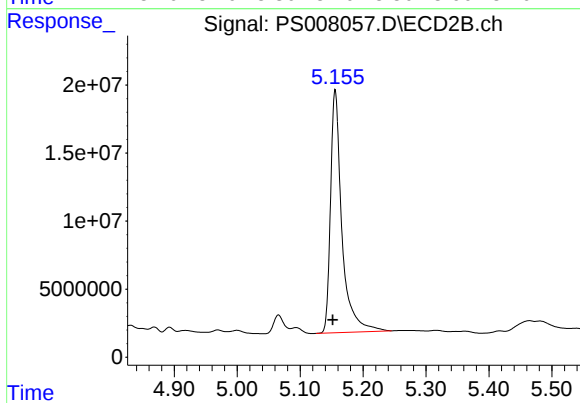

#4 2,4-DCAA


R.T.: 5.156 min
Delta R.T.: 0.004 min
Response: 224316028
Conc: 289.10 ng/ml

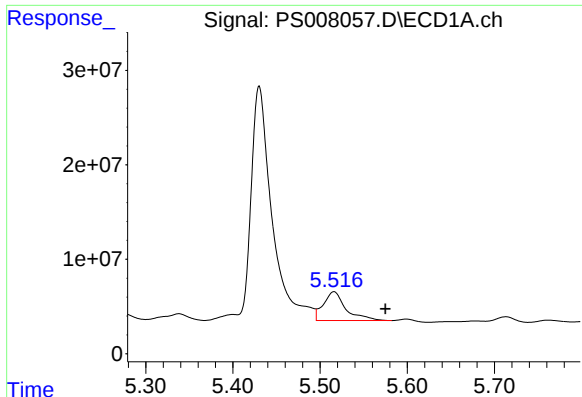

#5 DICAMBA


R.T.: 5.516 min
Delta R.T.: -0.059 min
Response: 55012874
Conc: 9.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

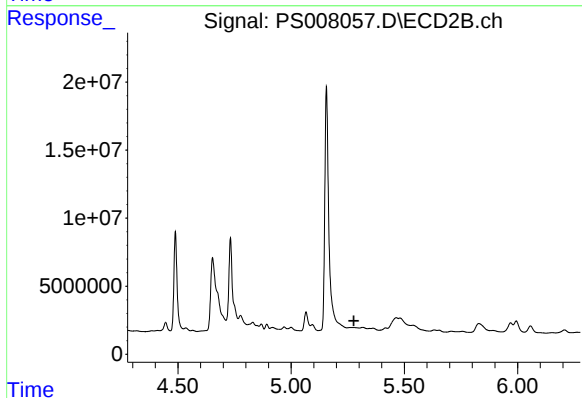


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

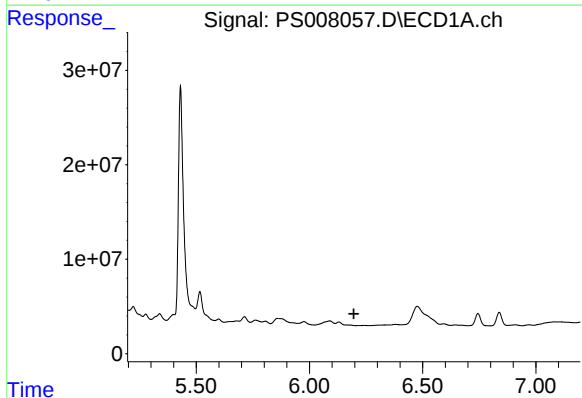


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

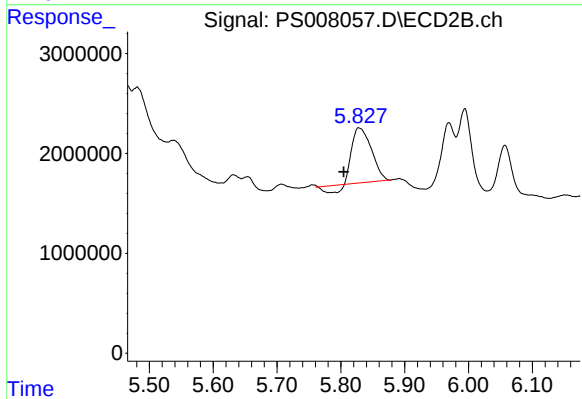

#8 DICHLORPROP


R.T.: 5.829 min
Delta R.T.: 0.025 min
Response: 10866691
Conc: 15.16 ng/ml

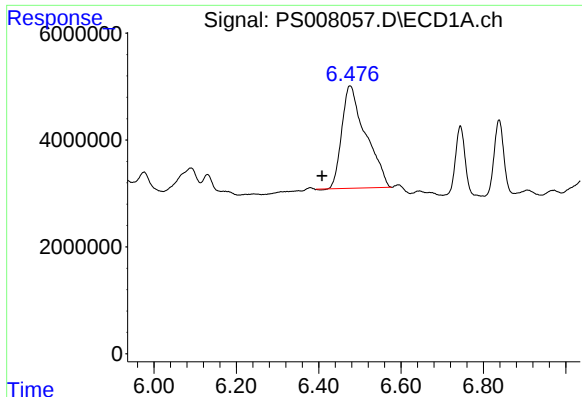

#9 2,4-D


R.T.: 6.476 min
Delta R.T.: 0.068 min
Response: 77265748
Conc: 48.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

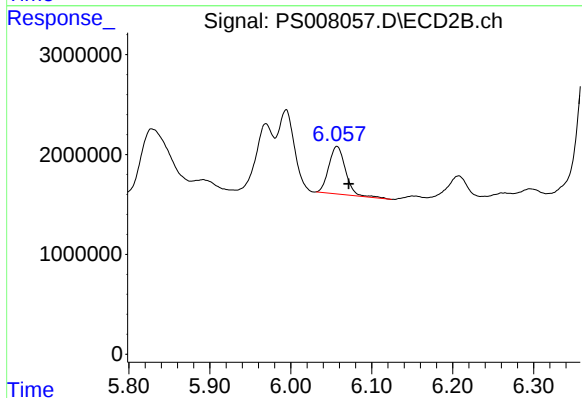


#9 2,4-D

R.T.: 6.057 min
Delta R.T.: -0.015 min
Response: 6848646
Conc: 7.75 ng/ml

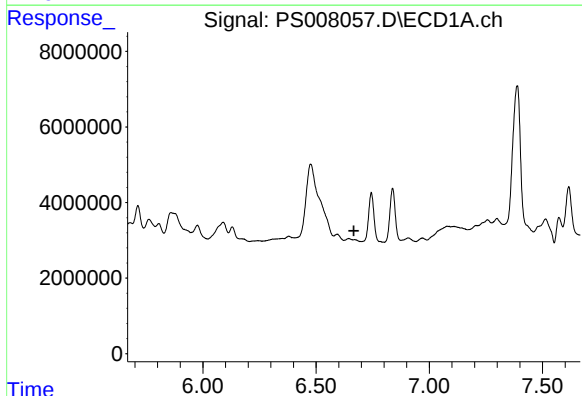


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

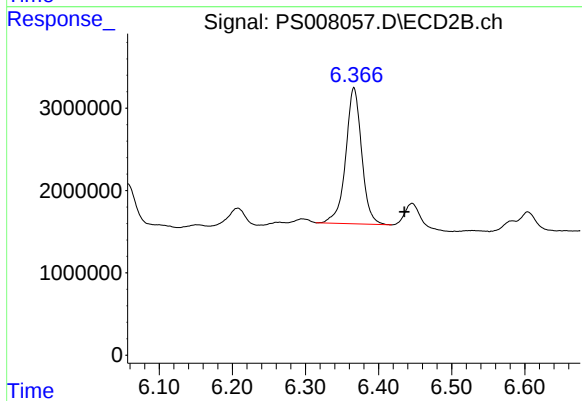

#10 Pentachlorophenol


R.T.: 6.366 min
Delta R.T.: -0.069 min
Response: 25072698
Conc: 2.30 ng/ml

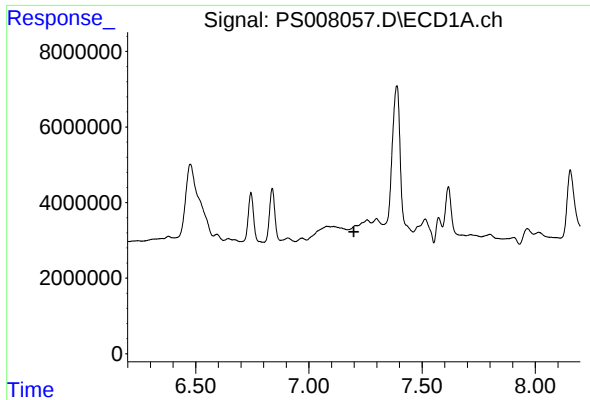

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

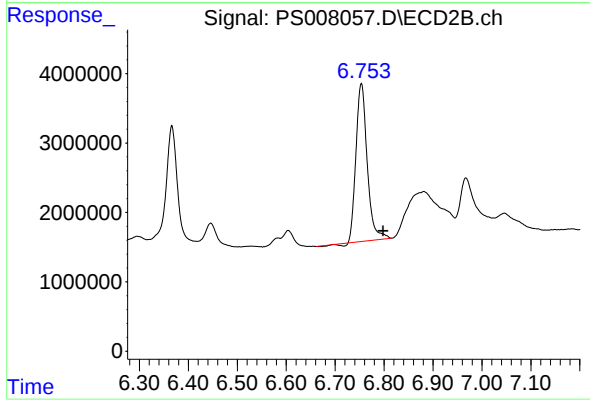

#11 2,4,5-TP (SILVEX)

R.T.: 6.754 min
Delta R.T.: -0.044 min
Response: 36124492
Conc: 8.42 ng/ml