

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
 Data File : PS008059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 14:33
 Operator : SM\AJ
 Sample : K6118-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 15:15:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.157	378.9E6	203.4E6	242.186	262.191
Target Compounds							
1) T	Dalapon	1.989	1.711	58479651	189.9E6	28.676	159.898 #
2) T	3,5-DICHL...	0.000	4.446	0	5063825	N.D.	4.893
3) T	4-Nitroph...	0.000	4.777	0	7364605	N.D.	16.263
5) T	DICAMBA	5.516	0.000	52861066	0	9.291	N.D. #
8) T	DICHLORPROP	0.000	5.829	0	9904503	N.D.	13.817
9) T	2,4-D	6.477	6.058	70648163	6829696	43.914	7.729 #
10) T	Pentachlo...	0.000	6.367	0	24995845	N.D.	2.290
11) T	2,4,5-TP ...	0.000	6.754	0	39757482	N.D.	9.270



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
Data File : PS008059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 14:33
Operator : SM\AJ
Sample : K6118-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 15:15:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

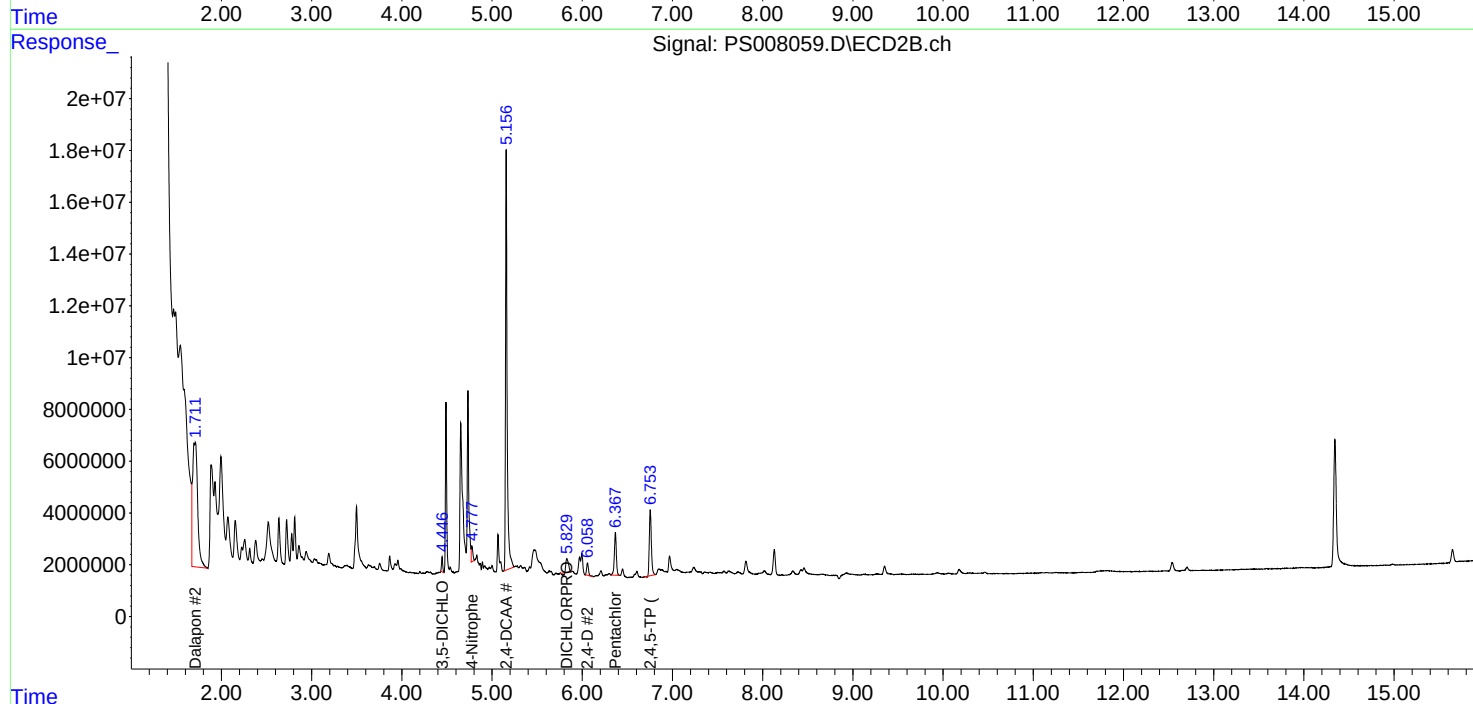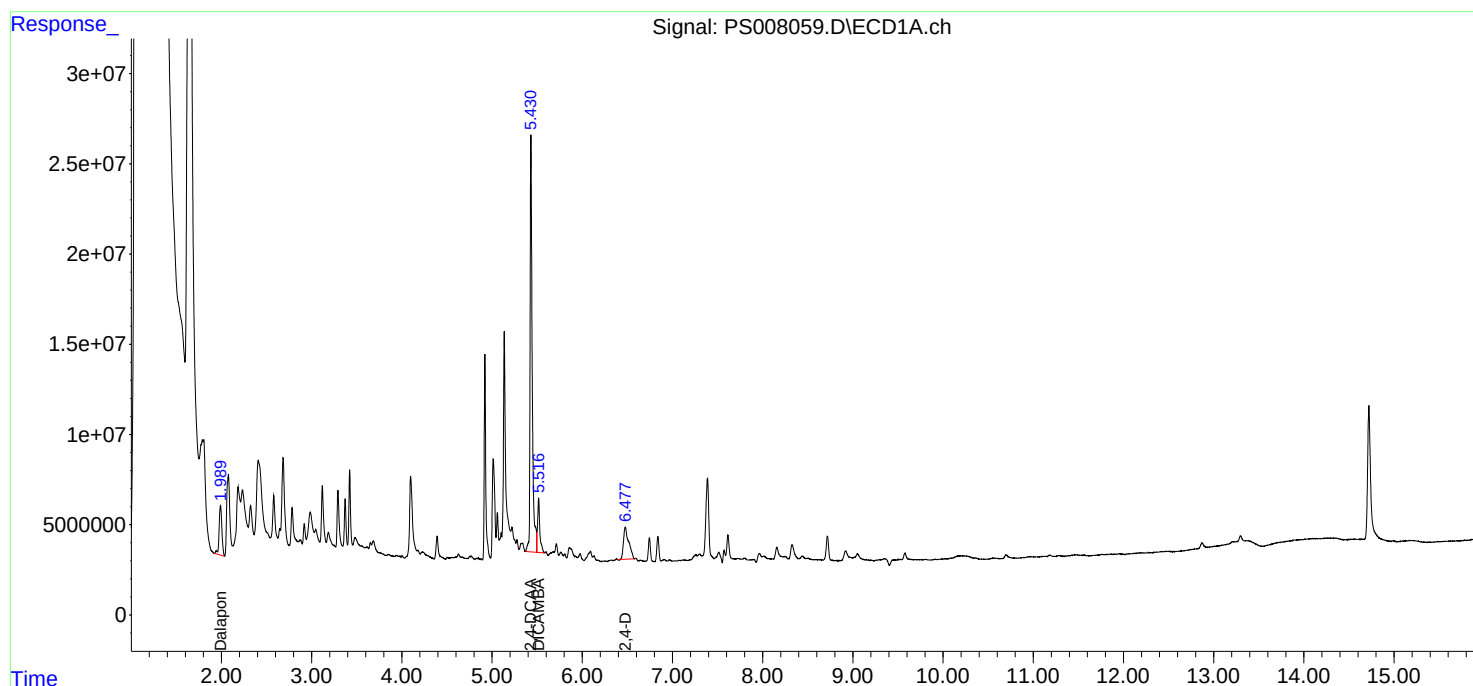


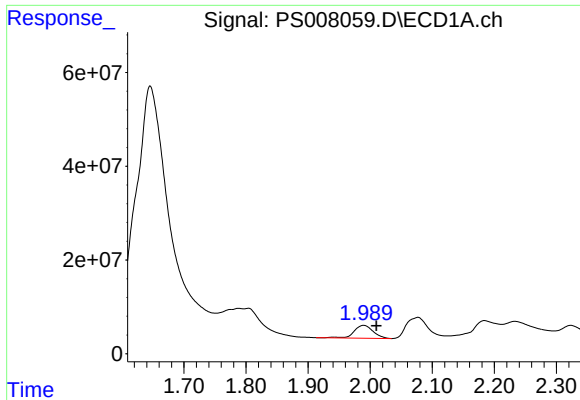

#1 Dalapon


R.T.: 1.989 min
Delta R.T.: -0.021 min
Response: 58479651
Conc: 28.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

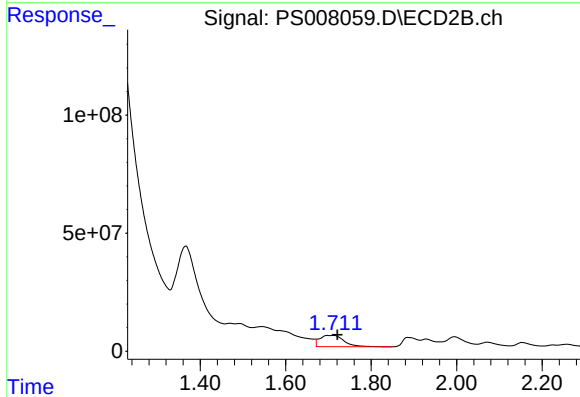


#1 Dalapon

R.T.: 1.711 min
Delta R.T.: -0.009 min
Response: 189925314
Conc: 159.90 ng/ml

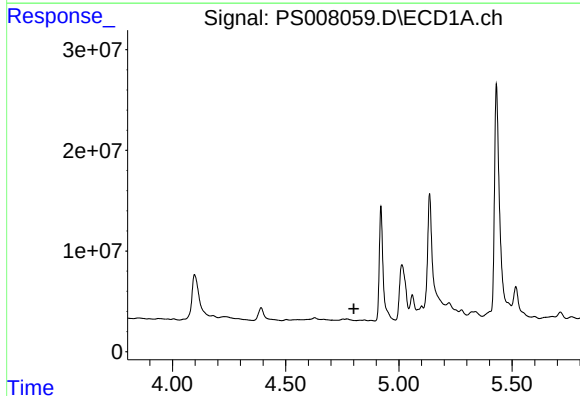


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

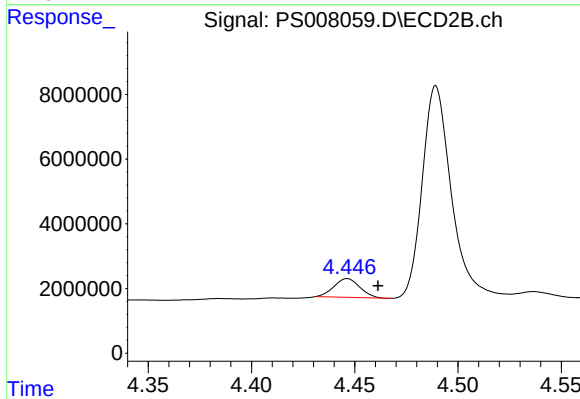

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.446 min
Delta R.T.: -0.015 min
Response: 5063825
Conc: 4.89 ng/ml

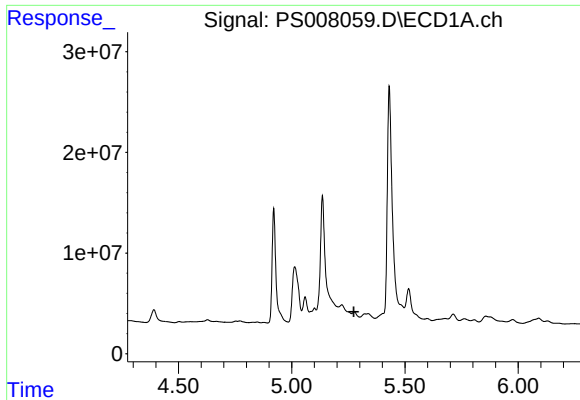

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

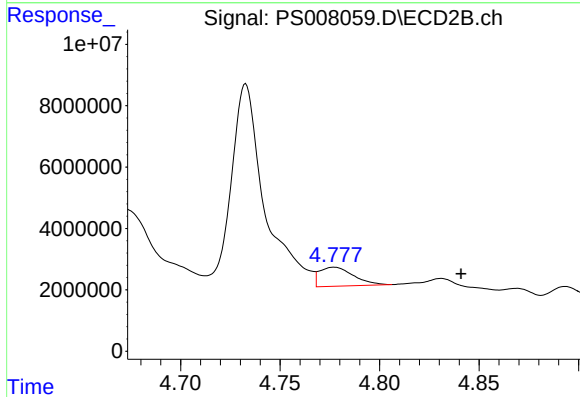


#3 4-Nitrophenol

R.T.: 4.777 min
Delta R.T.: -0.064 min
Response: 7364605
Conc: 16.26 ng/ml

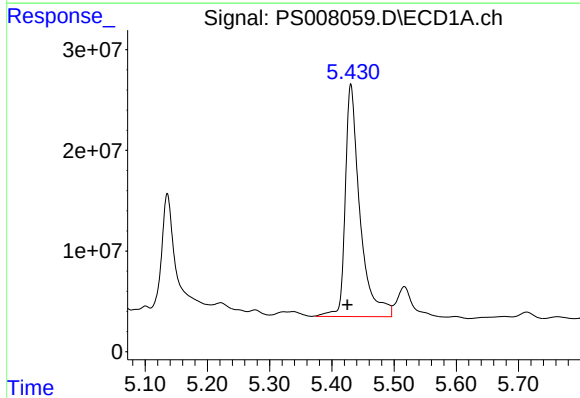


#4 2,4-DCAA

R.T.: 5.431 min
Delta R.T.: 0.006 min
Response: 378860046
Conc: 242.19 ng/ml

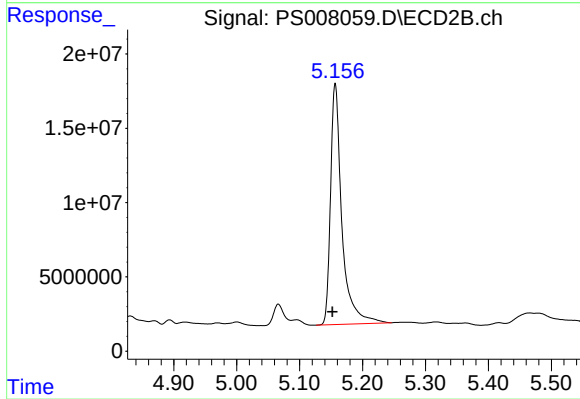

#4 2,4-DCAA


R.T.: 5.157 min
Delta R.T.: 0.005 min
Response: 203438485
Conc: 262.19 ng/ml

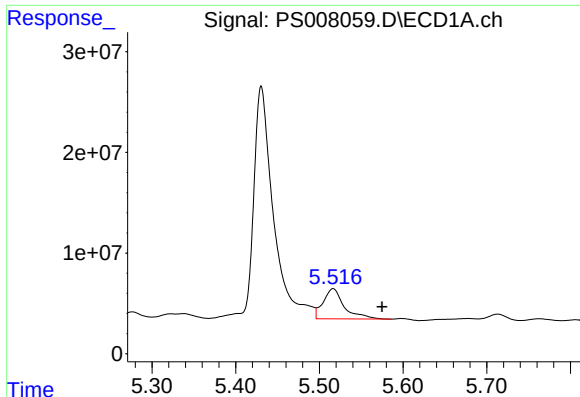

#5 DICAMBA


R.T.: 5.516 min
Delta R.T.: -0.058 min
Response: 52861066
Conc: 9.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

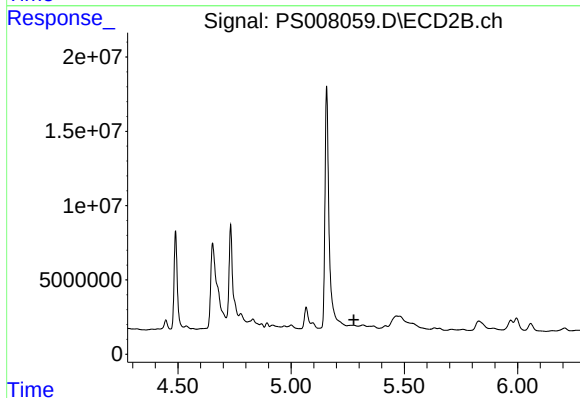


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

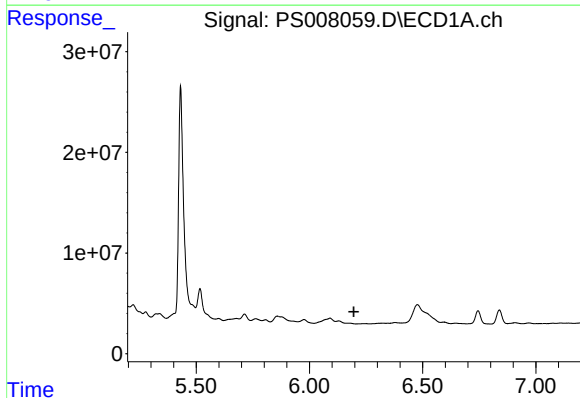


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

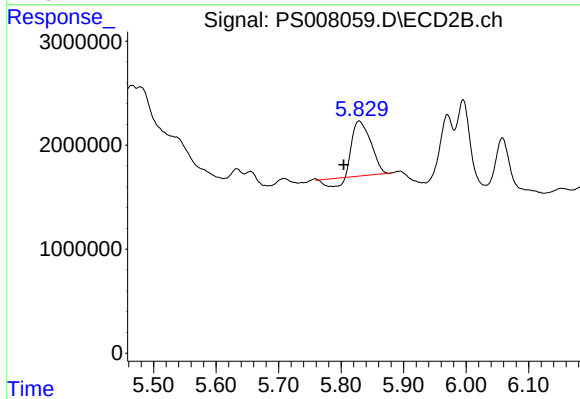

#8 DICHLORPROP


R.T.: 5.829 min
Delta R.T.: 0.025 min
Response: 9904503
Conc: 13.82 ng/ml

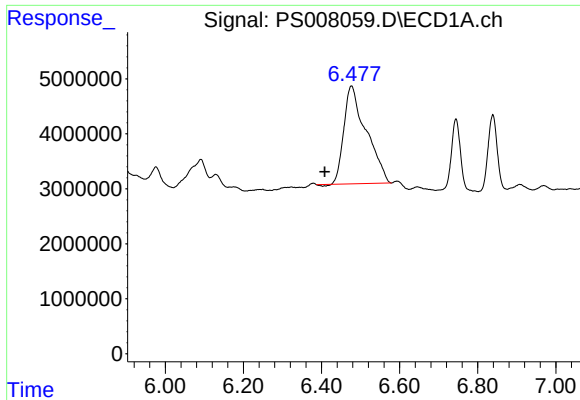

#9 2,4-D


R.T.: 6.477 min
Delta R.T.: 0.069 min
Response: 70648163
Conc: 43.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

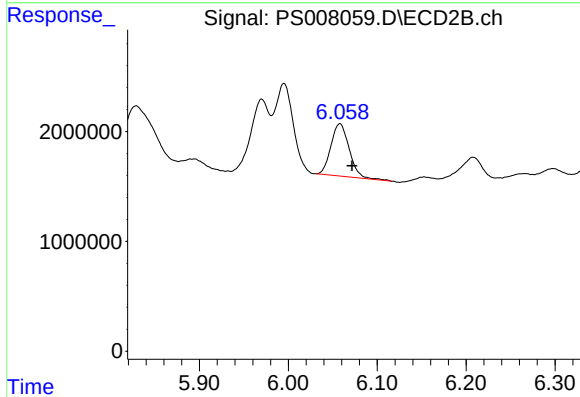


#9 2,4-D

R.T.: 6.058 min
Delta R.T.: -0.014 min
Response: 6829696
Conc: 7.73 ng/ml

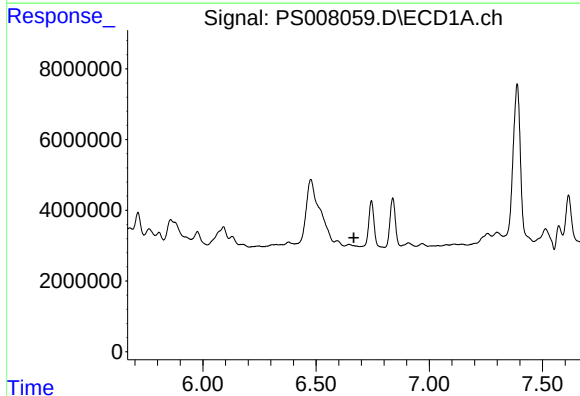


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

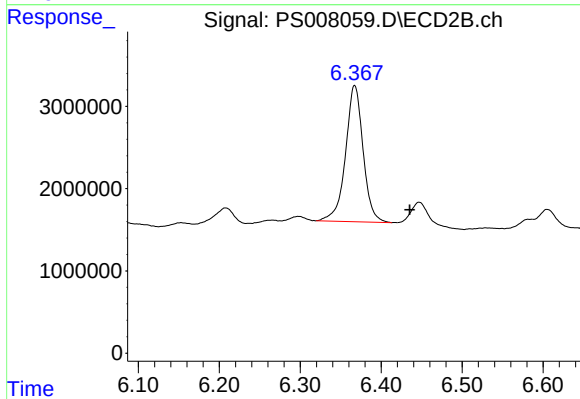

#10 Pentachlorophenol


R.T.: 6.367 min
Delta R.T.: -0.068 min
Response: 24995845
Conc: 2.29 ng/ml

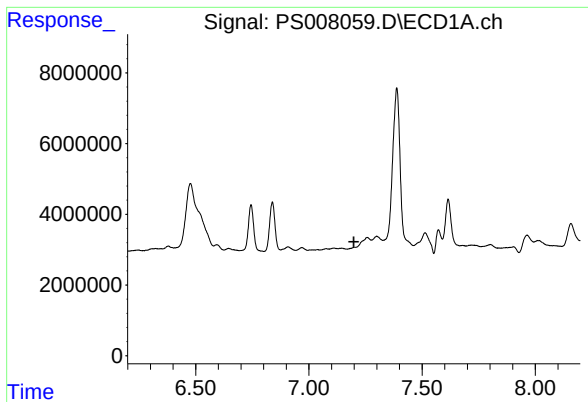

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

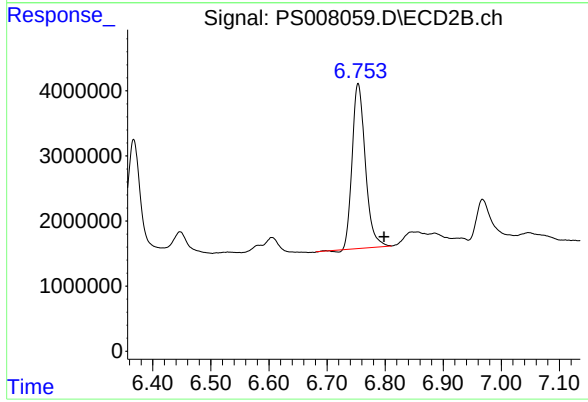

#11 2,4,5-TP (SILVEX)

R.T.: 6.754 min
Delta R.T.: -0.044 min
Response: 39757482
Conc: 9.27 ng/ml