

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
 Data File : PS008061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 15:17
 Operator : SM\AJ
 Sample : K6283-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 15:48:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.445	5.172	558.4E6	270.5E6	356.928	348.674
Target Compounds							
1) T	Dalapon	2.006	1.728	68220966	201.1E6	33.453	169.309 #
2) T	3,5-DICHL...	0.000	4.463	0	7365418	N.D.	7.117
3) T	4-Nitroph...	0.000	4.846	0	20591653	N.D.	45.471
5) T	DICAMBA	5.532	0.000	81997005	0	14.412	N.D. #
7) T	MCPA	0.000	5.480	0	46264327	N.D.	14.518
8) T	DICHLORPROP	0.000	5.845	0	8994970	N.D.	12.548
9) T	2,4-D	0.000	6.075	0	5337273	N.D.	6.040
10) T	Pentachlo...	0.000	6.384	0	31100710	N.D.	2.849
11) T	2,4,5-TP ...	0.000	6.770	0	49077607	N.D.	11.443
12) T	2,4,5-T	7.405	0.000	121.7E6	0	13.150	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
Data File : PS008061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 15:17
Operator : SM\AJ
Sample : K6283-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 15:48:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

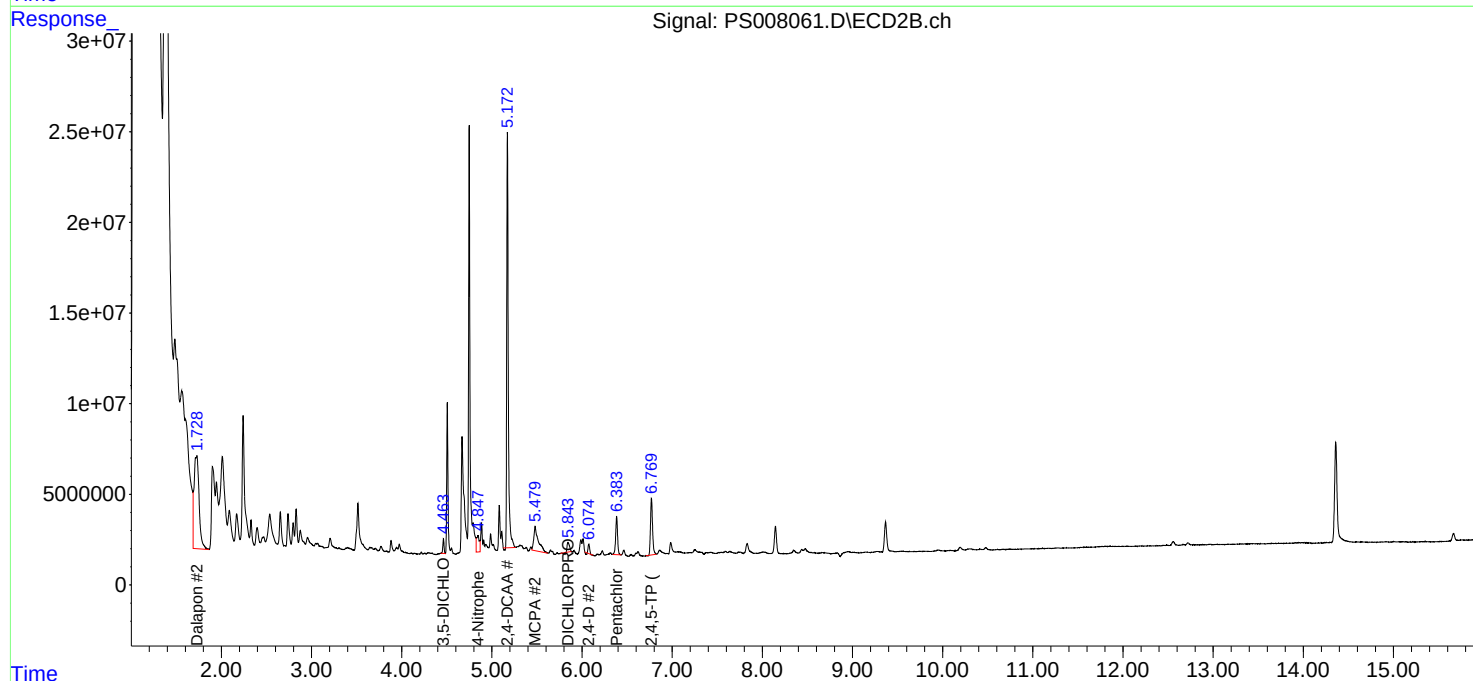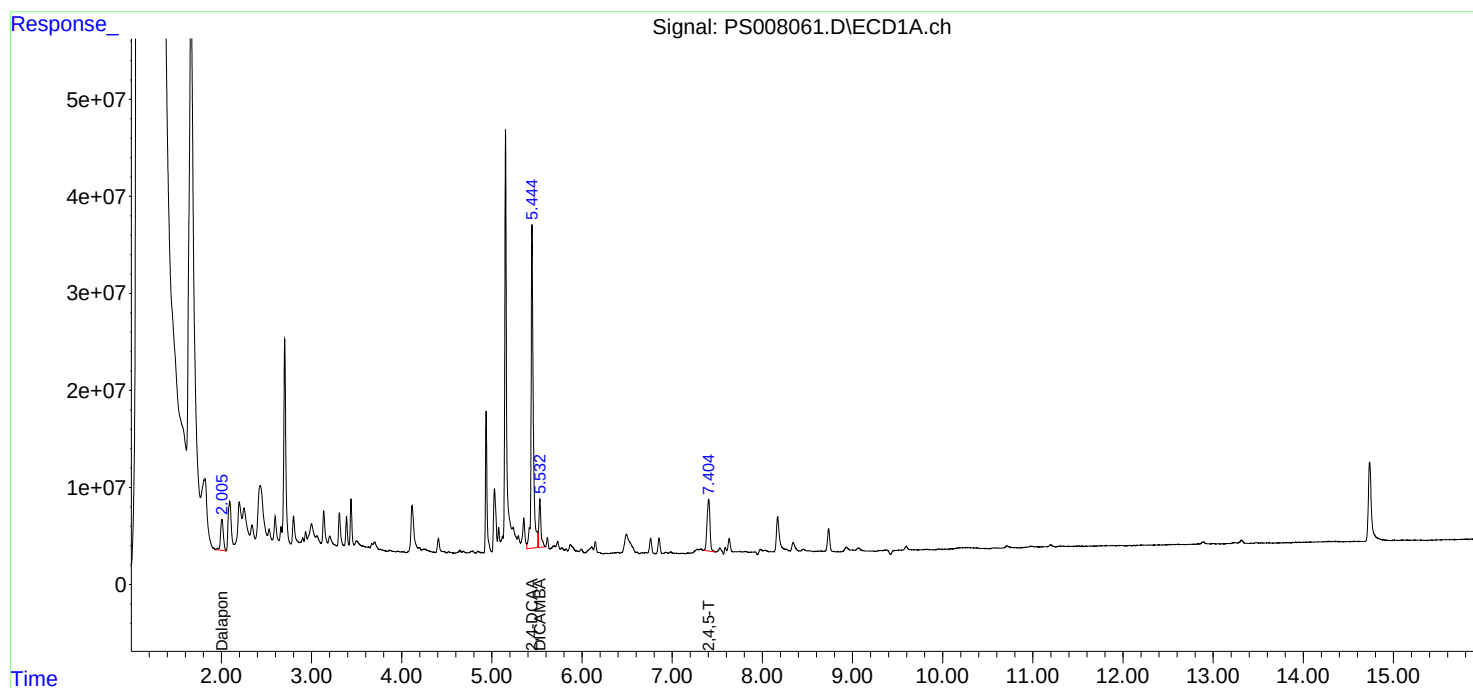


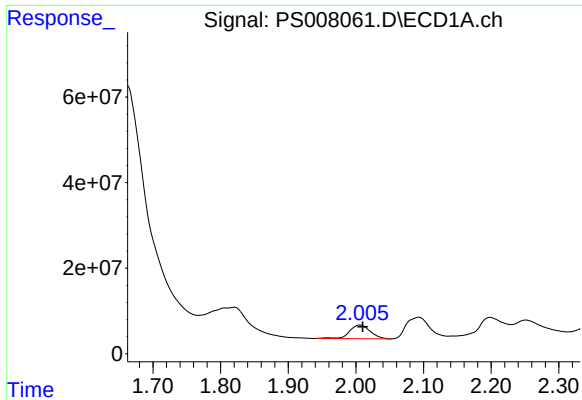

#1 Dalapon


R.T.: 2.006 min
Delta R.T.: -0.004 min
Response: 68220966
Conc: 33.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

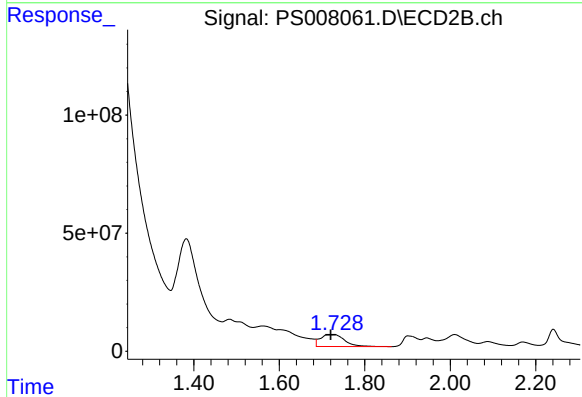


#1 Dalapon

R.T.: 1.728 min
Delta R.T.: 0.007 min
Response: 201103271
Conc: 169.31 ng/ml

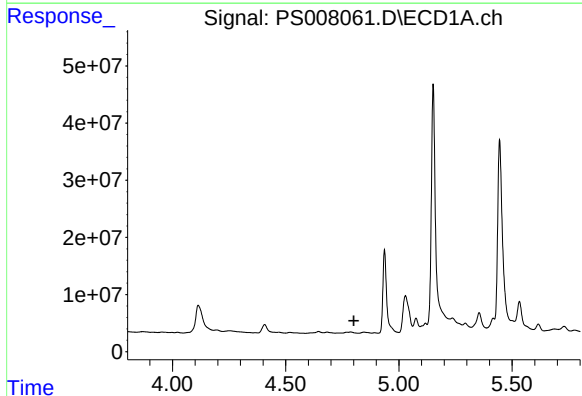


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

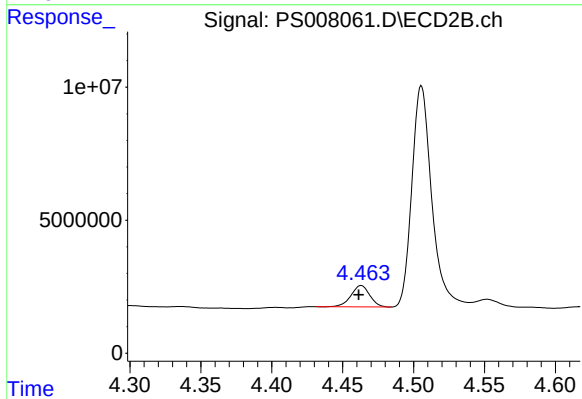

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.463 min
Delta R.T.: 0.002 min
Response: 7365418
Conc: 7.12 ng/ml

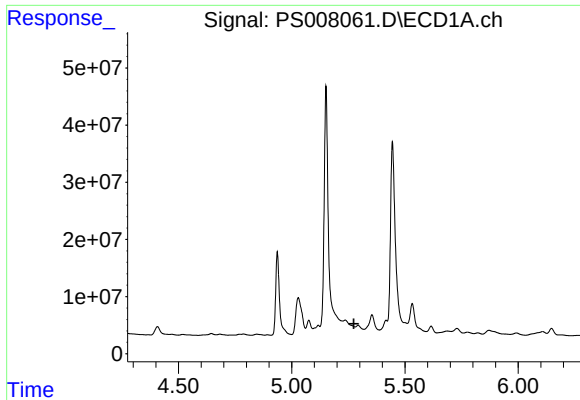

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

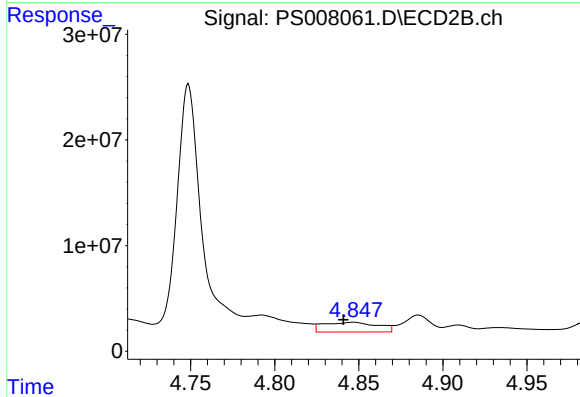


#3 4-Nitrophenol

R.T.: 4.846 min
Delta R.T.: 0.006 min
Response: 20591653
Conc: 45.47 ng/ml

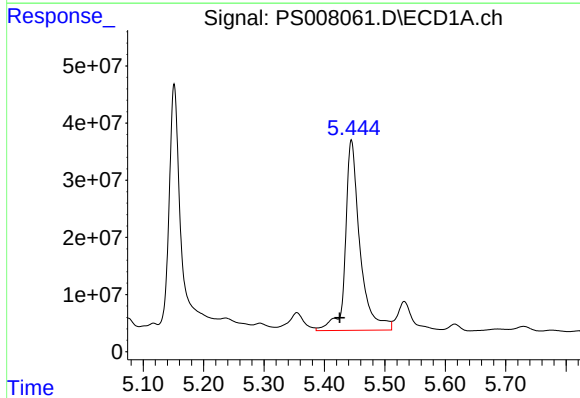


#4 2,4-DCAA

R.T.: 5.445 min
Delta R.T.: 0.020 min
Response: 558354419
Conc: 356.93 ng/ml

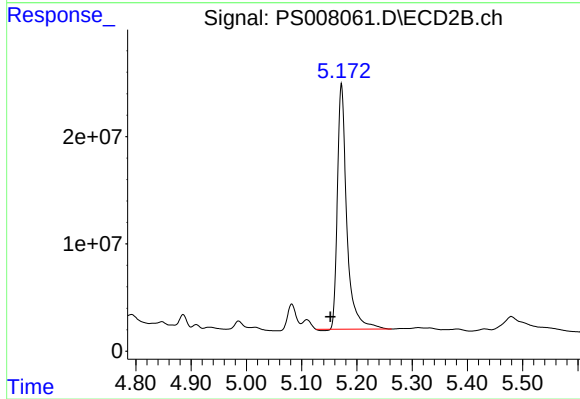

#4 2,4-DCAA


R.T.: 5.172 min
Delta R.T.: 0.020 min
Response: 270542039
Conc: 348.67 ng/ml

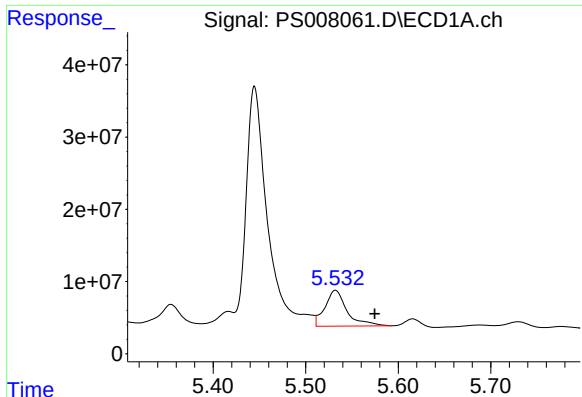

#5 DICAMBA


R.T.: 5.532 min
Delta R.T.: -0.043 min
Response: 81997005
Conc: 14.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

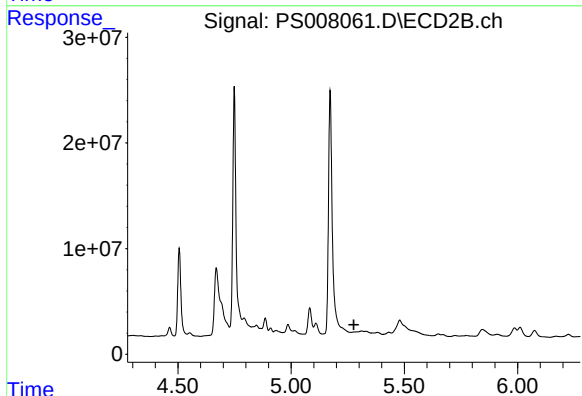


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

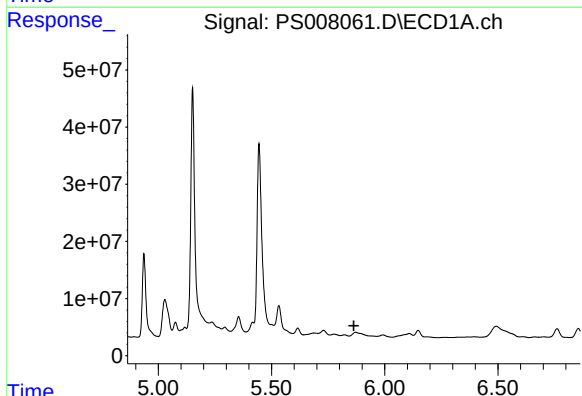


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.864 min
Response: 0
Conc: N.D.

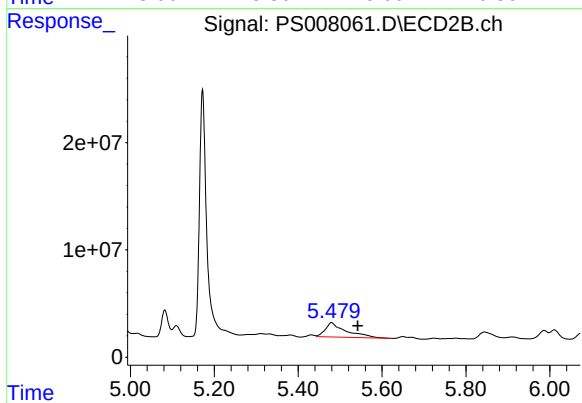

#7 MCPA


R.T.: 5.480 min
Delta R.T.: -0.063 min
Response: 46264327
Conc: 14.52 ug/ml

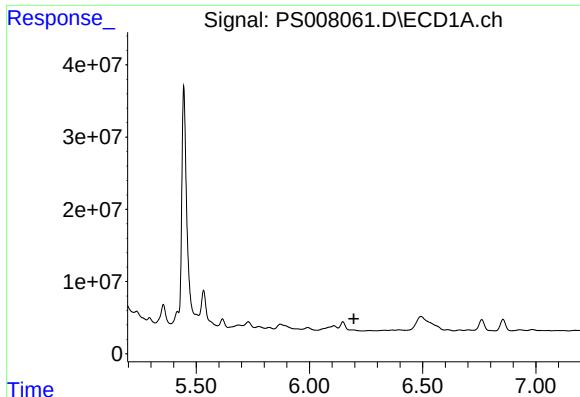

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

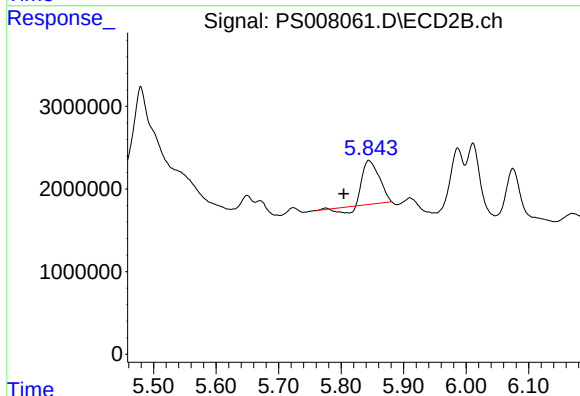


#8 DICHLORPROP

R.T.: 5.845 min
Delta R.T.: 0.040 min
Response: 8994970
Conc: 12.55 ng/ml

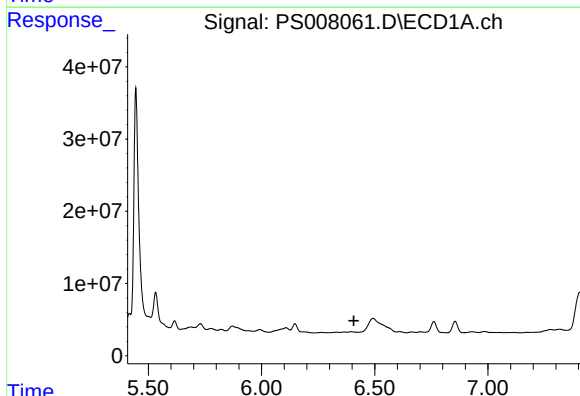


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

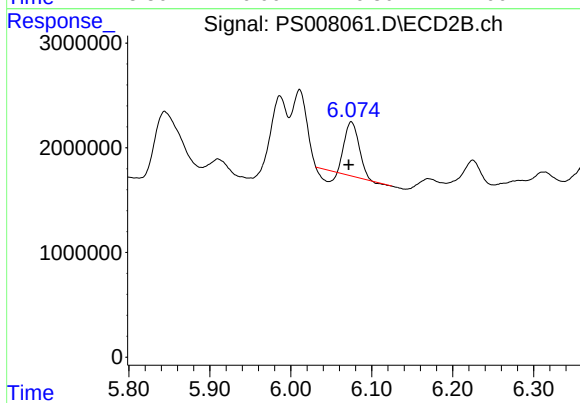

#9 2,4-D


R.T.: 6.075 min
Delta R.T.: 0.003 min
Response: 5337273
Conc: 6.04 ng/ml

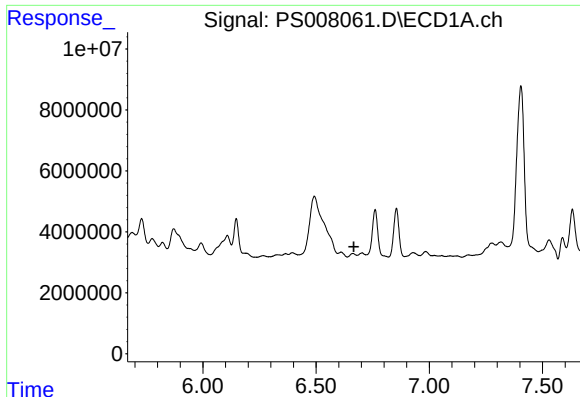

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

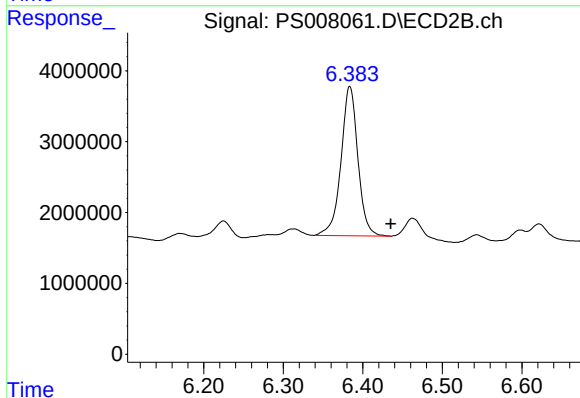


#10 Pentachlorophenol

R.T.: 6.384 min
Delta R.T.: -0.051 min
Response: 31100710
Conc: 2.85 ng/ml

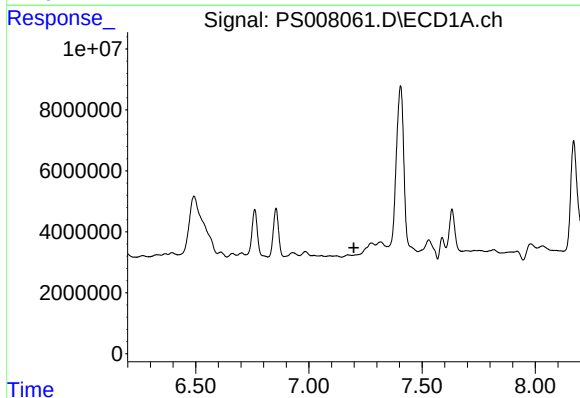


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

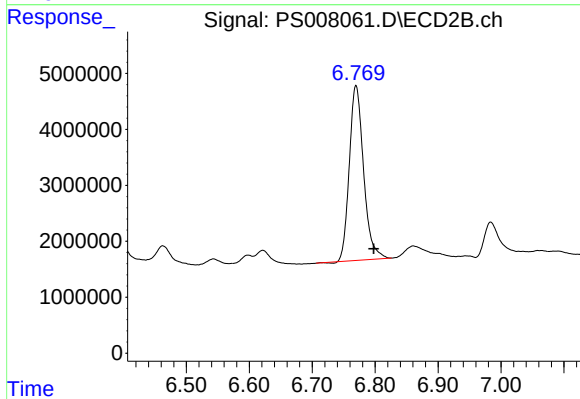

#11 2,4,5-TP (SILVEX)


R.T.: 6.770 min
Delta R.T.: -0.028 min
Response: 49077607
Conc: 11.44 ng/ml

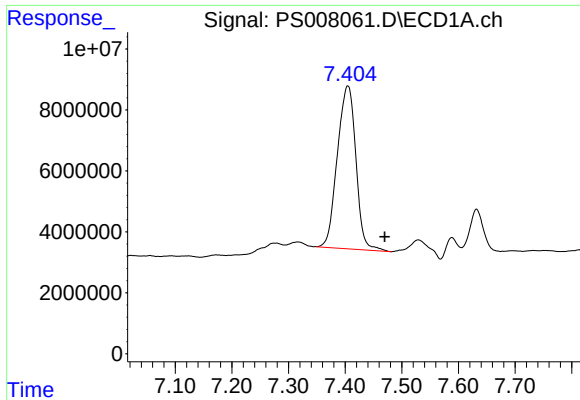

#12 2,4,5-T

R.T.: 7.405 min
Delta R.T.: -0.065 min
Response: 121703971
Conc: 13.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

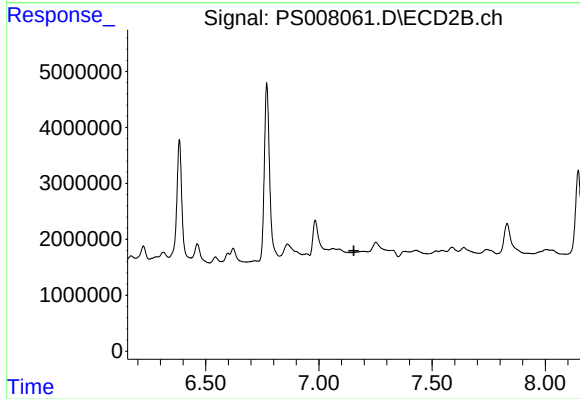

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.