

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
 Data File : PS008062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 15:39
 Operator : SM\AJ
 Sample : K6294-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 16:27:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.428	5.155	498.0E6	265.9E6	318.354	342.751
Target Compounds							
1) T	Dalapon	1.987	1.696	66600801	148.6E6	32.658	125.121 #
2) T	3,5-DICHL...	0.000	4.445	0	5489744	N.D.	5.305
3) T	4-Nitroph...	0.000	4.829	0	16267775	N.D.	35.923
5) T	DICAMBA	5.515	0.000	62030230	0	10.903	N.D. #
7) T	MCPA	0.000	5.480	0	40563551	N.D.	12.729
8) T	DICHLORPROP	0.000	5.829	0	10171923	N.D.	14.190
9) T	2,4-D	6.475	6.057	80061196	7944953	49.765	8.991 #
10) T	Pentachlo...	0.000	6.367	0	29317391	N.D.	2.686
11) T	2,4,5-TP ...	0.000	6.753	0	44635769	N.D.	10.407



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
Data File : PS008062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 15:39
Operator : SM\AJ
Sample : K6294-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 16:27:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

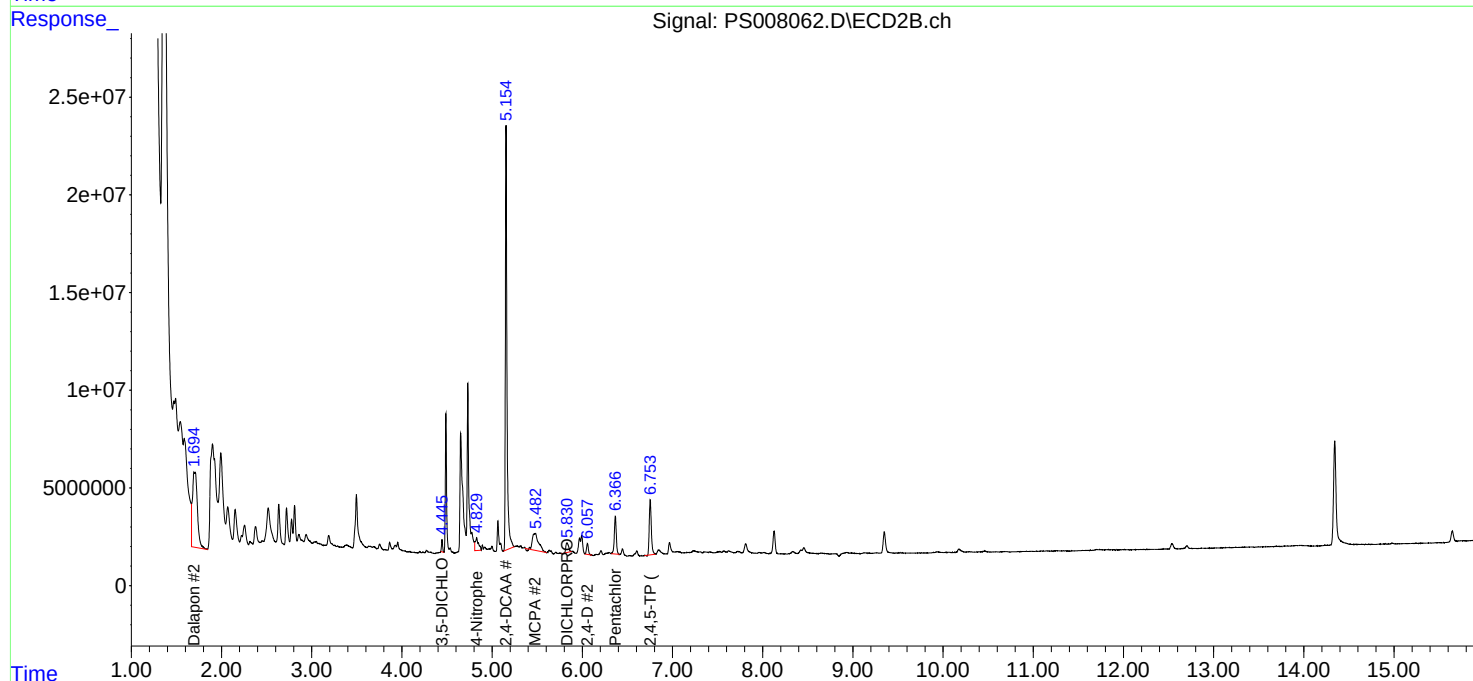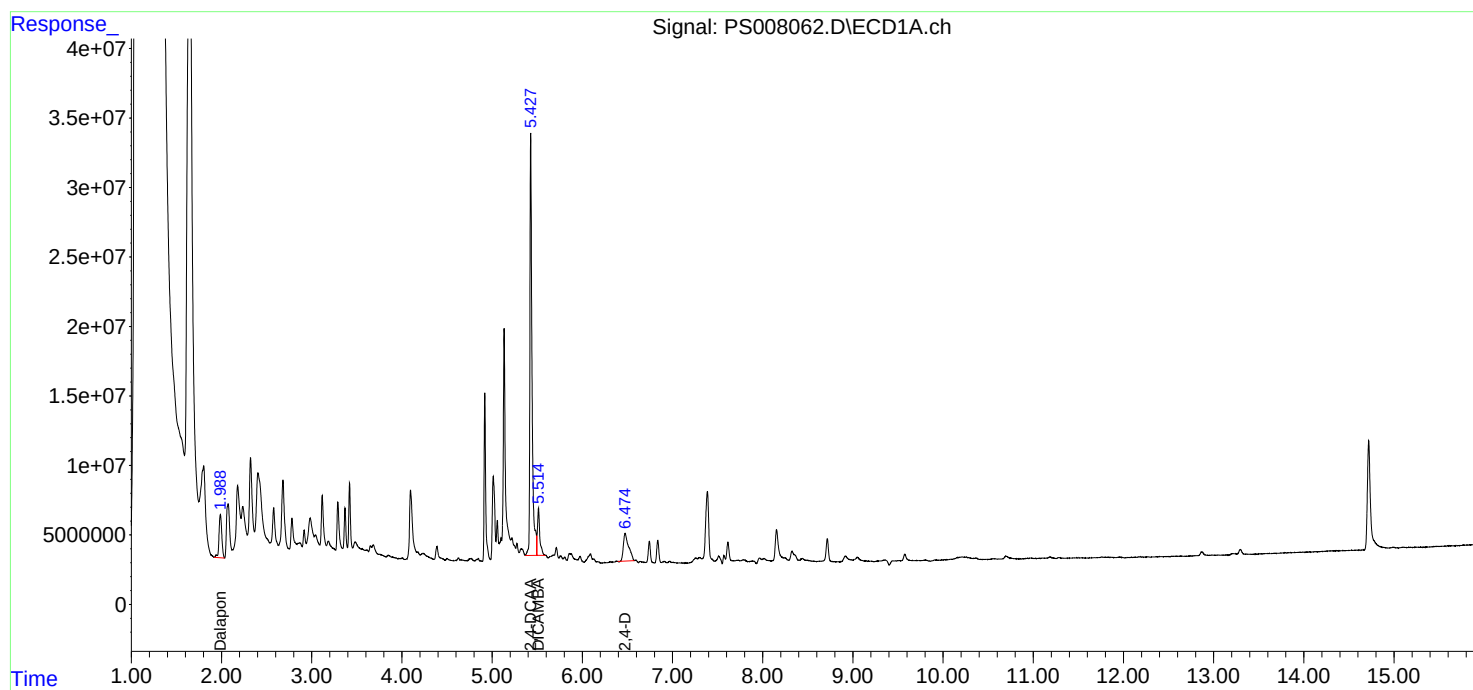


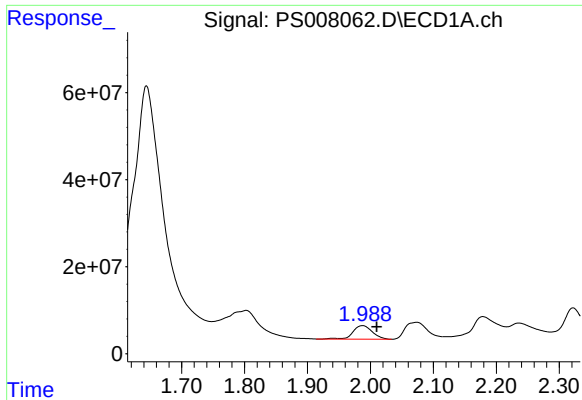

#1 Dalapon


R.T.: 1.987 min
Delta R.T.: -0.023 min
Response: 66600801
Conc: 32.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

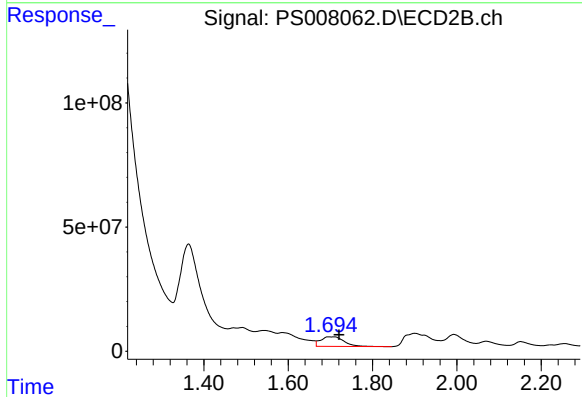


#1 Dalapon

R.T.: 1.696 min
Delta R.T.: -0.025 min
Response: 148617435
Conc: 125.12 ng/ml

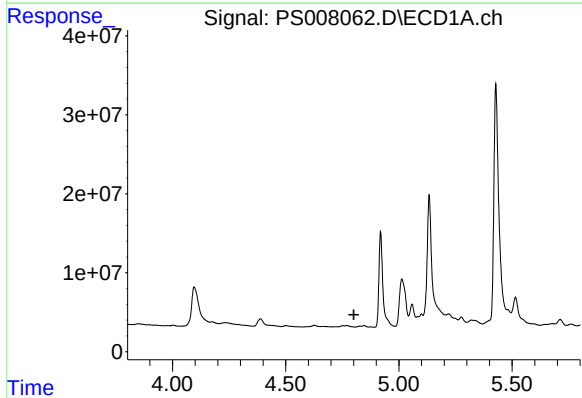


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

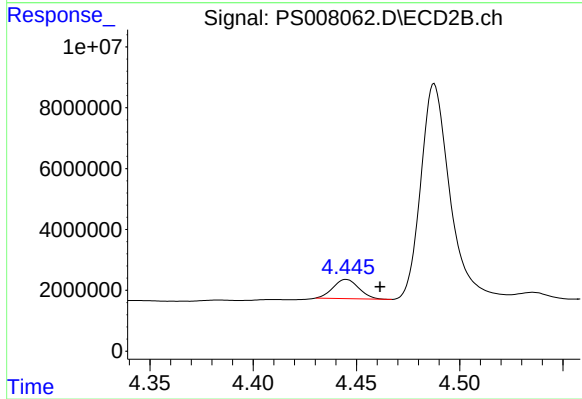

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.445 min
Delta R.T.: -0.016 min
Response: 5489744
Conc: 5.30 ng/ml

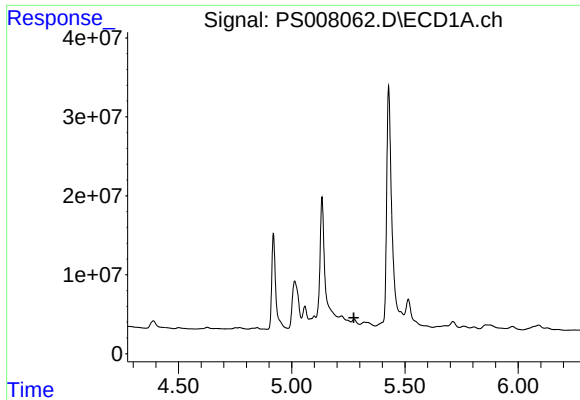

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

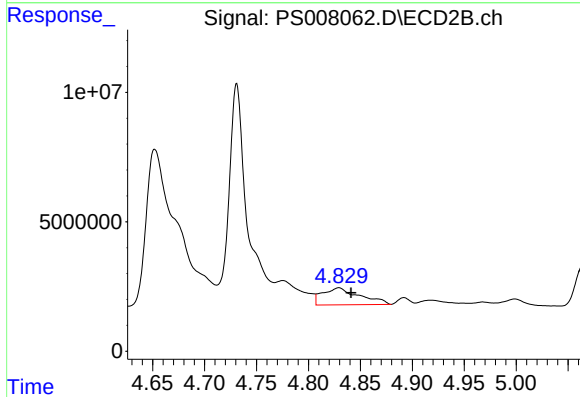


#3 4-Nitrophenol

R.T.: 4.829 min
Delta R.T.: -0.012 min
Response: 16267775
Conc: 35.92 ng/ml

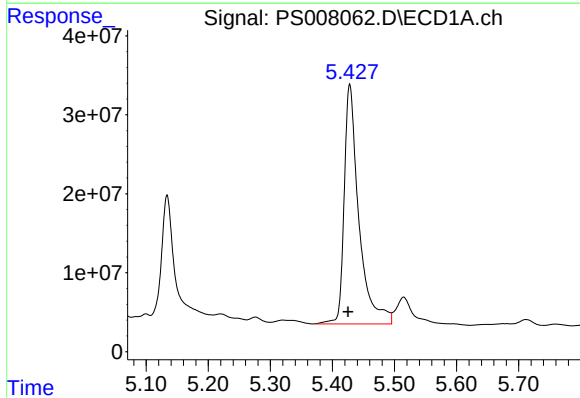


#4 2,4-DCAA

R.T.: 5.428 min
Delta R.T.: 0.003 min
Response: 498012445
Conc: 318.35 ng/ml

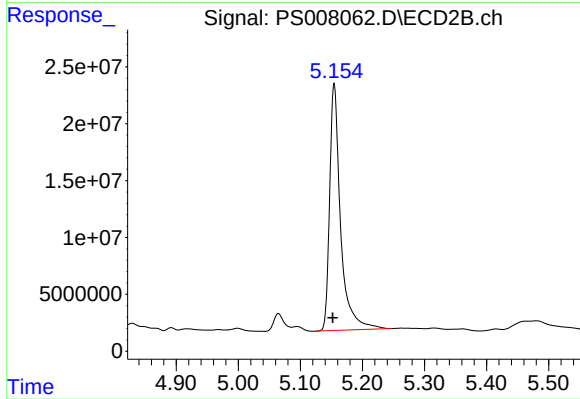

#4 2,4-DCAA


R.T.: 5.155 min
Delta R.T.: 0.003 min
Response: 265946481
Conc: 342.75 ng/ml

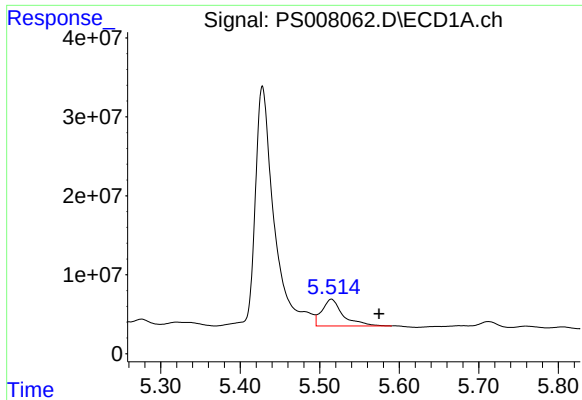

#5 DICAMBA


R.T.: 5.515 min
Delta R.T.: -0.060 min
Response: 62030230
Conc: 10.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

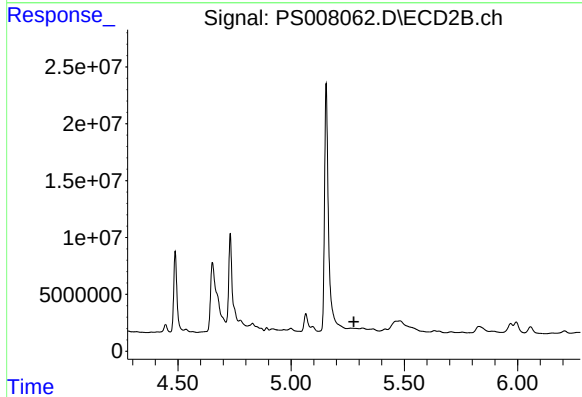


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

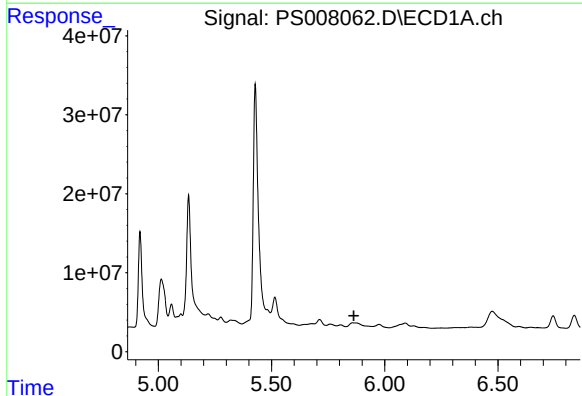


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.864 min
Response: 0
Conc: N.D.

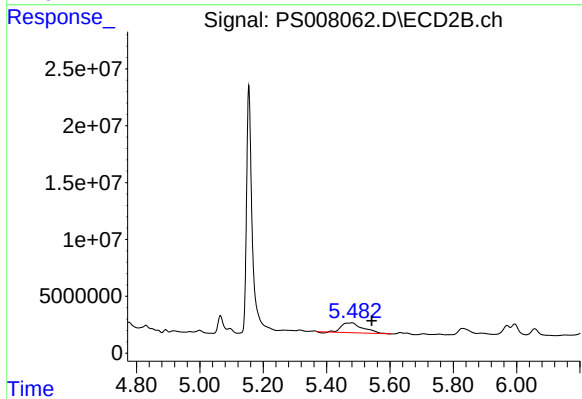

#7 MCPA


R.T.: 5.480 min
Delta R.T.: -0.063 min
Response: 40563551
Conc: 12.73 ug/ml

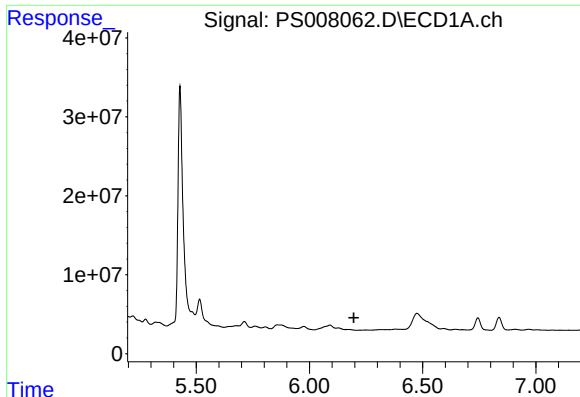

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

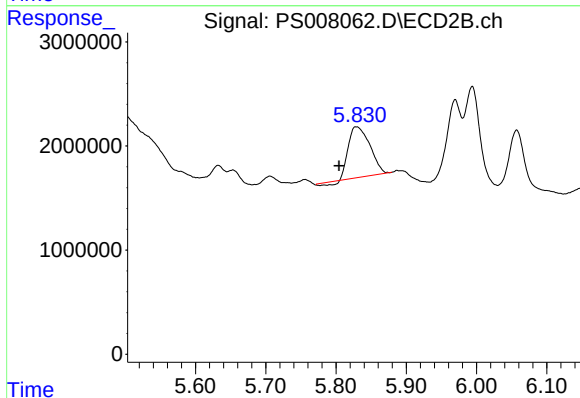


#8 DICHLORPROP

R.T.: 5.829 min
Delta R.T.: 0.025 min
Response: 10171923
Conc: 14.19 ng/ml

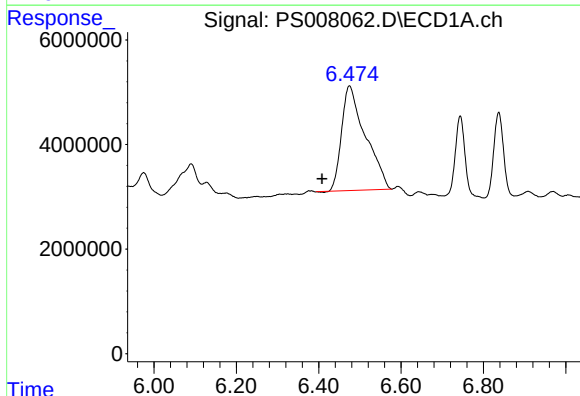


#9 2,4-D

R.T.: 6.475 min
Delta R.T.: 0.067 min
Response: 80061196
Conc: 49.76 ng/ml

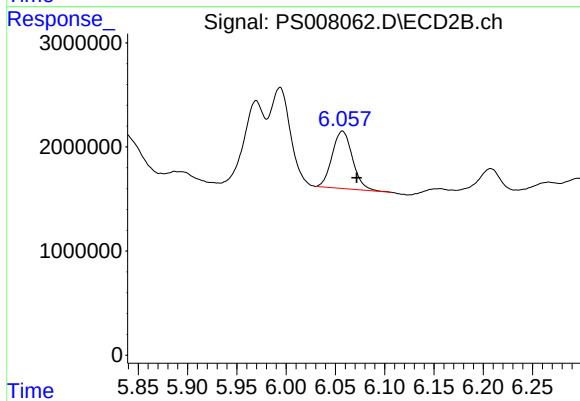

#9 2,4-D


R.T.: 6.057 min
Delta R.T.: -0.015 min
Response: 7944953
Conc: 8.99 ng/ml

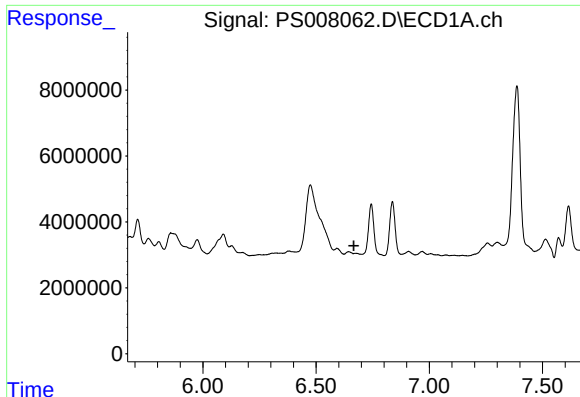

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

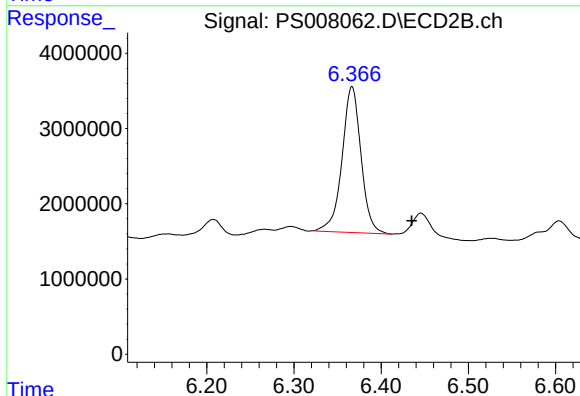


#10 Pentachlorophenol

R.T.: 6.367 min
Delta R.T.: -0.069 min
Response: 29317391
Conc: 2.69 ng/ml

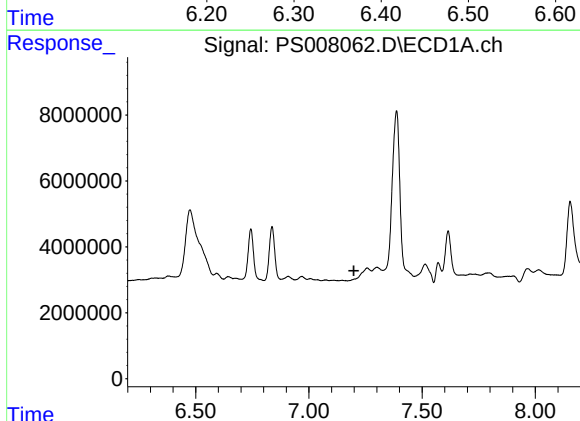

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

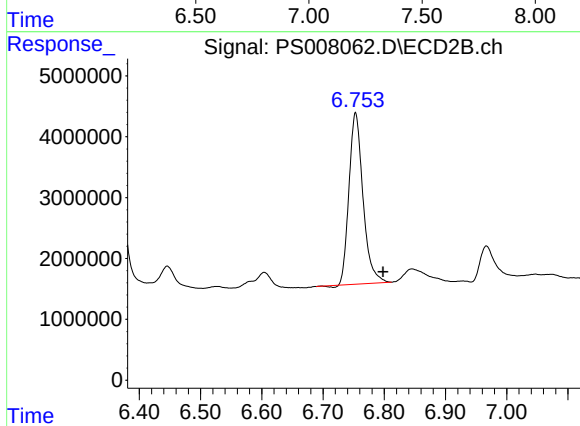

#11 2,4,5-TP (SILVEX)

R.T.: 6.753 min
Delta R.T.: -0.045 min
Response: 44635769
Conc: 10.41 ng/ml