

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
 Data File : PS008063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 16:01
 Operator : SM\AJ
 Sample : K6294-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 16:34:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.162	450.2E6	239.4E6	287.807	308.602
Target Compounds							
1) T	Dalapon	1.995	1.715	69148284	176.1E6	33.907	148.298 #
2) T	3,5-DICHL...	0.000	4.452	0	5880606	N.D.	5.682
3) T	4-Nitroph...	0.000	4.836	0	16363435	N.D.	36.134
5) T	DICAMBA	5.523	0.000	61214015	0	10.759	N.D. #
7) T	MCPA	0.000	5.485	0	42411804	N.D.	13.309
8) T	DICHLORPROP	0.000	5.835	0	11564236	N.D.	16.132
9) T	2,4-D	0.000	6.063	0	7324299	N.D.	8.289
10) T	Pentachlo...	0.000	6.373	0	27867365	N.D.	2.553
11) T	2,4,5-TP ...	0.000	6.759	0	43995270	N.D.	10.258



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121719\
Data File : PS008063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 16:01
Operator : SM\AJ
Sample : K6294-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 16:34:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

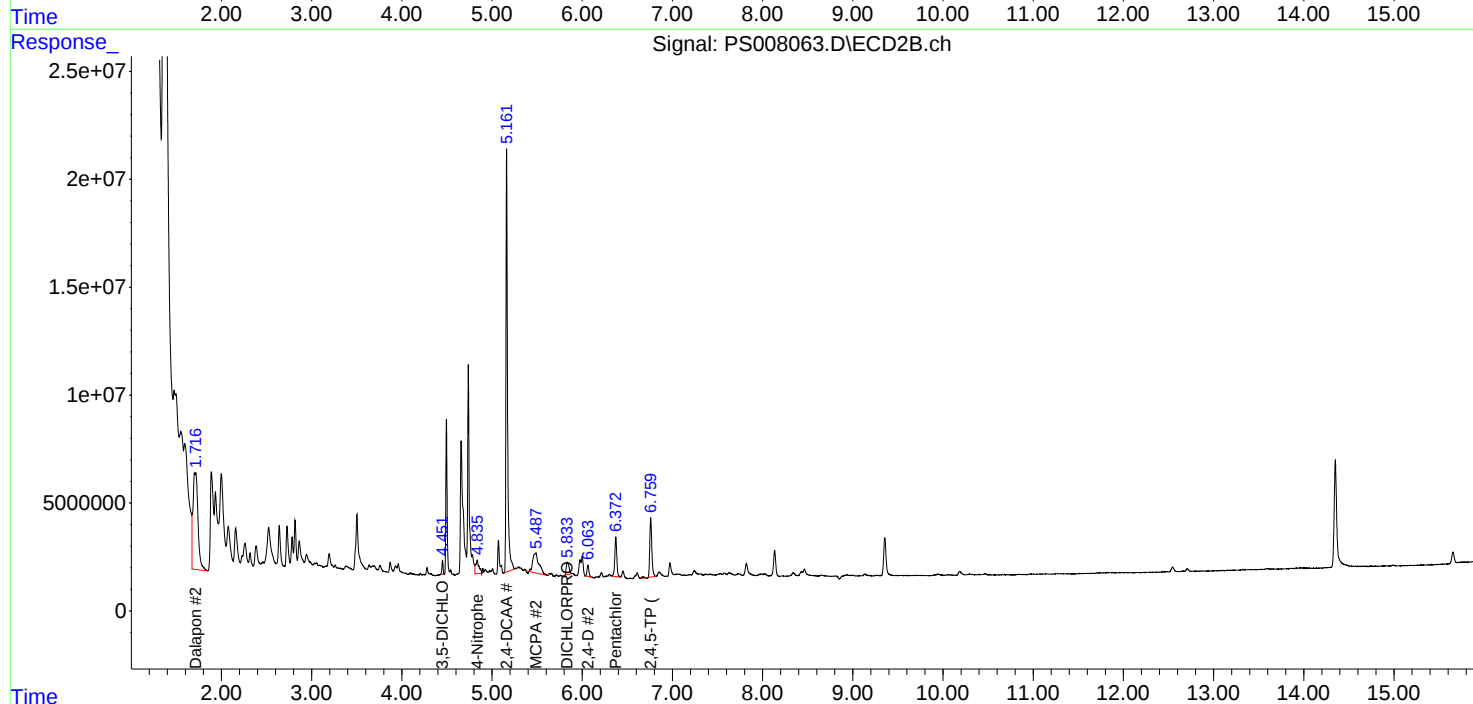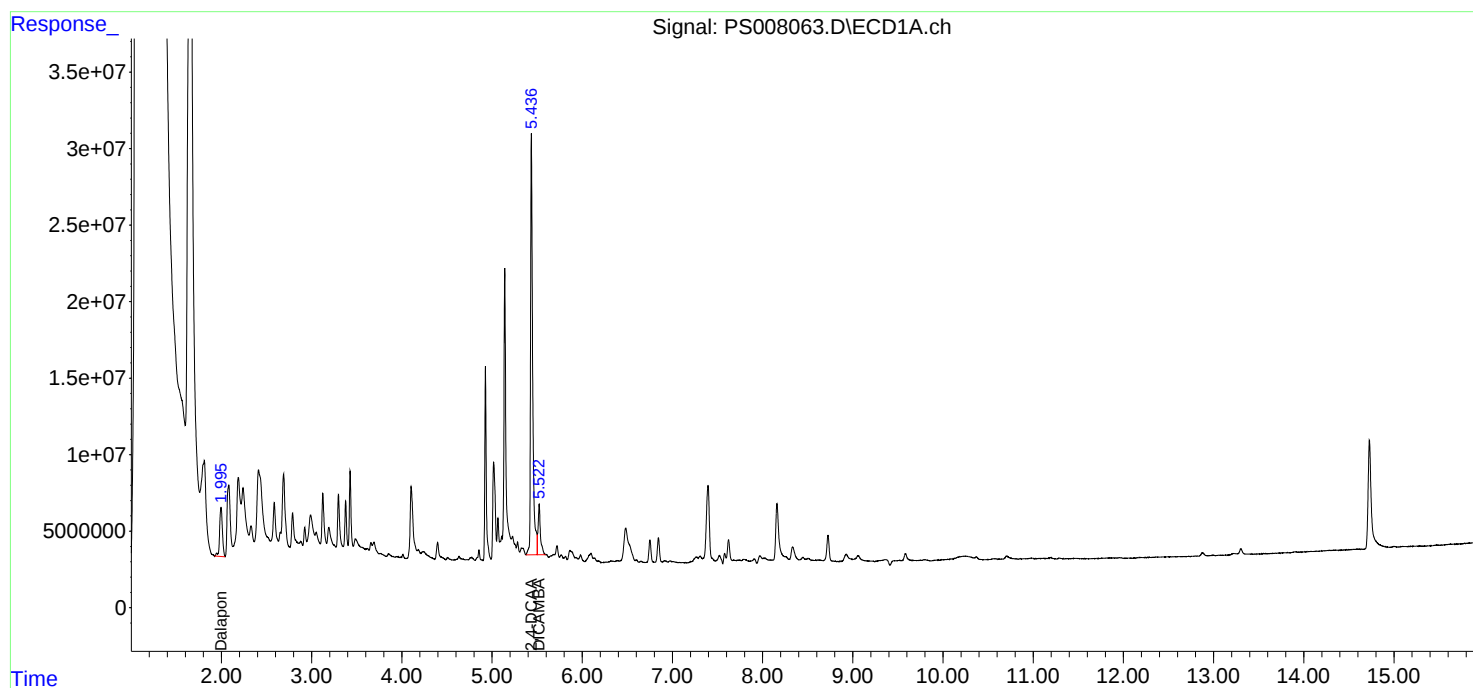


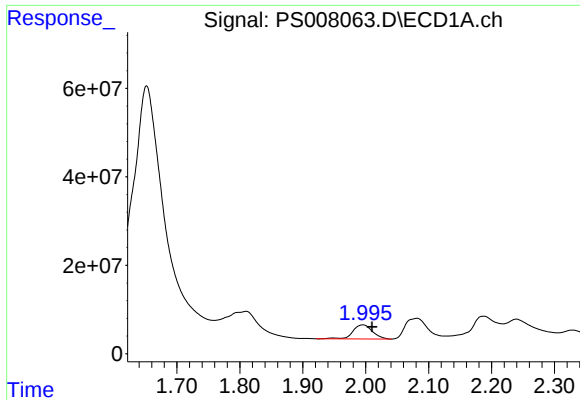

#1 Dalapon


R.T.: 1.995 min
Delta R.T.: -0.015 min
Response: 69148284
Conc: 33.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

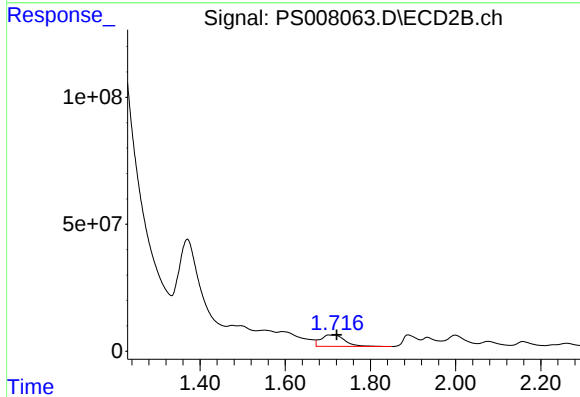


#1 Dalapon

R.T.: 1.715 min
Delta R.T.: -0.006 min
Response: 176147484
Conc: 148.30 ng/ml

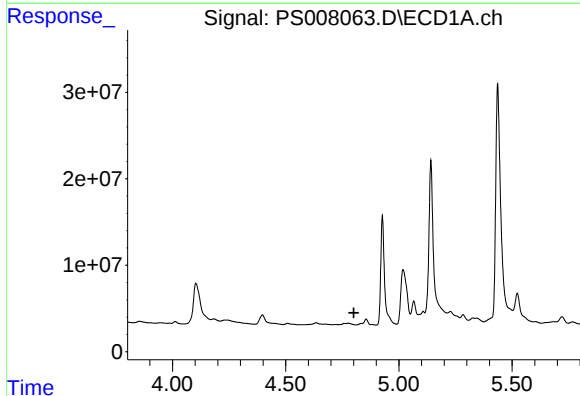


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

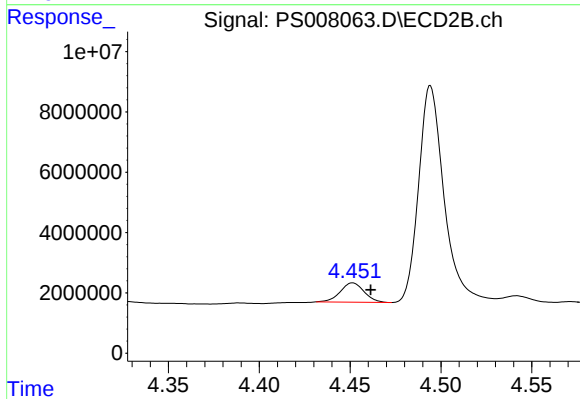

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.452 min
Delta R.T.: -0.010 min
Response: 5880606
Conc: 5.68 ng/ml

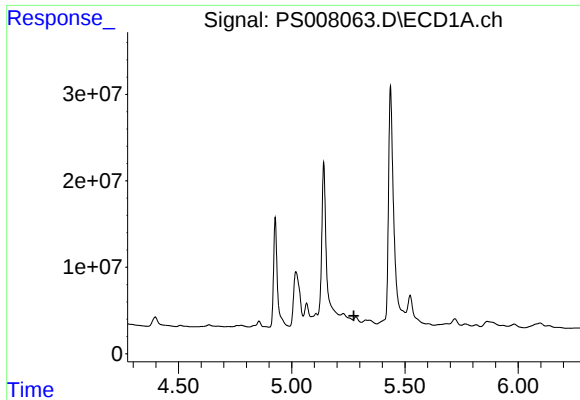

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

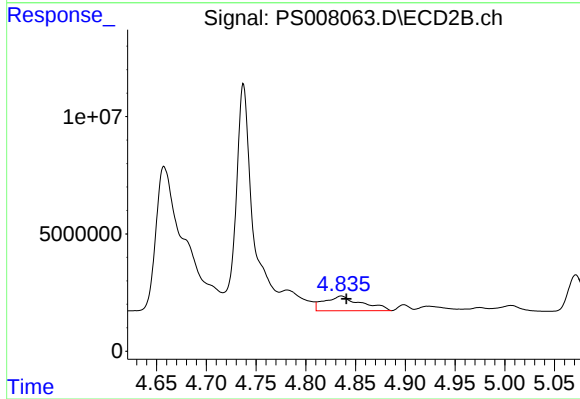


#3 4-Nitrophenol

R.T.: 4.836 min
Delta R.T.: -0.005 min
Response: 16363435
Conc: 36.13 ng/ml

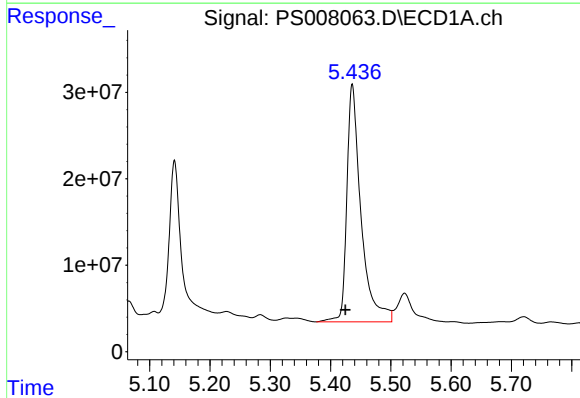


#4 2,4-DCAA

R.T.: 5.436 min
Delta R.T.: 0.011 min
Response: 450225603
Conc: 287.81 ng/ml

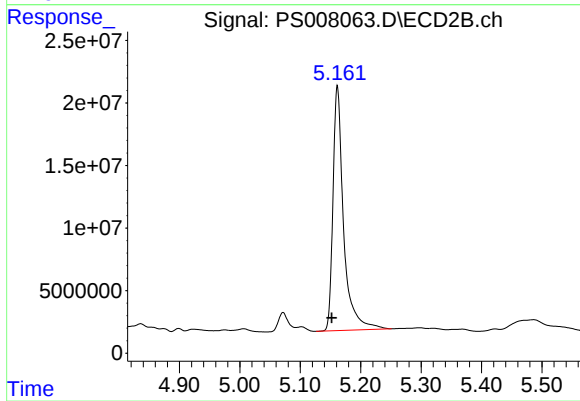

#4 2,4-DCAA


R.T.: 5.162 min
Delta R.T.: 0.010 min
Response: 239449586
Conc: 308.60 ng/ml

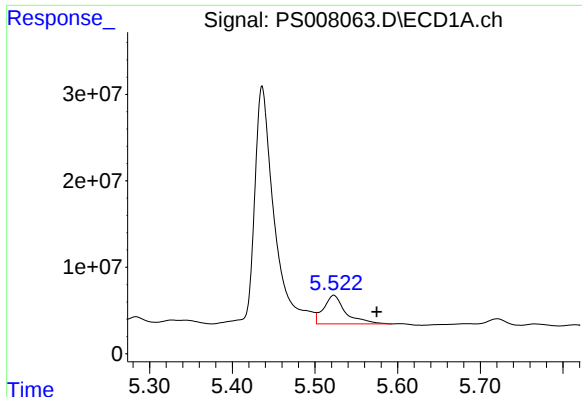

#5 DICAMBA


R.T.: 5.523 min
Delta R.T.: -0.052 min
Response: 61214015
Conc: 10.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

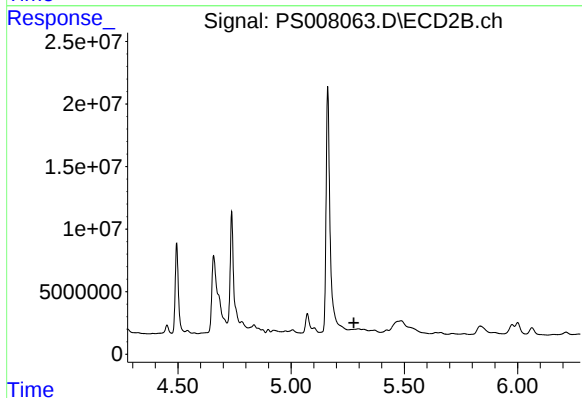


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

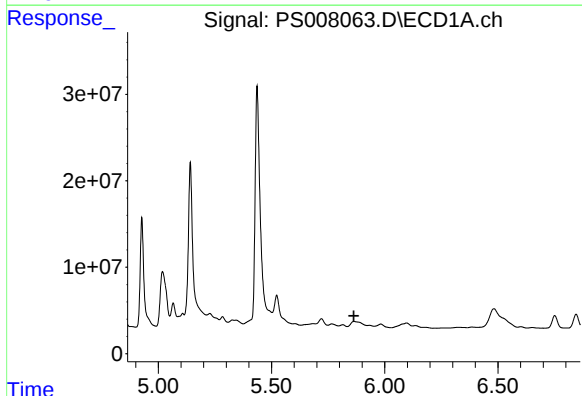


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.864 min
Response: 0
Conc: N.D.

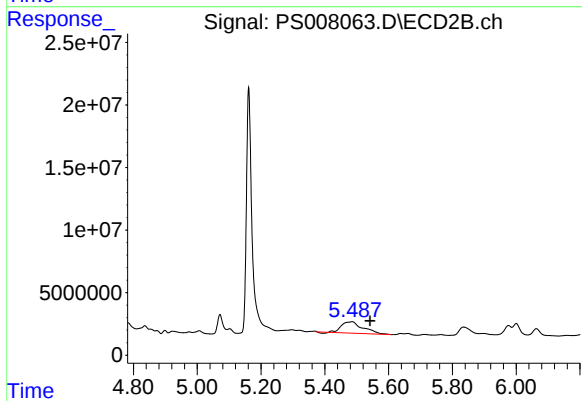

#7 MCPA


R.T.: 5.485 min
Delta R.T.: -0.057 min
Response: 42411804
Conc: 13.31 ug/ml

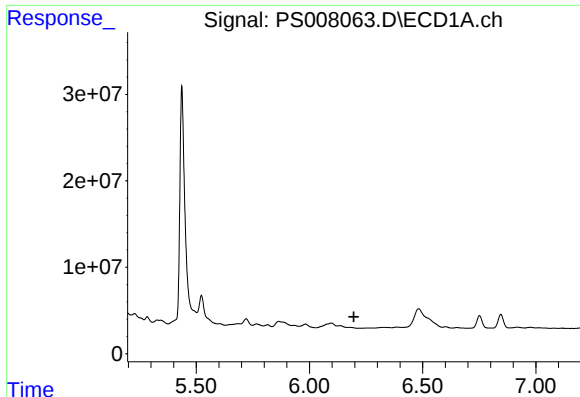

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

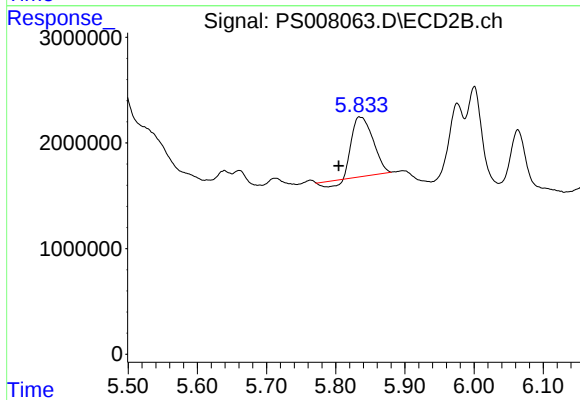


#8 DICHLORPROP

R.T.: 5.835 min
Delta R.T.: 0.031 min
Response: 11564236
Conc: 16.13 ng/ml

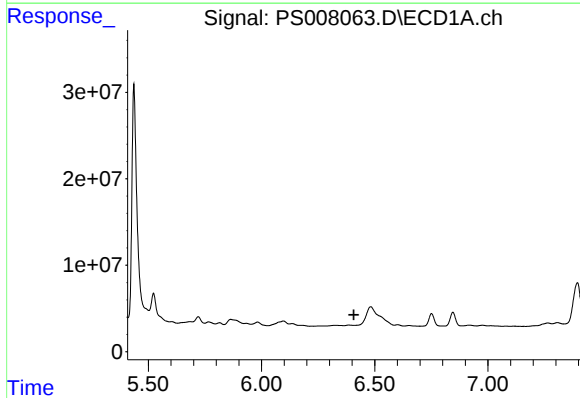


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

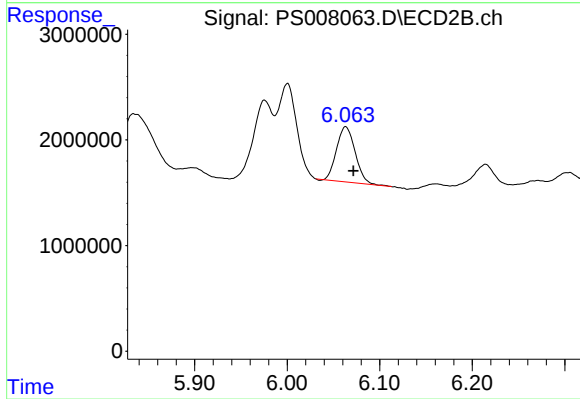

#9 2,4-D


R.T.: 6.063 min
Delta R.T.: -0.008 min
Response: 7324299
Conc: 8.29 ng/ml

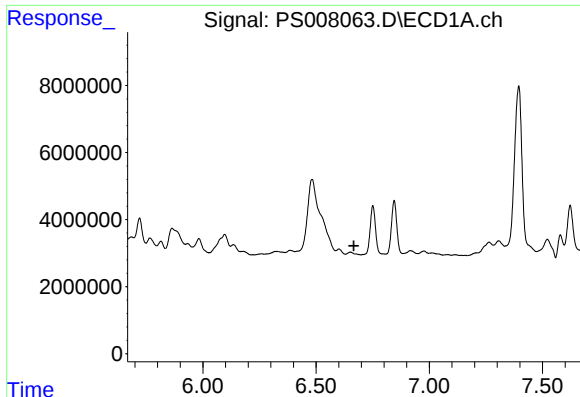

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

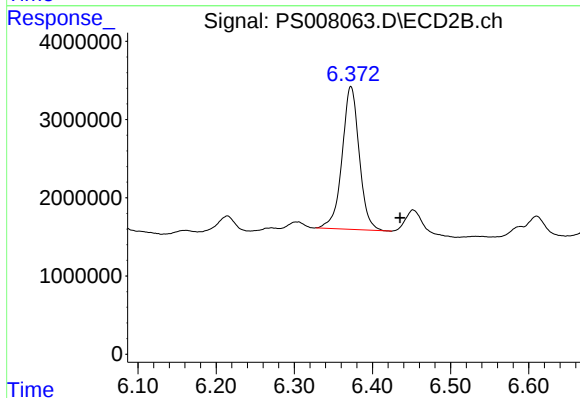


#10 Pentachlorophenol

R.T.: 6.373 min
Delta R.T.: -0.063 min
Response: 27867365
Conc: 2.55 ng/ml

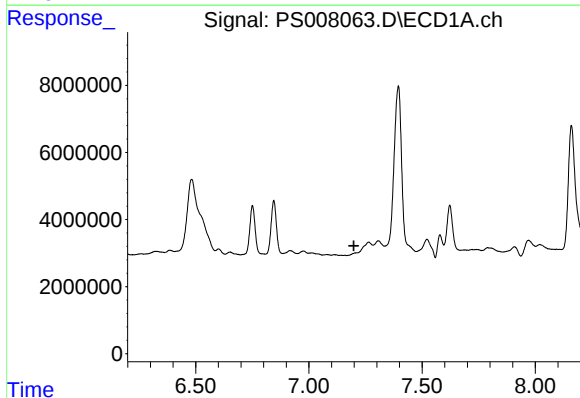

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

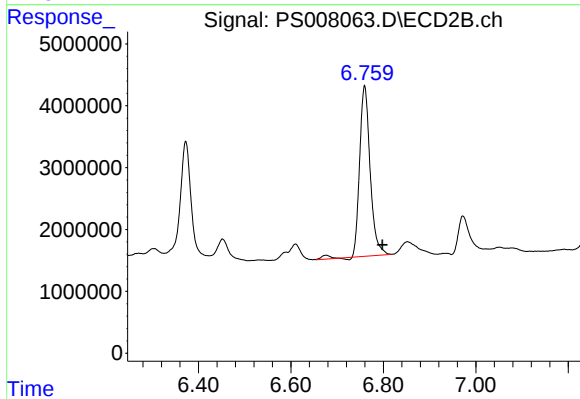

#11 2,4,5-TP (SILVEX)

R.T.: 6.759 min
Delta R.T.: -0.038 min
Response: 43995270
Conc: 10.26 ng/ml