

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121720\
 Data File : PS013556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 11:26
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 13:54:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.468f	0.000	507.8E6	0	396.208	N.D. #
3) T	4-Nitroph...	7.002f	0.000	521288	0	1.157	N.D. #
7) T	MCPA	7.692	0.000	11039791	0	2.824	N.D. #
8) T	DICHLORPROP	0.000	7.762f	0	8033657	N.D.	17.976
15) T	Picloram	11.038	11.032	59010830	29780952	8.567	8.553



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121720\
Data File : PS013556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 11:26
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 13:54:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

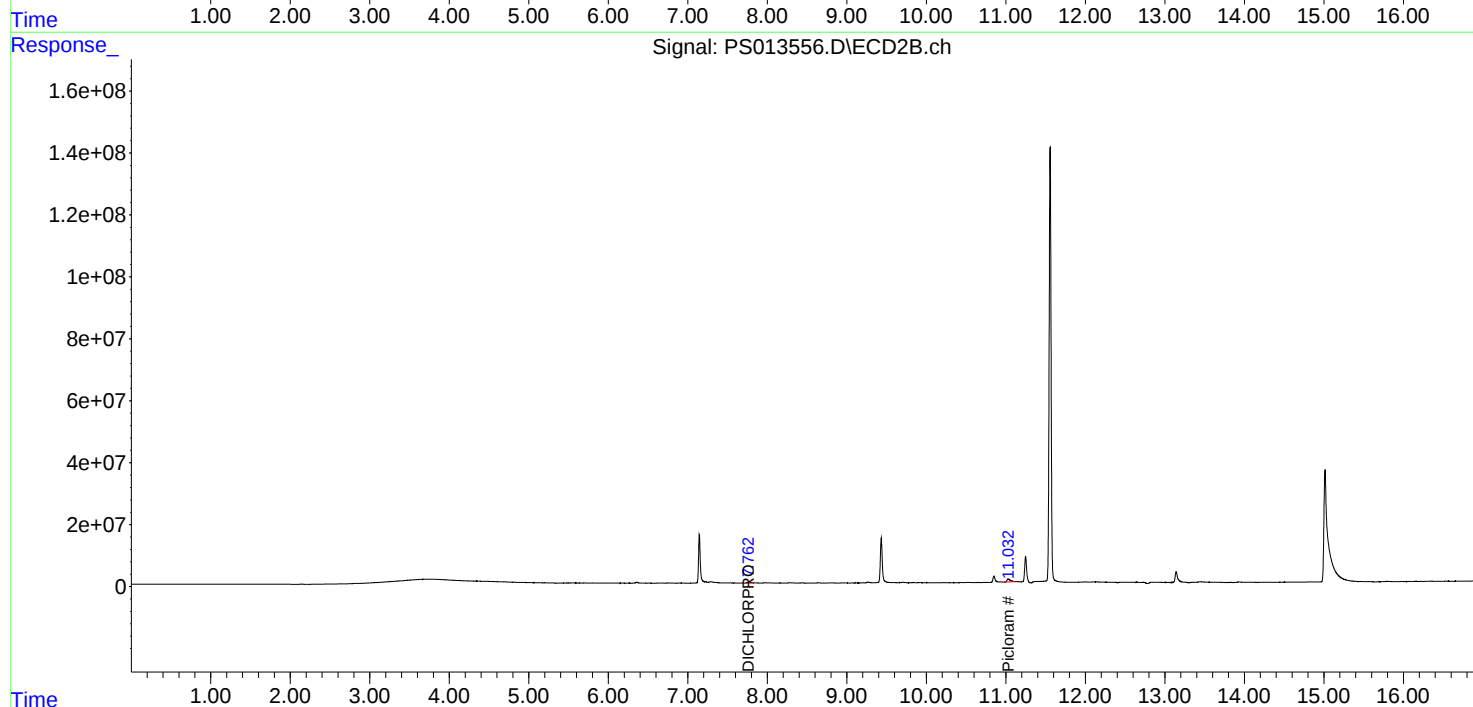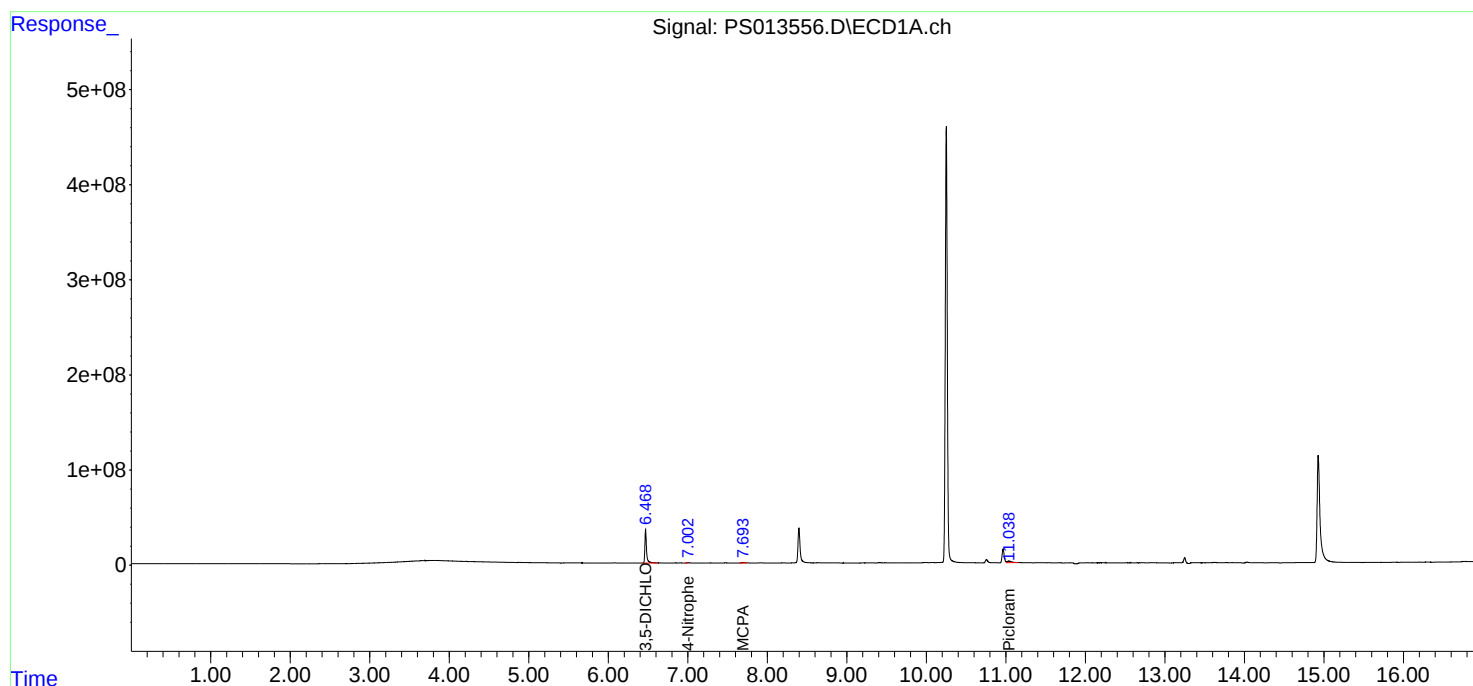


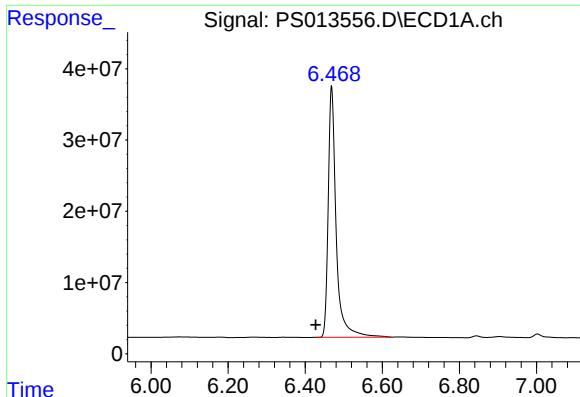

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.468 min
Delta R.T.: 0.041 min
Response: 507822914
Conc: 396.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

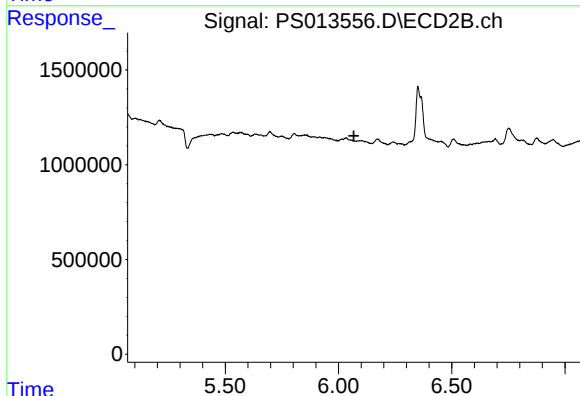


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.068 min
Response: 0
Conc: N.D.

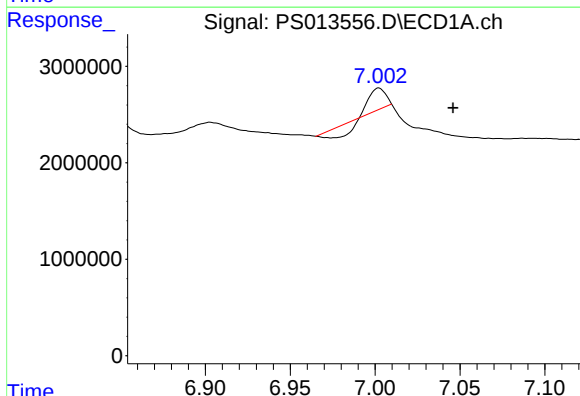


#3 4-Nitrophenol

R.T.: 7.002 min
Delta R.T.: -0.044 min
Response: 521288
Conc: 1.16 ng/ml

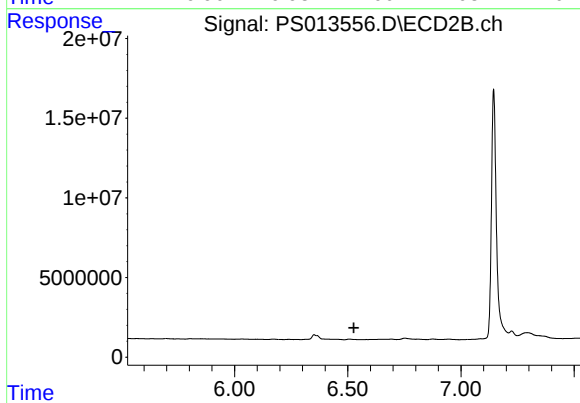

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

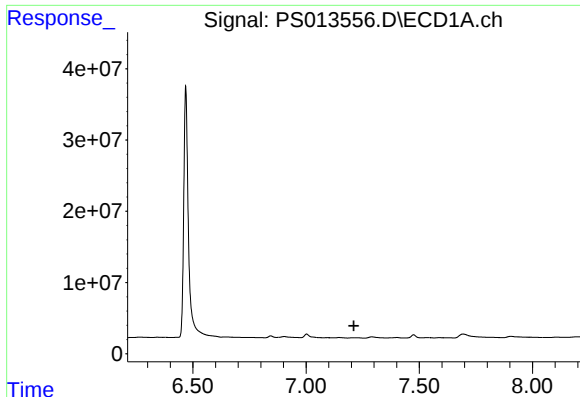

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

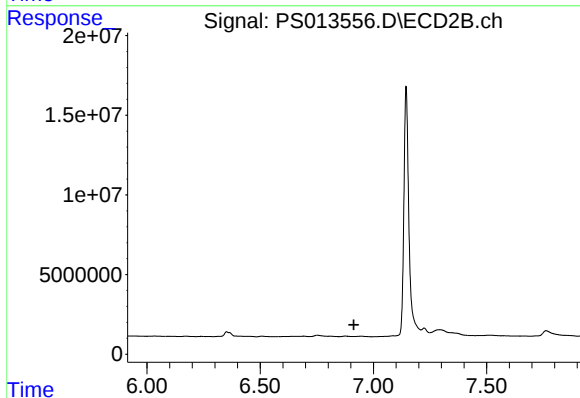


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.914 min
Response: 0
Conc: N.D.

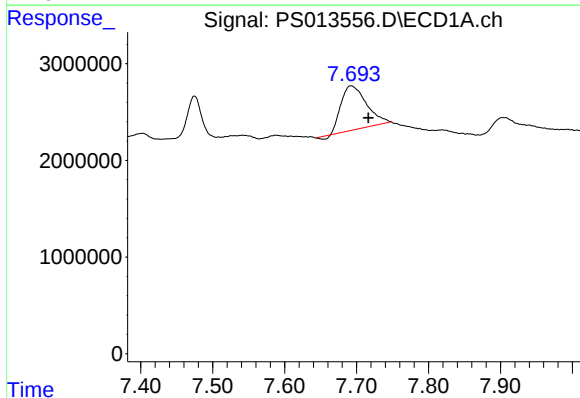


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.024 min
Response: 11039791
Conc: 2.82 ug/ml

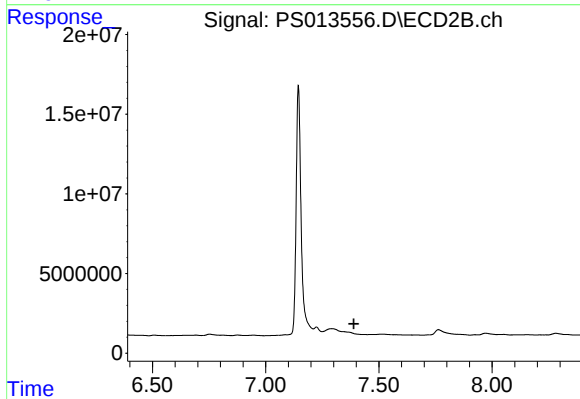

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

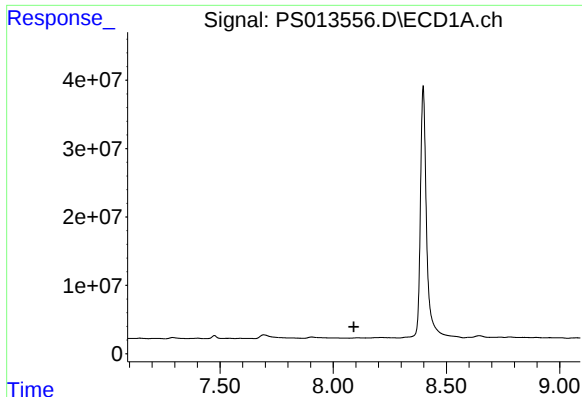

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

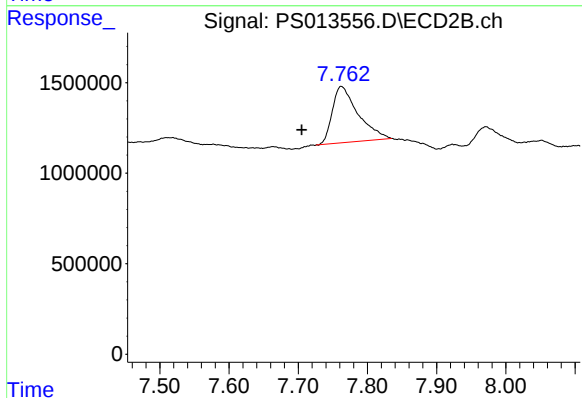


#8 DICHLORPROP

R.T.: 7.762 min
Delta R.T.: 0.057 min
Response: 8033657
Conc: 17.98 ng/ml

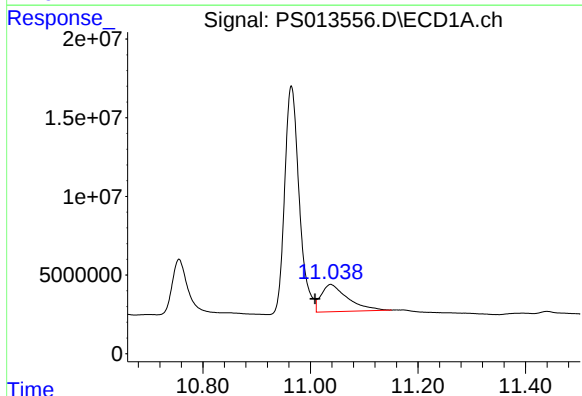

#15 Picloram

R.T.: 11.038 min
Delta R.T.: 0.029 min
Response: 59010830
Conc: 8.57 ng/ml

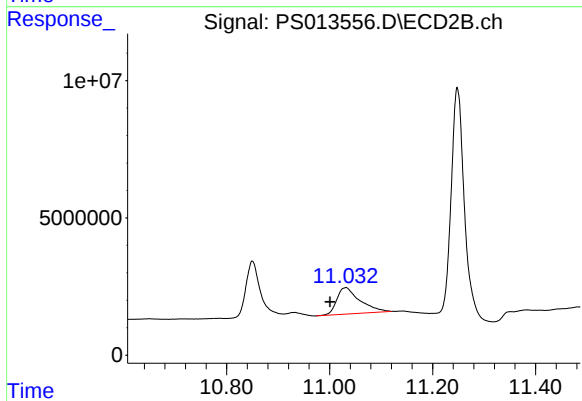

#15 Picloram

R.T.: 11.032 min
Delta R.T.: 0.031 min
Response: 29780952
Conc: 8.55 ng/ml