

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121720\
 Data File : PS013559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 14:29
 Operator : DD\AJ
 Sample : L5115-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 15:36:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	135.1E6	67087183	145.071	170.548
Target Compounds							
7) T	MCPA	7.705	0.000	155.4E6	0	39.750	N.D. #
8) T	DICHLORPROP	0.000	7.759f	0	7798588	N.D.	17.450
9) T	2,4-D	0.000	8.051f	0	5310990	N.D.	9.842
11) T	2,4,5-TP ...	9.186	0.000	11612080	0	2.178	N.D. #
12) T	2,4,5-T	9.404f	0.000	27462486	0	4.967	N.D. #
15) T	Picloram	11.038	11.024	115.1E6	85978733	16.712	24.694 #
16) T	DCPA	0.000	10.929	0	4617348	N.D.	1.518



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121720\
Data File : PS013559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 14:29
Operator : DD\AJ
Sample : L5115-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 15:36:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

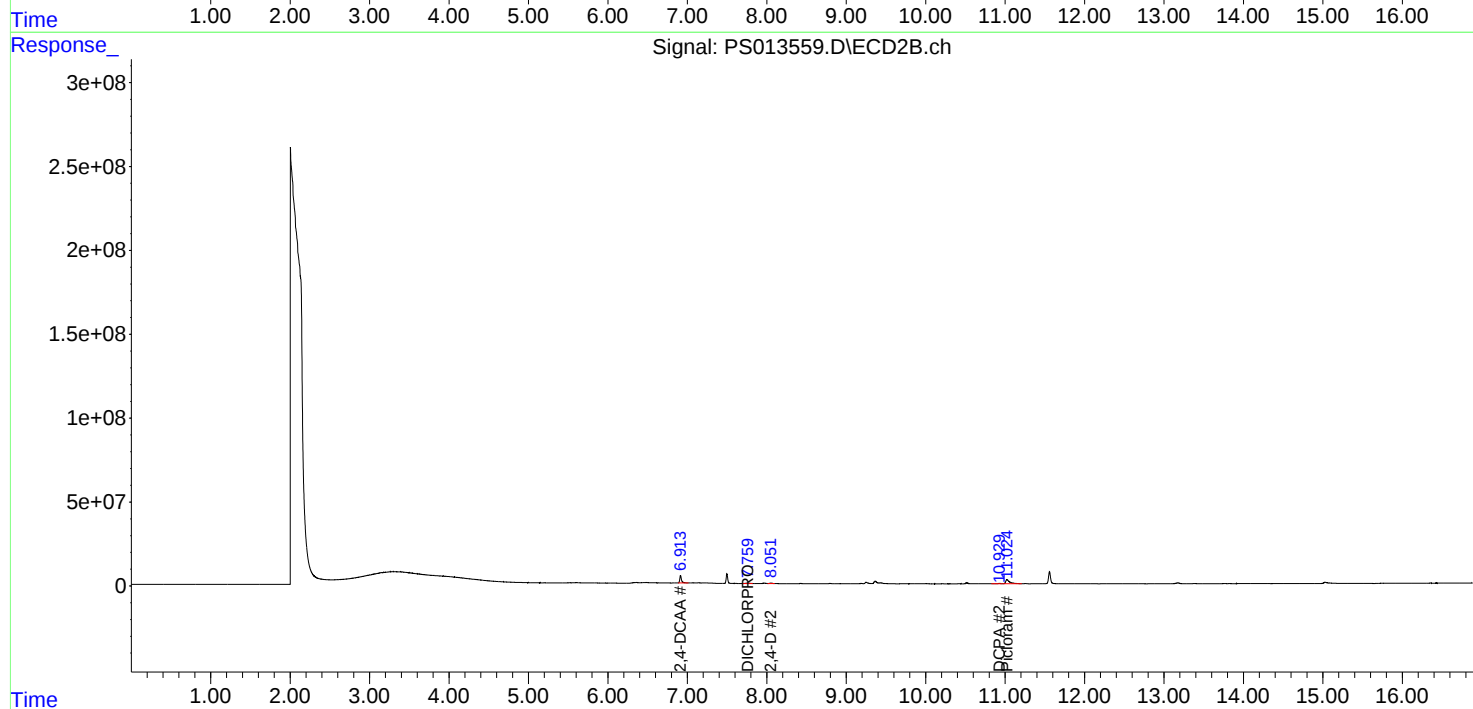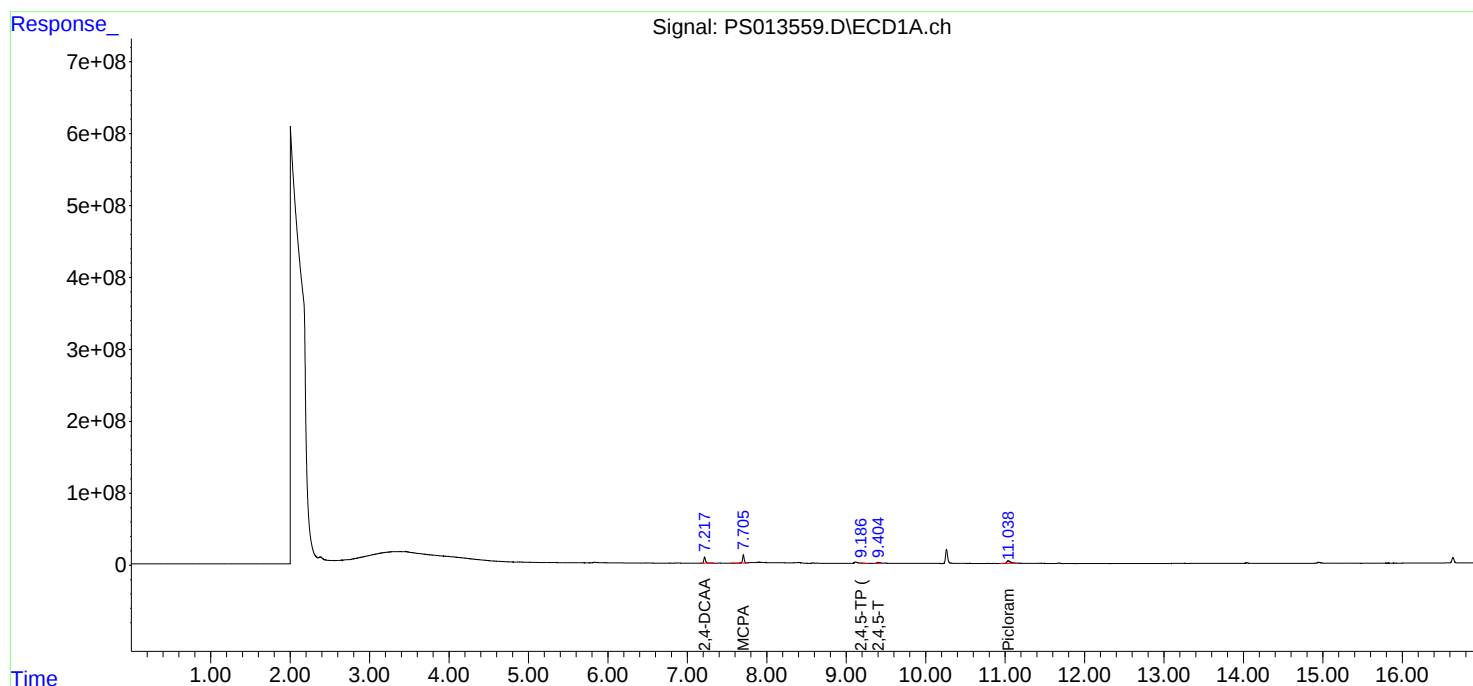


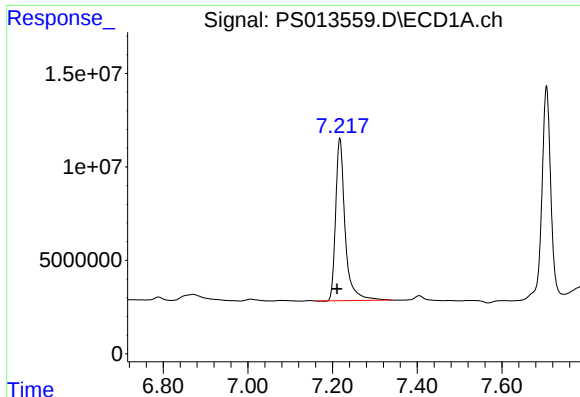

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.006 min
Response: 135070019
Conc: 145.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

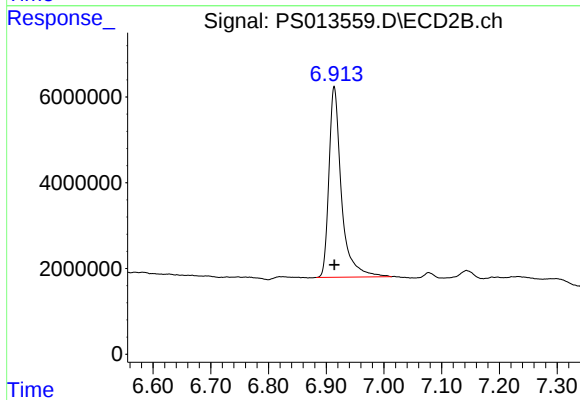


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 67087183
Conc: 170.55 ng/ml

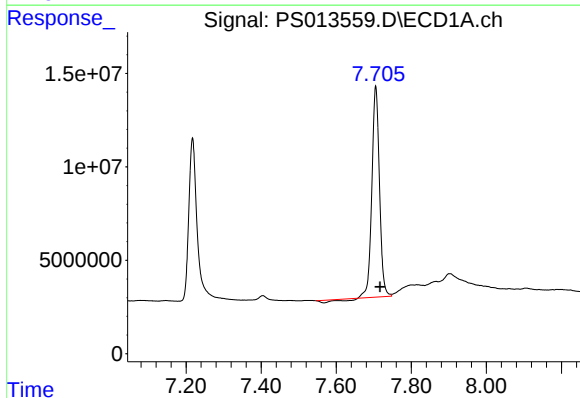


#7 MCPA

R.T.: 7.705 min
Delta R.T.: -0.011 min
Response: 155366555
Conc: 39.75 ug/ml

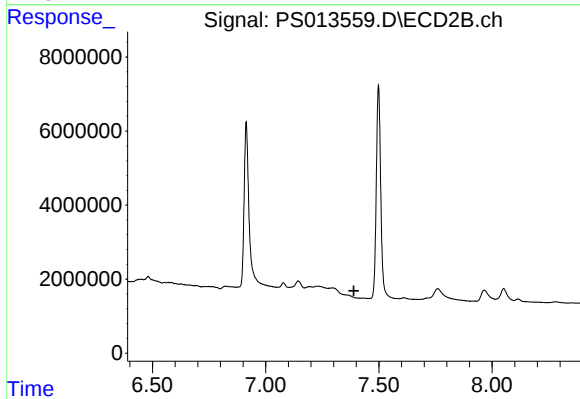

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

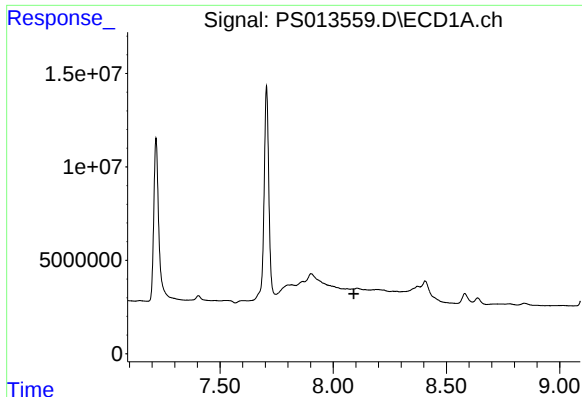

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

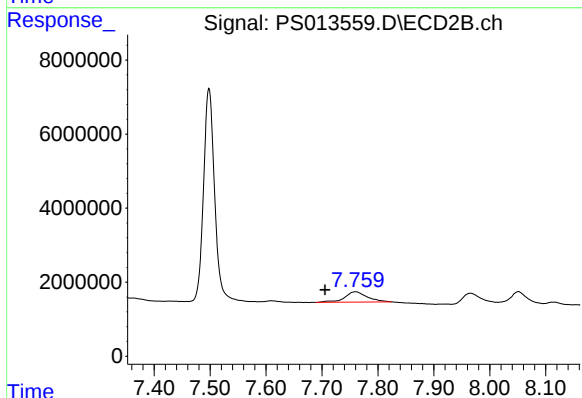


#8 DICHLORPROP

R.T.: 7.759 min
Delta R.T.: 0.054 min
Response: 7798588
Conc: 17.45 ng/ml

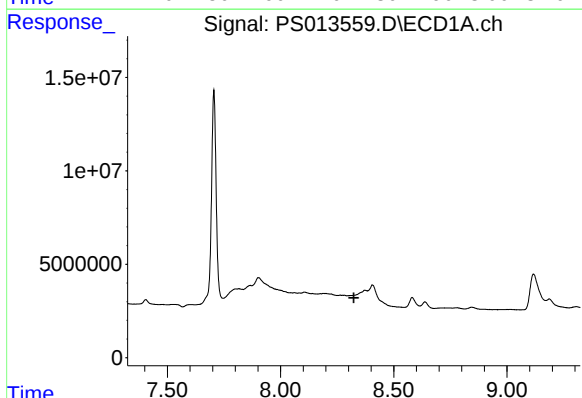


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

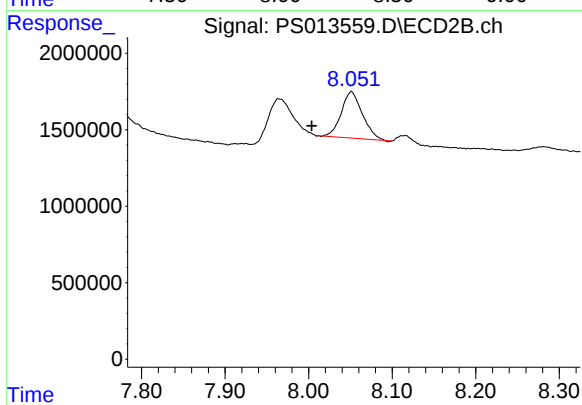

#9 2,4-D


R.T.: 8.051 min
Delta R.T.: 0.048 min
Response: 5310990
Conc: 9.84 ng/ml

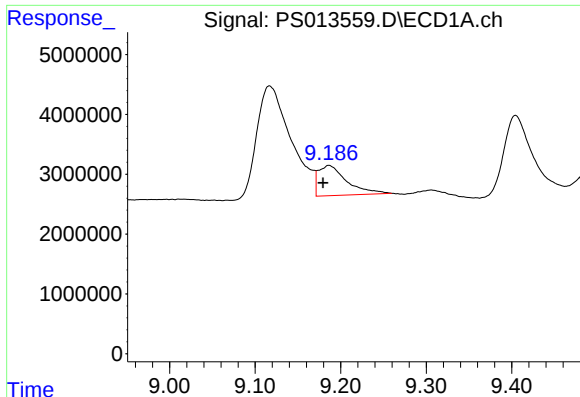

#11 2,4,5-TP (SILVEX)


R.T.: 9.186 min
Delta R.T.: 0.007 min
Response: 11612080
Conc: 2.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

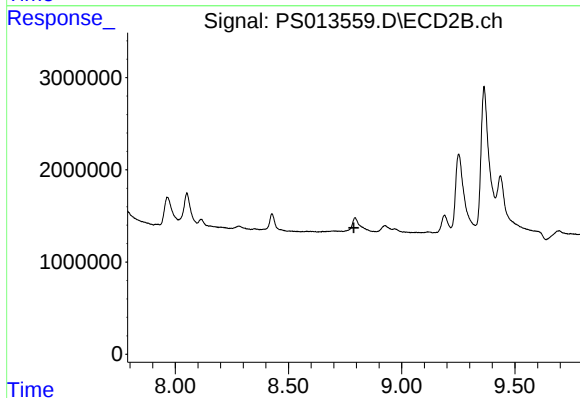


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.789 min
Response: 0
Conc: N.D.

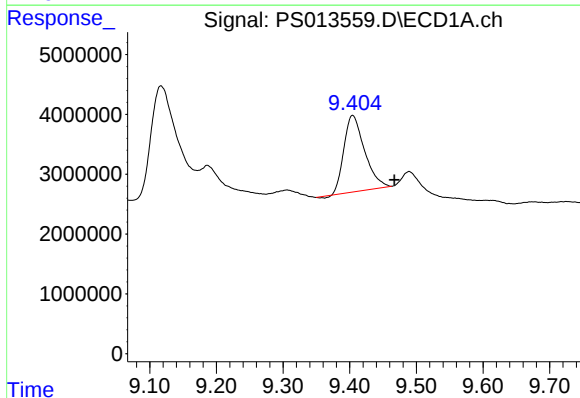


#12 2,4,5-T

R.T.: 9.404 min
Delta R.T.: -0.063 min
Response: 27462486
Conc: 4.97 ng/ml

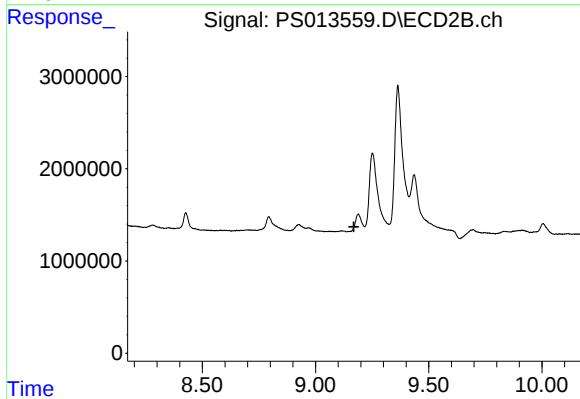

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

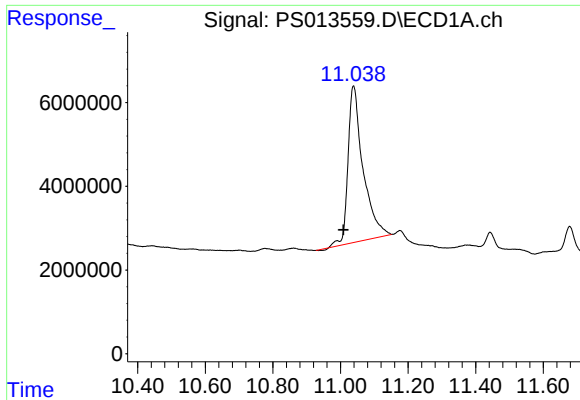

#15 Picloram


R.T.: 11.038 min
Delta R.T.: 0.029 min
Response: 115109408
Conc: 16.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

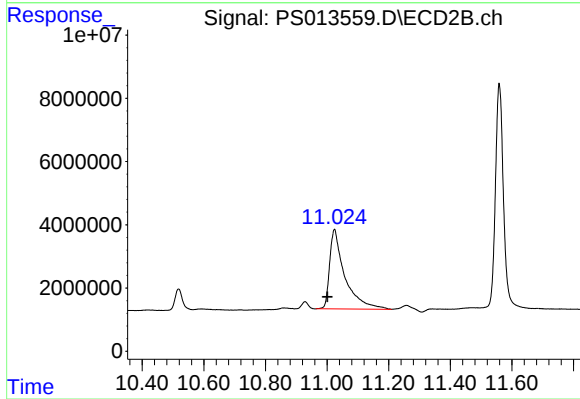


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.023 min
Response: 85978733
Conc: 24.69 ng/ml

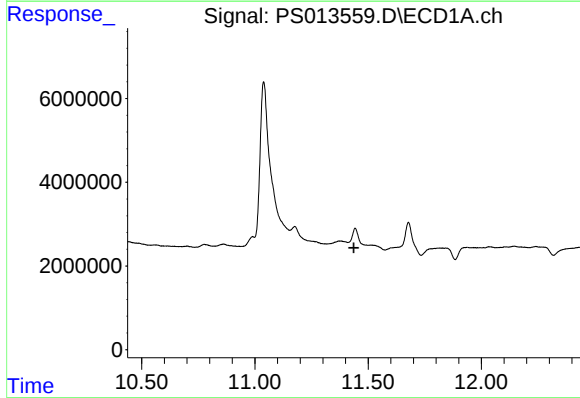

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.437 min
Response: 0
Conc: N.D.

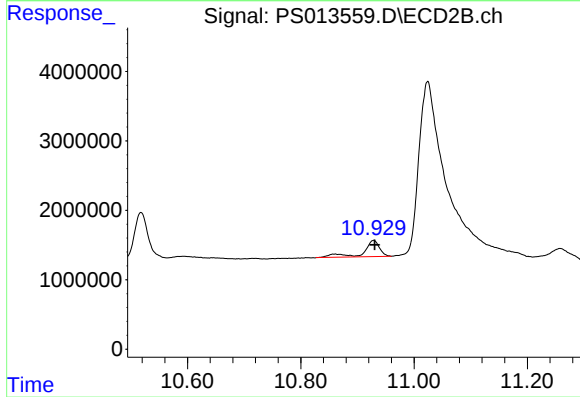

#16 DCPA

R.T.: 10.929 min
Delta R.T.: -0.002 min
Response: 4617348
Conc: 1.52 ng/ml