

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121721\
 Data File : PS017742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2021 09:54
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 22:28:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.127	6.716	738.8E6	305.2E6	472.727	512.018
Target Compounds							
2) T	3,5-DICHL...	6.396	0.000	32393343	0	14.499	N.D. #
5) T	DICAMBA	0.000	6.935f	0	8438422	N.D.	3.168
6) T	MCP	0.000	6.935	0	8438422	N.D.	3.877
9) T	2,4-D	8.306f	0.000	85551184	0	48.392	N.D. #
15) T	Picloram	10.886	10.802f	5728786	14708865	<MDL	2.995 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121721\
Data File : PS017742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 09:54
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 22:28:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

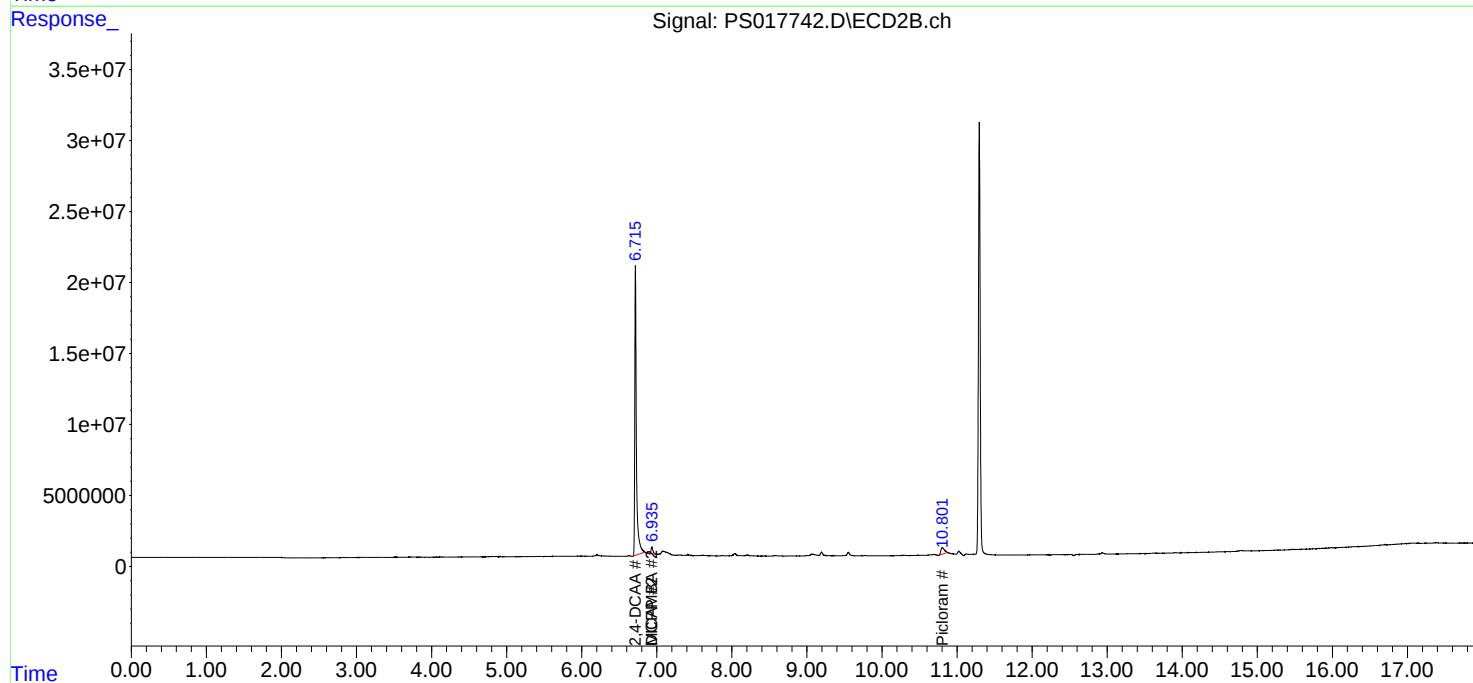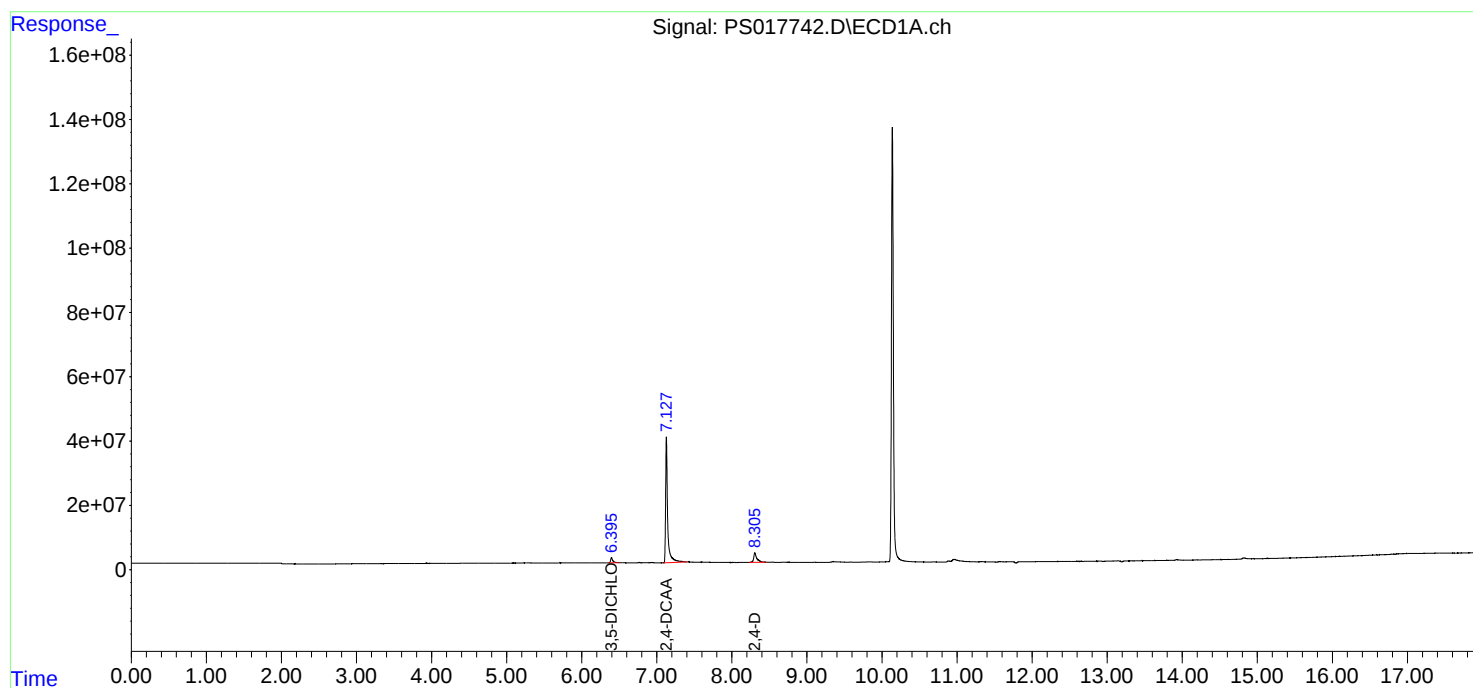


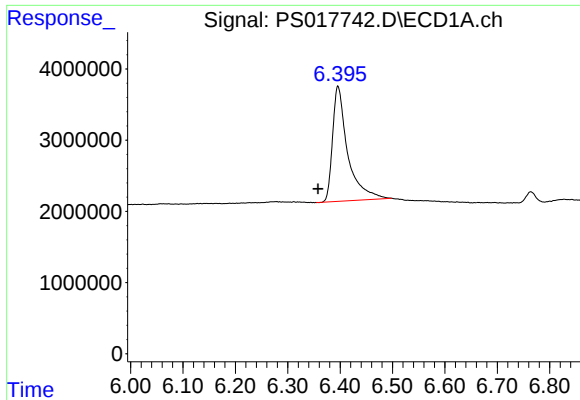

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.396 min
Delta R.T.: 0.037 min
Response: 32393343
Conc: 14.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

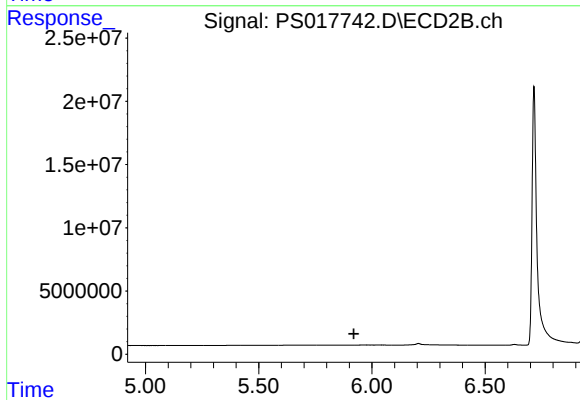


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

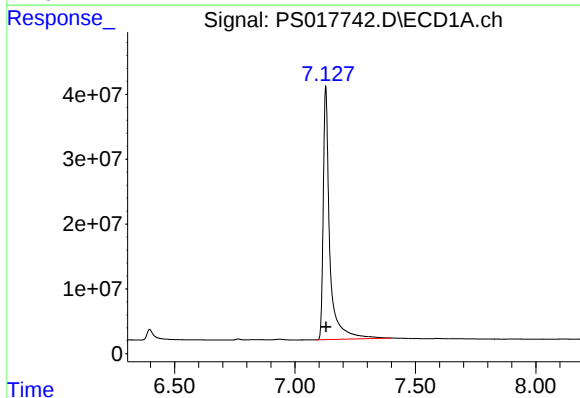


#4 2,4-DCAA

R.T.: 7.127 min
Delta R.T.: -0.003 min
Response: 738845877
Conc: 472.73 ng/ml

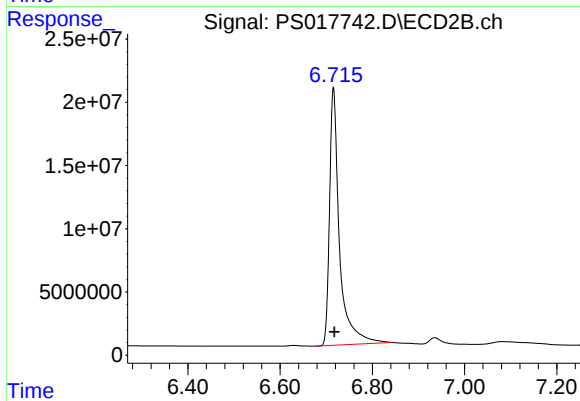

#4 2,4-DCAA


R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 305214895
Conc: 512.02 ng/ml

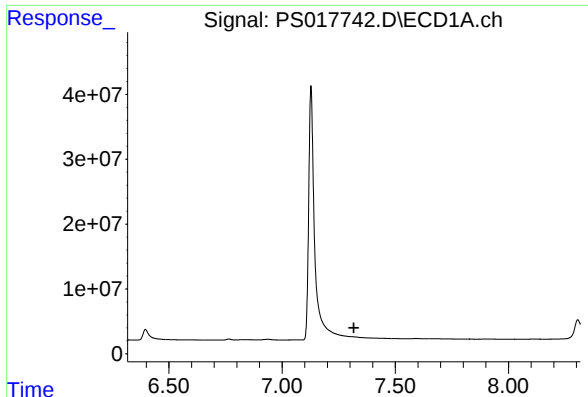

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

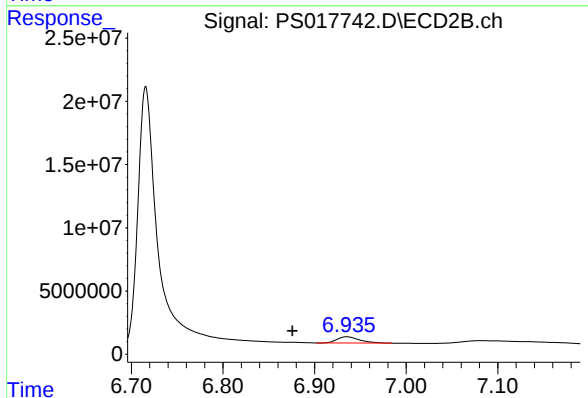


#5 DICAMBA

R.T.: 6.935 min
Delta R.T.: 0.059 min
Response: 8438422
Conc: 3.17 ng/ml

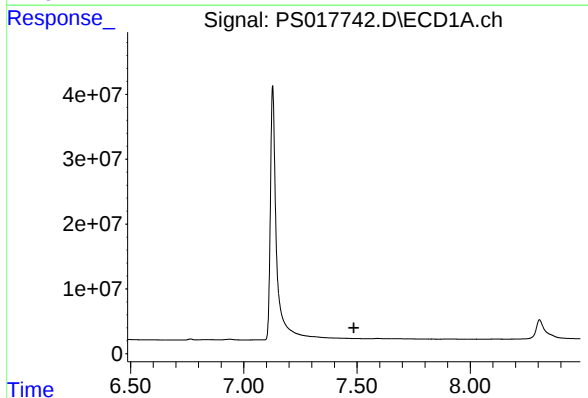


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

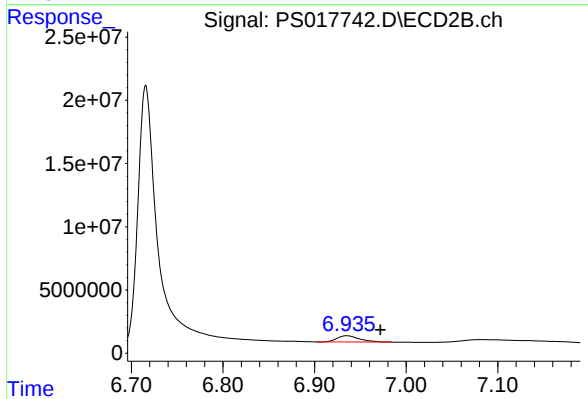

#6 MCPP


R.T.: 6.935 min
Delta R.T.: -0.037 min
Response: 8438422
Conc: 3.88 ug/ml

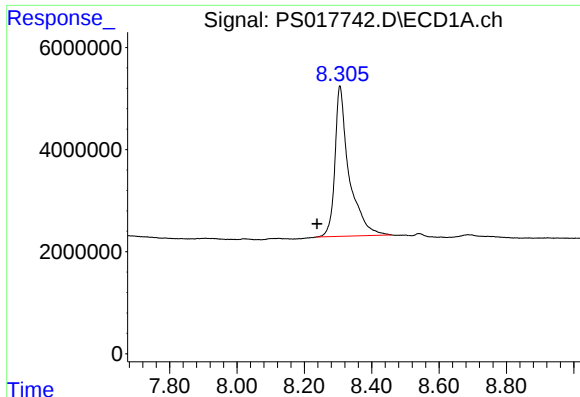

#9 2,4-D


R.T.: 8.306 min
Delta R.T.: 0.067 min
Response: 85551184
Conc: 48.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

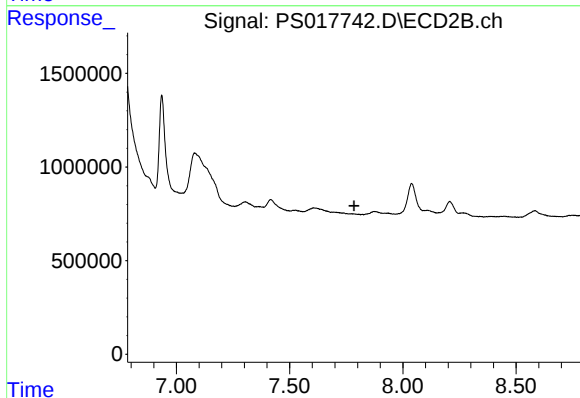


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

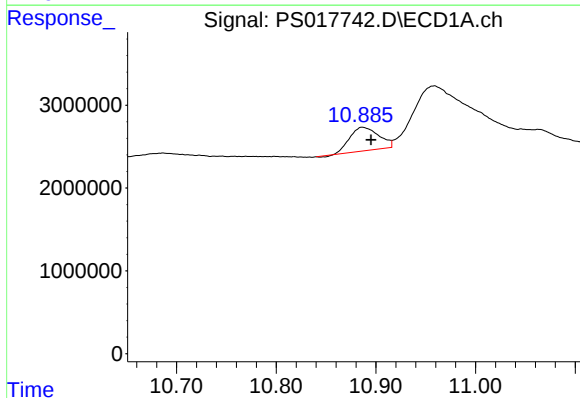

#15 Picloram

R.T.: 10.886 min
Delta R.T.: -0.009 min
Response: 5728786
Conc: N.D.

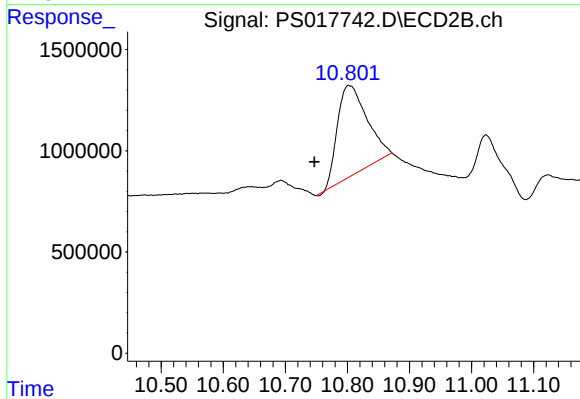

#15 Picloram

R.T.: 10.802 min
Delta R.T.: 0.055 min
Response: 14708865
Conc: 2.99 ng/ml