

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121721\
 Data File : PS017764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2021 21:12
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 22:38:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.128	6.716	747.3E6	310.2E6	478.116	520.311
Target Compounds							
2) T	3,5-DICHL...	6.398	0.000	37753728	0	16.899	N.D. #
5) T	DICAMBA	0.000	6.935f	0	15333171	N.D.	5.756
6) T	MCP	0.000	6.935	0	15333171	N.D.	7.045
9) T	2,4-D	8.306f	0.000	109.3E6	0	61.816	N.D. #
15) T	Picloram	10.886	0.000	11629159	0	1.072	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121721\
Data File : PS017764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 21:12
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 22:38:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

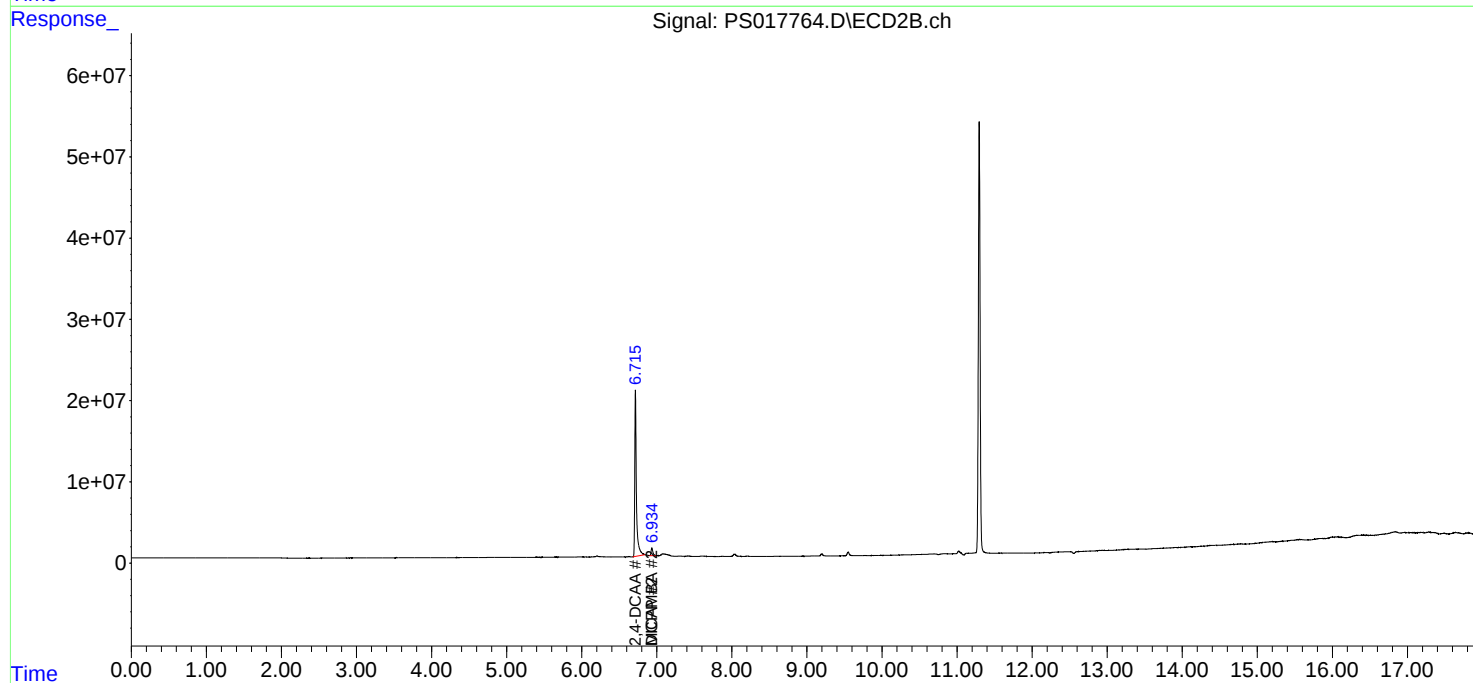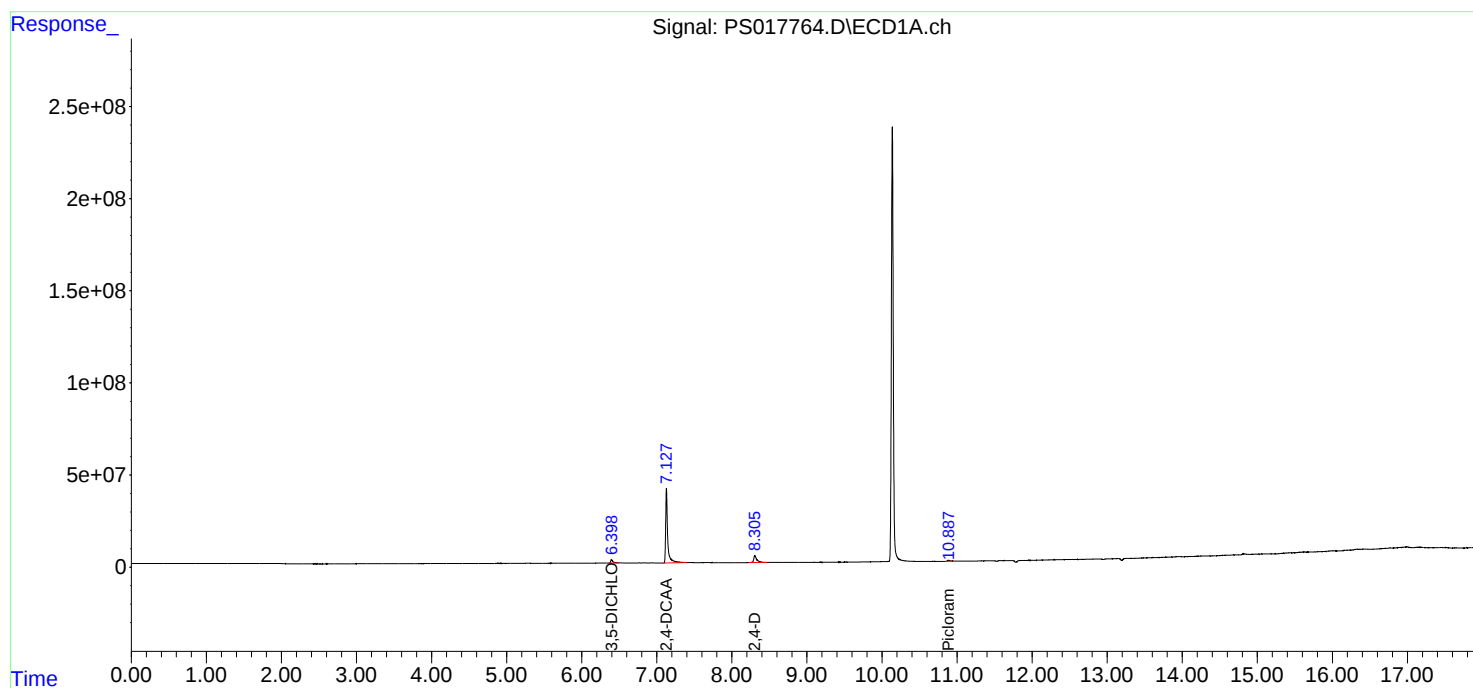


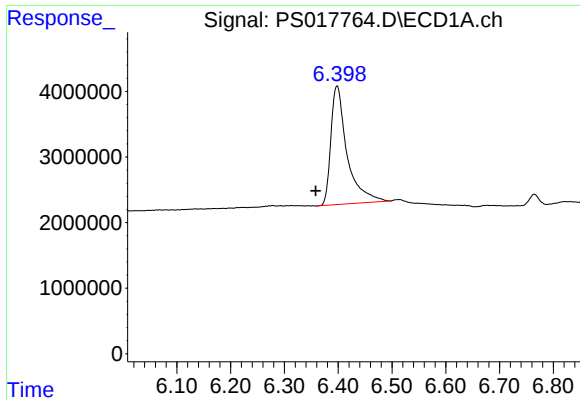

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.398 min
Delta R.T.: 0.040 min
Response: 37753728
Conc: 16.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

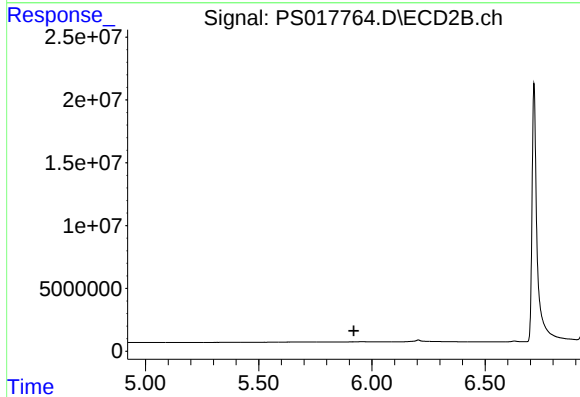


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

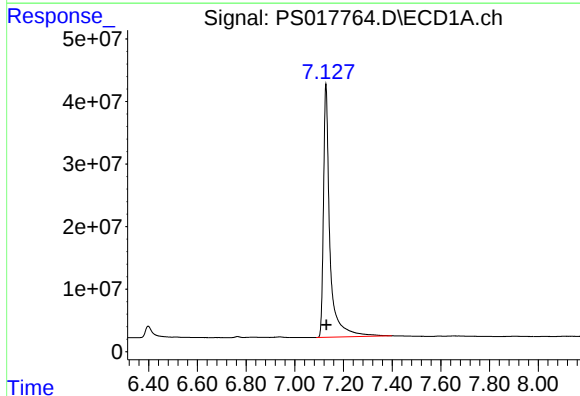


#4 2,4-DCAA

R.T.: 7.128 min
Delta R.T.: -0.002 min
Response: 747269710
Conc: 478.12 ng/ml

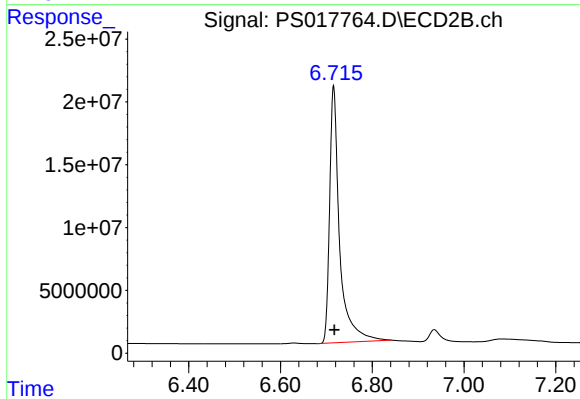

#4 2,4-DCAA


R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 310158336
Conc: 520.31 ng/ml

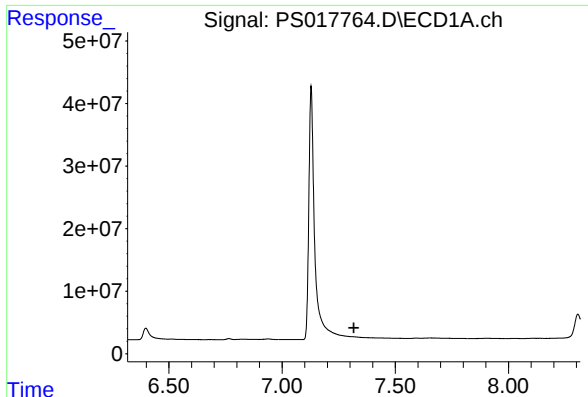

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

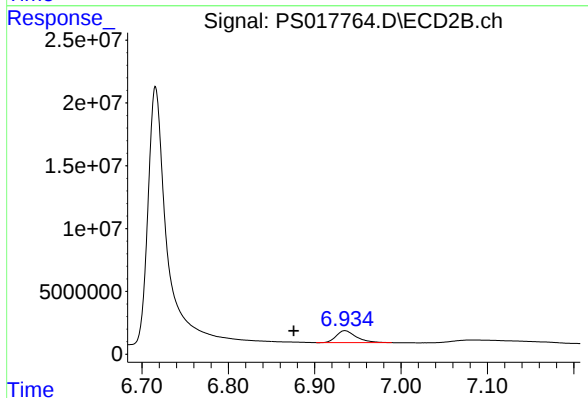


#5 DICAMBA

R.T.: 6.935 min
Delta R.T.: 0.059 min
Response: 15333171
Conc: 5.76 ng/ml

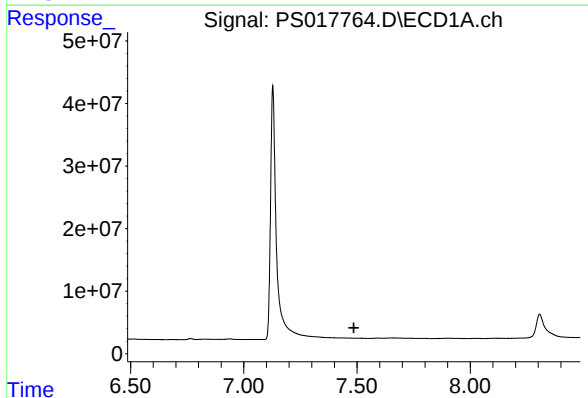


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

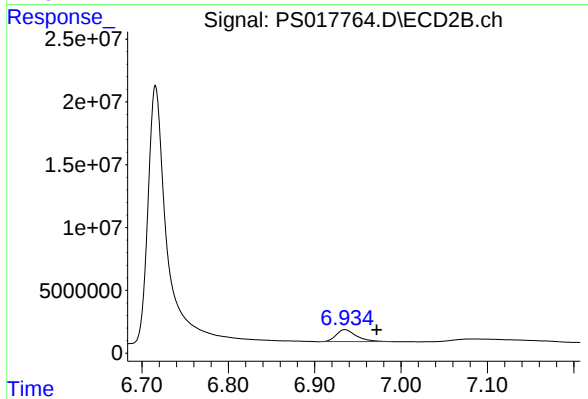

#6 MCPP


R.T.: 6.935 min
Delta R.T.: -0.037 min
Response: 15333171
Conc: 7.04 ug/ml

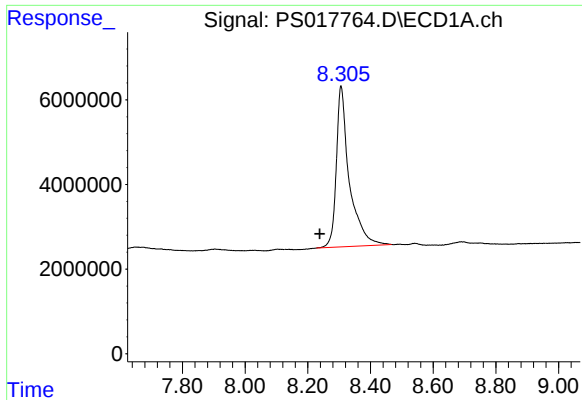

#9 2,4-D


R.T.: 8.306 min
Delta R.T.: 0.067 min
Response: 109282784
Conc: 61.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

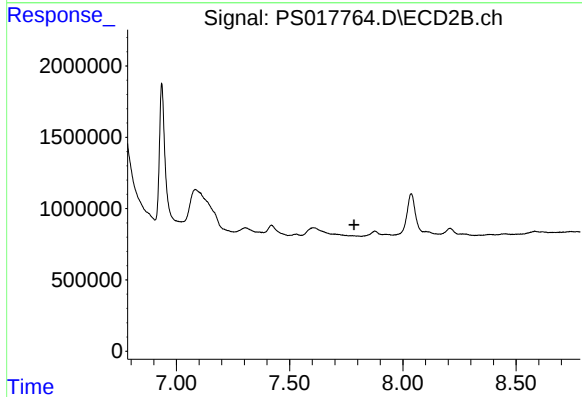


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

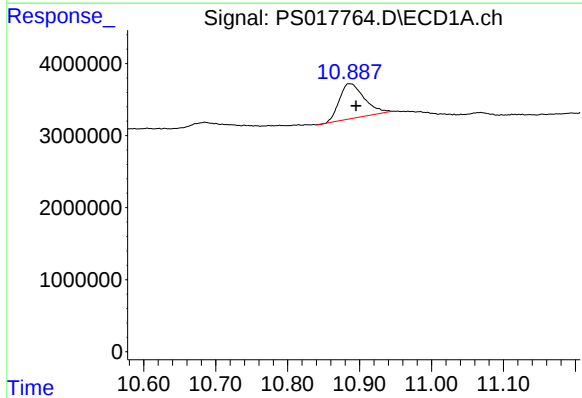

#15 Picloram

R.T.: 10.886 min
Delta R.T.: -0.009 min
Response: 11629159
Conc: 1.07 ng/ml

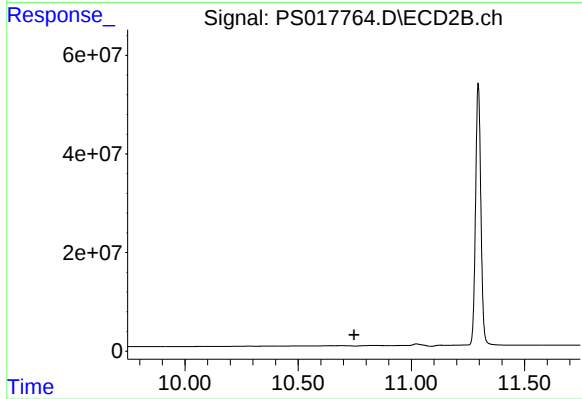

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.747 min
Response: 0
Conc: N.D.