

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121723\
 Data File : PS025132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 09:20
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:53:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.512	2.553	4962141	3497289	1.721 3.049 #
2) T	3,5-DICHL...	5.696	6.023f	10117643	119932	2.993 <MDL #
3) T	4-Nitroph...	6.191	0.000	10563453	0	7.173 N.D. #
5) T	DICAMBA	0.000	6.966	0	7532909	N.D. 2.431
6) T	MCP	6.674	6.966f	5074043	7532909	<MDL 3.632 #
7) T	MCPA	0.000	7.167f	0	3344952	N.D. 1.017
8) T	DICHLORPROP	0.000	7.548	0	1975053	N.D. 2.511
9) T	2,4-D	7.245	7.763f	74485957	865857	24.523 <MDL #
10) T	Pentachlo...	0.000	8.244	0	1151069	N.D. <MDL
11) T	2,4,5-TP ...	0.000	8.605	0	200286	N.D. <MDL
12) T	2,4,5-T	0.000	8.972	0	1118225	N.D. <MDL
13) T	2,4-DB	0.000	9.505	0	758457	N.D. 1.370
14) T	DINOSEB	0.000	9.803	0	556522	N.D. <MDL
15) T	Picloram	9.676	10.754	120.4E6	40048587	6.179 6.119
16) T	DCPA	0.000	10.754	0	40048587	N.D. 7.389



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121723\
Data File : PS025132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 09:20
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:53:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

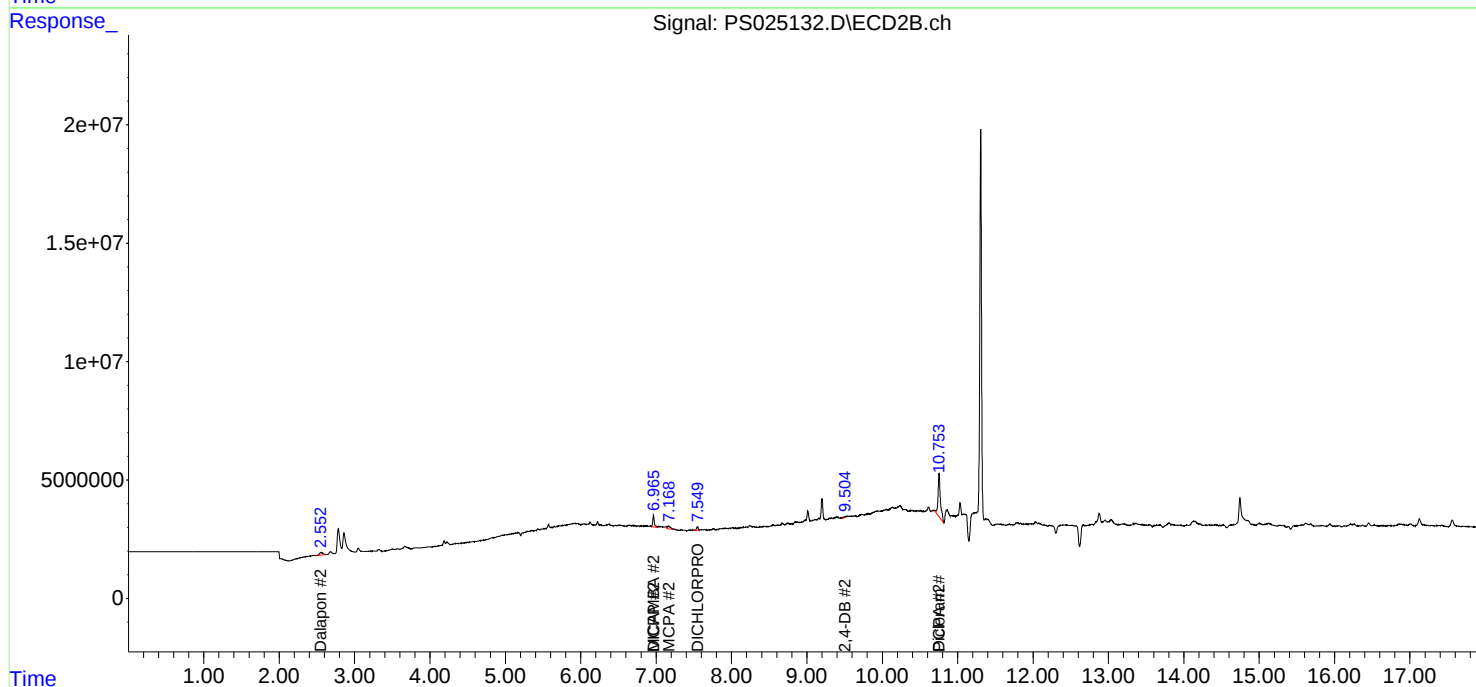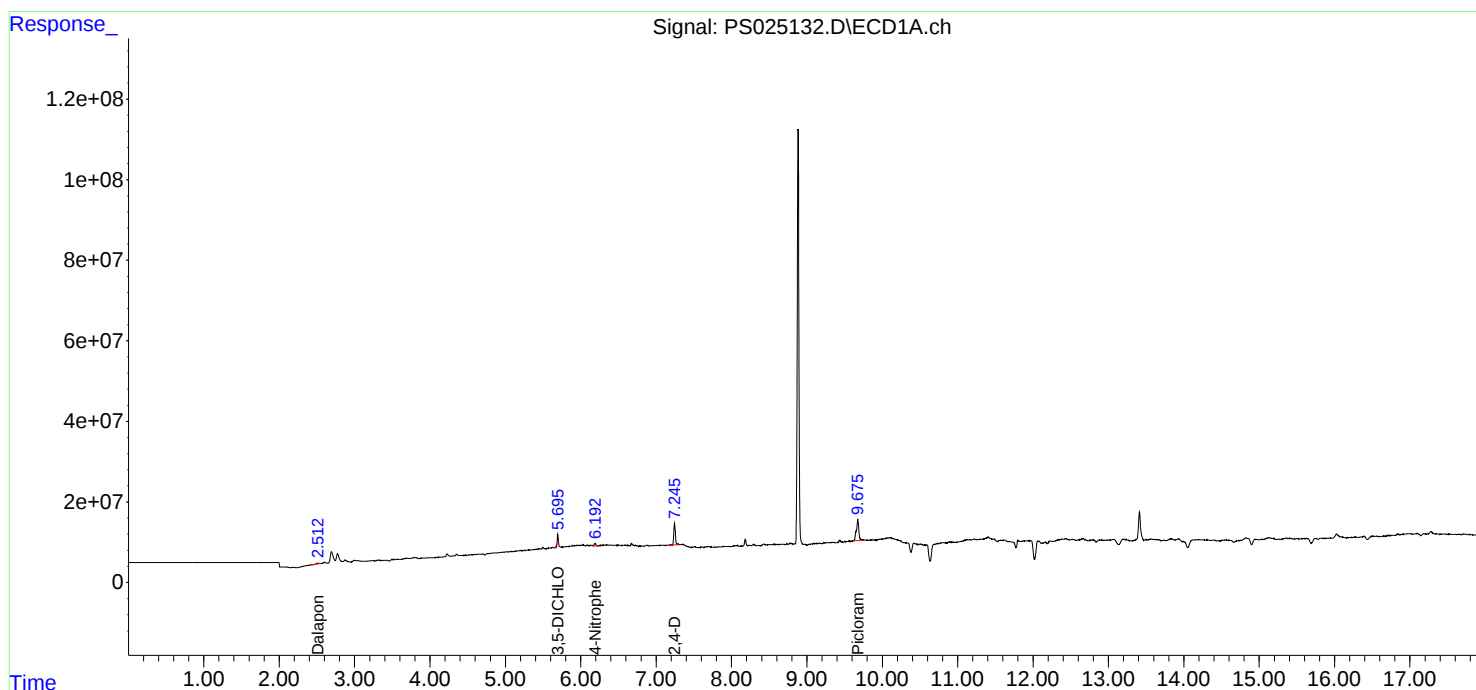


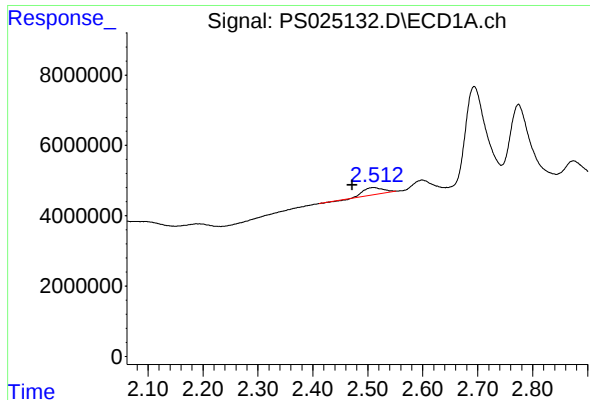

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.040 min
Response: 4962141
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

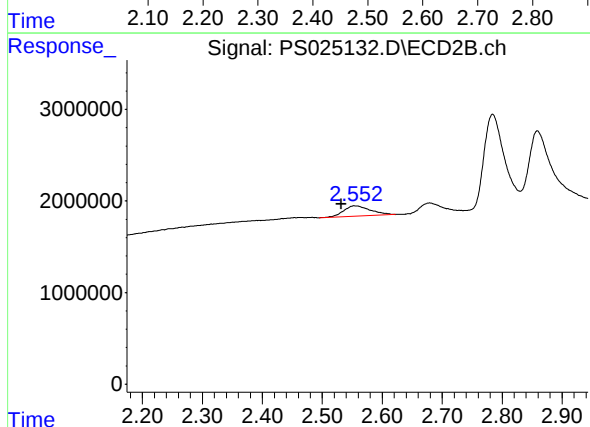


#1 Dalapon

R.T.: 2.553 min
Delta R.T.: 0.021 min
Response: 3497289
Conc: 3.05 ng/ml

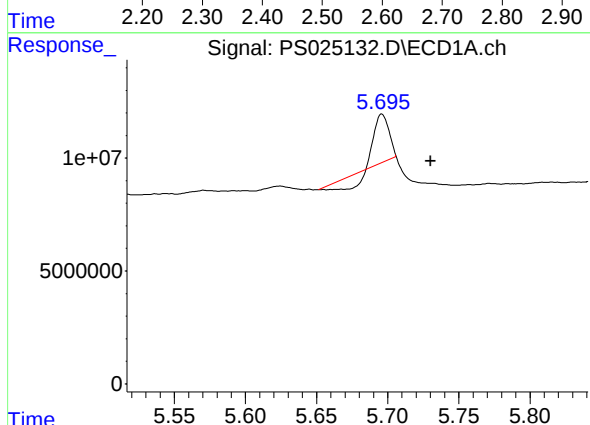


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.696 min
Delta R.T.: -0.034 min
Response: 10117643
Conc: 2.99 ng/ml

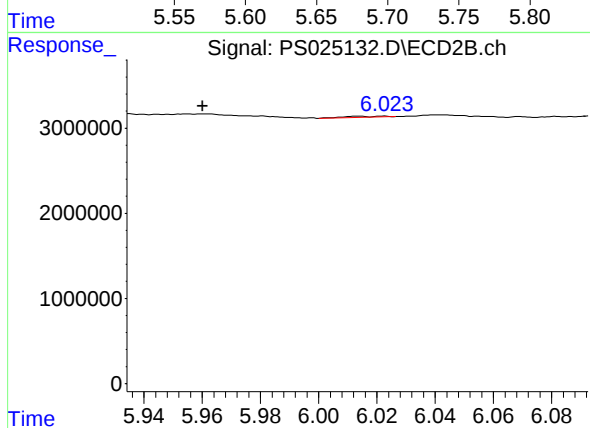

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.023 min
Delta R.T.: 0.062 min
Response: 119932
Conc: N.D.

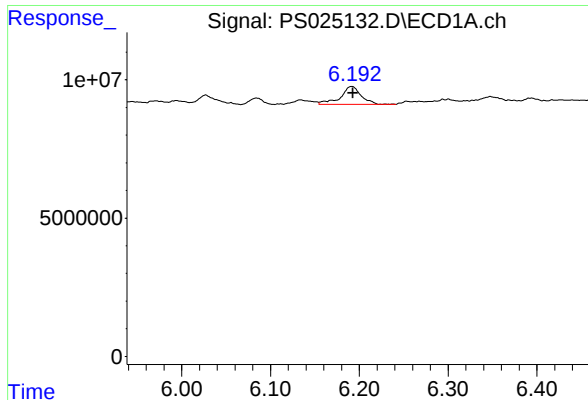

#3 4-Nitrophenol


R.T.: 6.191 min
Delta R.T.: -0.002 min
Response: 10563453
Conc: 7.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

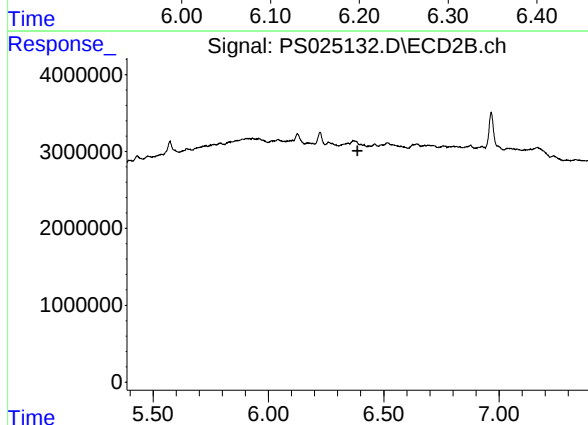


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

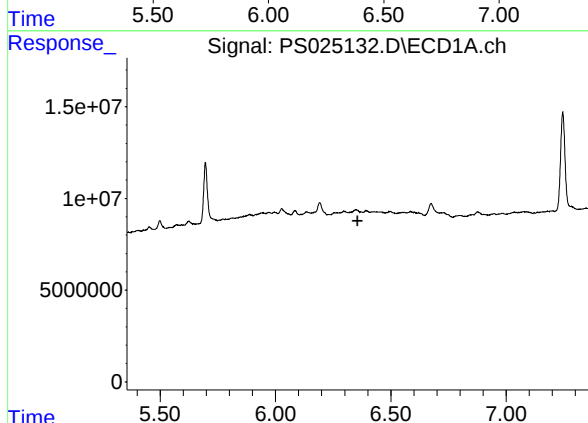


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

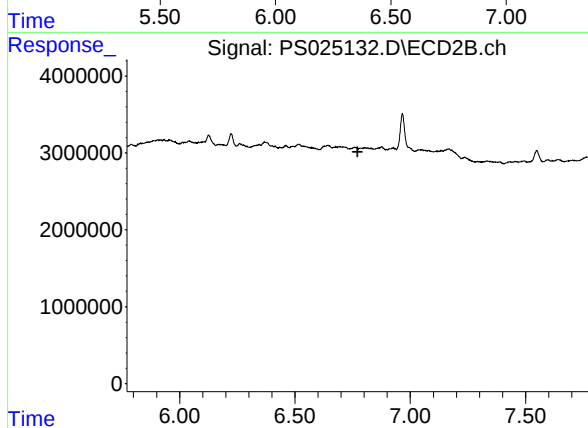

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

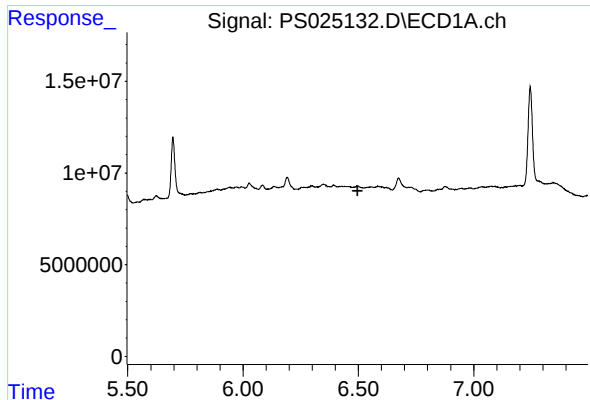

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

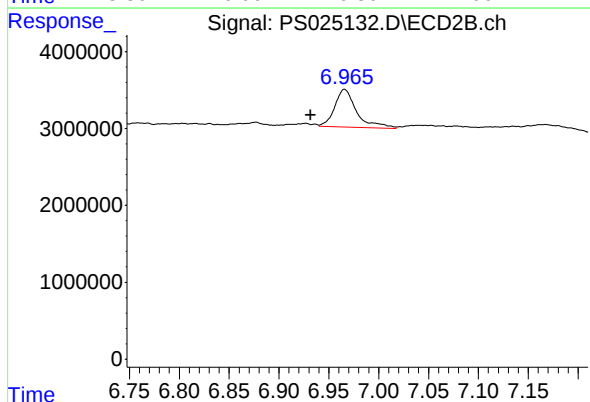


#5 DICAMBA

R.T.: 6.966 min
Delta R.T.: 0.034 min
Response: 7532909
Conc: 2.43 ng/ml

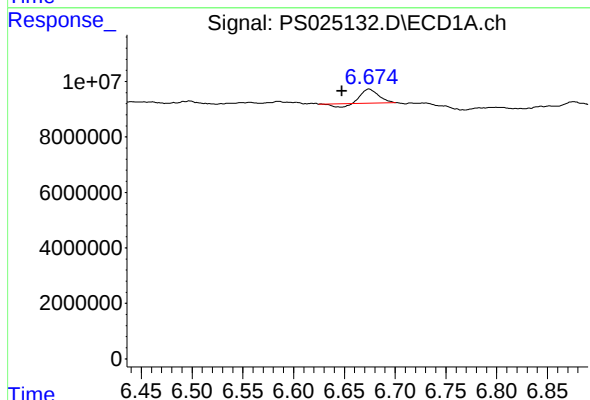


#6 MCPP

R.T.: 6.674 min
Delta R.T.: 0.027 min
Response: 5074043
Conc: N.D.

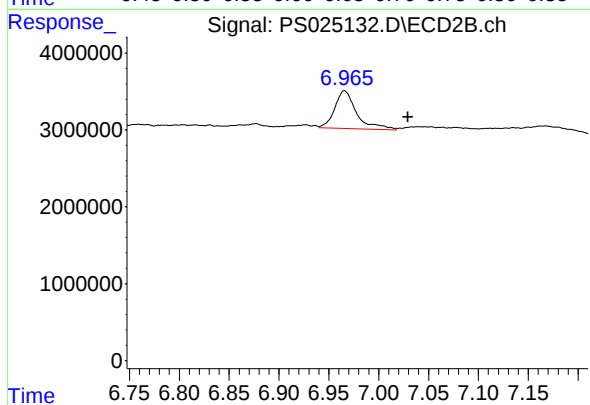

#6 MCPP


R.T.: 6.966 min
Delta R.T.: -0.064 min
Response: 7532909
Conc: 3.63 ug/ml

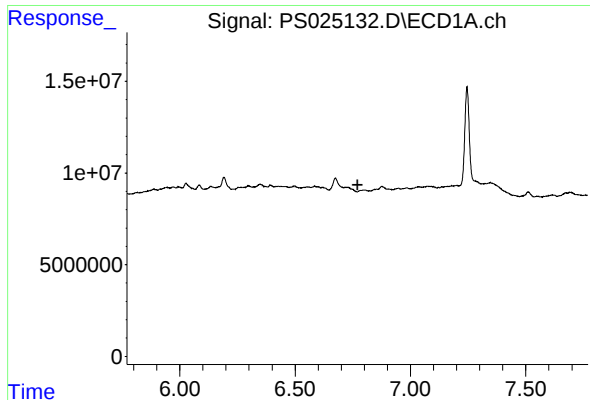

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

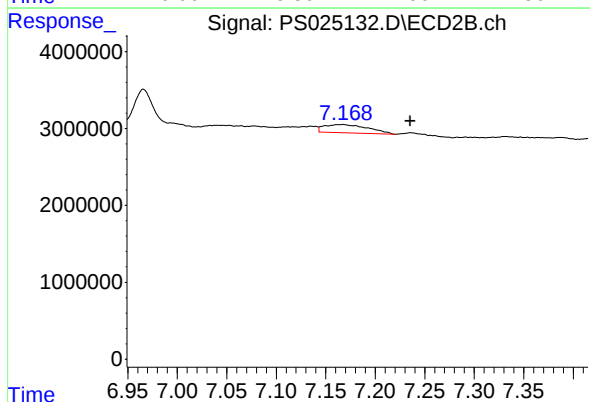


#7 MCPA

R.T.: 7.167 min
Delta R.T.: -0.068 min
Response: 3344952
Conc: 1.02 ug/ml

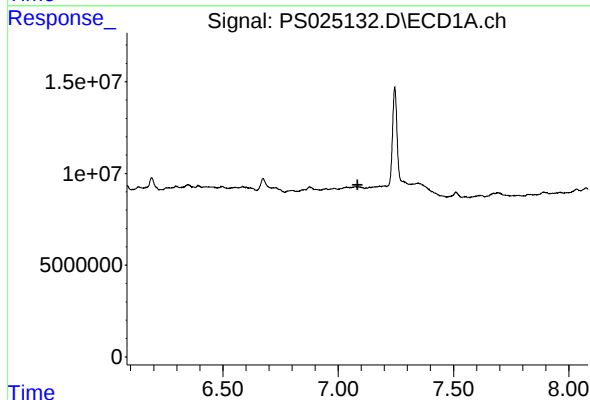


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

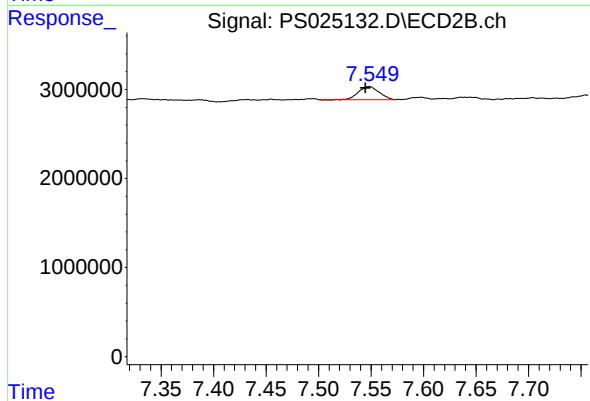

#8 DICHLORPROP


R.T.: 7.548 min
Delta R.T.: 0.003 min
Response: 1975053
Conc: 2.51 ng/ml

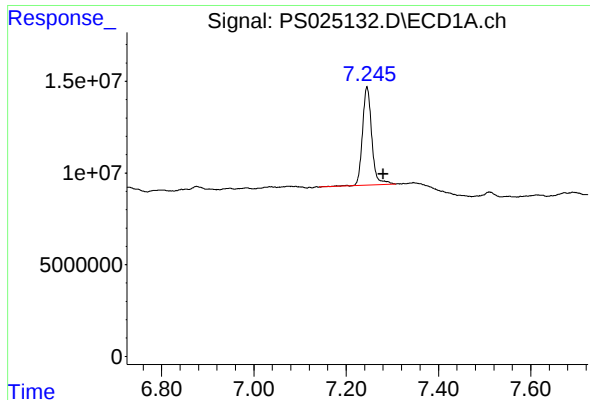

#9 2,4-D


R.T.: 7.245 min
Delta R.T.: -0.036 min
Response: 74485957
Conc: 24.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

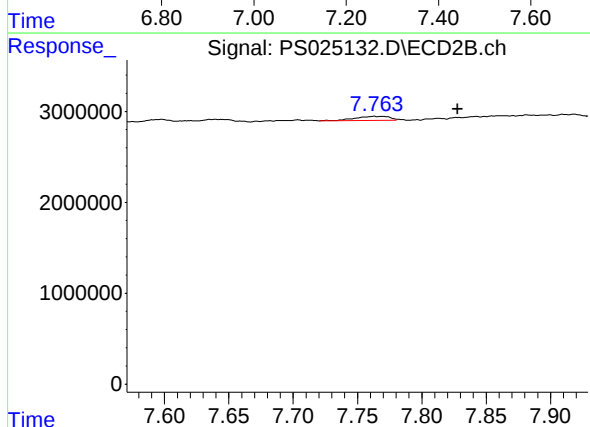


#9 2,4-D

R.T.: 7.763 min
Delta R.T.: -0.065 min
Response: 865857
Conc: N.D.

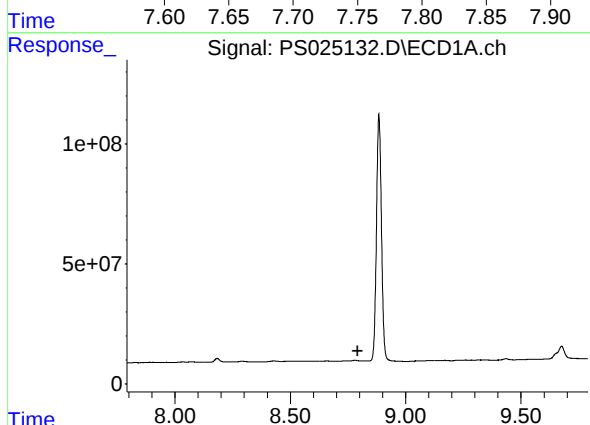


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

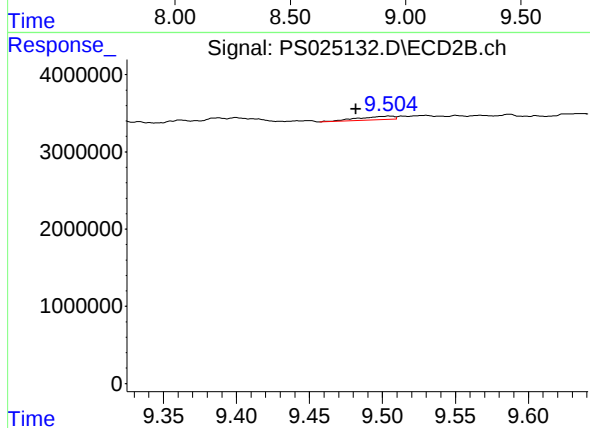

#13 2,4-DB


R.T.: 9.505 min
Delta R.T.: 0.023 min
Response: 758457
Conc: 1.37 ng/ml

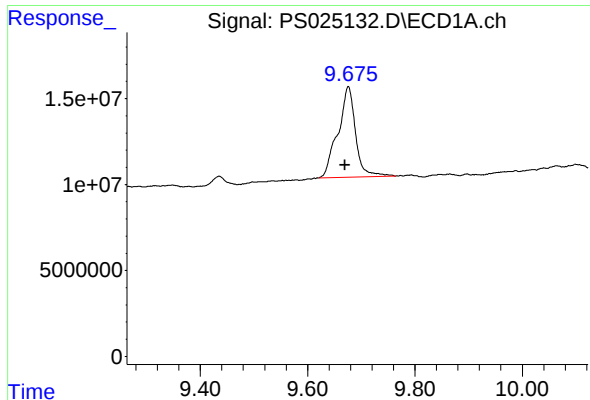

#15 Picloram


R.T.: 9.676 min
Delta R.T.: 0.006 min
Response: 120396710
Conc: 6.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

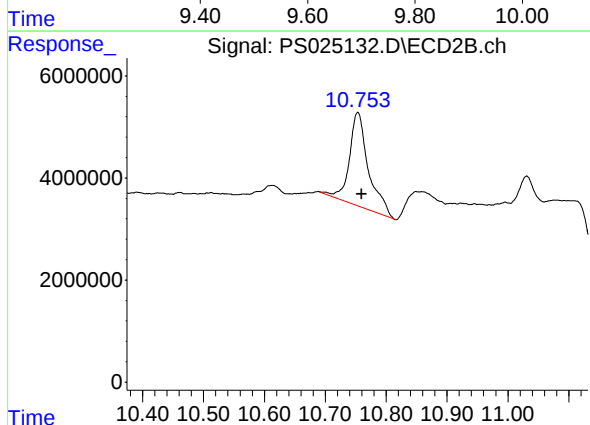


#15 Picloram

R.T.: 10.754 min
Delta R.T.: -0.006 min
Response: 40048587
Conc: 6.12 ng/ml

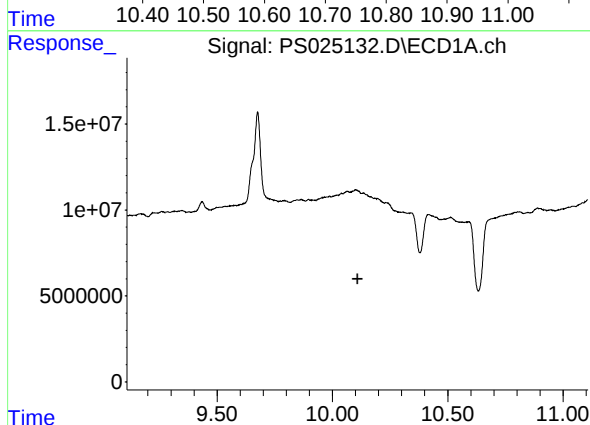

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

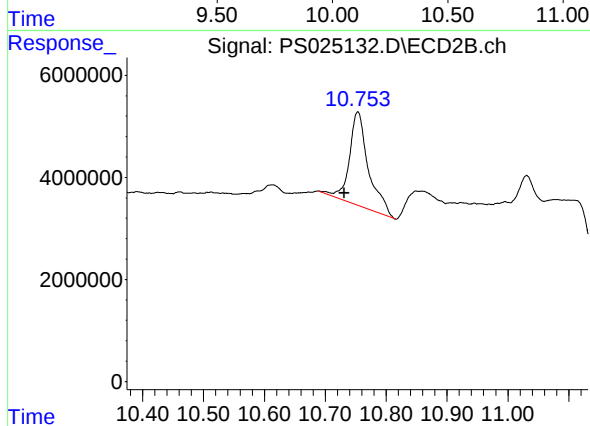

#16 DCPA

R.T.: 10.754 min
Delta R.T.: 0.022 min
Response: 40048587
Conc: 7.39 ng/ml