

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121723\
 Data File : PS025133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 09:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:53:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.768	1291.8E6	411.1E6	577.244	567.316
Target Compounds							
1) T	Dalapon	2.508	2.562	7992226	3977912	2.772	3.468 #
2) T	3,5-DICHL...	5.696	0.000	4049807	0	1.198	N.D. #
3) T	4-Nitroph...	6.195	0.000	9238755	0	6.274	N.D. #
5) T	DICAMBA	0.000	6.968	0	3224081	N.D.	1.041
6) T	MCP	0.000	6.968f	0	3224081	N.D.	1.554
8) T	DICHLORPROP	0.000	7.555	0	2528612	N.D.	3.214
9) T	2,4-D	7.245	7.766f	24190004	207549	7.964	<MDL #
11) T	2,4,5-TP ...	0.000	8.604	0	494040	N.D.	<MDL
12) T	2,4,5-T	0.000	8.976	0	491634	N.D.	<MDL
15) T	Picloram	9.679	10.757	81813374	22149470	4.199	3.384
16) T	DCPA	0.000	10.757	0	22149470	N.D.	4.087



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121723\
Data File : PS025133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 09:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:53:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

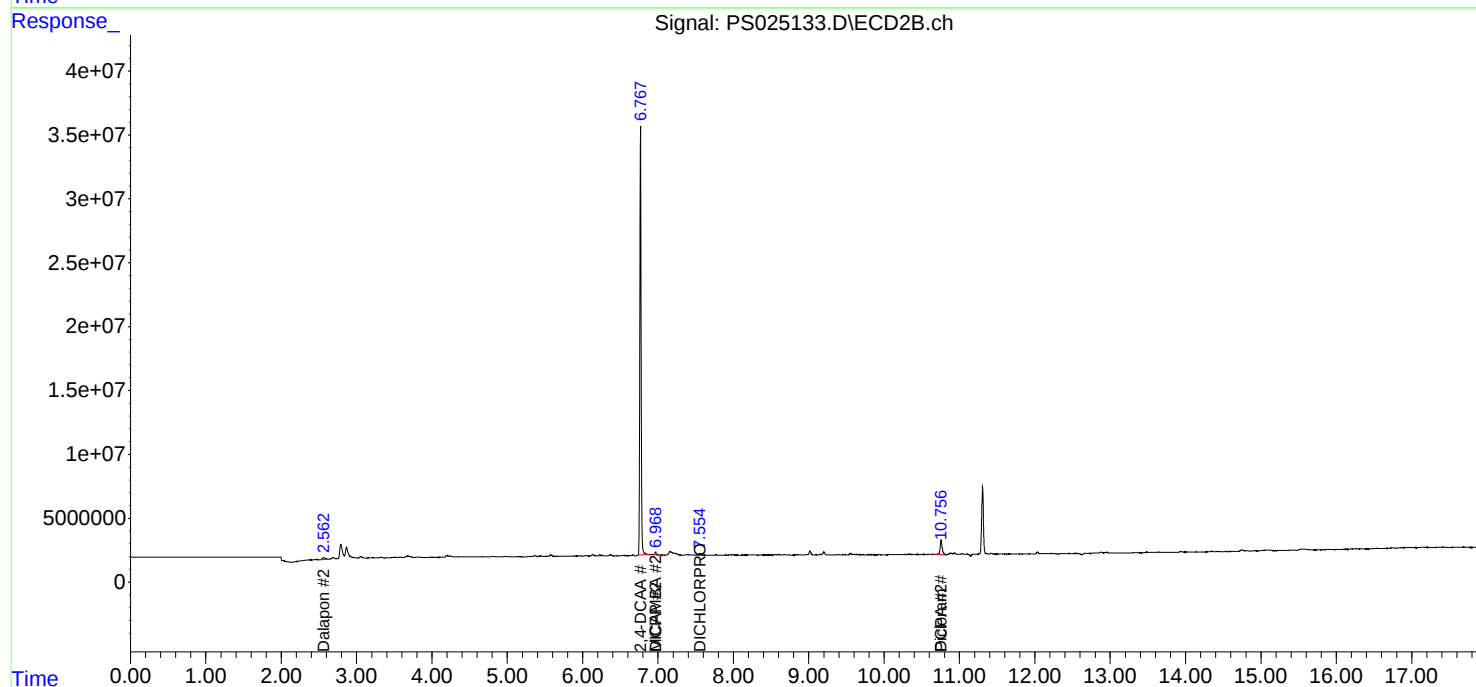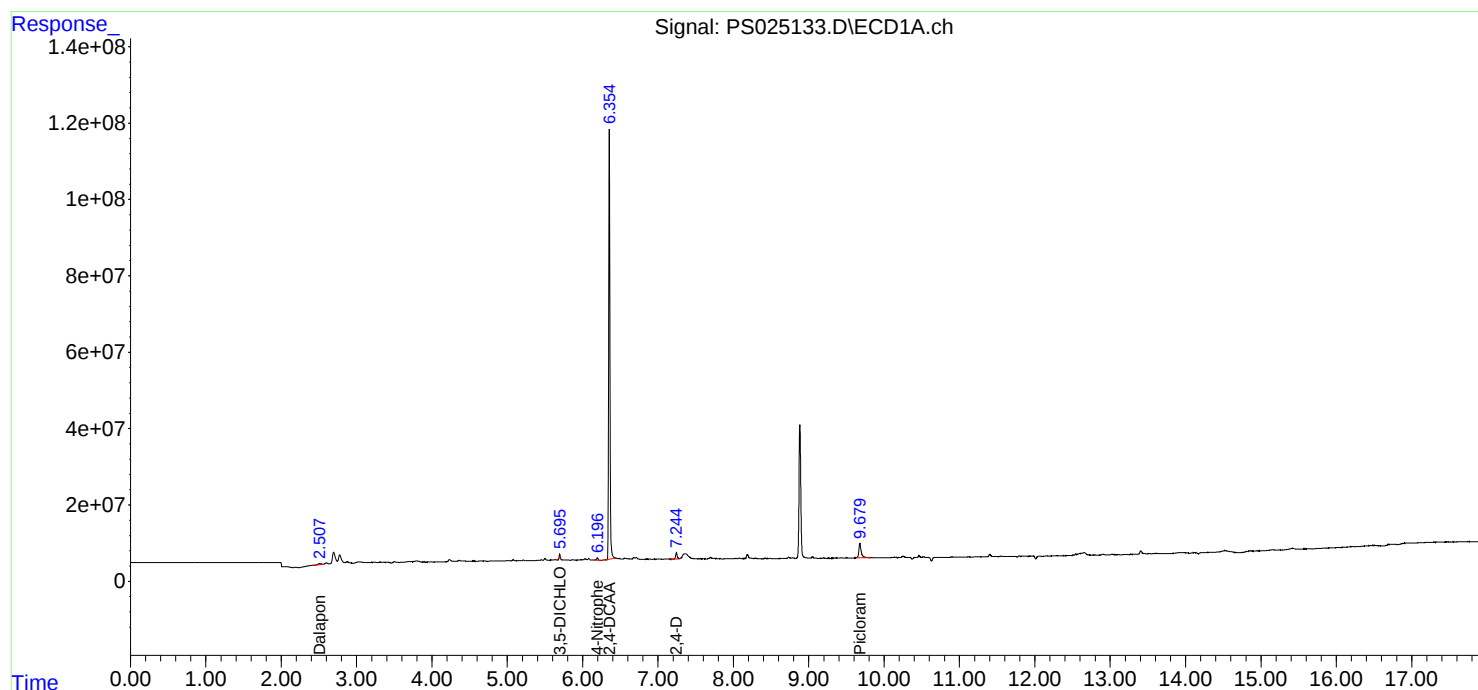


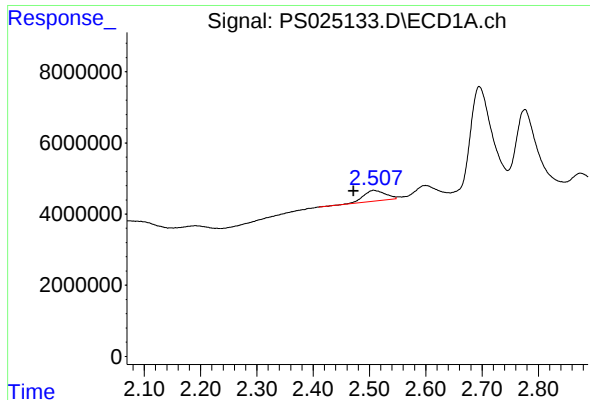

#1 Dalapon


R.T.: 2.508 min
Delta R.T.: 0.036 min
Response: 7992226
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

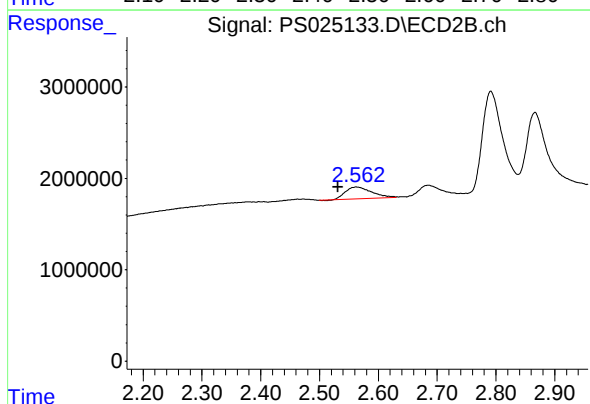


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.031 min
Response: 3977912
Conc: 3.47 ng/ml

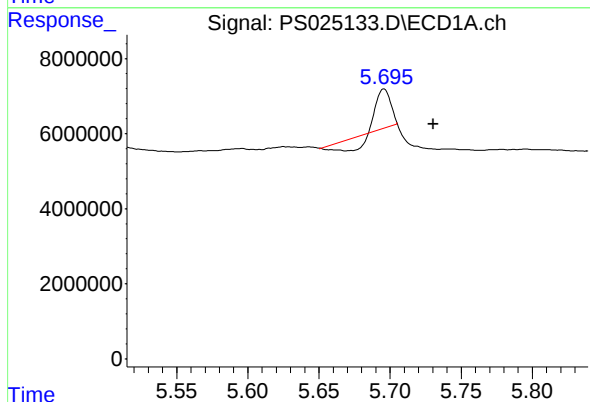


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.696 min
Delta R.T.: -0.035 min
Response: 4049807
Conc: 1.20 ng/ml

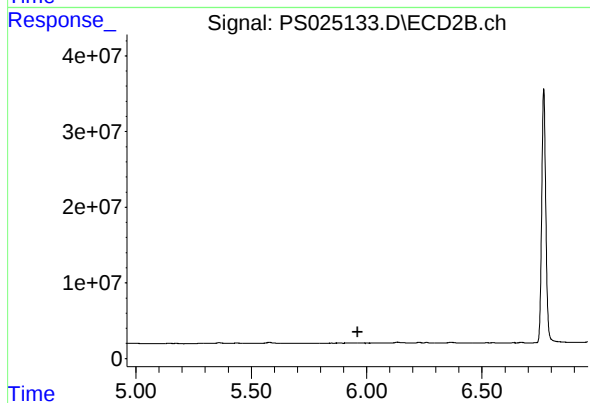

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

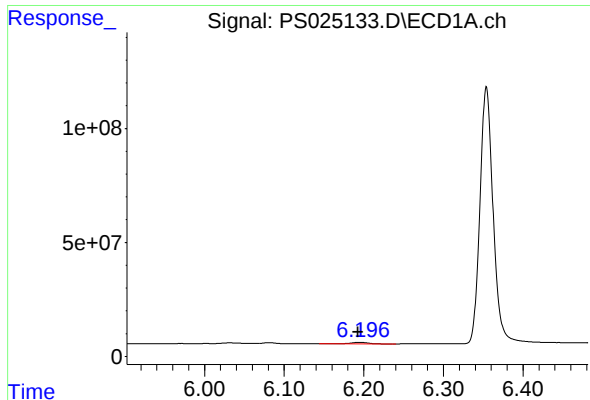

#3 4-Nitrophenol


R.T.: 6.195 min
Delta R.T.: 0.002 min
Response: 9238755
Conc: 6.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

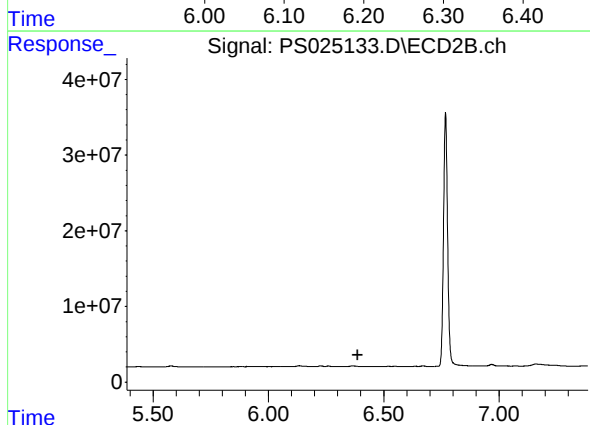


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

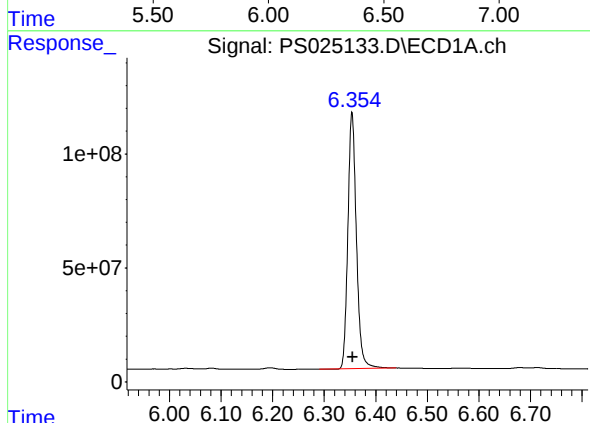


#4 2,4-DCAA

R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 1291782849
Conc: 577.24 ng/ml

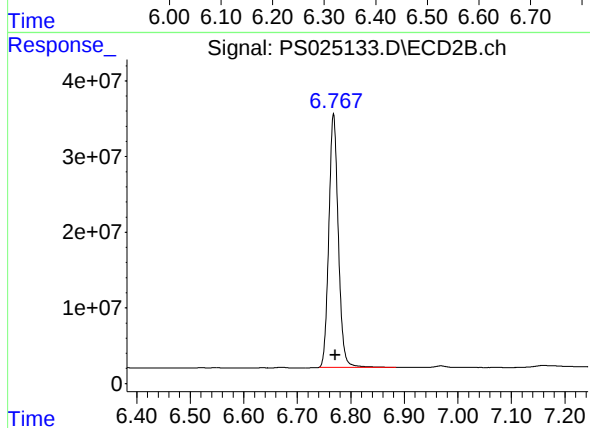

#4 2,4-DCAA


R.T.: 6.768 min
Delta R.T.: -0.003 min
Response: 411051591
Conc: 567.32 ng/ml

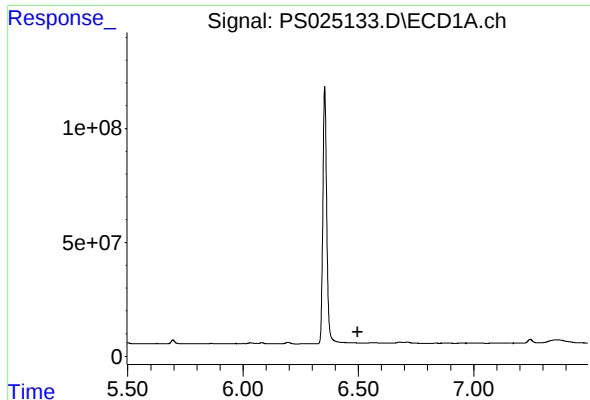

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

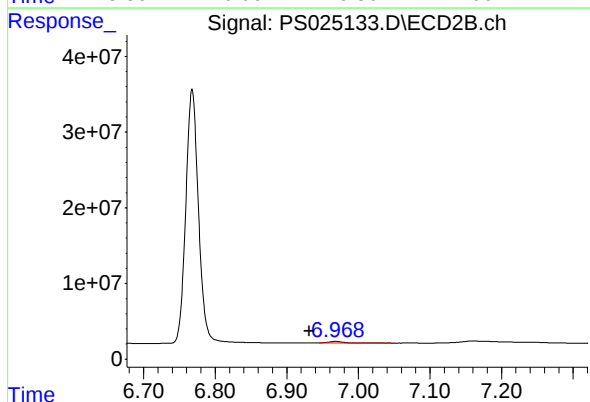


#5 DICAMBA

R.T.: 6.968 min
Delta R.T.: 0.036 min
Response: 3224081
Conc: 1.04 ng/ml

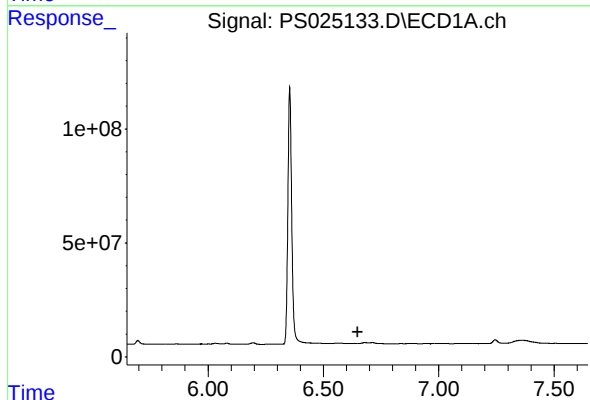


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.648 min
Response: 0
Conc: N.D.

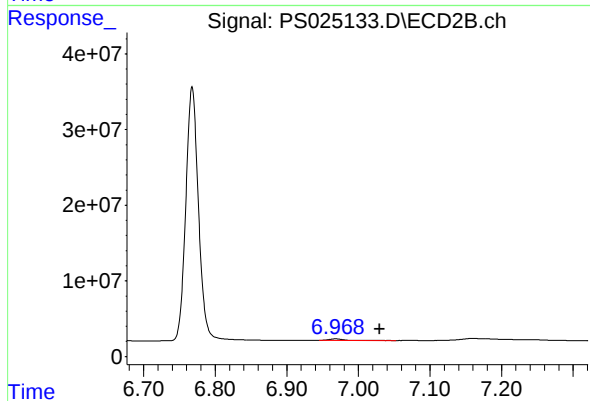

#6 MCPP


R.T.: 6.968 min
Delta R.T.: -0.061 min
Response: 3224081
Conc: 1.55 ug/ml

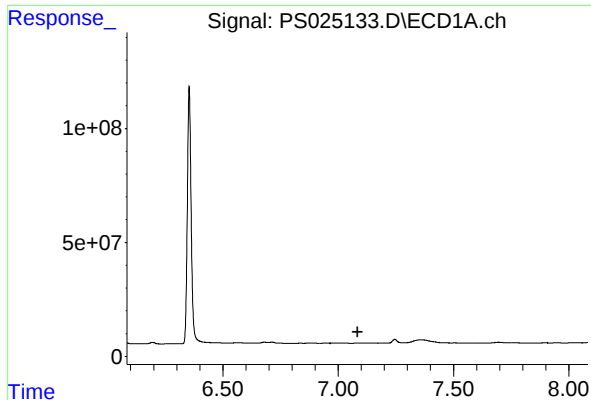

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

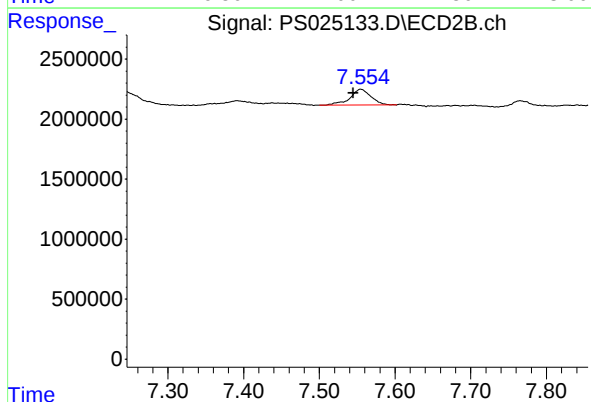


#8 DICHLORPROP

R.T.: 7.555 min
Delta R.T.: 0.010 min
Response: 2528612
Conc: 3.21 ng/ml

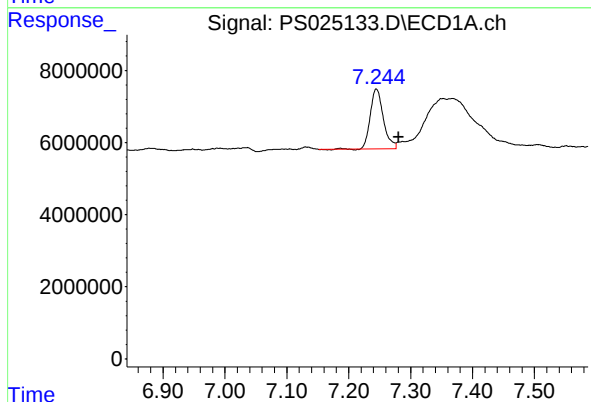


#9 2,4-D

R.T.: 7.245 min
Delta R.T.: -0.036 min
Response: 24190004
Conc: 7.96 ng/ml

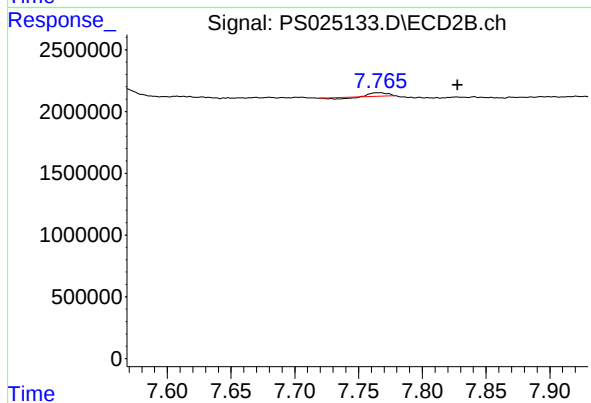

#9 2,4-D


R.T.: 7.766 min
Delta R.T.: -0.062 min
Response: 207549
Conc: N.D.

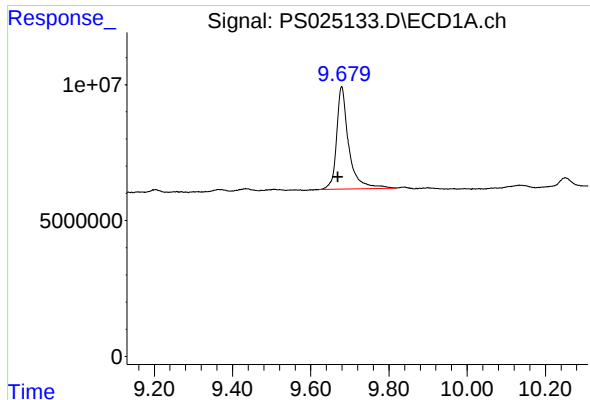

#15 Picloram


R.T.: 9.679 min
Delta R.T.: 0.009 min
Response: 81813374
Conc: 4.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

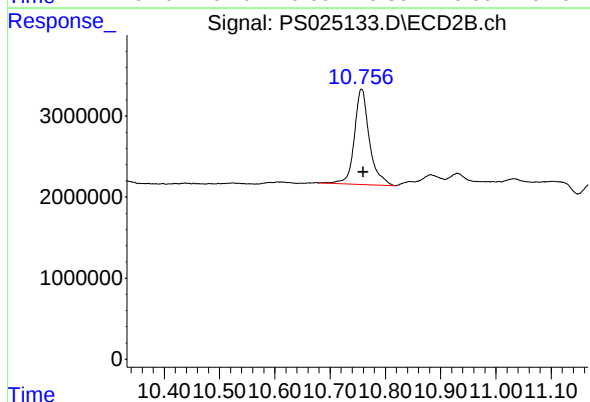


#15 Picloram

R.T.: 10.757 min
Delta R.T.: -0.003 min
Response: 22149470
Conc: 3.38 ng/ml

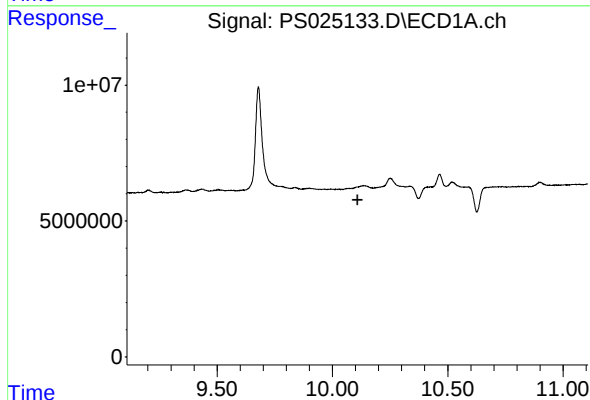

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

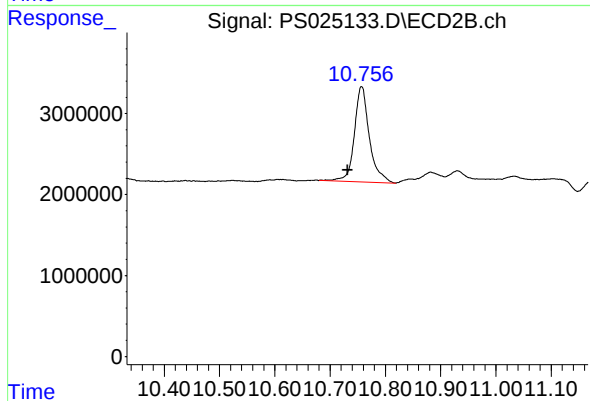

#16 DCPA

R.T.: 10.757 min
Delta R.T.: 0.025 min
Response: 22149470
Conc: 4.09 ng/ml