

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121723\
 Data File : PS025136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 13:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:54:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.356	6.766	1168.8E6	363.5E6	522.295	501.629
Target Compounds							
1) T	Dalapon	2.509	2.557	8594648	3677248	2.980	3.206
3) T	4-Nitroph...	6.199	0.000	6234174	0	4.233	N.D. #
7) T	MCPA	6.794	0.000	5969803	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.554	0	1377229	N.D.	1.751
9) T	2,4-D	0.000	7.762f	0	249653	N.D.	<MDL
10) T	Pentachlo...	0.000	8.242	0	969904	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.602	0	866455	N.D.	<MDL
12) T	2,4,5-T	8.299	8.973	2109771	851617	<MDL	<MDL #
14) T	DINOSEB	0.000	9.860f	0	872291	N.D.	<MDL
15) T	Picloram	9.686	10.756	64226355	18114794	3.296	2.768
16) T	DCPA	0.000	10.756	0	18114794	N.D.	3.342



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121723\
Data File : PS025136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 13:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:54:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

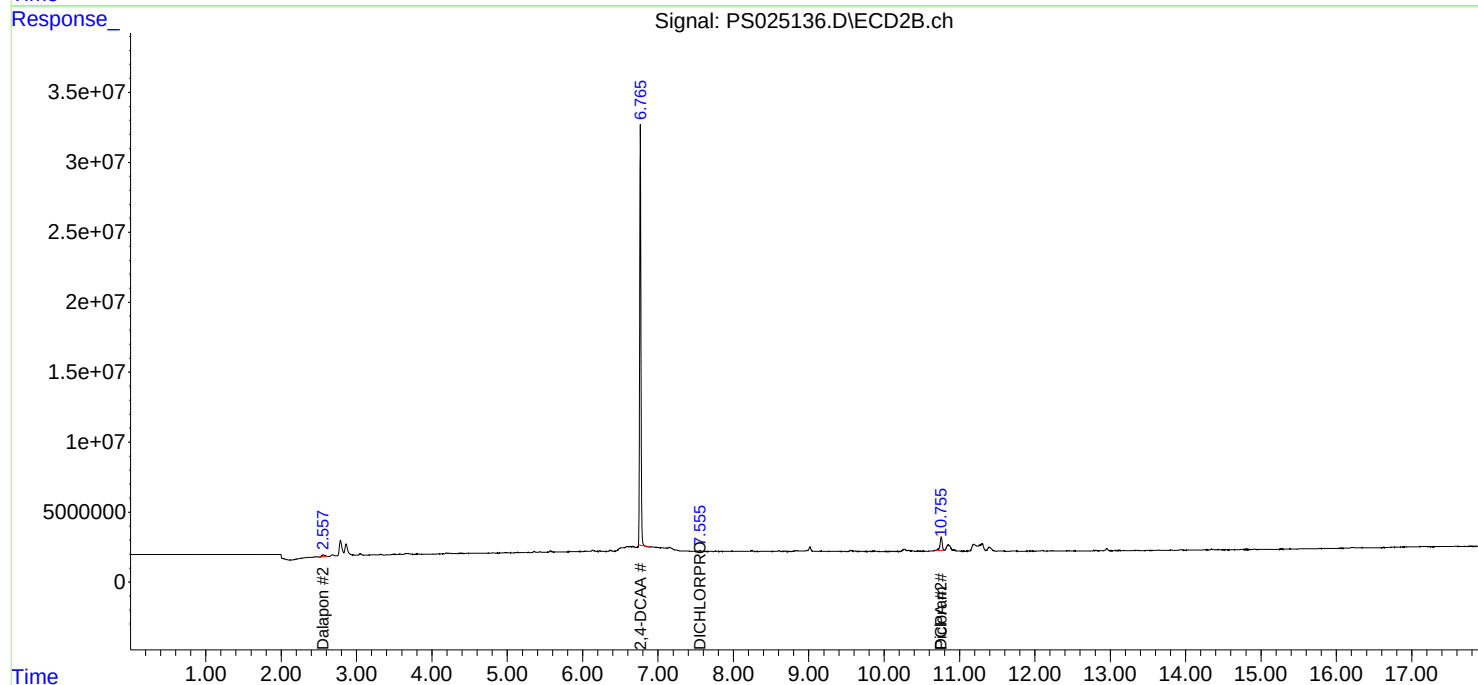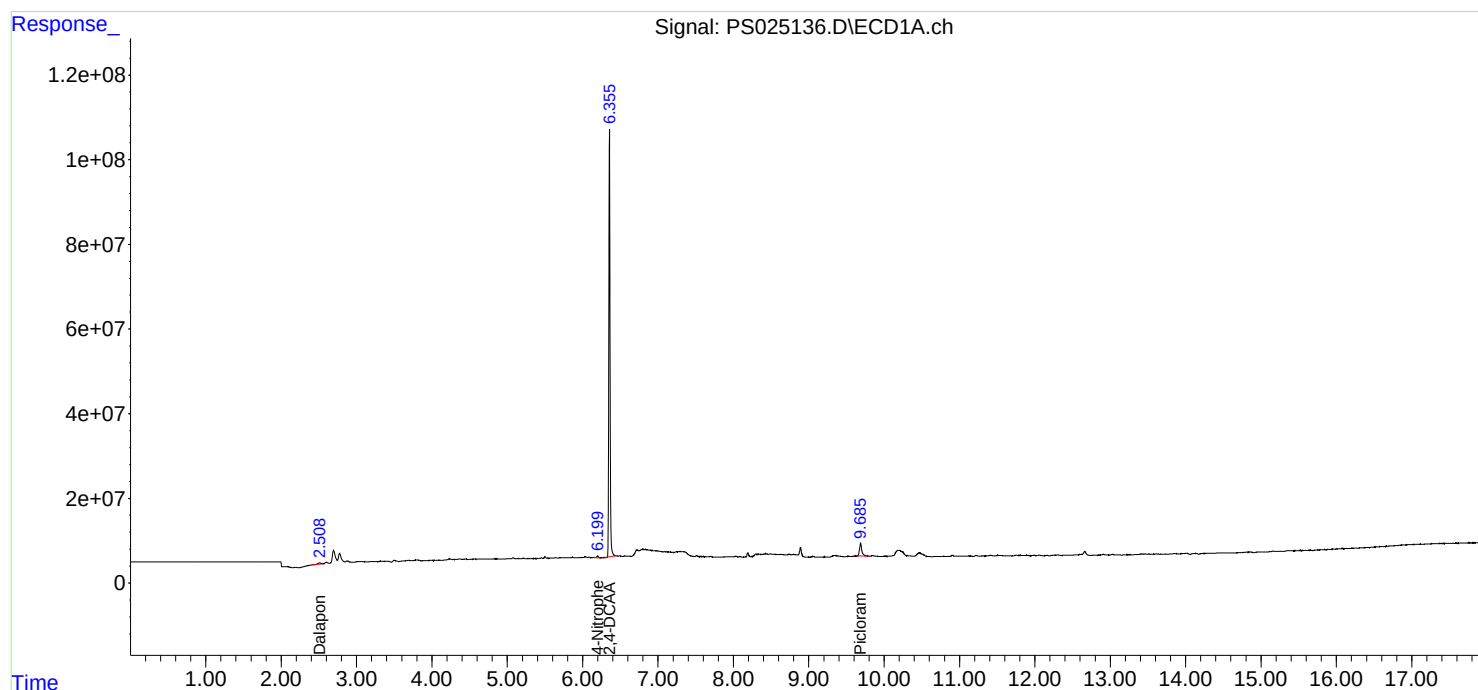


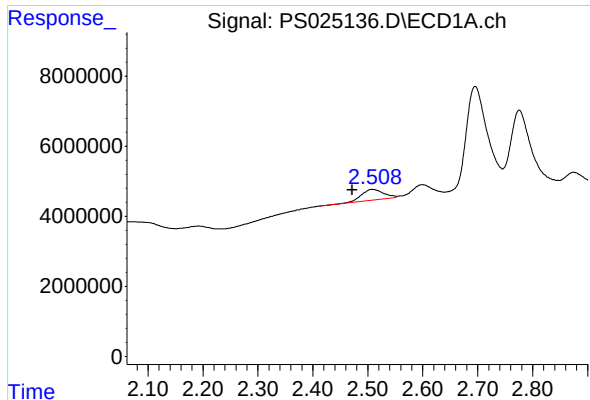

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 8594648
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

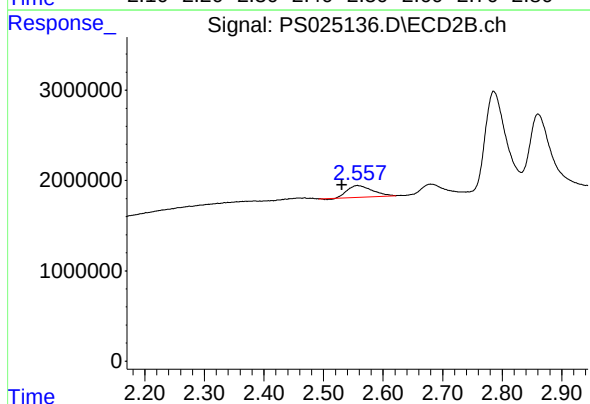


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: 0.026 min
Response: 3677248
Conc: 3.21 ng/ml

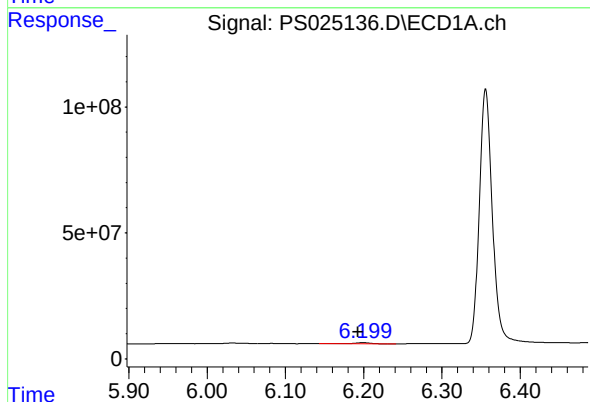


#3 4-Nitrophenol

R.T.: 6.199 min
Delta R.T.: 0.006 min
Response: 6234174
Conc: 4.23 ng/ml

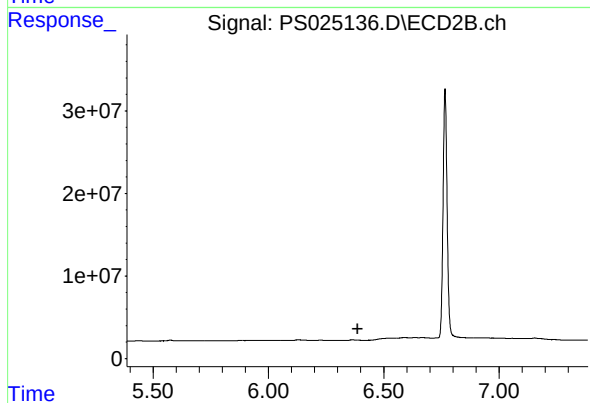

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

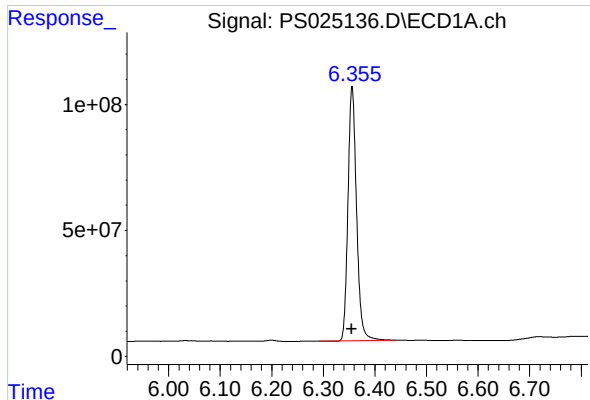

#4 2,4-DCAA


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 1168815602
Conc: 522.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

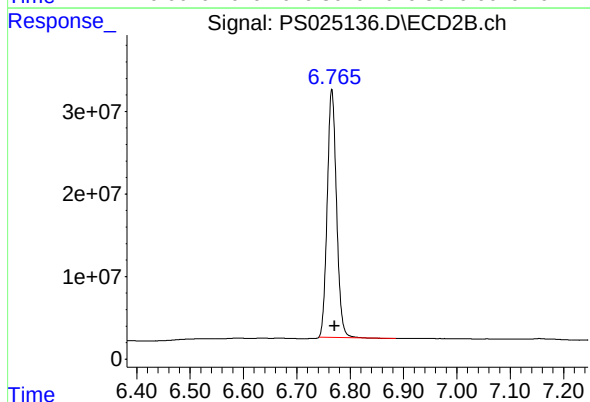


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.006 min
Response: 363457309
Conc: 501.63 ng/ml

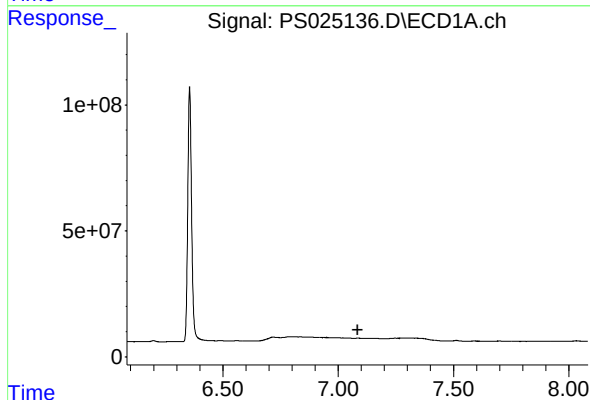


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

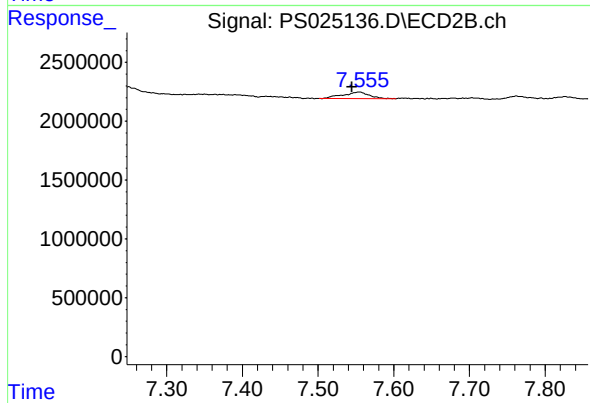

#8 DICHLORPROP


R.T.: 7.554 min
Delta R.T.: 0.009 min
Response: 1377229
Conc: 1.75 ng/ml

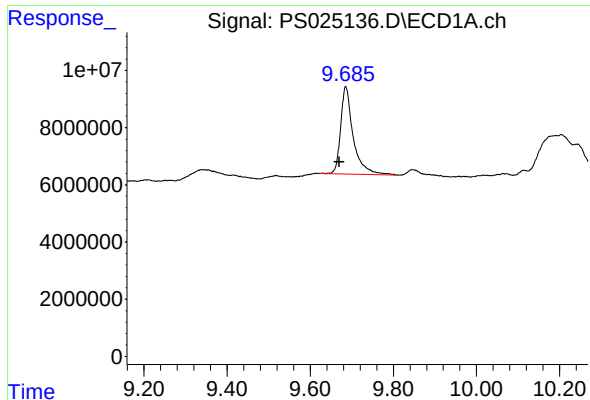

#15 Picloram


R.T.: 9.686 min
Delta R.T.: 0.016 min
Response: 64226355
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

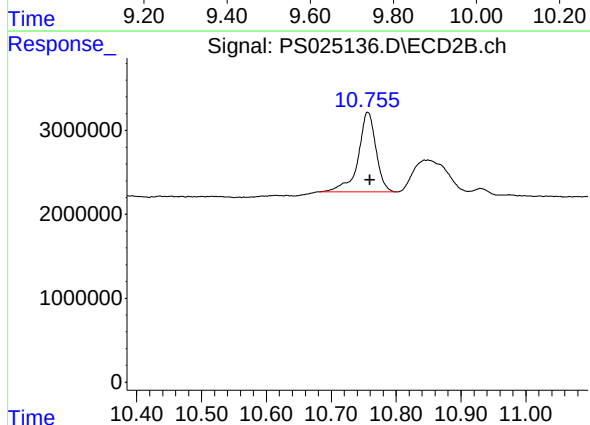


#15 Picloram

R.T.: 10.756 min
Delta R.T.: -0.004 min
Response: 18114794
Conc: 2.77 ng/ml

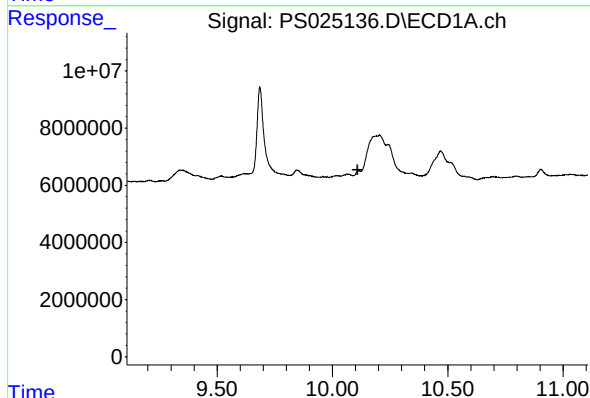

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

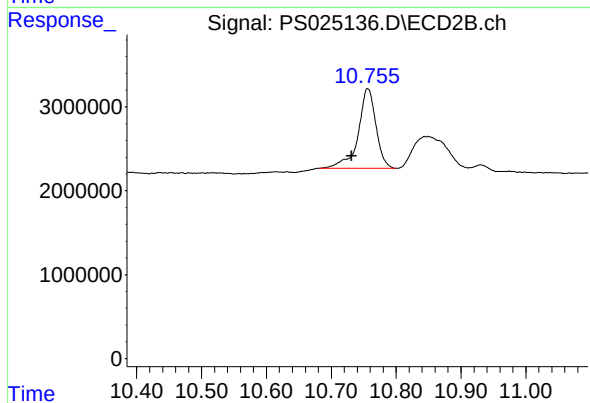

#16 DCPA

R.T.: 10.756 min
Delta R.T.: 0.025 min
Response: 18114794
Conc: 3.34 ng/ml