

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS121819\  
 Data File : PS008067.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Dec 2019 08:42  
 Operator : SM\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 18 11:16:05 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS121819.M  
 Quant Title : 8080.M  
 QLast Update : Wed Dec 18 11:09:54 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |          |       |       |            |      |        |
|------------------|----------|-------|-------|------------|------|--------|
| 7) T             | MCPA     | 0.000 | 5.483 | 0 48014301 | N.D. | 16.078 |
| 15) T            | Picloram | 0.000 | 8.926 | 0 31934237 | N.D. | 5.306  |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS121819\  
Data File : PS008067.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2019 08:42  
Operator : SM\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampled :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 18 11:16:05 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS121819.M  
Quant Title : 8080.M  
QLast Update : Wed Dec 18 11:09:54 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

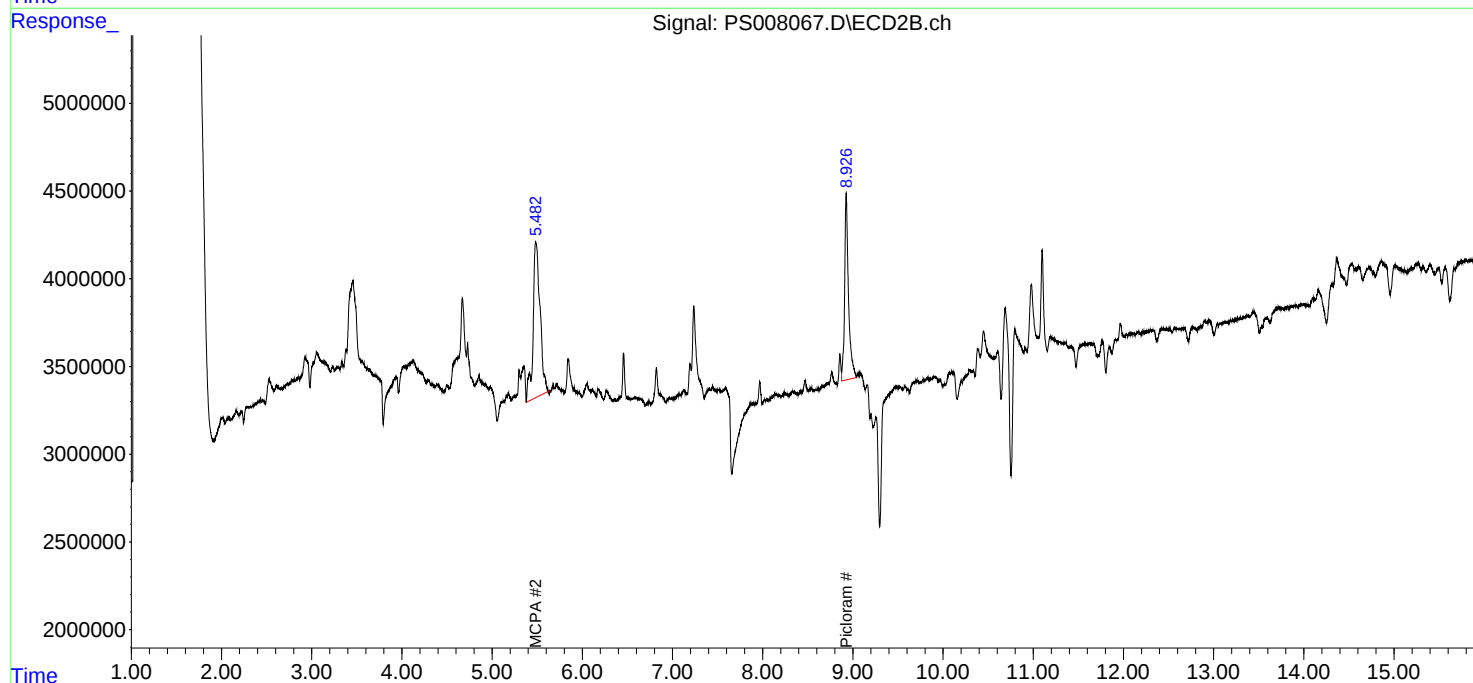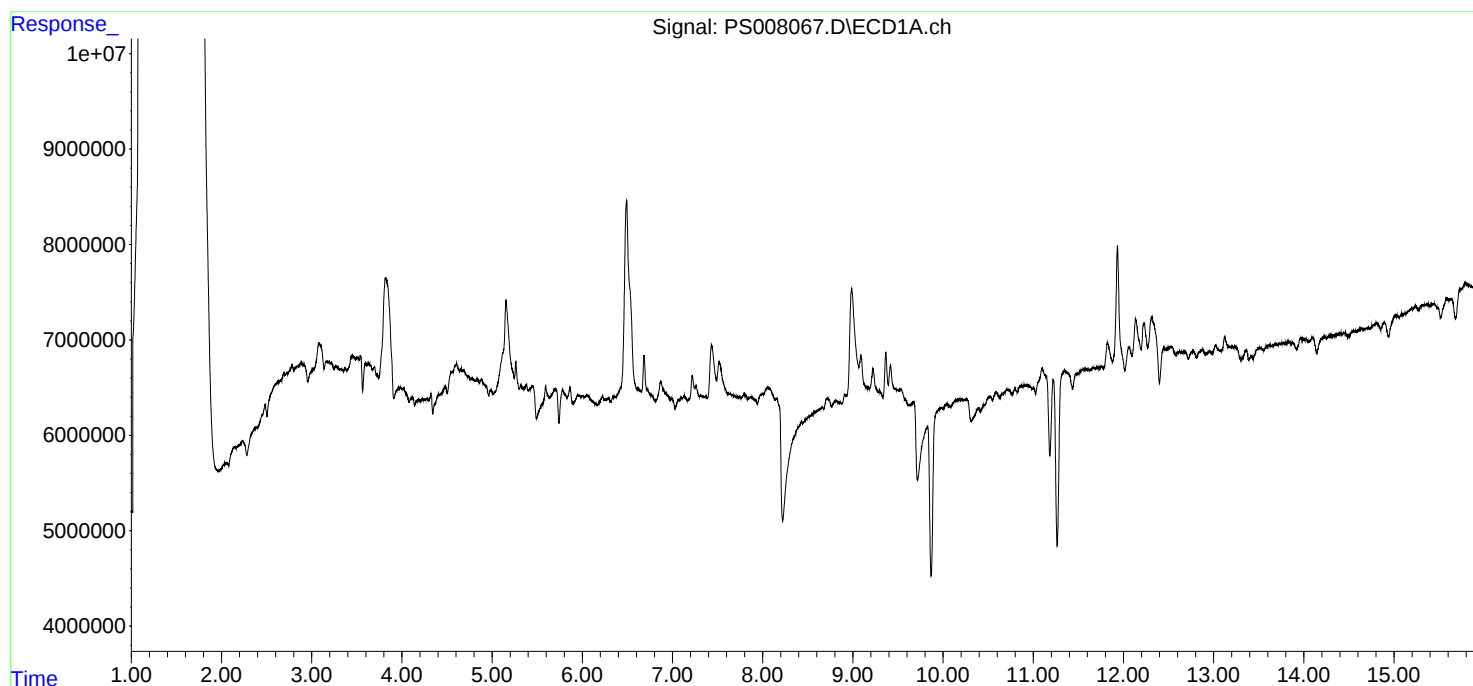


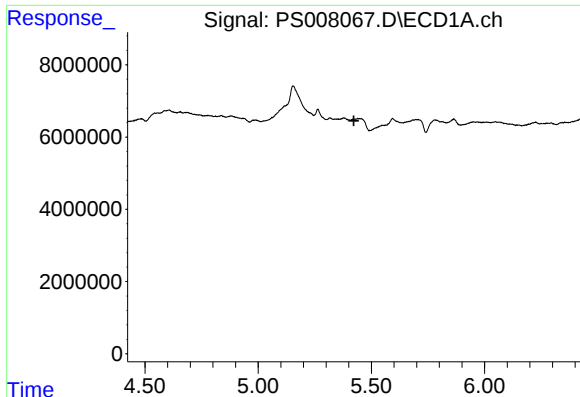

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T. : 5.423 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

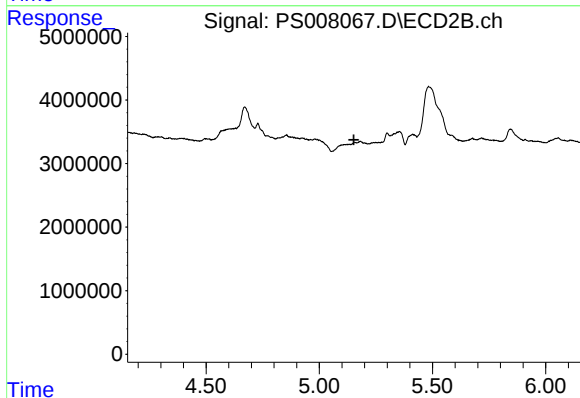


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 5.153 min  
Response: 0  
Conc: N.D.

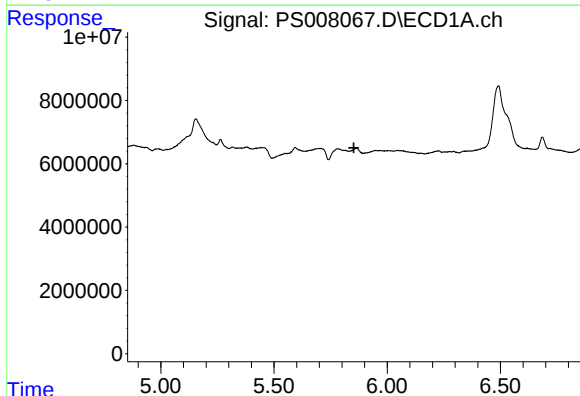


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 5.853 min  
Response: 0  
Conc: N.D.

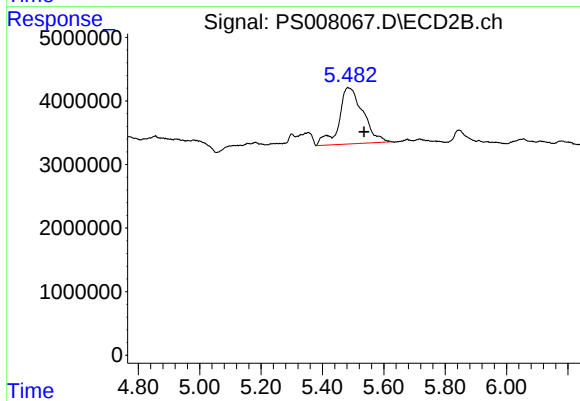

#7 MCPA


R.T.: 5.483 min  
Delta R.T.: -0.053 min  
Response: 48014301  
Conc: 16.08 ug/ml

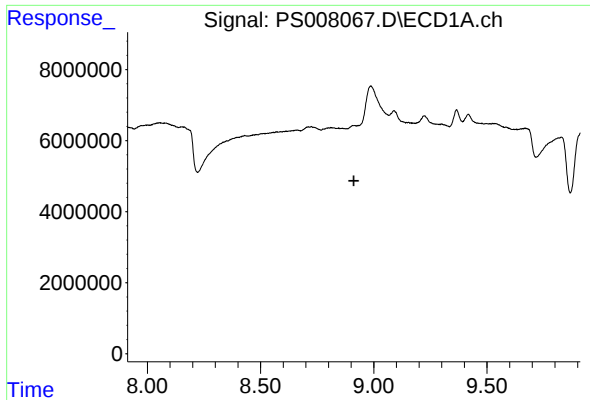

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 8.912 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

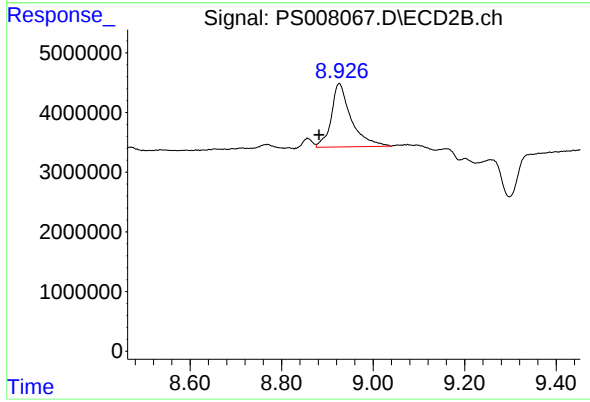

#15 Picloram

R.T.: 8.926 min  
Delta R.T.: 0.044 min  
Response: 31934237  
Conc: 5.31 ng/ml