

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121819\
 Data File : PS008068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 09:04
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 11:16:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.425	5.154	657.6E6	326.3E6	438.940	444.567
Target Compounds							
7) T	MCPA	0.000	5.477	0	41873801	N.D.	14.022
9) T	2,4-D	6.474	0.000	85055707	0	56.452	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121819\
Data File : PS008068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 09:04
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 11:16:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

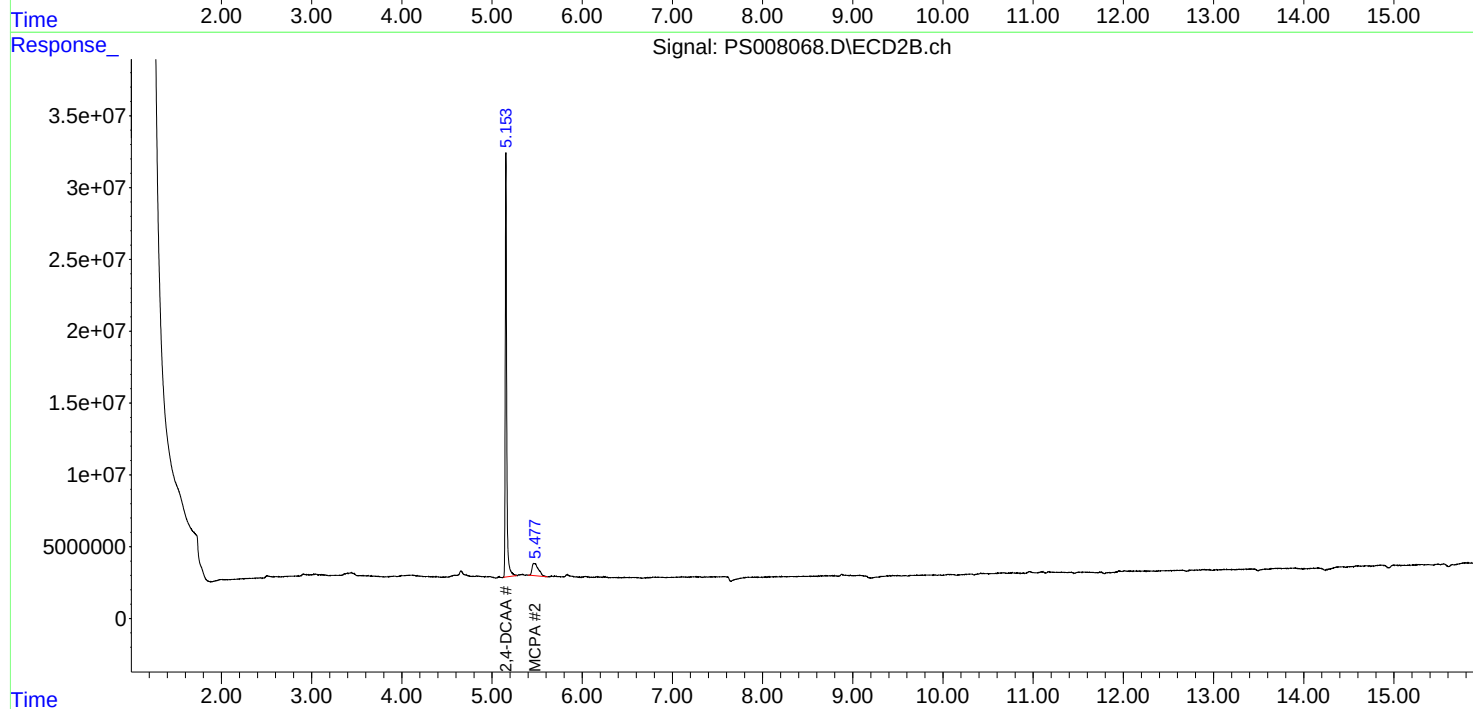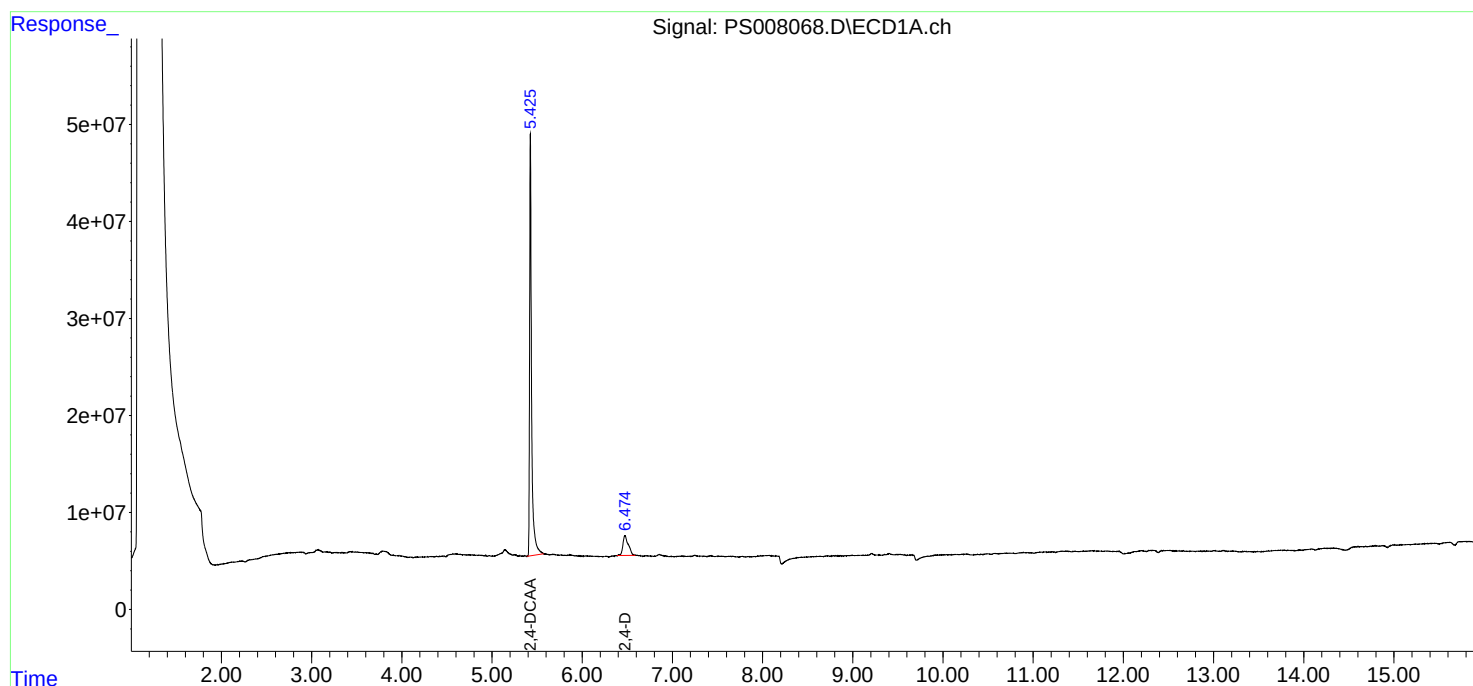


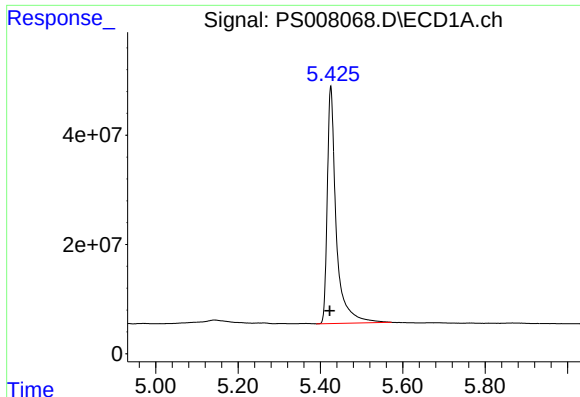

#4 2,4-DCAA


R.T.: 5.425 min
Delta R.T.: 0.003 min
Response: 657579697
Conc: 438.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

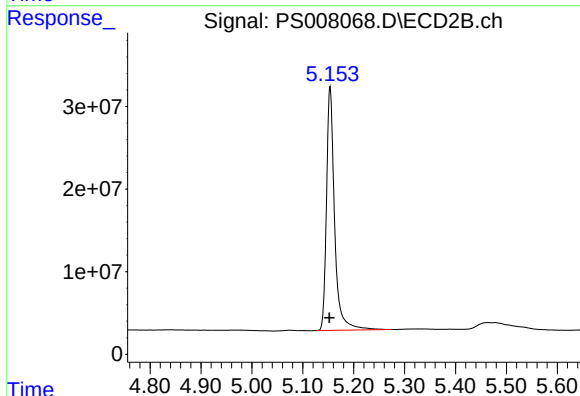


#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.001 min
Response: 326282839
Conc: 444.57 ng/ml

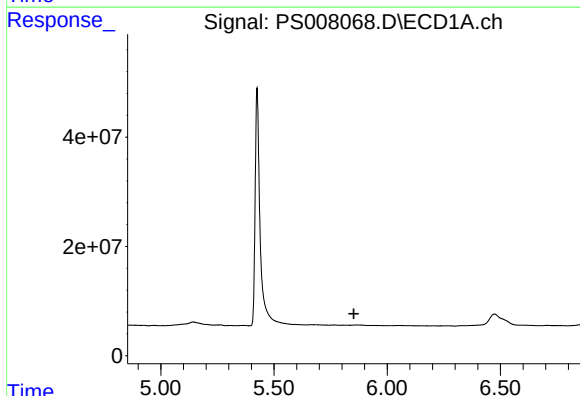


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.853 min
Response: 0
Conc: N.D.

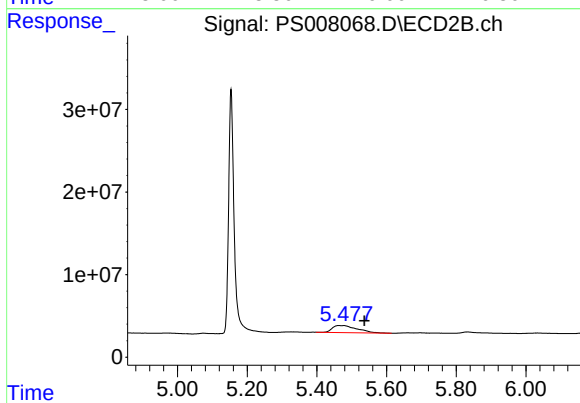

#7 MCPA


R.T.: 5.477 min
Delta R.T.: -0.059 min
Response: 41873801
Conc: 14.02 ug/ml

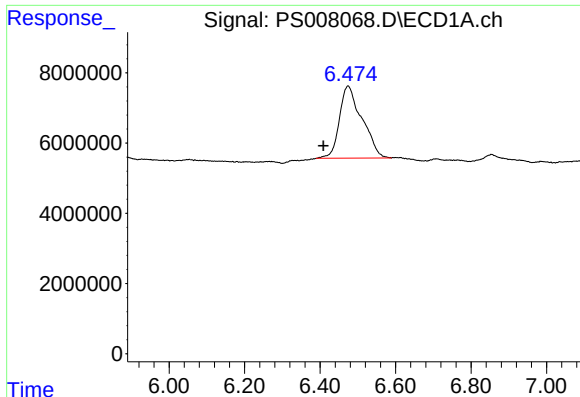

#9 2,4-D

R.T.: 6.474 min
Delta R.T.: 0.065 min
Response: 85055707
Conc: 56.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

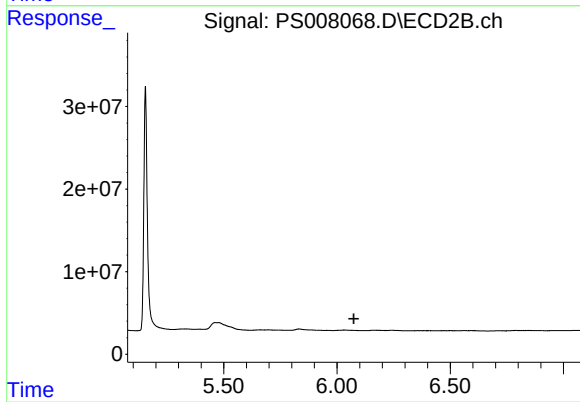

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.075 min
Response: 0
Conc: N.D.