

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121922\
 Data File : PS021457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 08:50
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 20:17:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.397	0.000	856860	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.513	0.000	1024743	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.752	0.000	485962	0	<MDL	N.D. #
3) T	4-Nitroph...	6.219	0.000	2164432	0	1.204	N.D. #
5) T	DICAMBA	6.513	0.000	928842	0	<MDL	N.D. #
6) T	MCPD	6.644	7.049	-23615	1287899	N.D.	<MDL
7) T	MCPA	6.820	0.000	573272	0	<MDL	N.D. #
8) T	DICHLORPROP	7.121	7.620	1542743	672646	<MDL	<MDL #
9) T	2,4-D	7.333	0.000	3984026	0	1.043	N.D. #
10) T	Pentachlo...	7.551	8.318	1477210	653350	<MDL	<MDL #
11) T	2,4,5-TP ...	8.085	8.678	1486885	881692	<MDL	<MDL #
12) T	2,4,5-T	8.353	9.060	2377373	4490212	<MDL	<MDL #
13) T	2,4-DB	8.868	9.581	544959	189859	<MDL	<MDL #
14) T	DINOSEB	9.895	0.000	1872025	0	<MDL	N.D. #
15) T	Picloram	9.761	10.870	50771571	28651047	1.773	1.762
16) T	DCPA	10.173	10.814	693866	2053875	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121922\
Data File : PS021457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 08:50
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 20:17:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

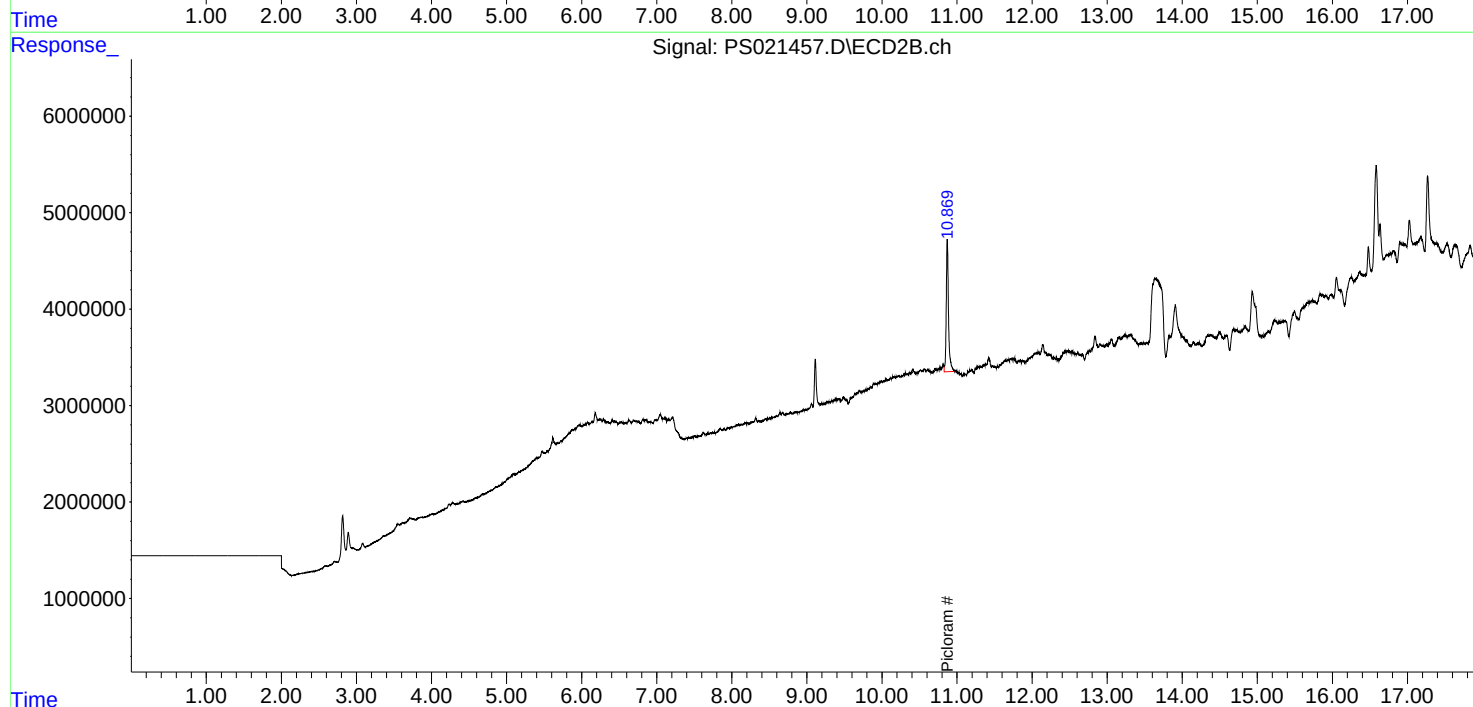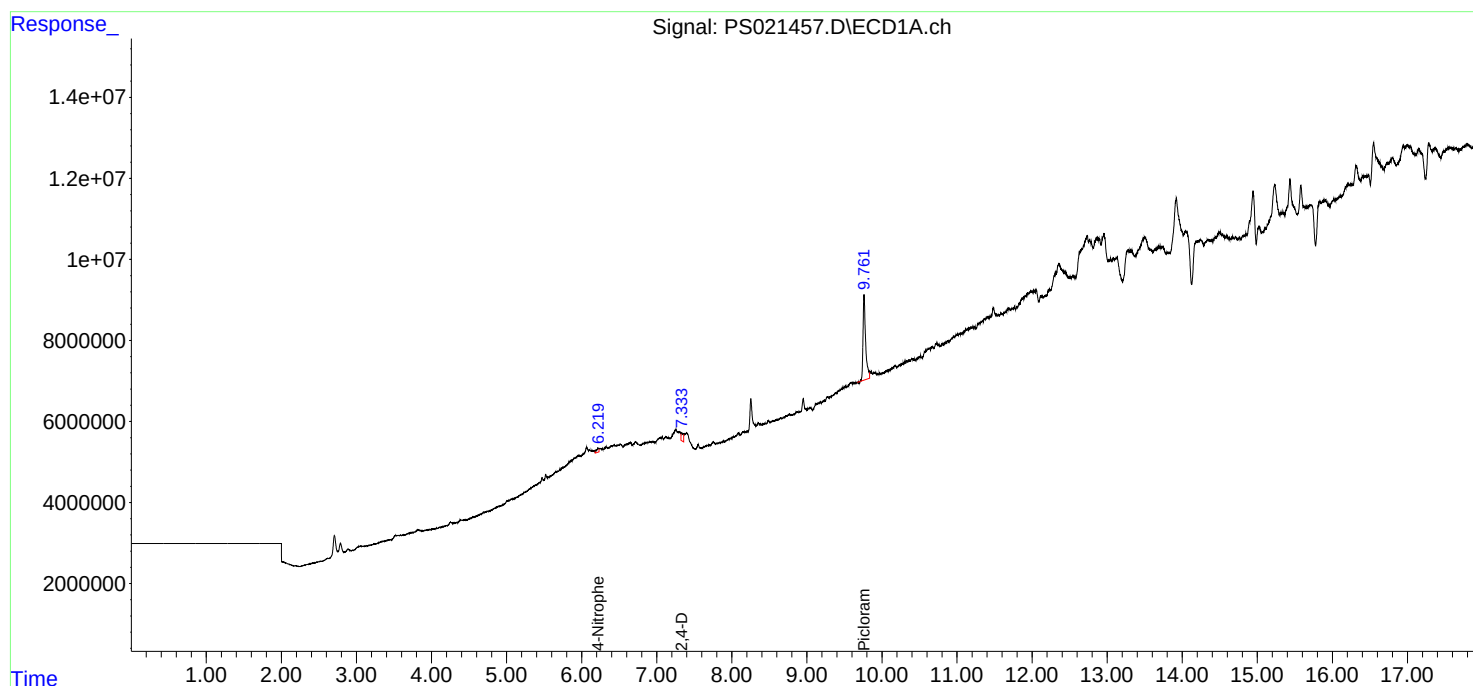


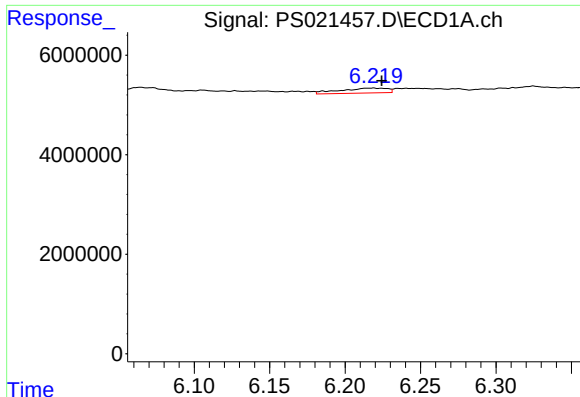

#3 4-Nitrophenol


R.T.: 6.219 min
Delta R.T.: -0.006 min
Response: 2164432
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

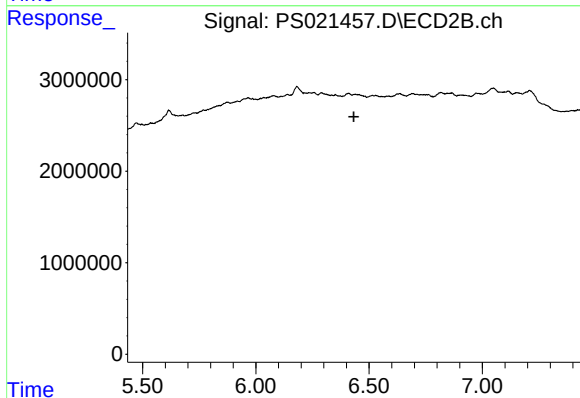


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

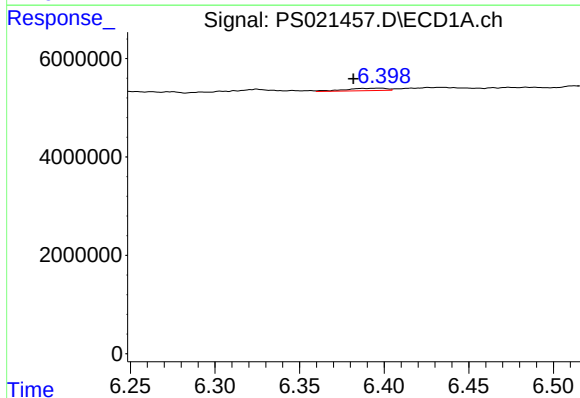


#4 2,4-DCAA

R.T.: 6.397 min
Delta R.T.: 0.015 min
Response: 856860
Conc: N.D.

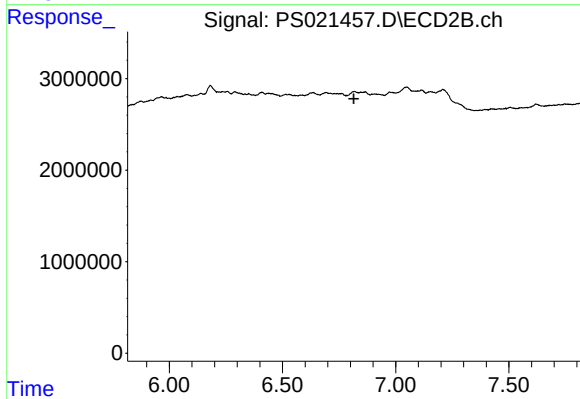

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

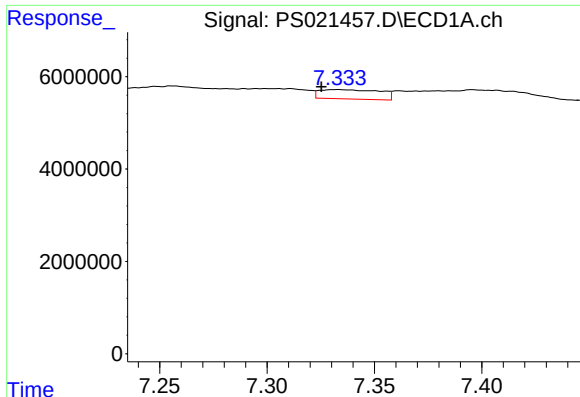

#9 2,4-D


R.T.: 7.333 min
Delta R.T.: 0.008 min
Response: 3984026
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

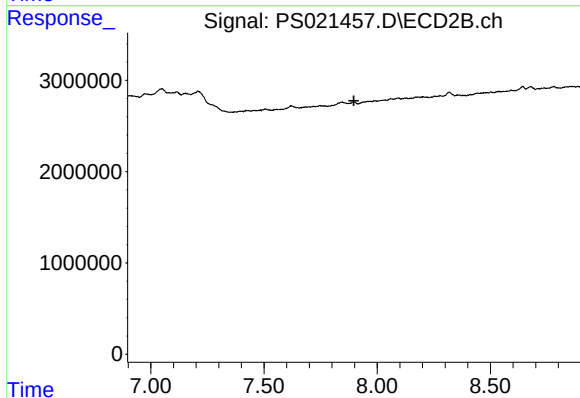


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

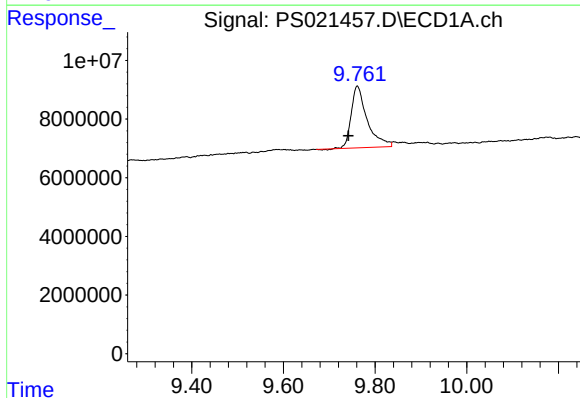

#15 Picloram

R.T.: 9.761 min
Delta R.T.: 0.019 min
Response: 50771571
Conc: 1.77 ng/ml

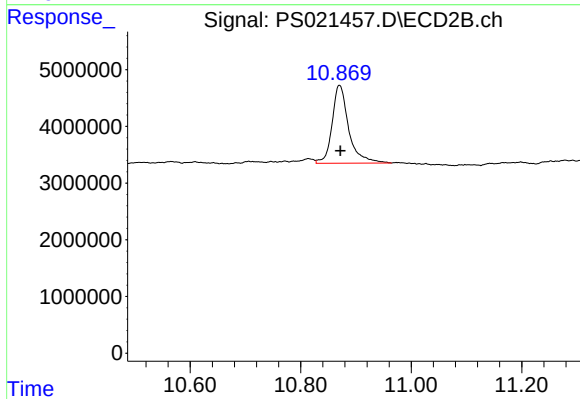

#15 Picloram

R.T.: 10.870 min
Delta R.T.: -0.002 min
Response: 28651047
Conc: 1.76 ng/ml