

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121922\
 Data File : PS021458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 09:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 20:18:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.811	1303.4E6	893.9E6	448.613	518.498
Target Compounds							
1) T	Dalapon	2.537f	0.000	174809	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.743	0.000	1317611	0	<MDL	N.D. #
3) T	4-Nitroph...	6.226	0.000	4999677	0	2.781	N.D. #
6) T	MCP	0.000	7.122f	0	364301	N.D.	<MDL
7) T	MCPA	6.759	7.219f	908221	14930603	<MDL	1.688 #
10) T	Pentachlo...	7.549	0.000	683822	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.088	0.000	2762089	0	<MDL	N.D. #
12) T	2,4,5-T	8.323	0.000	16291689	0	<MDL	N.D. #
13) T	2,4-DB	8.845	9.638f	1883032	1723449	<MDL	1.199 #
15) T	Picloram	9.761	10.902	1356952	27129982	<MDL	1.668 #
16) T	DCPA	10.165	0.000	339491	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121922\
Data File : PS021458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 09:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 20:18:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

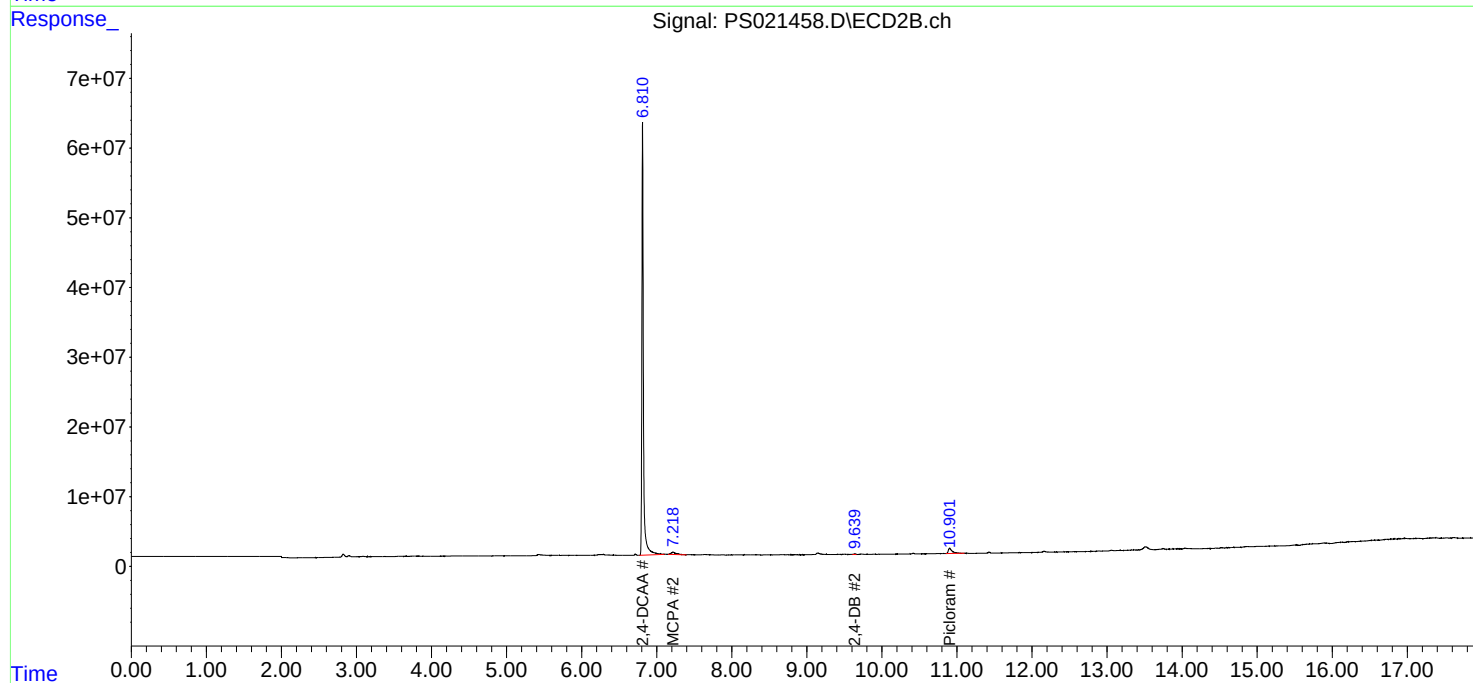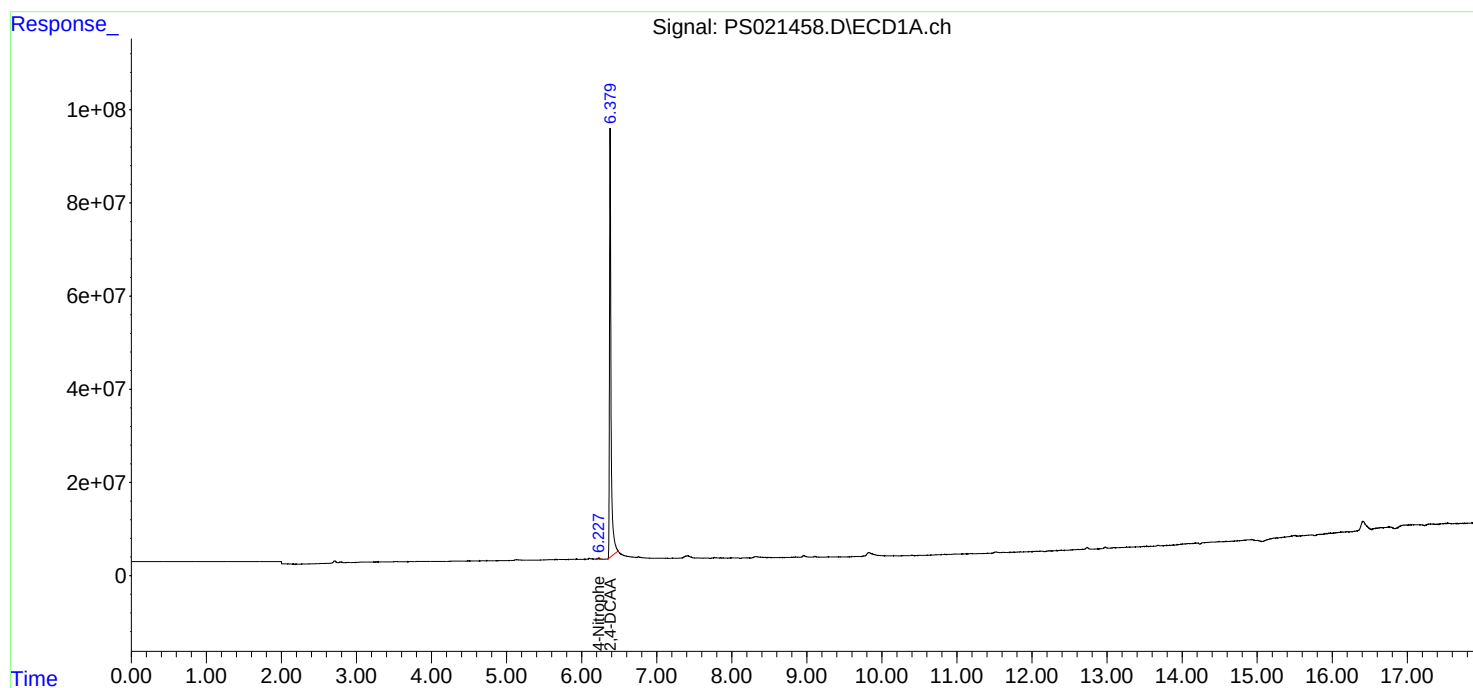


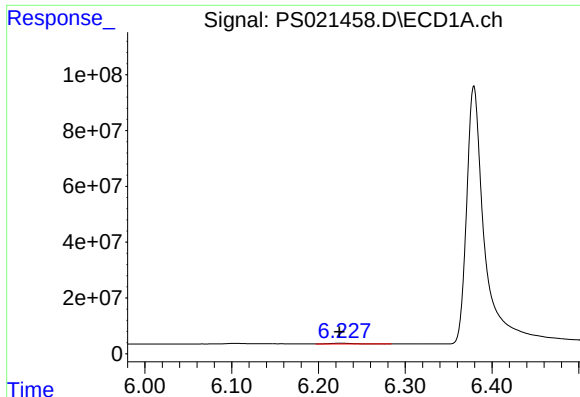

#3 4-Nitrophenol


R.T.: 6.226 min
Delta R.T.: 0.002 min
Response: 4999677
Conc: 2.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

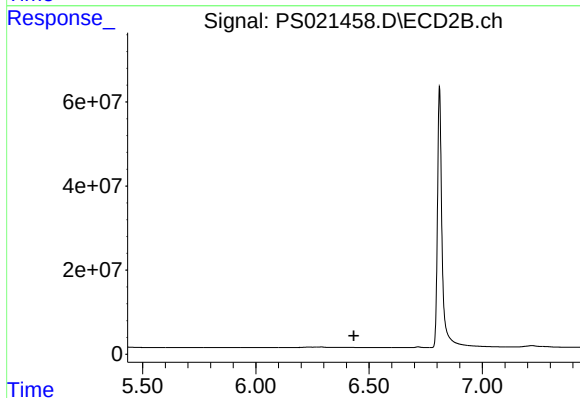


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

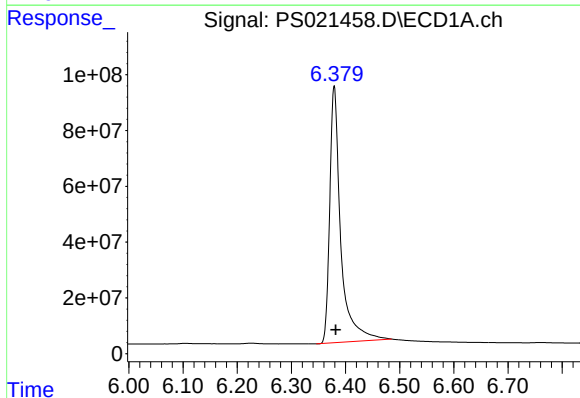


#4 2,4-DCAA

R.T.: 6.379 min
Delta R.T.: -0.003 min
Response: 1303441611
Conc: 448.61 ng/ml

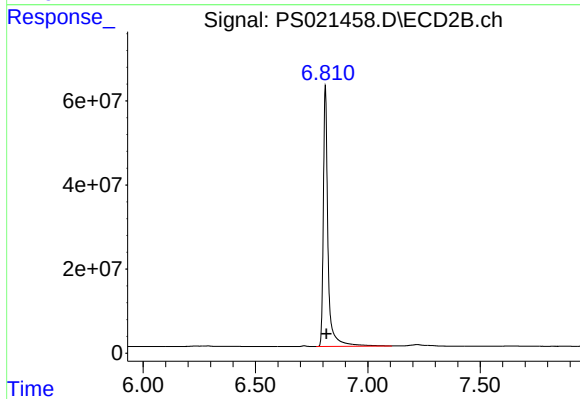

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: -0.005 min
Response: 893886840
Conc: 518.50 ng/ml

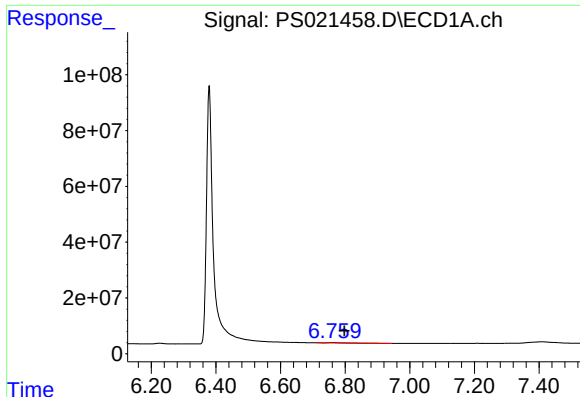

#7 MCPA


R.T.: 6.759 min
Delta R.T.: -0.038 min
Response: 908221
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

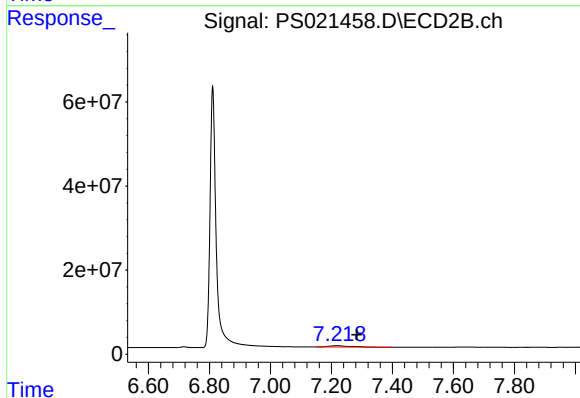


#7 MCPA

R.T.: 7.219 min
Delta R.T.: -0.064 min
Response: 14930603
Conc: 1.69 ug/ml

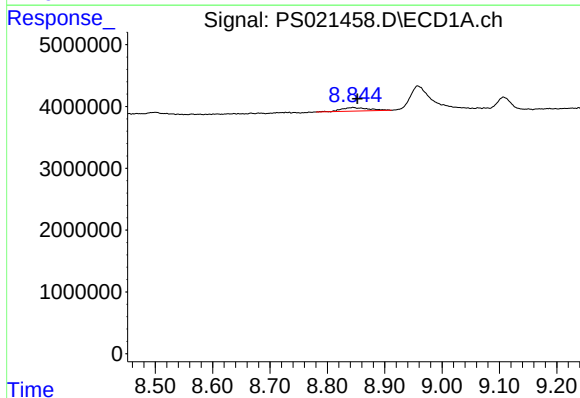


#13 2,4-DB

R.T.: 8.845 min
Delta R.T.: -0.008 min
Response: 1883032
Conc: N.D.

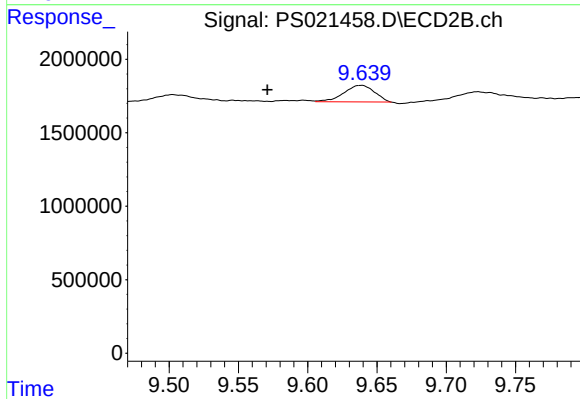

#13 2,4-DB


R.T.: 9.638 min
Delta R.T.: 0.068 min
Response: 1723449
Conc: 1.20 ng/ml

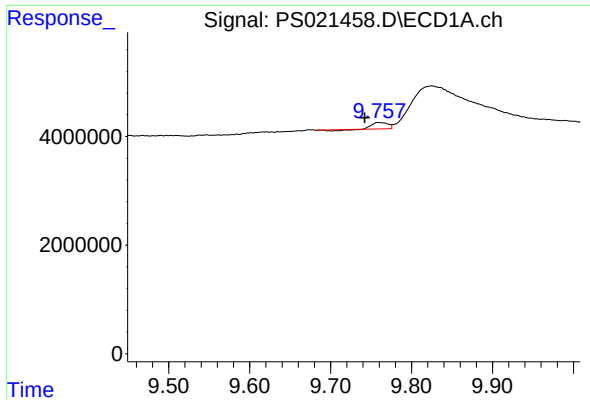

#15 Picloram

R.T.: 9.761 min
Delta R.T.: 0.018 min
Response: 1356952
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

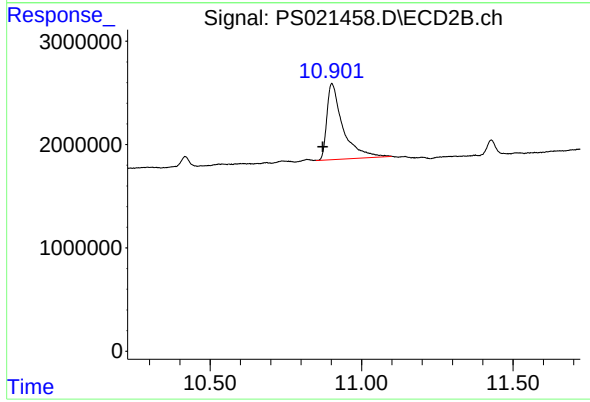

#15 Picloram

R.T.: 10.902 min
Delta R.T.: 0.030 min
Response: 27129982
Conc: 1.67 ng/ml