

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121923\
 Data File : PS025138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 11:06
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 22:22:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.510	2.562	10543950	4022629	3.656	3.507
2) T	3,5-DICHL...	5.697	0.000	30909305	0	9.145	N.D. #
3) T	4-Nitroph...	6.191	0.000	15527670	0	10.544	N.D. #
5) T	DICAMBA	0.000	6.969	0	12896483	N.D.	4.162
6) T	MCP	6.682	6.969f	2990623	12896483	<MDL	6.217 #
7) T	MCPA	0.000	7.232	0	2869986	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.554	0	2970583	N.D.	3.776
9) T	2,4-D	7.246	7.768f	142.4E6	864589	46.878	<MDL #
11) T	2,4,5-TP ...	0.000	8.604	0	413601	N.D.	<MDL
12) T	2,4,5-T	0.000	8.976	0	402650	N.D.	<MDL
15) T	Picloram	9.683	10.759	62016460	25868394	3.183	3.952
16) T	DCPA	0.000	10.759	0	25868394	N.D.	4.773



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121923\
Data File : PS025138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 11:06
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 22:22:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

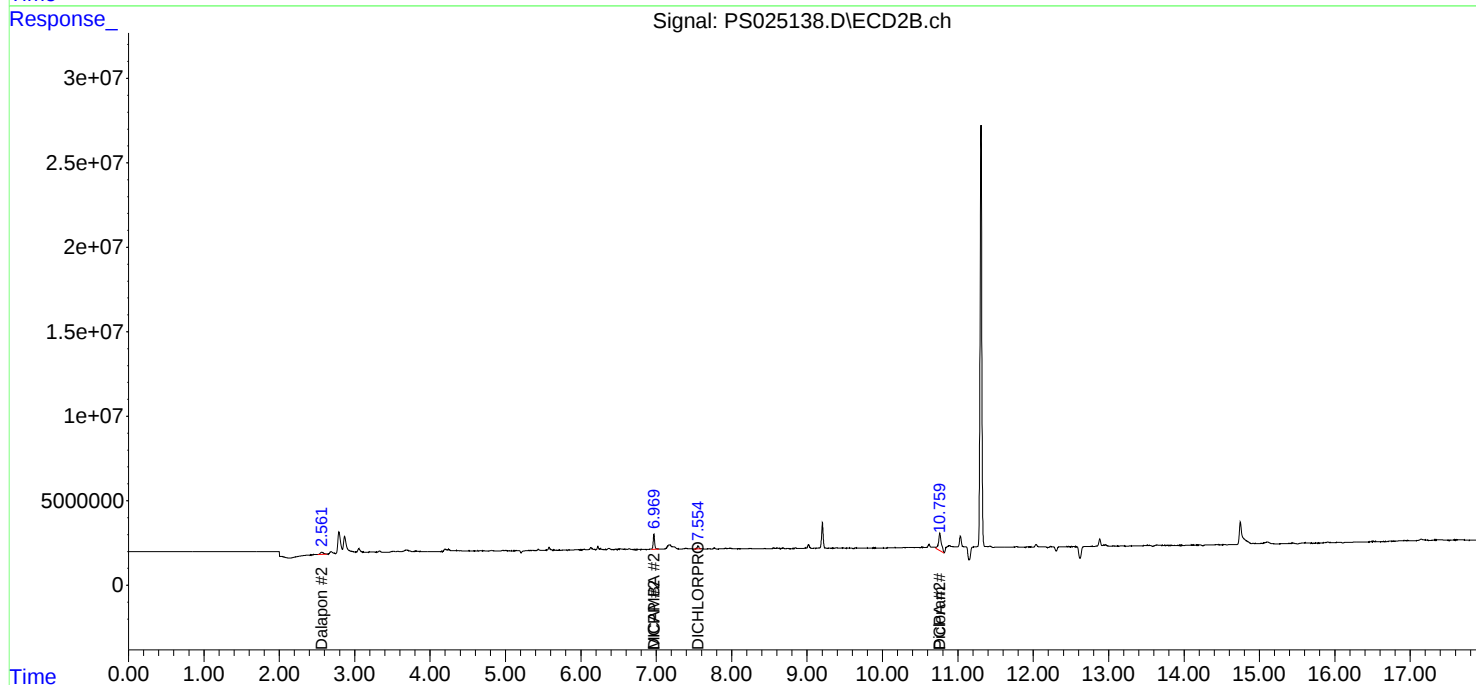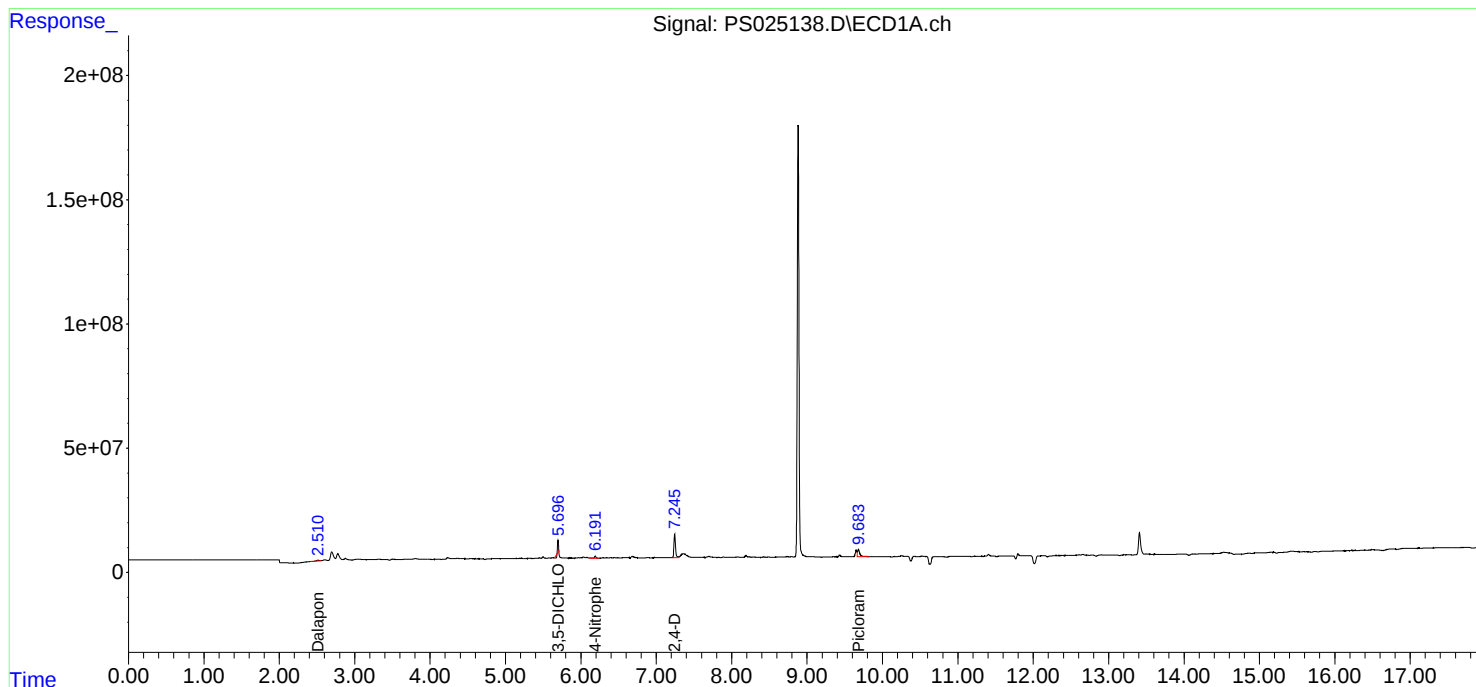


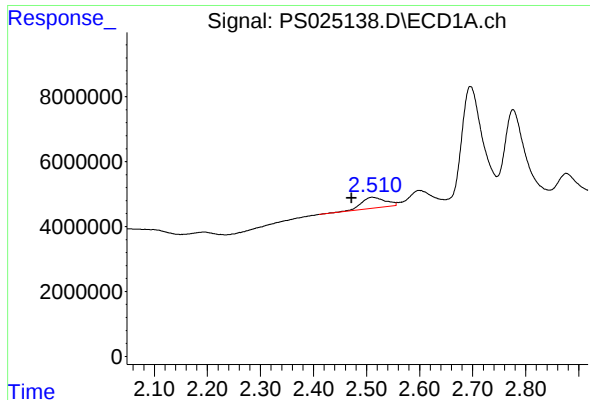

#1 Dalapon


R.T.: 2.510 min
Delta R.T.: 0.038 min
Response: 10543950
Conc: 3.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

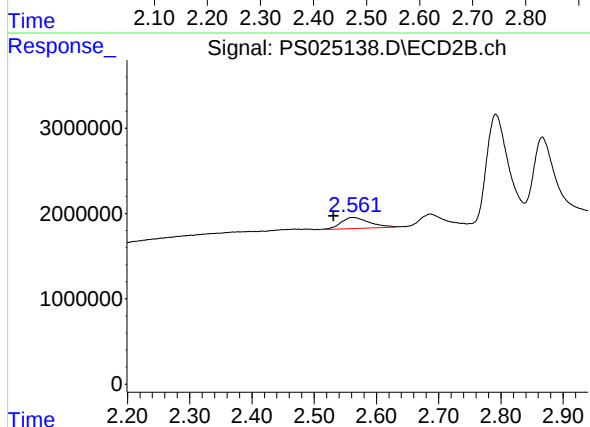


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.031 min
Response: 4022629
Conc: 3.51 ng/ml

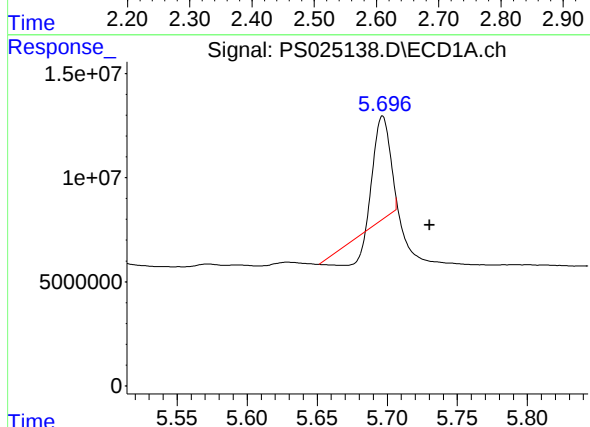


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.697 min
Delta R.T.: -0.033 min
Response: 30909305
Conc: 9.14 ng/ml

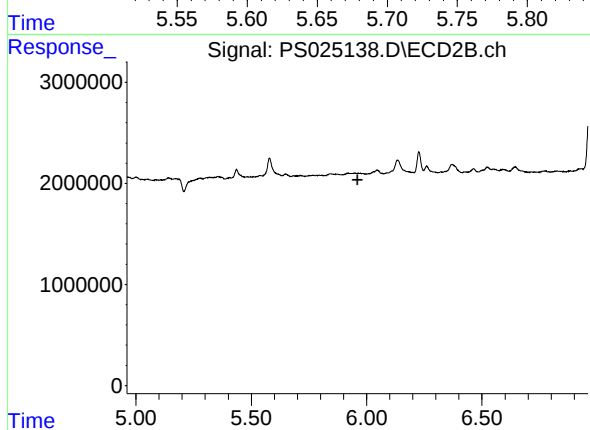

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

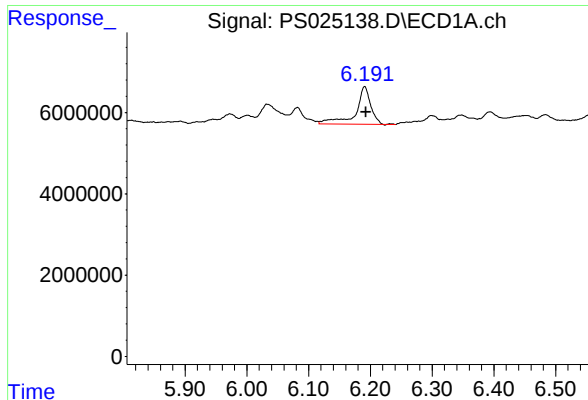

#3 4-Nitrophenol


R.T.: 6.191 min
Delta R.T.: -0.002 min
Response: 15527670
Conc: 10.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

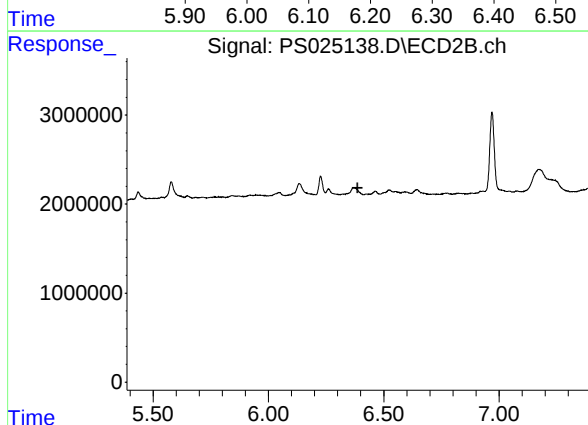


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

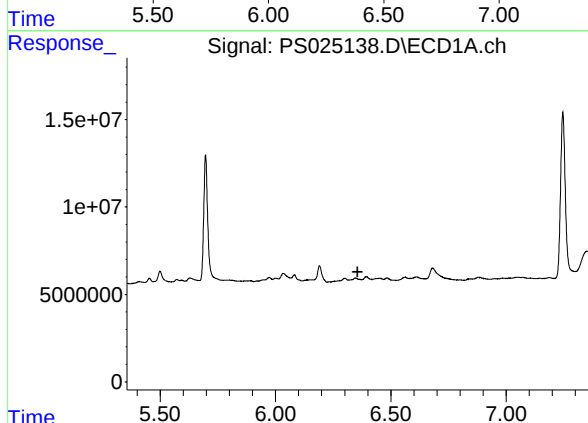


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

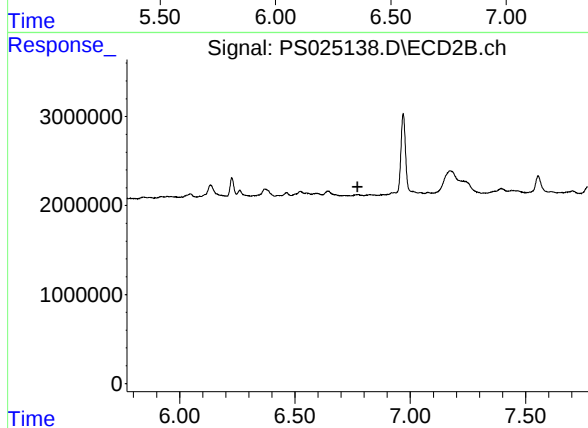

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

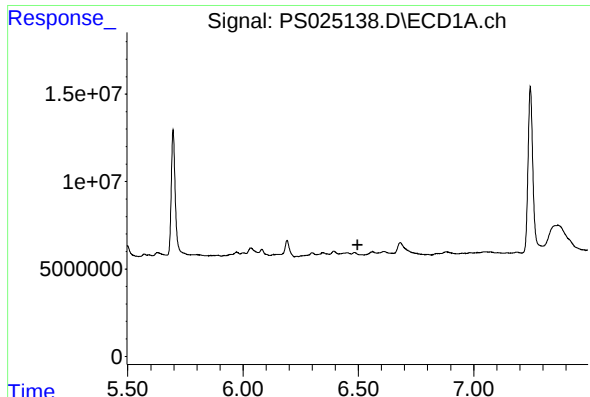

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

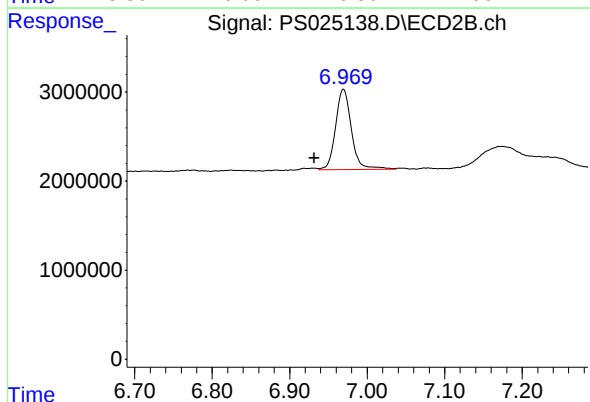


#5 DICAMBA

R.T.: 6.969 min
Delta R.T.: 0.038 min
Response: 12896483
Conc: 4.16 ng/ml

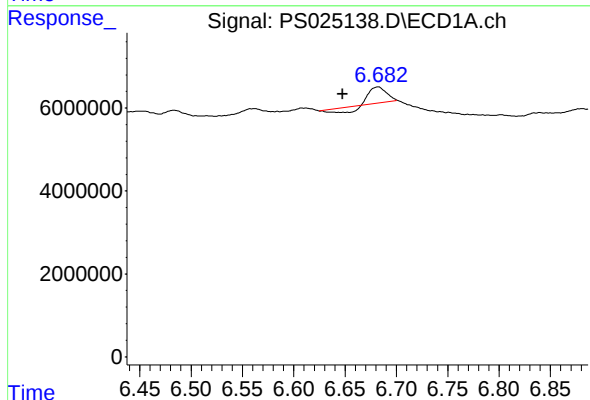


#6 MCPP

R.T.: 6.682 min
Delta R.T.: 0.034 min
Response: 2990623
Conc: N.D.

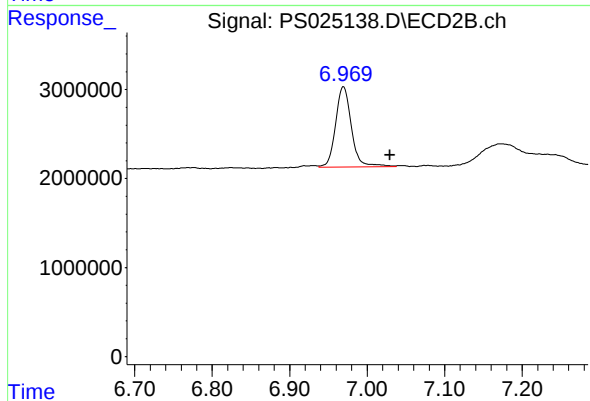

#6 MCPP


R.T.: 6.969 min
Delta R.T.: -0.060 min
Response: 12896483
Conc: 6.22 ug/ml

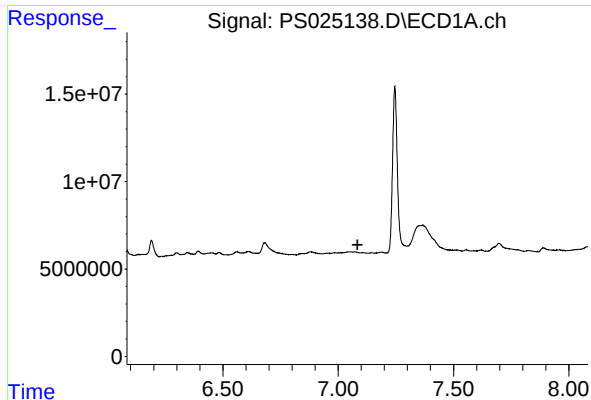

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

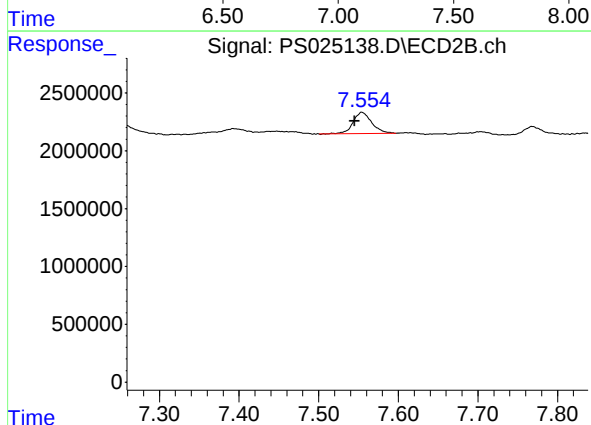


#8 DICHLORPROP

R.T.: 7.554 min
Delta R.T.: 0.009 min
Response: 2970583
Conc: 3.78 ng/ml

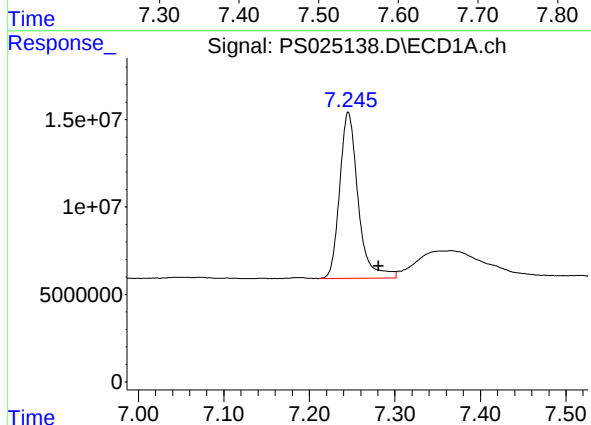


#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.035 min
Response: 142383235
Conc: 46.88 ng/ml

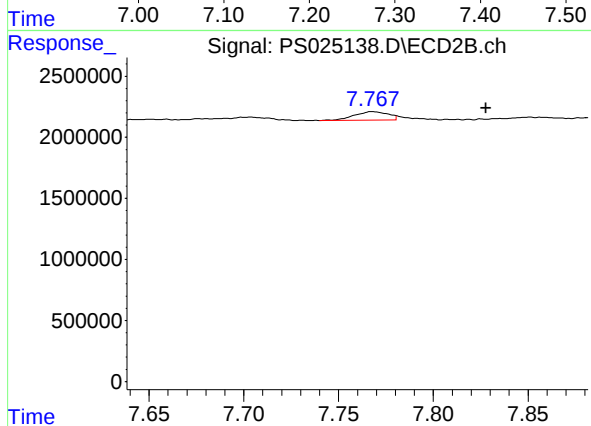

#9 2,4-D


R.T.: 7.768 min
Delta R.T.: -0.060 min
Response: 864589
Conc: N.D.

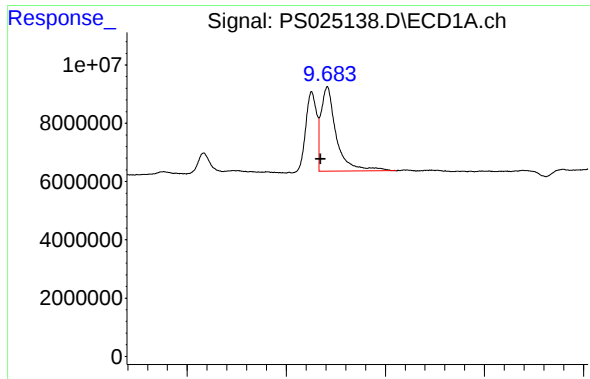

#15 Picloram


R.T.: 9.683 min
Delta R.T.: 0.013 min
Response: 62016460
Conc: 3.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

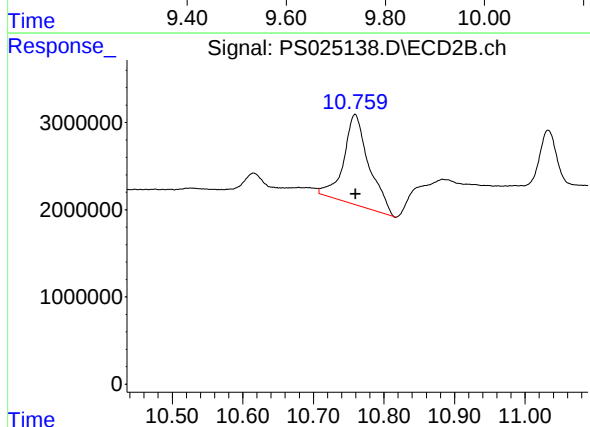


#15 Picloram

R.T.: 10.759 min
Delta R.T.: 0.000 min
Response: 25868394
Conc: 3.95 ng/ml

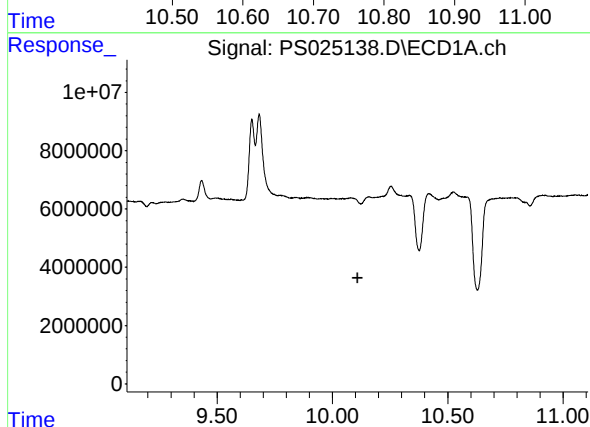

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

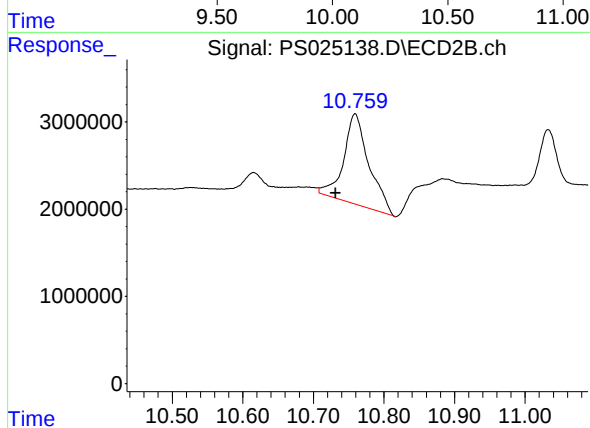

#16 DCPA

R.T.: 10.759 min
Delta R.T.: 0.027 min
Response: 25868394
Conc: 4.77 ng/ml