

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121923\
 Data File : PS025139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 11:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 22:23:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.768	1213.7E6	381.8E6	542.331	526.955
Target Compounds							
1) T	Dalapon	2.509	2.563	10265943	4478241	3.560	3.904
5) T	DICAMBA	0.000	6.967	0	689671	N.D.	<MDL
6) T	MCPP	0.000	6.967f	0	689671	N.D.	<MDL
7) T	MCPA	0.000	7.224	0	3726033	N.D.	1.133
8) T	DICHLORPROP	0.000	7.562	0	1182670	N.D.	1.503
9) T	2,4-D	0.000	7.769f	0	399486	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.559f	0	220787	N.D.	<MDL
12) T	2,4,5-T	0.000	9.020f	0	1930426	N.D.	<MDL
15) T	Picloram	9.687	10.761	35057877	9529300	1.799	1.456
16) T	DCPA	0.000	10.761	0	9529300	N.D.	1.758



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121923\
Data File : PS025139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 11:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 22:23:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

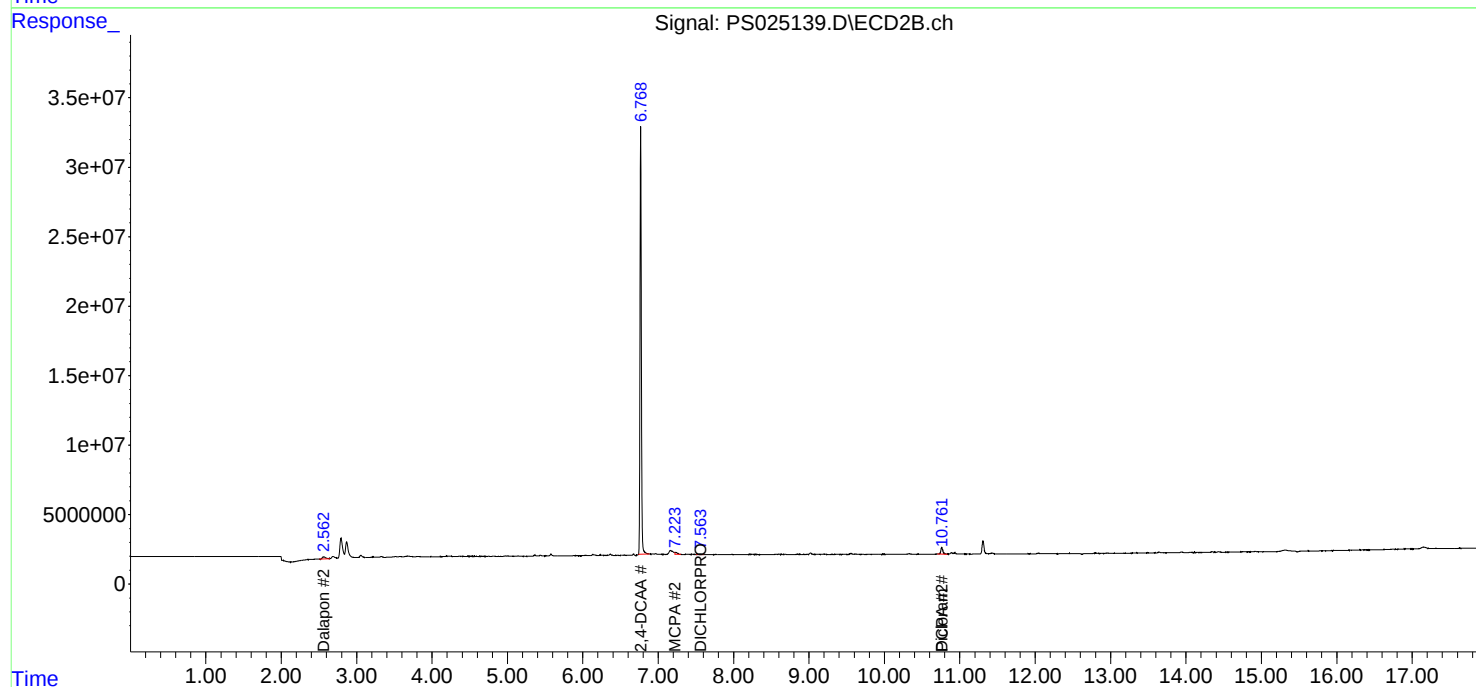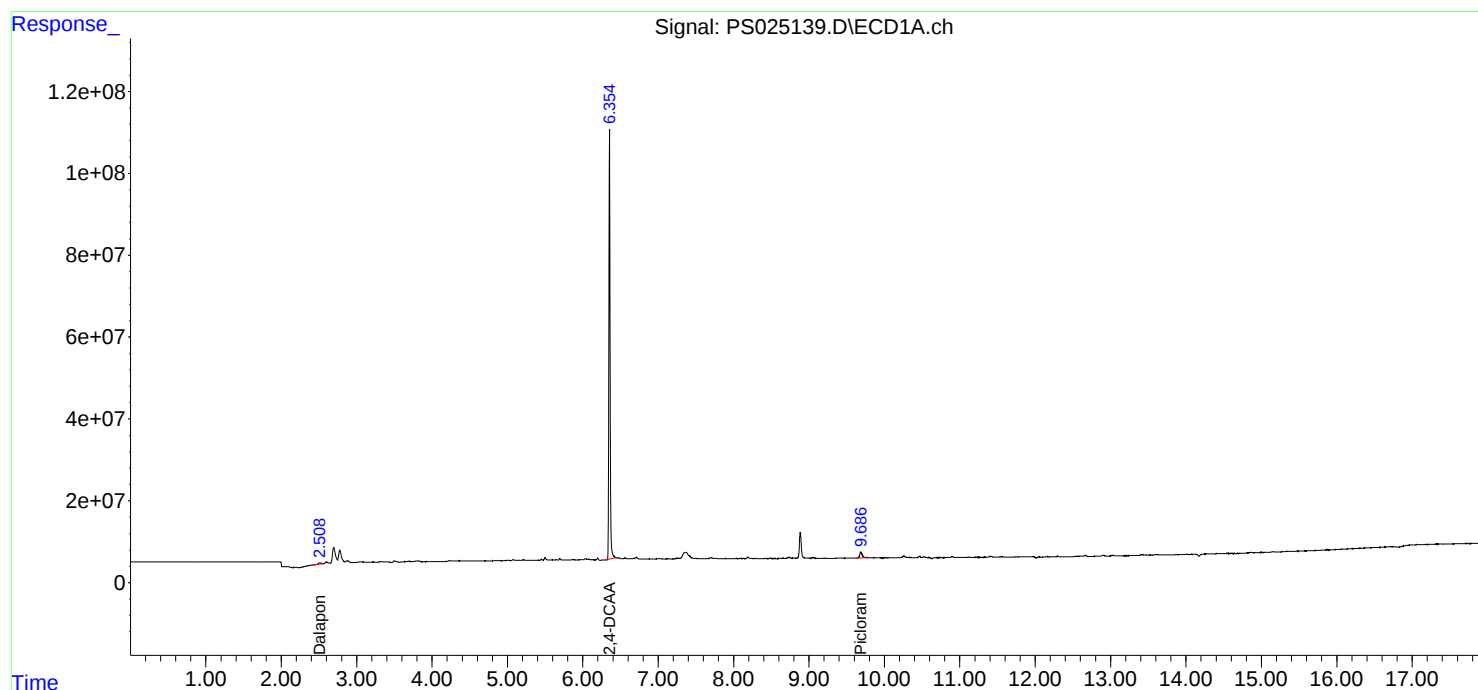


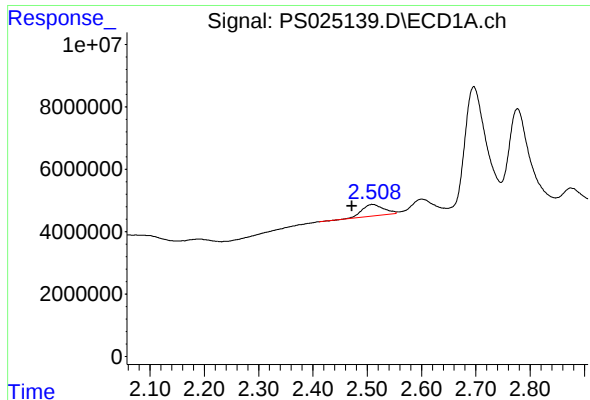

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 10265943
Conc: 3.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

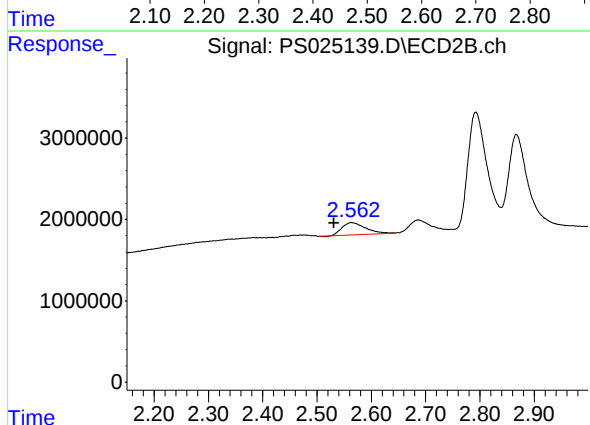


#1 Dalapon

R.T.: 2.563 min
Delta R.T.: 0.032 min
Response: 4478241
Conc: 3.90 ng/ml

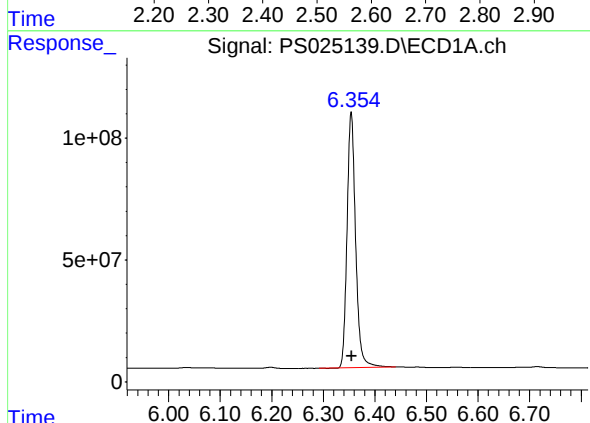


#4 2,4-DCAA

R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 1213651492
Conc: 542.33 ng/ml

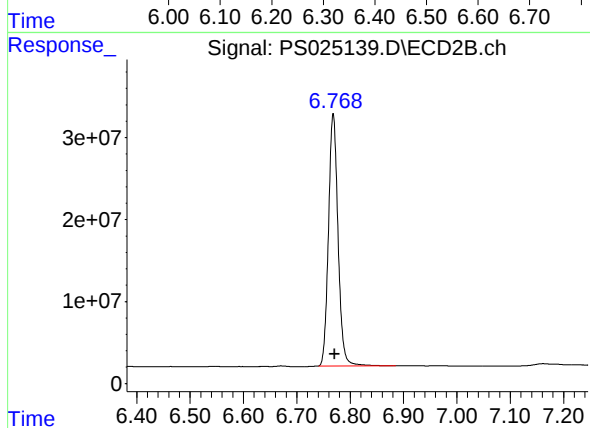

#4 2,4-DCAA


R.T.: 6.768 min
Delta R.T.: -0.003 min
Response: 381807699
Conc: 526.96 ng/ml

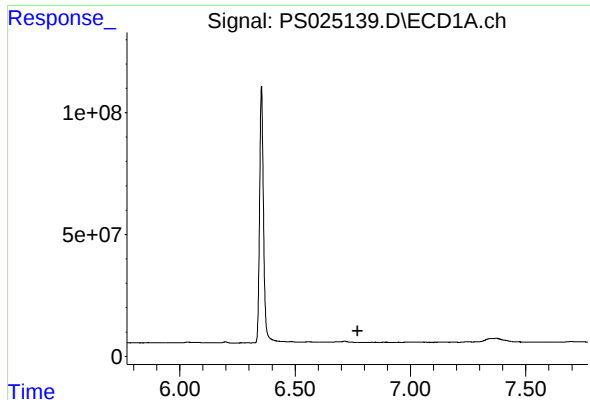

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

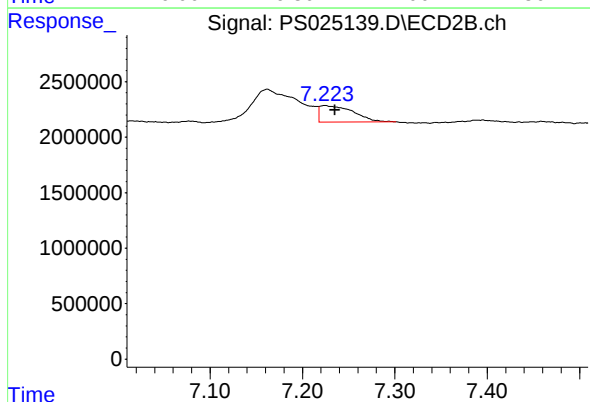


#7 MCPA

R.T.: 7.224 min
Delta R.T.: -0.011 min
Response: 3726033
Conc: 1.13 ug/ml

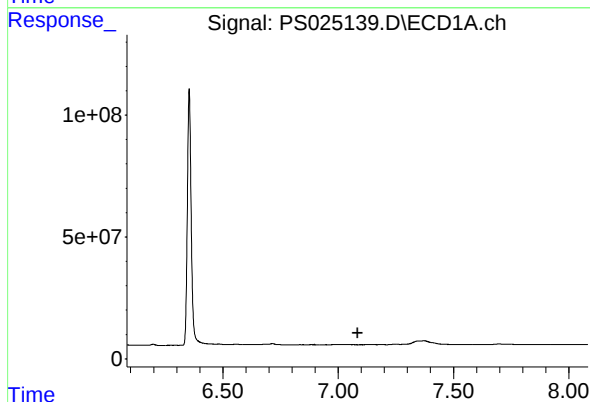


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

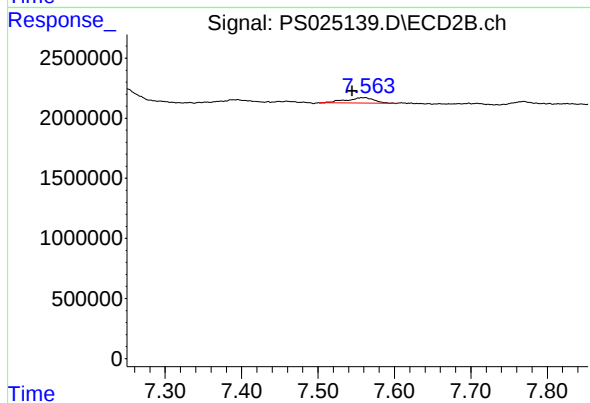

#8 DICHLORPROP


R.T.: 7.562 min
Delta R.T.: 0.017 min
Response: 1182670
Conc: 1.50 ng/ml

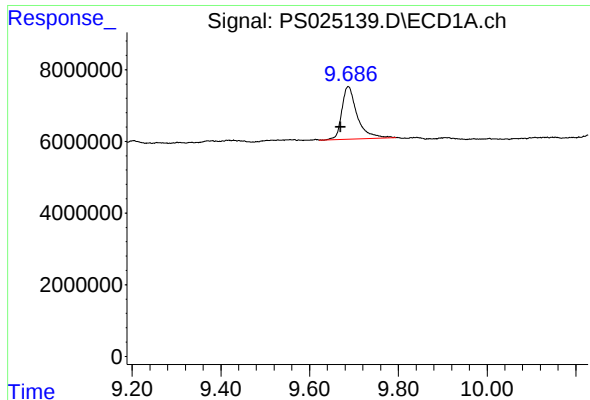

#15 Picloram


R.T.: 9.687 min
Delta R.T.: 0.017 min
Response: 35057877
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

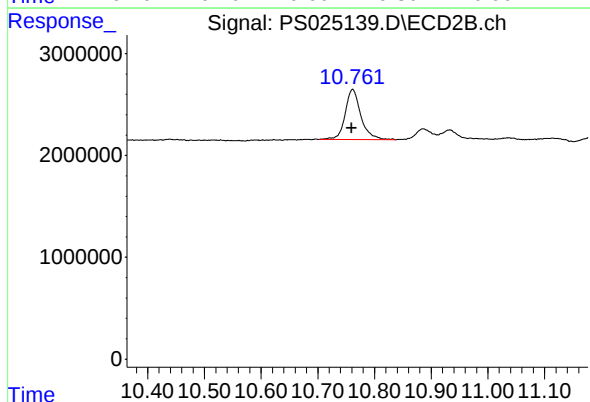


#15 Picloram

R.T.: 10.761 min
Delta R.T.: 0.002 min
Response: 9529300
Conc: 1.46 ng/ml

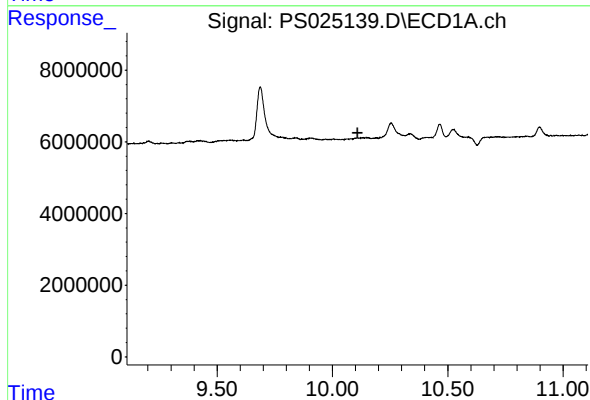

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

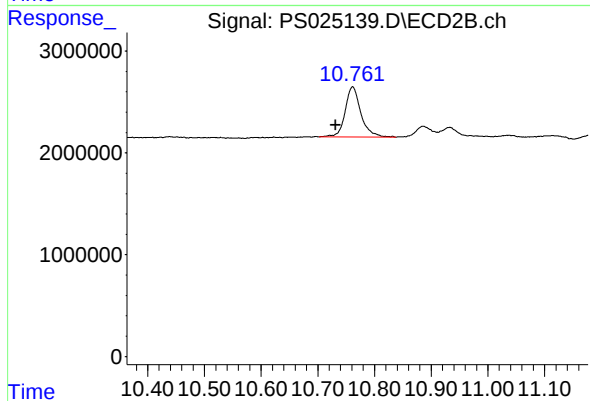

#16 DCPA

R.T.: 10.761 min
Delta R.T.: 0.030 min
Response: 9529300
Conc: 1.76 ng/ml