

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121923\
 Data File : PS025142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 14:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 22:23:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.769	1190.6E6	377.3E6	532.038	520.669
Target Compounds							
1) T	Dalapon	0.000	2.558	0	3108817	N.D.	2.710
2) T	3,5-DICHL...	5.697	0.000	1267974	0	<MDL	N.D. #
3) T	4-Nitroph...	6.197	0.000	6795125	0	4.614	N.D. #
5) T	DICAMBA	0.000	6.969	0	2485751	N.D.	<MDL
6) T	MCP	6.681	7.075f	2056984	459299	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.555	0	3607297	N.D.	4.586
9) T	2,4-D	7.246	7.768f	17265484	182730	5.684	<MDL #
10) T	Pentachlo...	0.000	8.246	0	776983	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.623	0	4101137	N.D.	<MDL
12) T	2,4,5-T	8.303	8.978	31550589	707271	2.184	<MDL #
13) T	2,4-DB	0.000	9.471	0	979104	N.D.	1.769
15) T	Picloram	9.685	10.760	26499080	10321060	1.360	1.577
16) T	DCPA	0.000	10.760	0	10321060	N.D.	1.904



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121923\
Data File : PS025142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 14:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 22:23:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

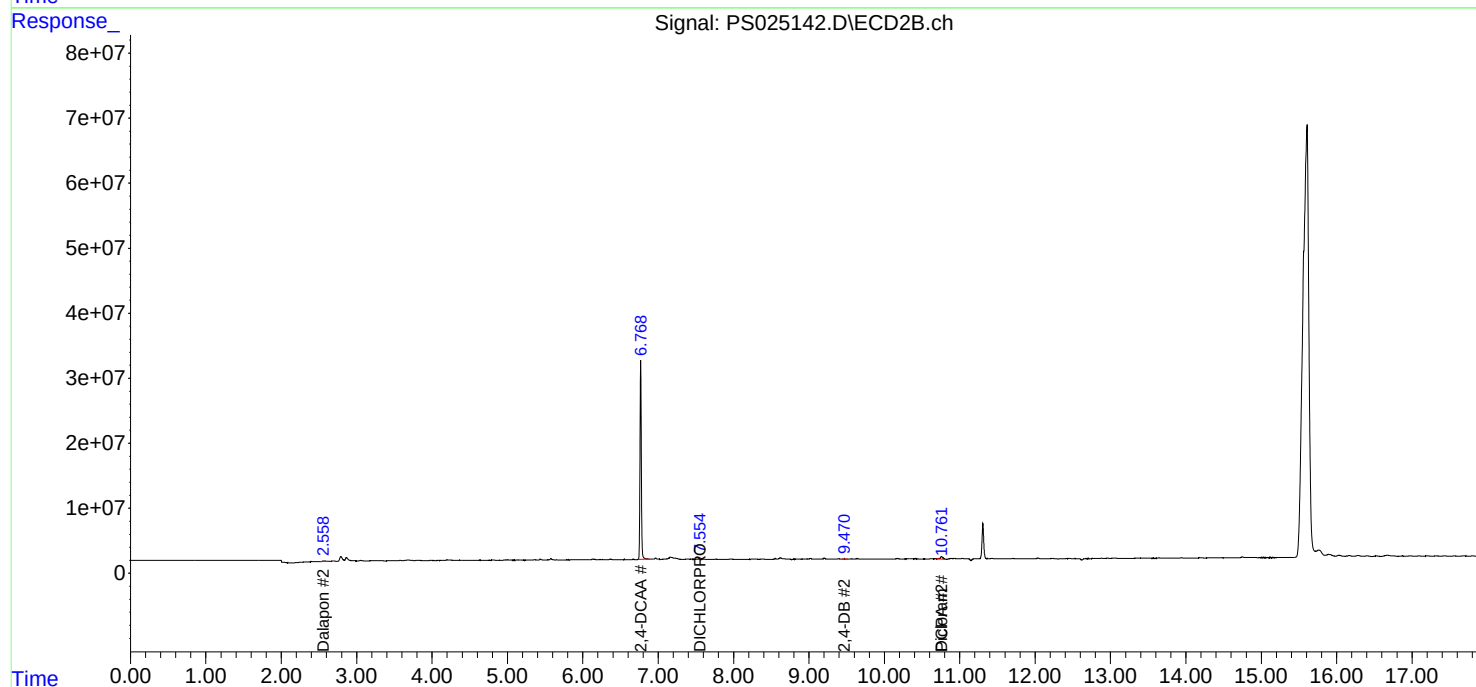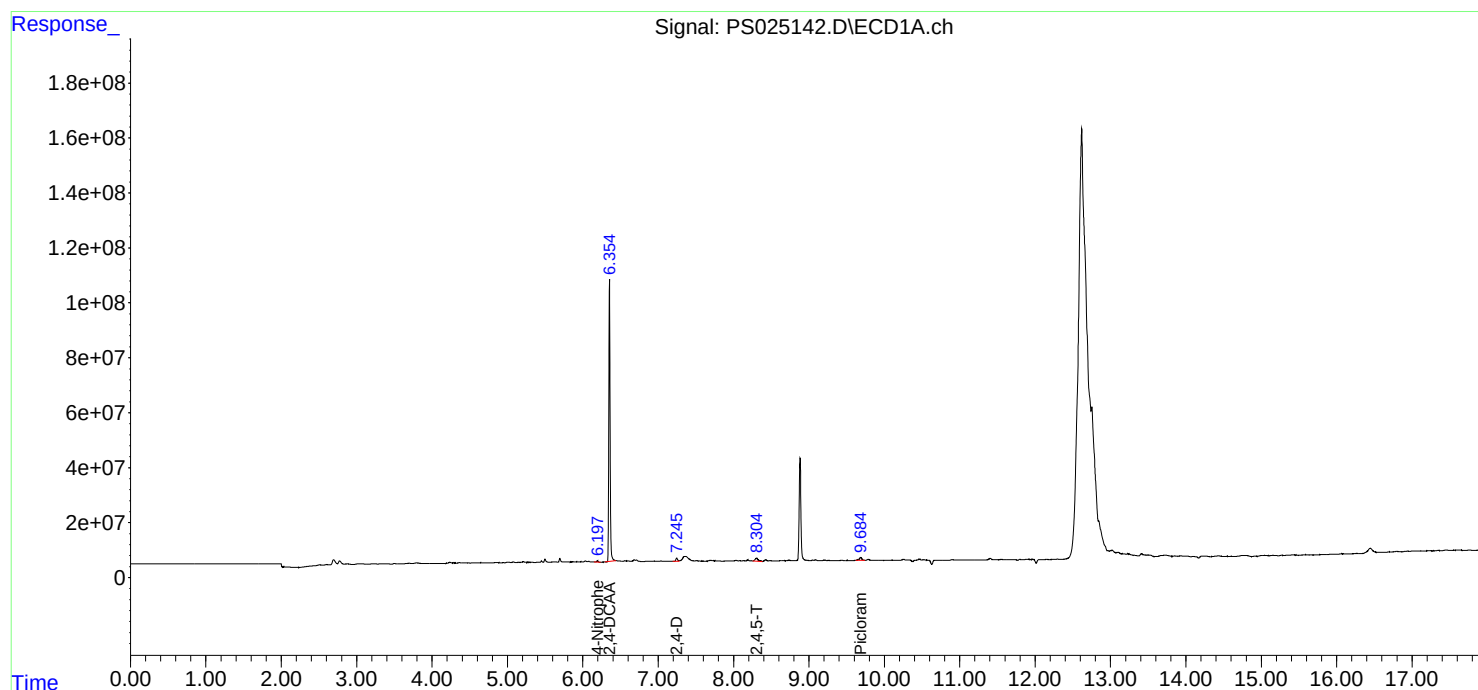


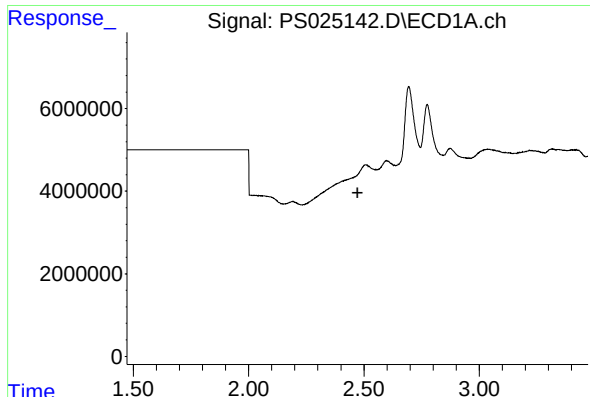

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

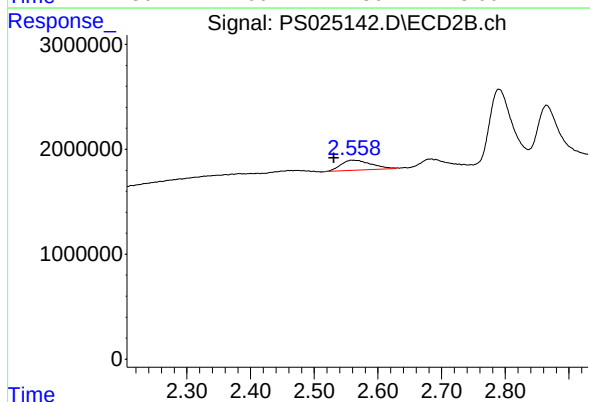


#1 Dalapon

R.T.: 2.558 min
Delta R.T.: 0.027 min
Response: 3108817
Conc: 2.71 ng/ml

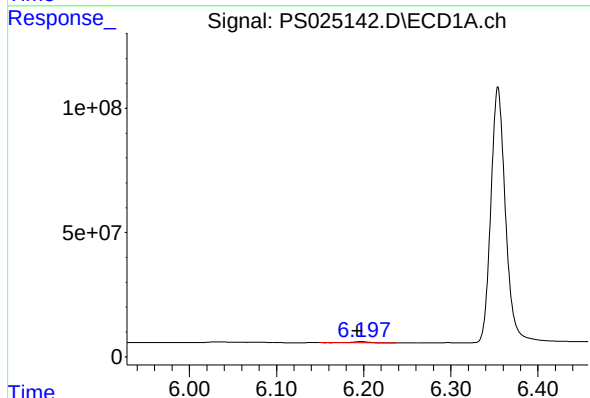


#3 4-Nitrophenol

R.T.: 6.197 min
Delta R.T.: 0.004 min
Response: 6795125
Conc: 4.61 ng/ml

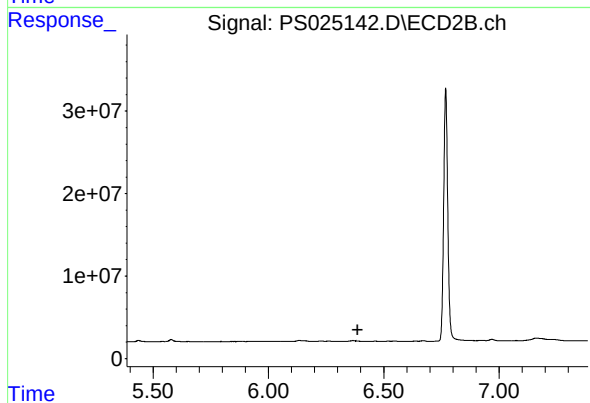

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

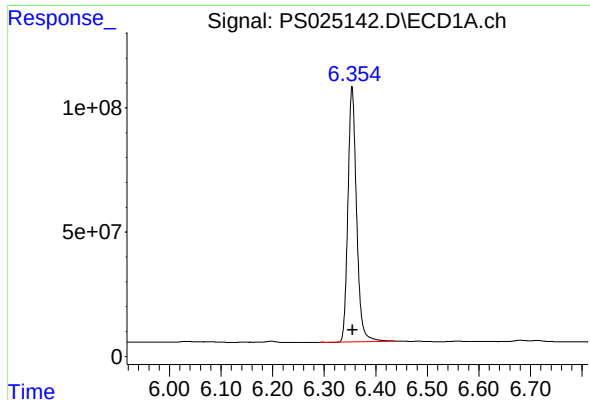

#4 2,4-DCAA


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 1190619267
Conc: 532.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

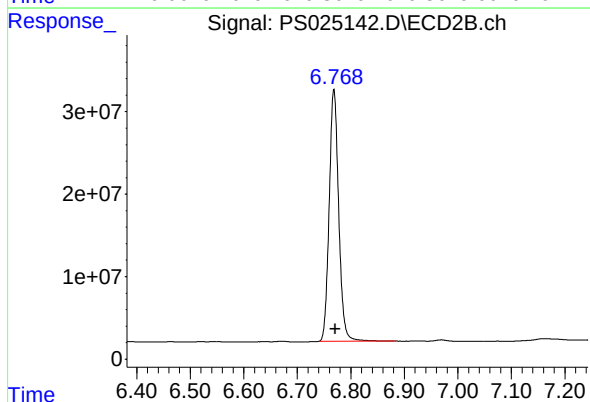


#4 2,4-DCAA

R.T.: 6.769 min
Delta R.T.: -0.003 min
Response: 377252932
Conc: 520.67 ng/ml

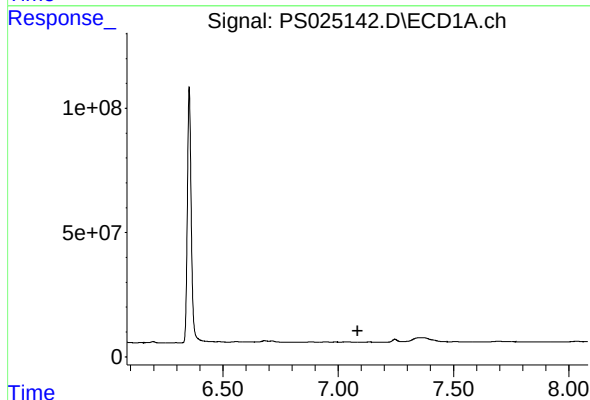


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

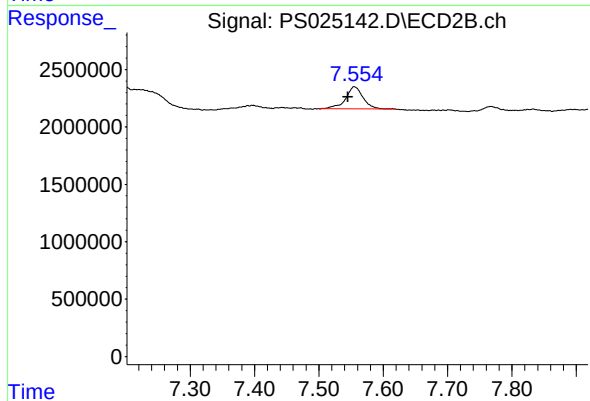

#8 DICHLORPROP


R.T.: 7.555 min
Delta R.T.: 0.010 min
Response: 3607297
Conc: 4.59 ng/ml

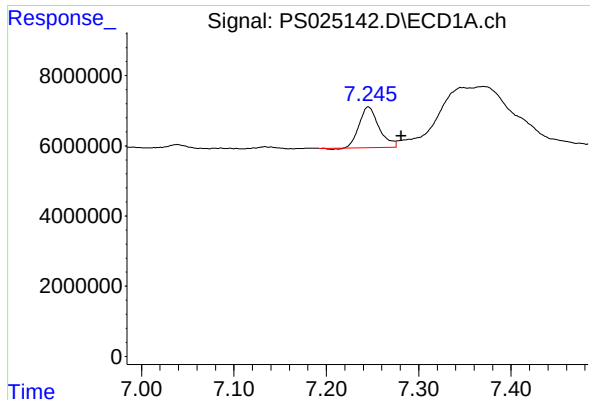

#9 2,4-D


R.T.: 7.246 min
Delta R.T.: -0.035 min
Response: 17265484
Conc: 5.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

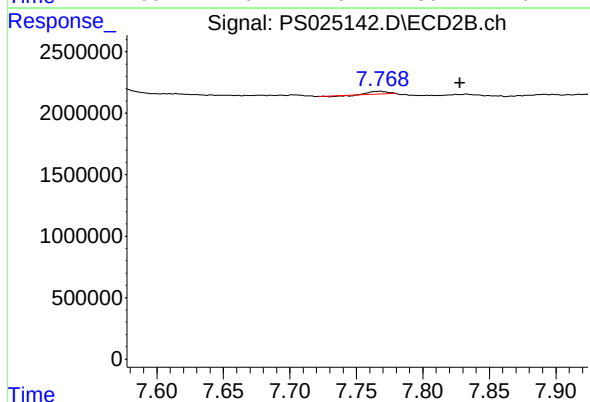


#9 2,4-D

R.T.: 7.768 min
Delta R.T.: -0.060 min
Response: 182730
Conc: N.D.

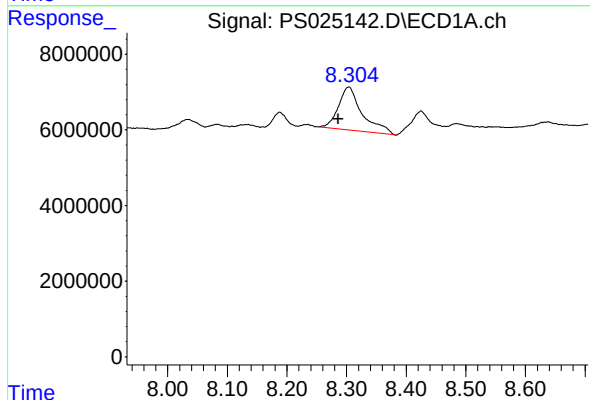


#12 2,4,5-T

R.T.: 8.303 min
Delta R.T.: 0.017 min
Response: 31550589
Conc: 2.18 ng/ml

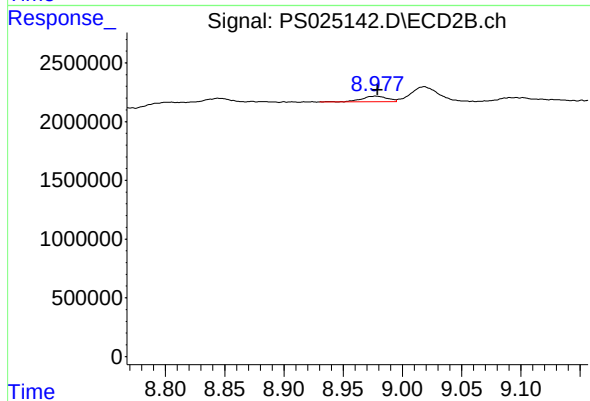

#12 2,4,5-T


R.T.: 8.978 min
Delta R.T.: -0.001 min
Response: 707271
Conc: N.D.

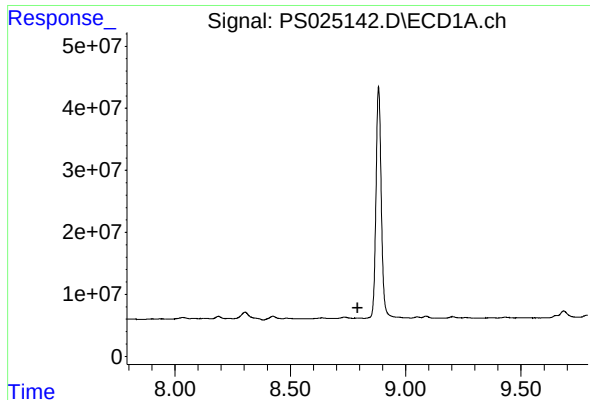

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

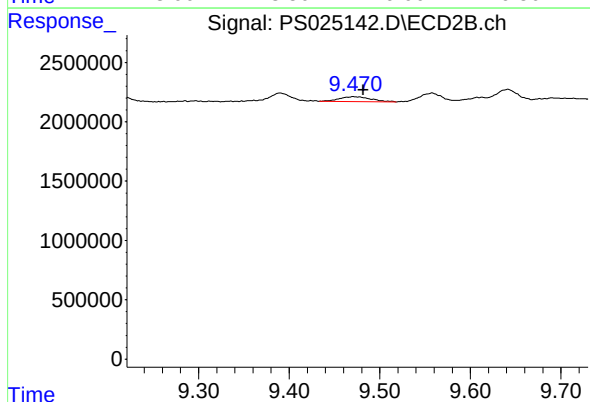


#13 2,4-DB

R.T.: 9.471 min
Delta R.T.: -0.011 min
Response: 979104
Conc: 1.77 ng/ml

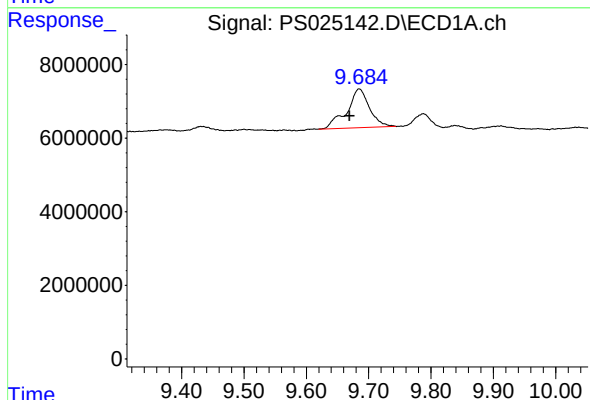


#15 Picloram

R.T.: 9.685 min
Delta R.T.: 0.015 min
Response: 26499080
Conc: 1.36 ng/ml

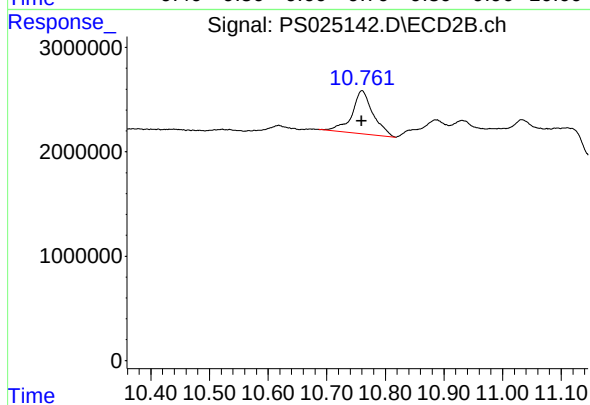

#15 Picloram


R.T.: 10.760 min
Delta R.T.: 0.000 min
Response: 10321060
Conc: 1.58 ng/ml

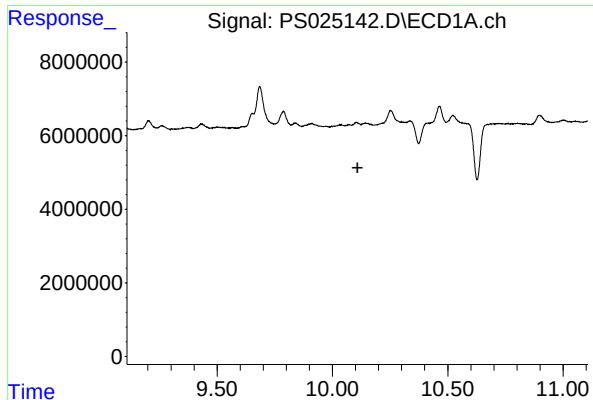

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

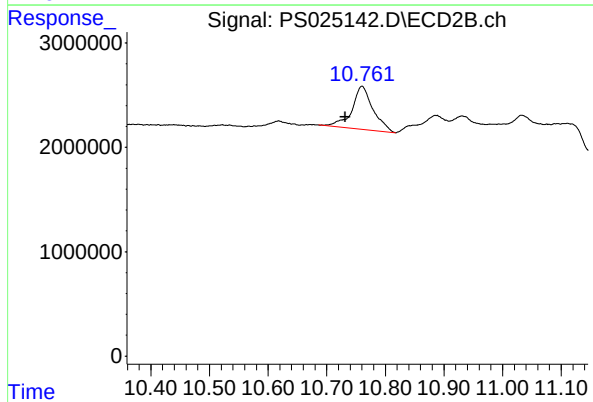

#16 DCPA

R.T.: 10.760 min
Delta R.T.: 0.029 min
Response: 10321060
Conc: 1.90 ng/ml