

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122021\
 Data File : PS017775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2021 16:58
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 00:19:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.395	0.000	33784980	0	15.122	N.D. #
5) T	DICAMBA	7.320	0.000	12424562	0	1.965	N.D. #
8) T	DICHLORPROP	8.015	0.000	3816082	0	2.442	N.D. #
9) T	2,4-D	8.300f	0.000	73949060	0	41.829	N.D. #
10) T	Pentachlo...	8.540	8.199	22400931	9250900	1.038	1.080
11) T	2,4,5-TP ...	9.094	8.568	18222916	7485794	2.142	2.059
12) T	2,4,5-T	9.395	8.960	48276003	10541558	5.549	3.083 #
13) T	2,4-DB	9.975f	0.000	2278110	0	1.543	N.D. #
14) T	DINOSEB	11.067	9.761	42809243	7128052	6.261	2.759 #
15) T	Picloram	10.922	10.764	243.5E6	105.5E6	22.441	21.478
16) T	DCPA	11.335	10.686	27079472	10717327	2.493	2.393



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122021\
Data File : PS017775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2021 16:58
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 00:19:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

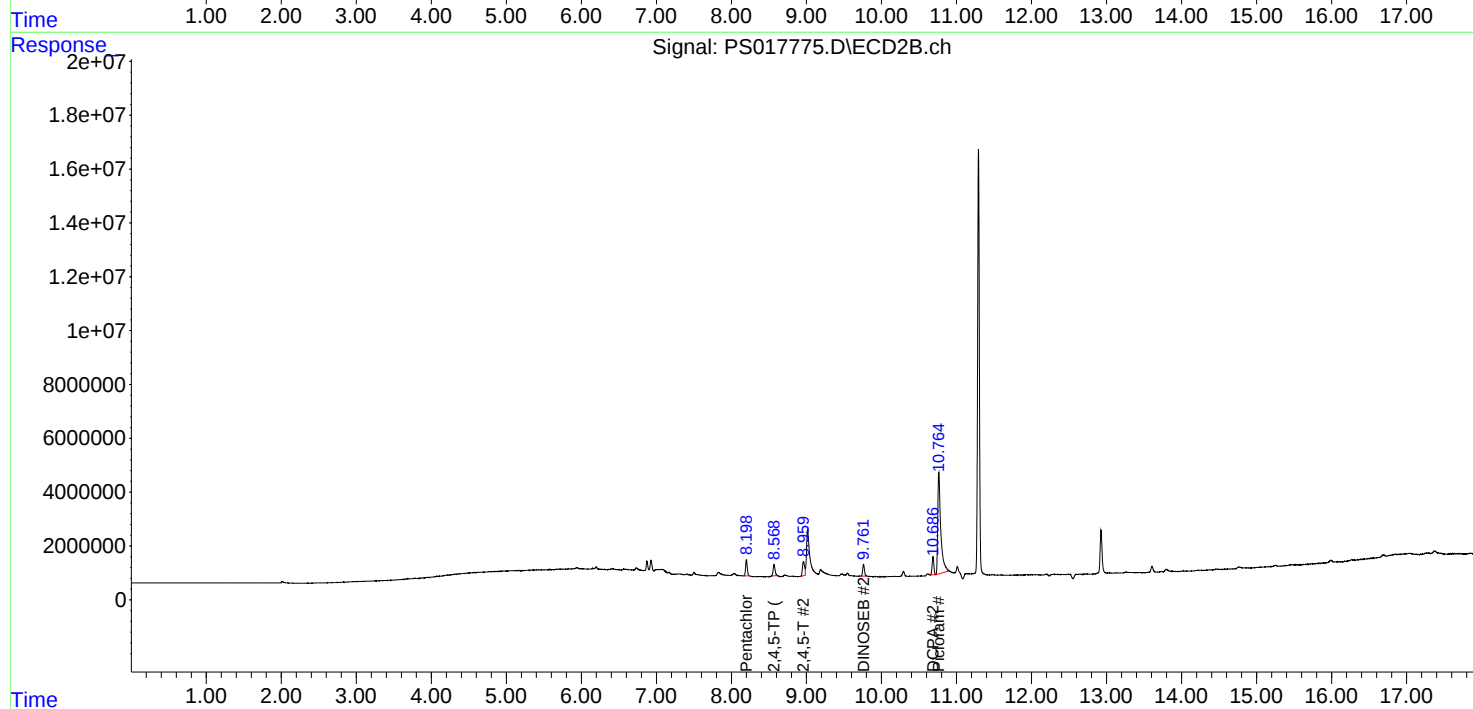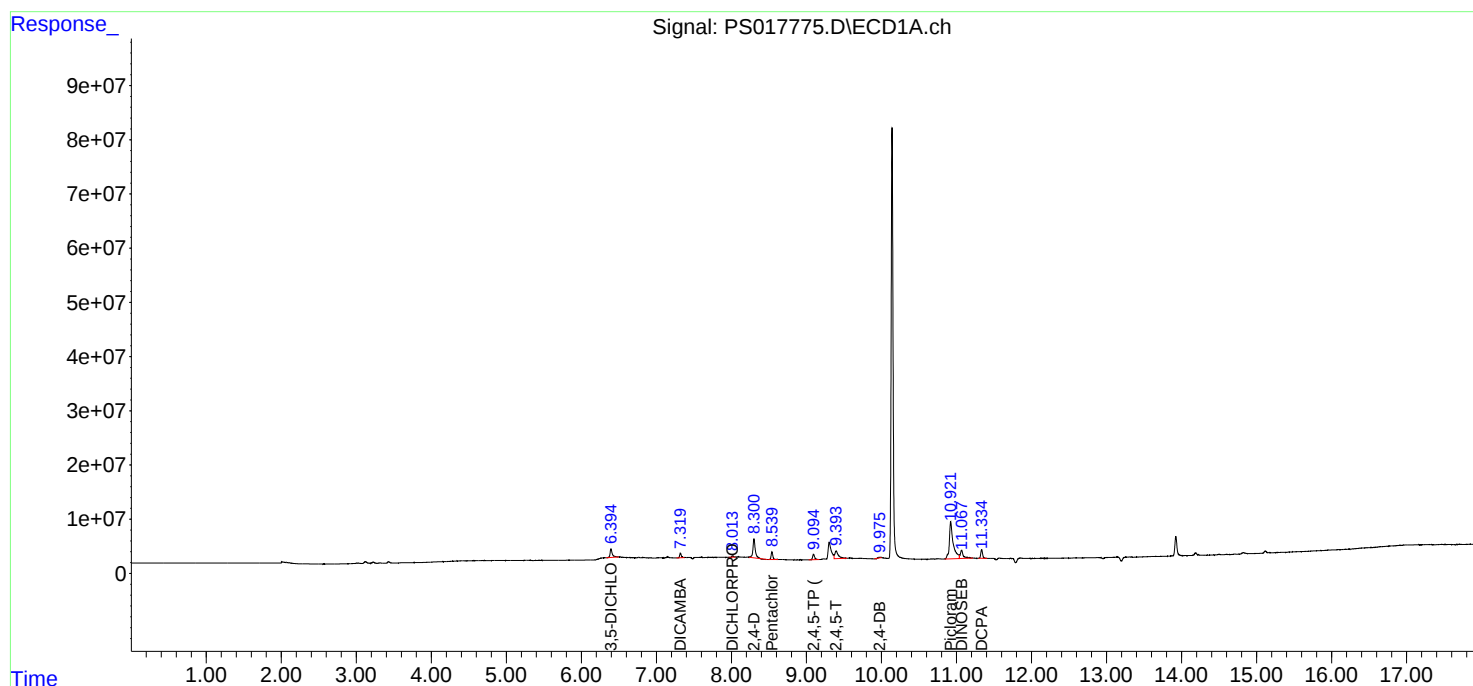


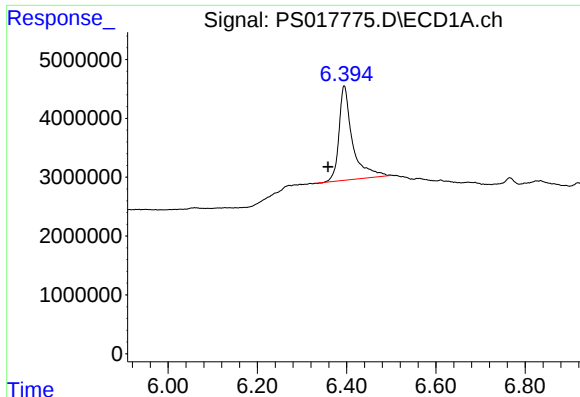

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.395 min
Delta R.T.: 0.036 min
Response: 33784980
Conc: 15.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

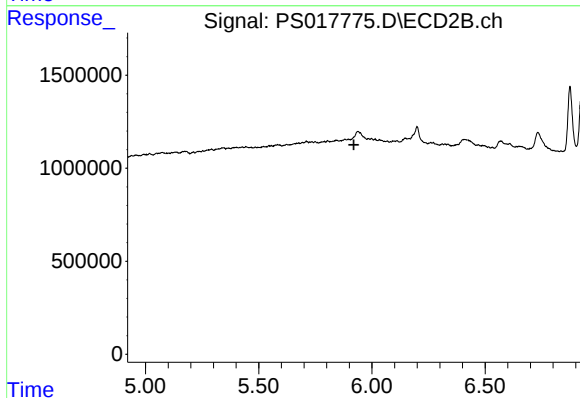


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

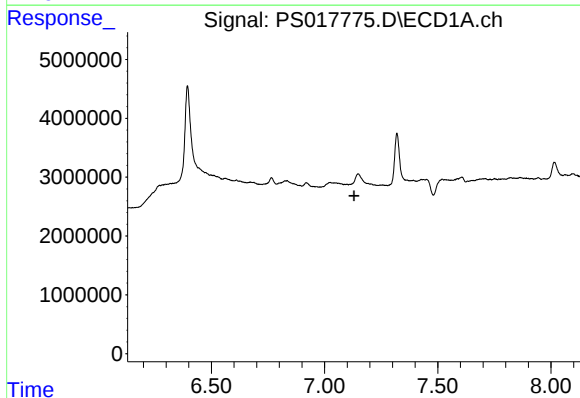


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.130 min
Response: 0
Conc: N.D.

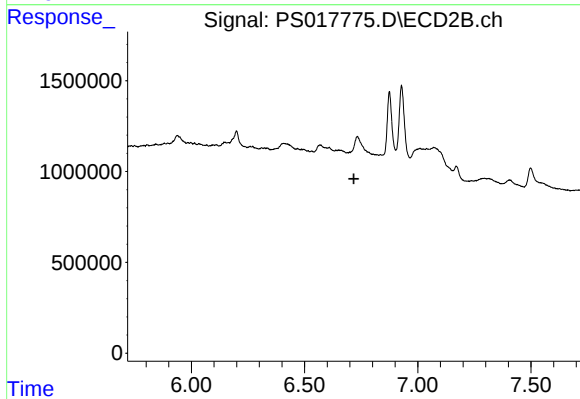

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.718 min
Response: 0
Conc: N.D.

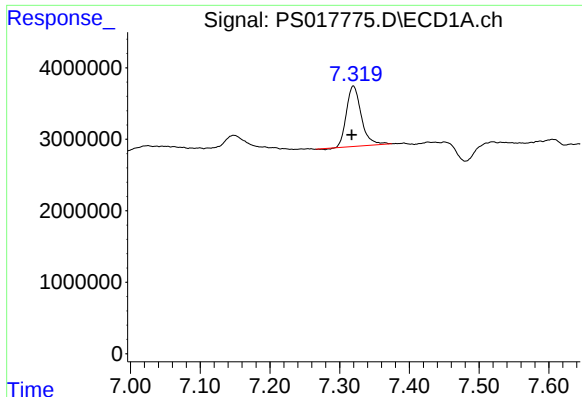

#5 DICAMBA


R.T.: 7.320 min
Delta R.T.: 0.002 min
Response: 12424562
Conc: 1.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

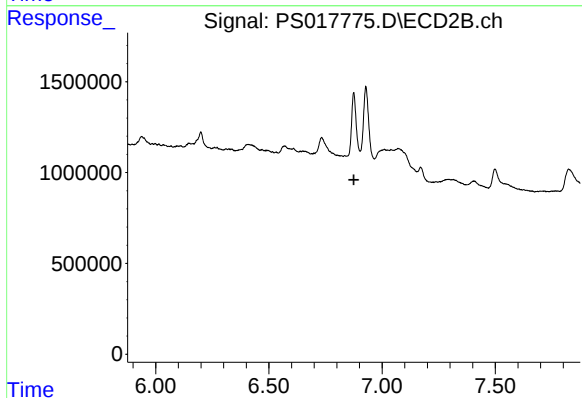


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

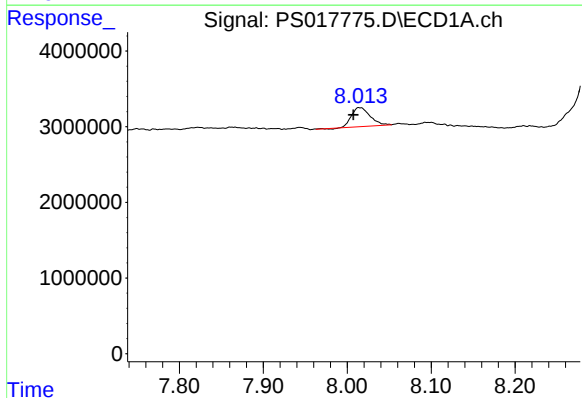


#8 DICHLORPROP

R.T.: 8.015 min
Delta R.T.: 0.007 min
Response: 3816082
Conc: 2.44 ng/ml

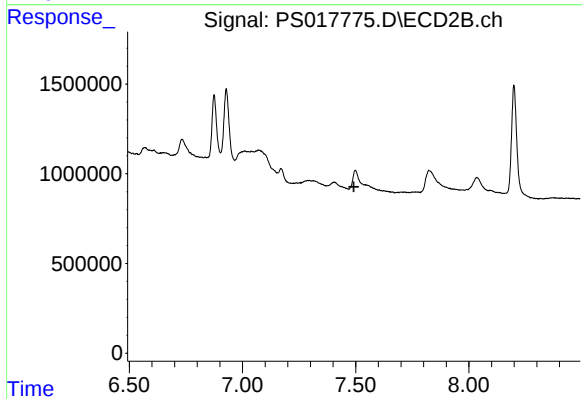

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.492 min
Response: 0
Conc: N.D.

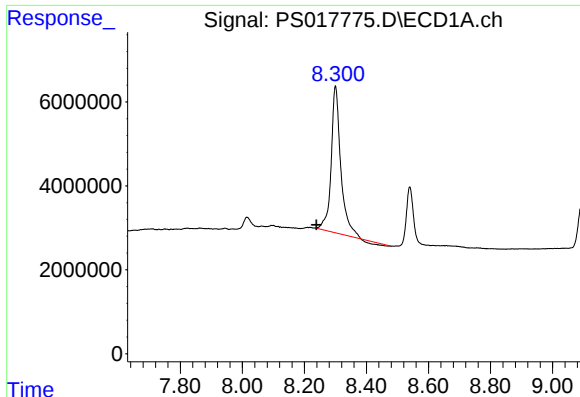

#9 2,4-D


R.T.: 8.300 min
Delta R.T.: 0.062 min
Response: 73949060
Conc: 41.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

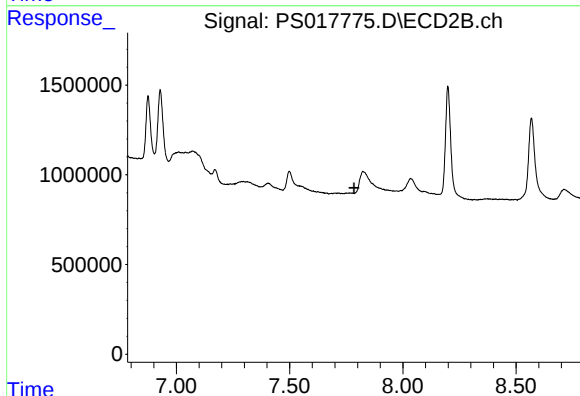


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

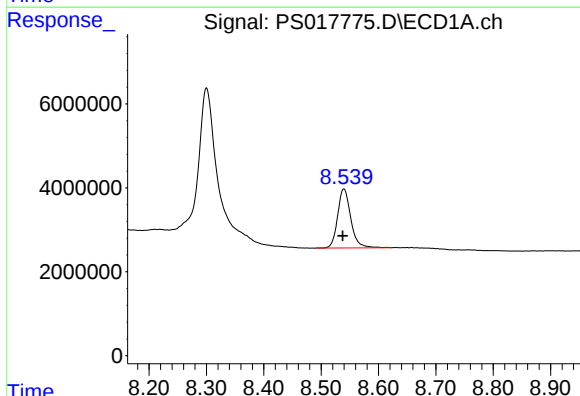


#10 Pentachlorophenol

R.T.: 8.540 min
Delta R.T.: 0.002 min
Response: 22400931
Conc: 1.04 ng/ml

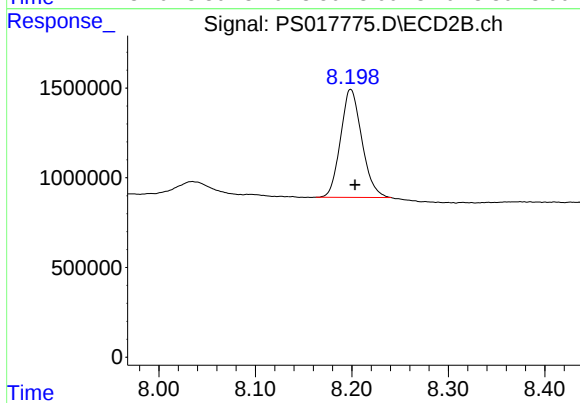

#10 Pentachlorophenol


R.T.: 8.199 min
Delta R.T.: -0.005 min
Response: 9250900
Conc: 1.08 ng/ml

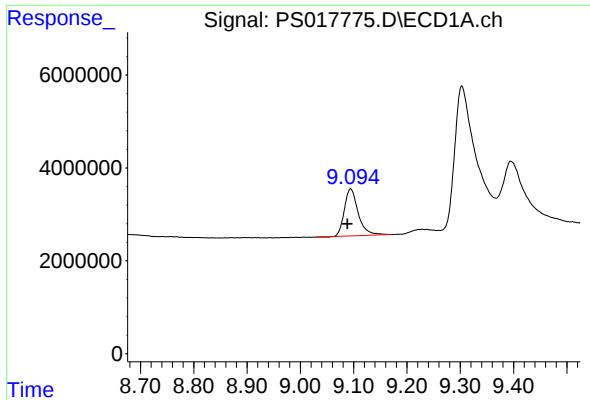

#11 2,4,5-TP (SILVEX)


R.T.: 9.094 min
Delta R.T.: 0.006 min
Response: 18222916
Conc: 2.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

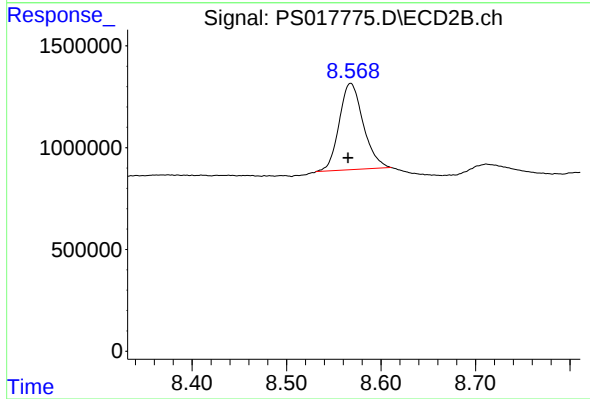


#11 2,4,5-TP (SILVEX)

R.T.: 8.568 min
Delta R.T.: 0.003 min
Response: 7485794
Conc: 2.06 ng/ml

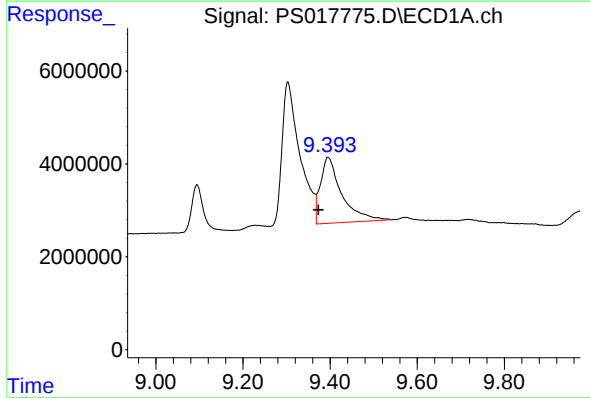


#12 2,4,5-T

R.T.: 9.395 min
Delta R.T.: 0.021 min
Response: 48276003
Conc: 5.55 ng/ml

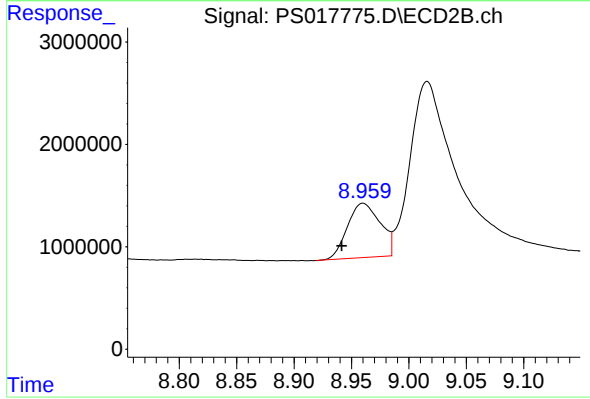

#12 2,4,5-T


R.T.: 8.960 min
Delta R.T.: 0.019 min
Response: 10541558
Conc: 3.08 ng/ml

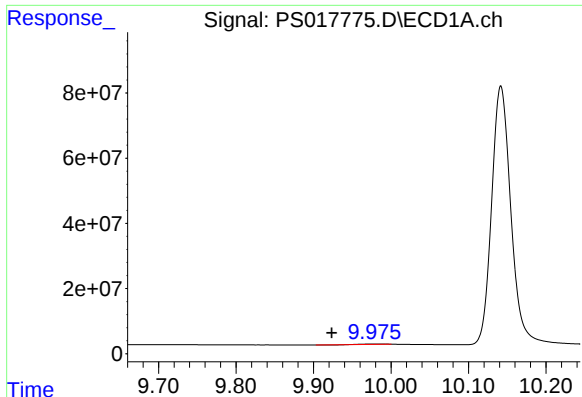

#13 2,4-DB


R.T.: 9.975 min
Delta R.T.: 0.052 min
Response: 2278110
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

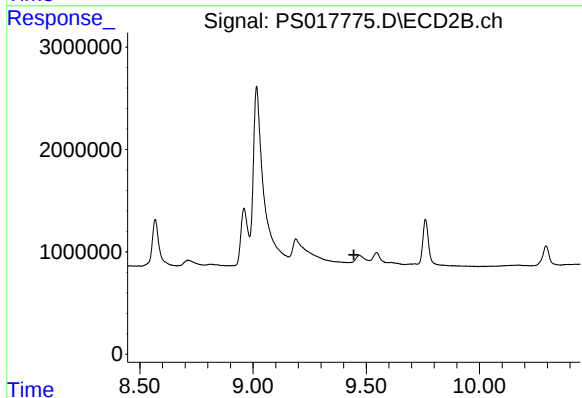


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.445 min
Response: 0
Conc: N.D.

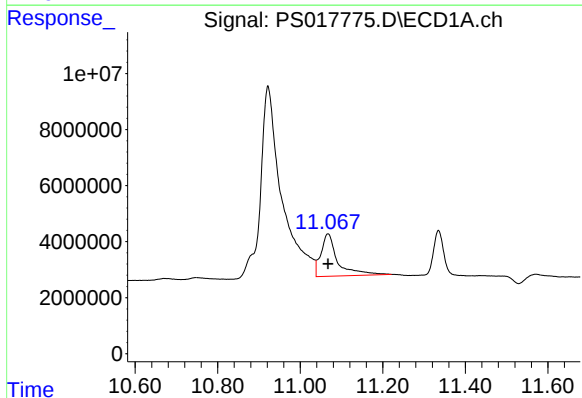


#14 DINOSEB

R.T.: 11.067 min
Delta R.T.: 0.000 min
Response: 42809243
Conc: 6.26 ng/ml

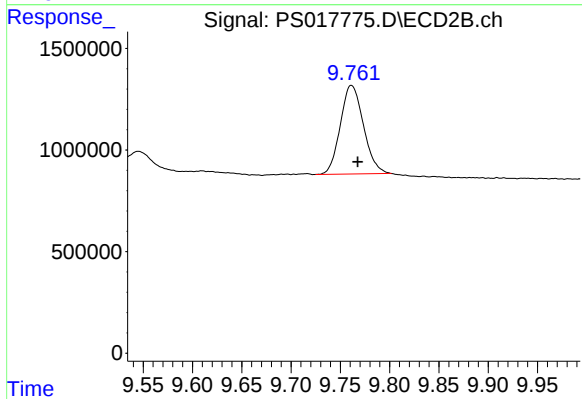

#14 DINOSEB


R.T.: 9.761 min
Delta R.T.: -0.006 min
Response: 7128052
Conc: 2.76 ng/ml

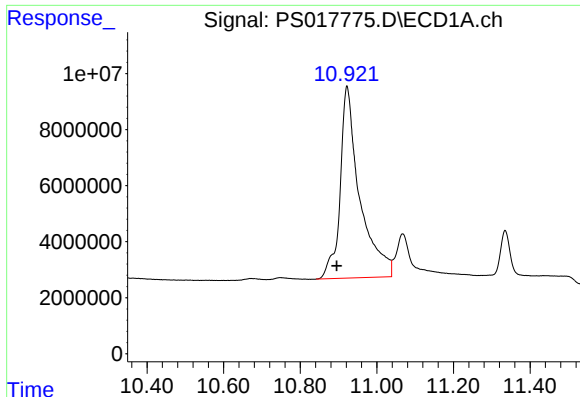

#15 Picloram


R.T.: 10.922 min
Delta R.T.: 0.027 min
Response: 243512443
Conc: 22.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

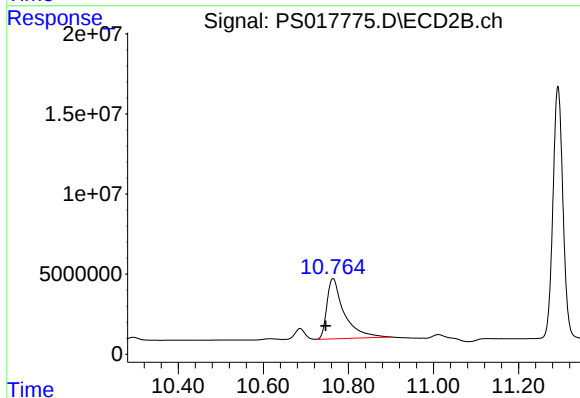


#15 Picloram

R.T.: 10.764 min
Delta R.T.: 0.017 min
Response: 105487816
Conc: 21.48 ng/ml

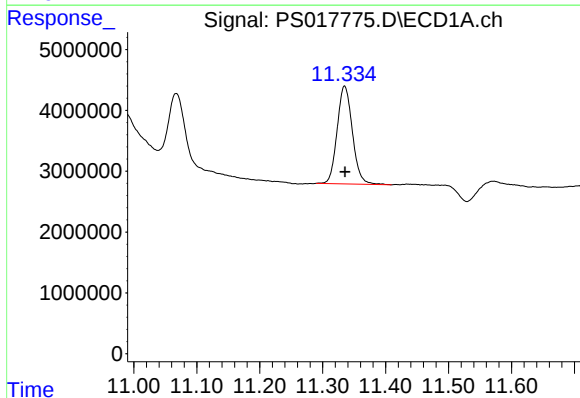

#16 DCPA

R.T.: 11.335 min
Delta R.T.: -0.001 min
Response: 27079472
Conc: 2.49 ng/ml

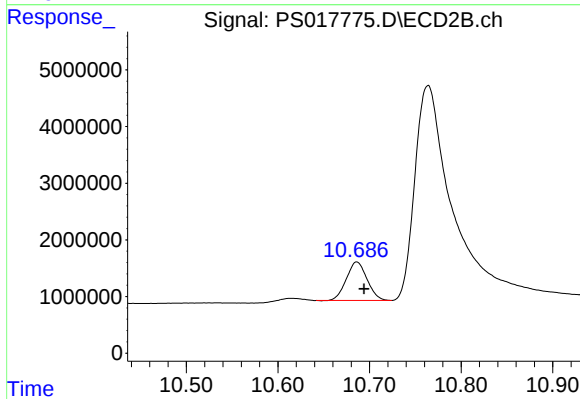

#16 DCPA

R.T.: 10.686 min
Delta R.T.: -0.008 min
Response: 10717327
Conc: 2.39 ng/ml