

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122021\
 Data File : PS017776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2021 17:22
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 00:20:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.128	6.715	799.6E6	339.2E6	511.605	569.016
Target Compounds							
2) T	3,5-DICHL...	6.392	0.000	173.0E6	0	77.439	N.D. #
5) T	DICAMBA	7.315	6.932f	9448412	48153393	1.494	18.076 #
6) T	MCP	0.000	6.932f	0	48153393	N.D.	22.123
9) T	2,4-D	8.299f	0.000	283.9E6	0	160.562	N.D. #
12) T	2,4,5-T	9.336	0.000	36109322	0	4.151	N.D. #
14) T	DINOSEB	11.065	0.000	17559418	0	2.568	N.D. #
15) T	Picloram	10.884	10.789f	21078864	55812172	1.943	11.364 #
16) T	DCPA	11.335	0.000	5016663	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122021\
Data File : PS017776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2021 17:22
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 00:20:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

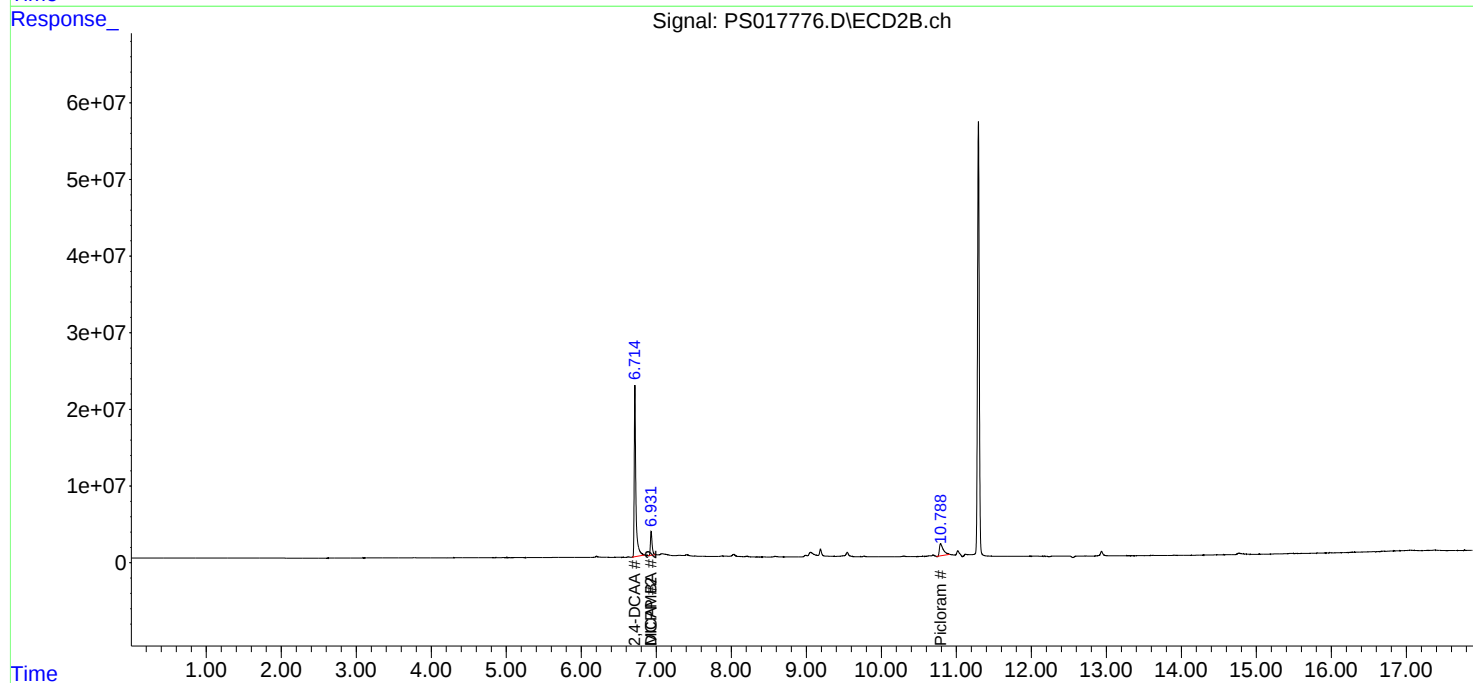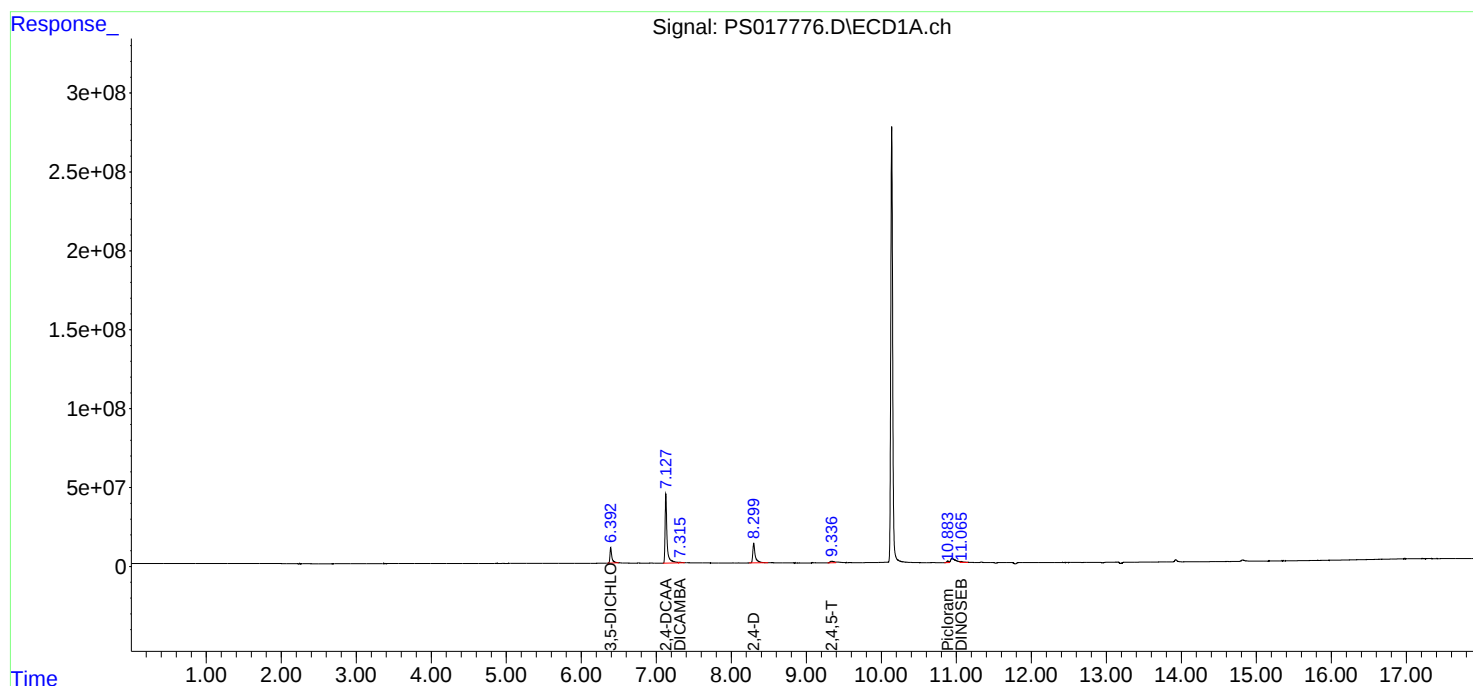


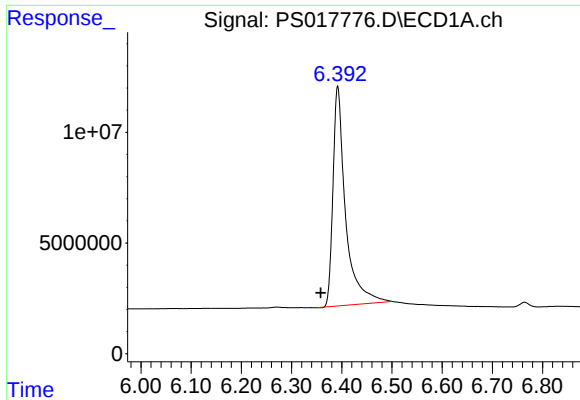

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.392 min
Delta R.T.: 0.034 min
Response: 173009673
Conc: 77.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

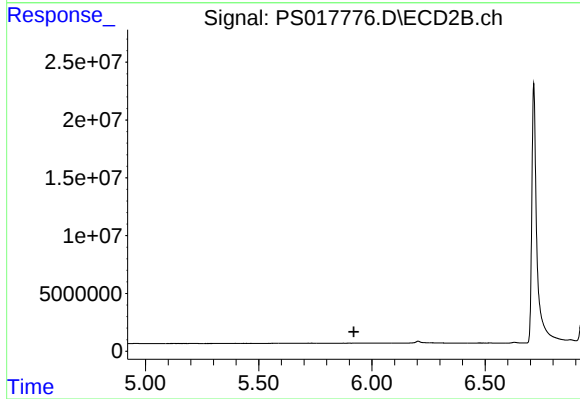


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

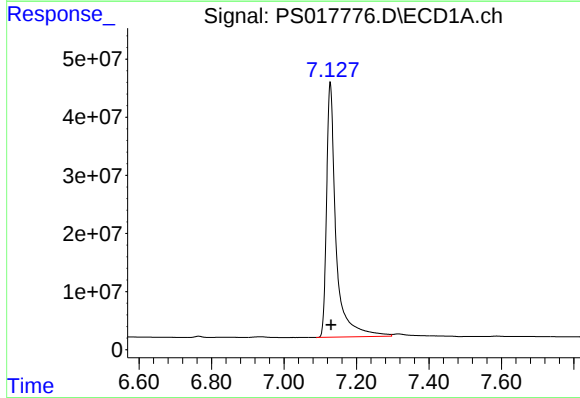


#4 2,4-DCAA

R.T.: 7.128 min
Delta R.T.: -0.002 min
Response: 799610643
Conc: 511.60 ng/ml

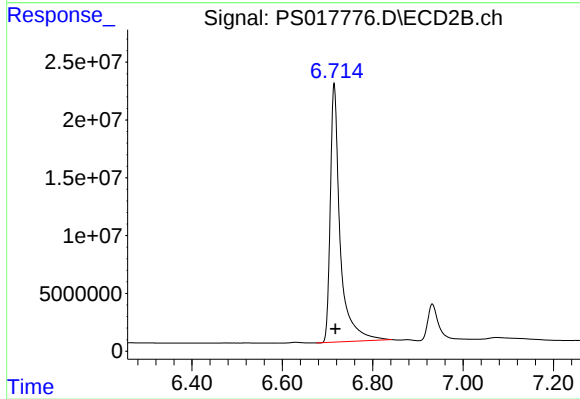

#4 2,4-DCAA


R.T.: 6.715 min
Delta R.T.: -0.003 min
Response: 339191494
Conc: 569.02 ng/ml

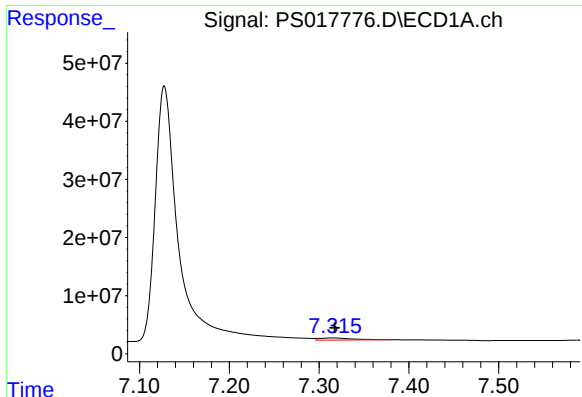

#5 DICAMBA


R.T.: 7.315 min
Delta R.T.: -0.002 min
Response: 9448412
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

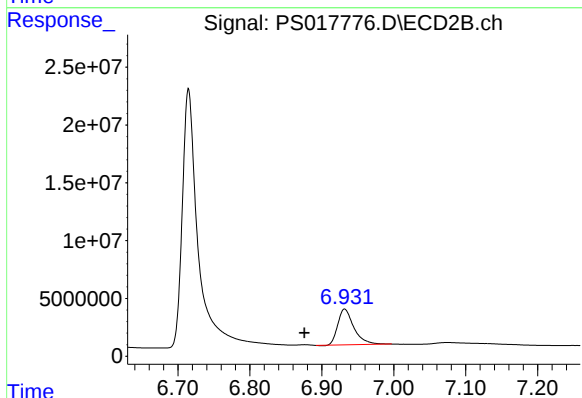


#5 DICAMBA

R.T.: 6.932 min
Delta R.T.: 0.056 min
Response: 48153393
Conc: 18.08 ng/ml

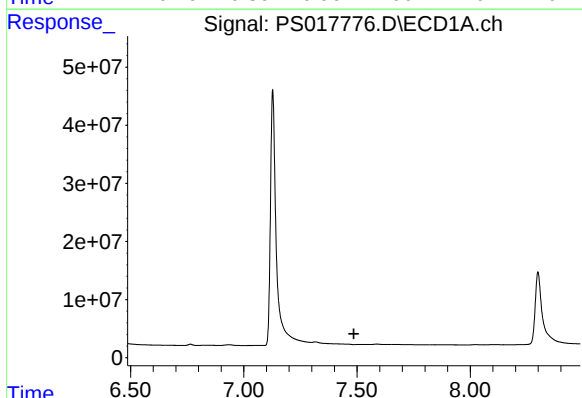


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

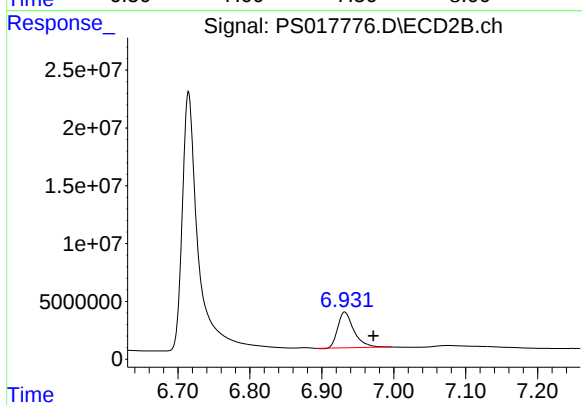

#6 MCP


R.T.: 6.932 min
Delta R.T.: -0.040 min
Response: 48153393
Conc: 22.12 ug/ml

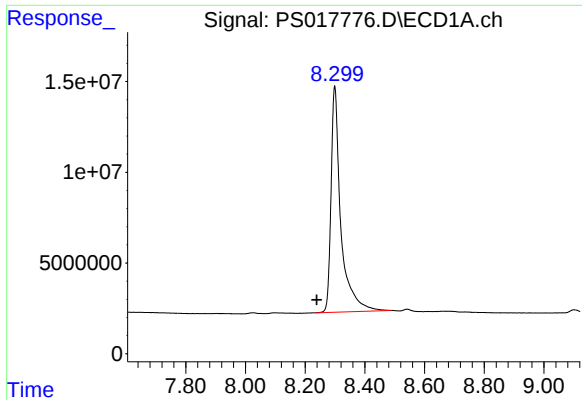

#9 2,4-D


R.T.: 8.299 min
Delta R.T.: 0.061 min
Response: 283853580
Conc: 160.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

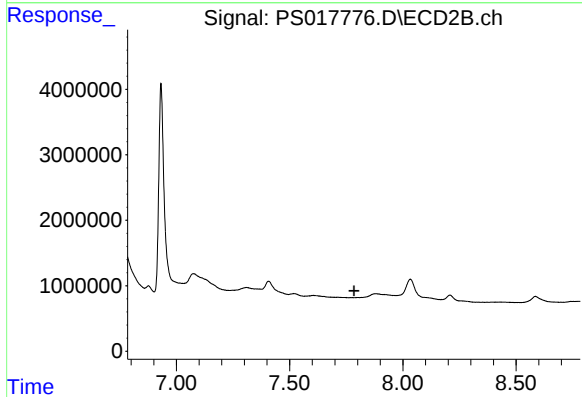


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

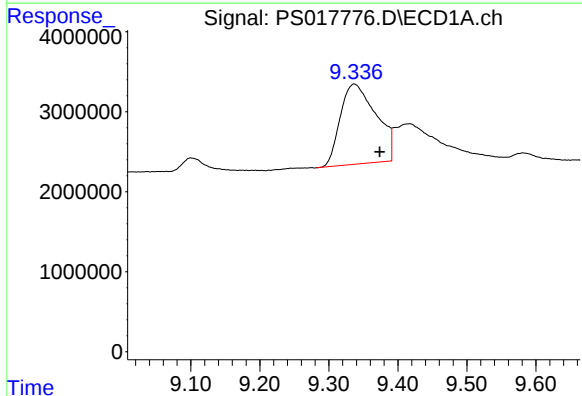


#12 2,4,5-T

R.T.: 9.336 min
Delta R.T.: -0.037 min
Response: 36109322
Conc: 4.15 ng/ml

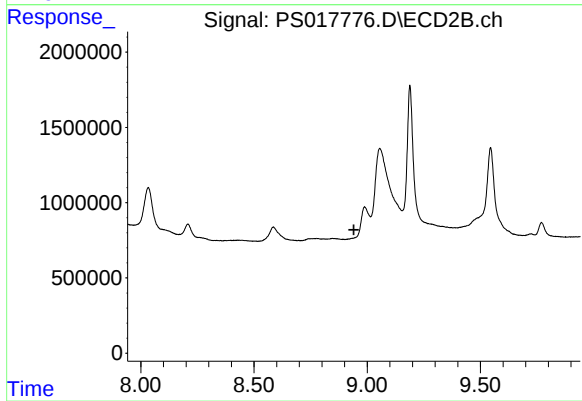

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

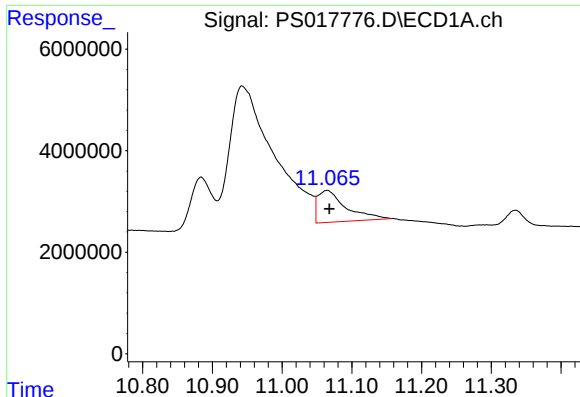

#14 DINOSEB


R.T.: 11.065 min
Delta R.T.: -0.003 min
Response: 17559418
Conc: 2.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

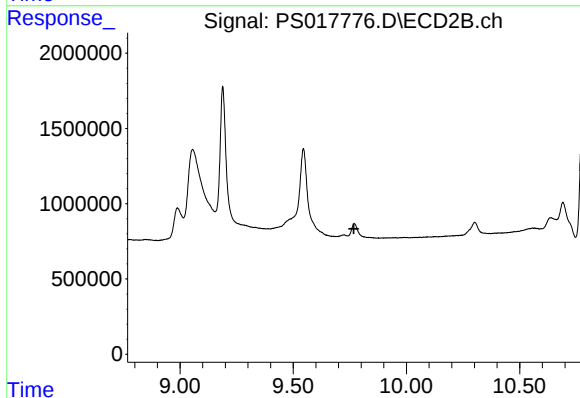


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

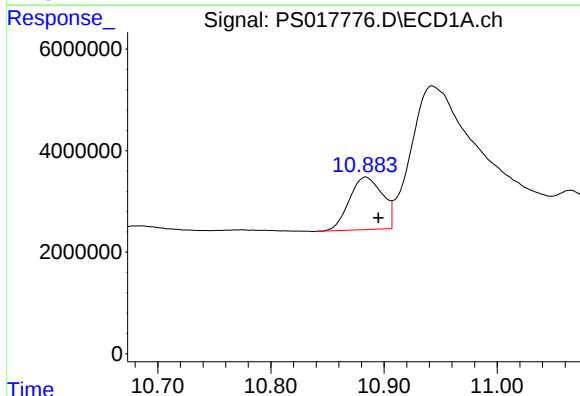

#15 Picloram

R.T.: 10.884 min
Delta R.T.: -0.011 min
Response: 21078864
Conc: 1.94 ng/ml

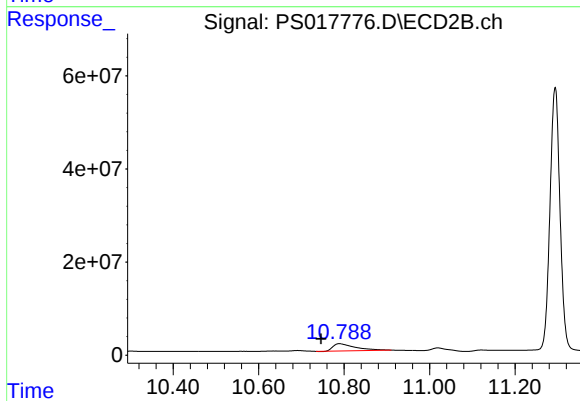

#15 Picloram

R.T.: 10.789 min
Delta R.T.: 0.042 min
Response: 55812172
Conc: 11.36 ng/ml