

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122021\
 Data File : PS017783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2021 20:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 00:23:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.126	6.714	793.8E6	341.4E6	507.910	572.716
Target Compounds							
2) T	3,5-DICHL...	6.391	0.000	154.0E6	0	68.940	N.D. #
5) T	DICAMBA	7.315	6.931f	6891674	40947773	1.090	15.371 #
6) T	MCP	0.000	6.931f	0	40947773	N.D.	18.813
9) T	2,4-D	8.296f	0.000	247.5E6	0	140.025	N.D. #
10) T	Pentachlo...	8.537	0.000	3448877	0	<MDL	N.D. #
15) T	Picloram	10.873	0.000	23975454	0	2.209	N.D. #
16) T	DCPA	11.331	0.000	5347054	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122021\
Data File : PS017783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2021 20:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 00:23:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

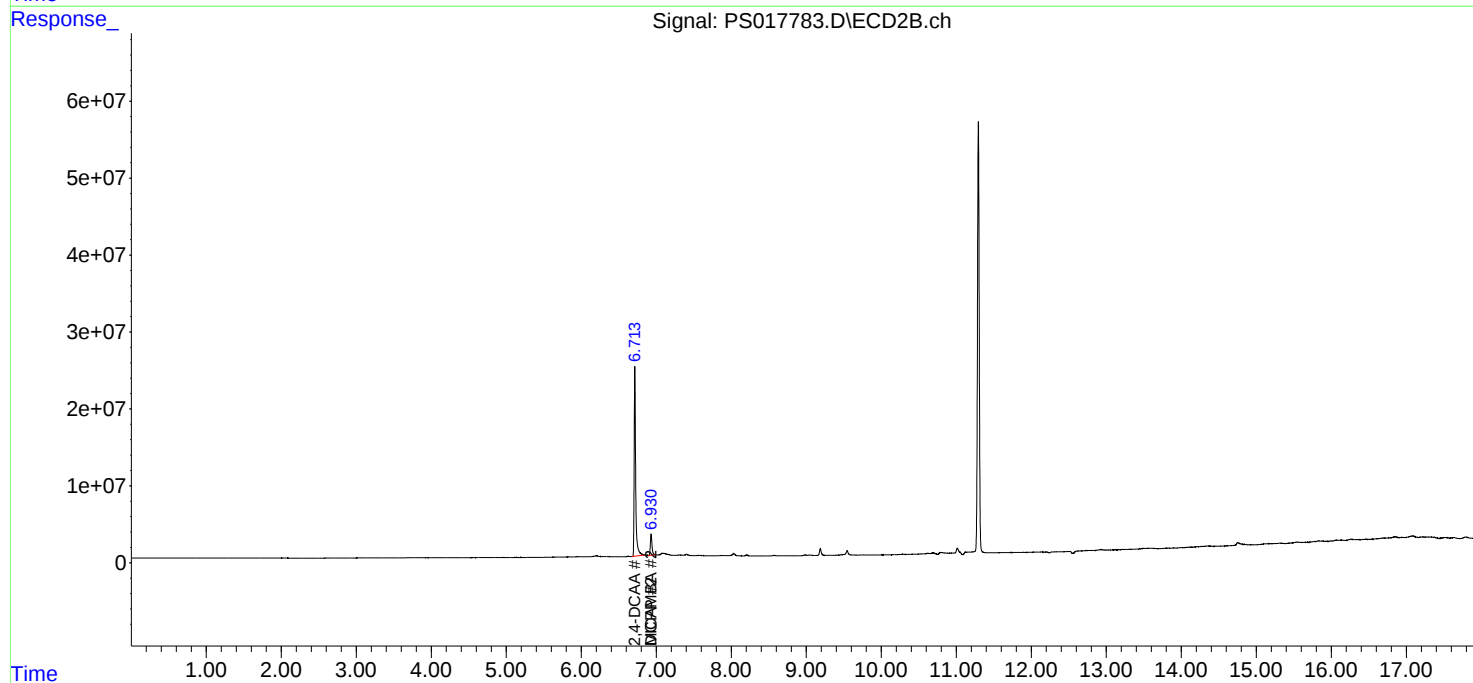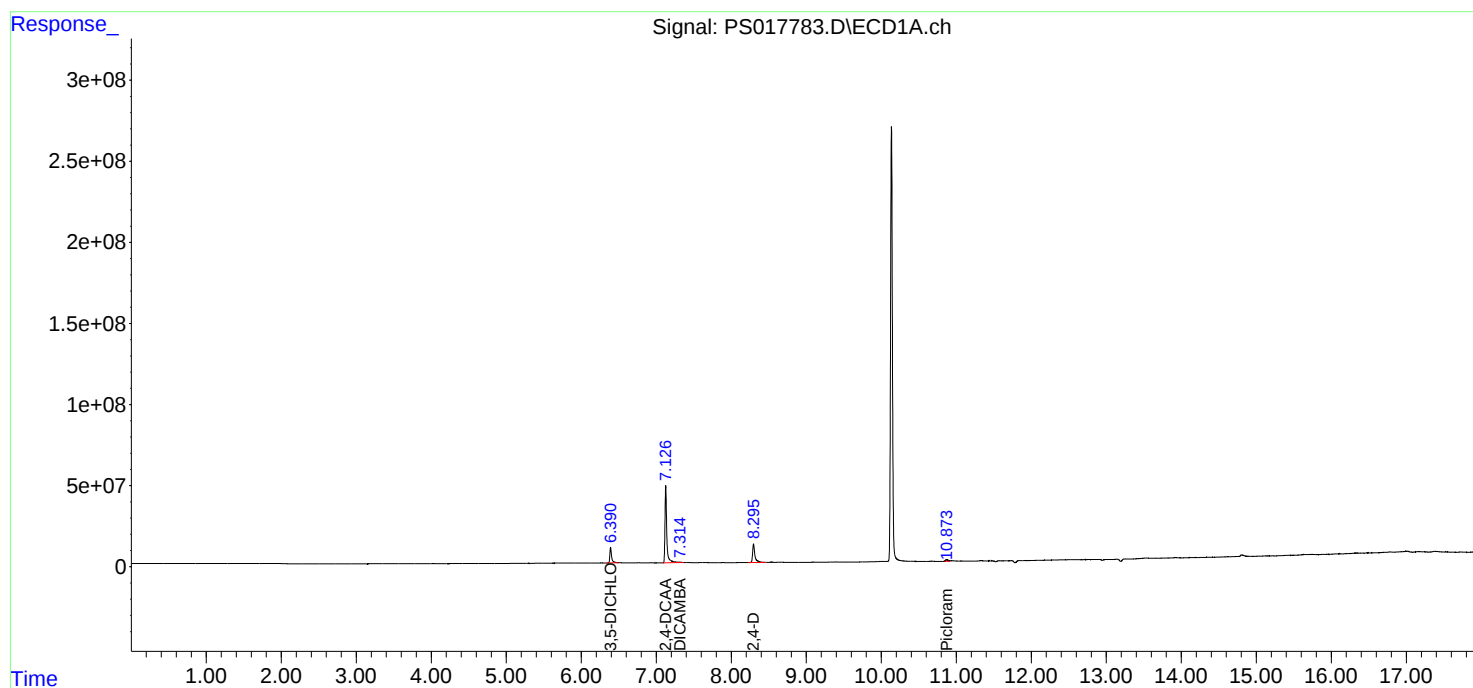


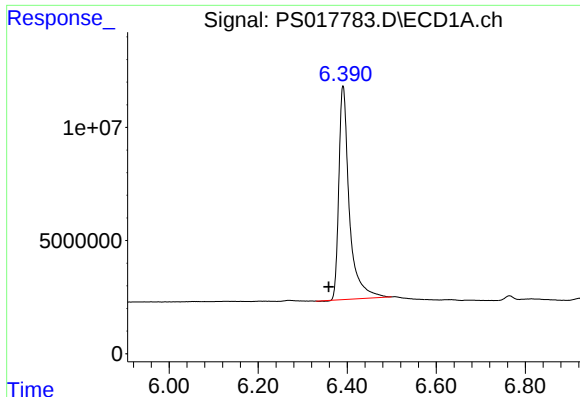

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.391 min
Delta R.T.: 0.032 min
Response: 154021309
Conc: 68.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

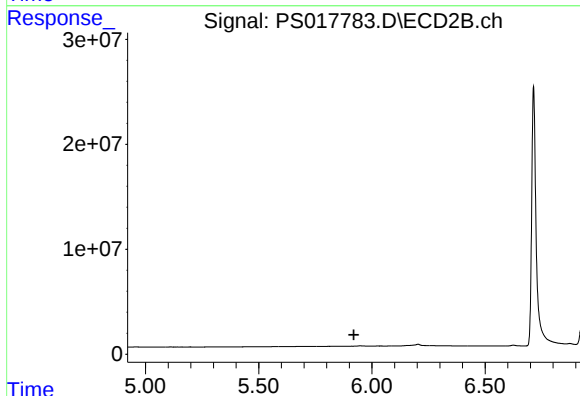


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

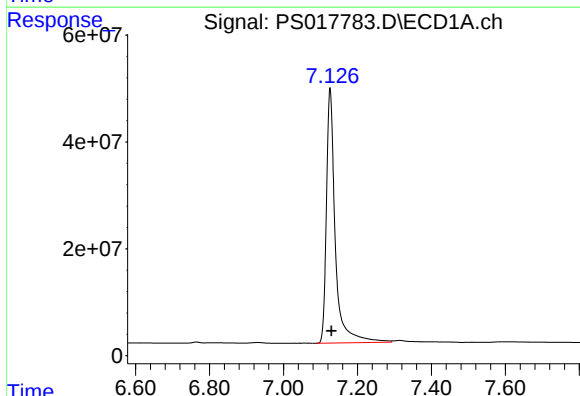


#4 2,4-DCAA

R.T.: 7.126 min
Delta R.T.: -0.004 min
Response: 793835809
Conc: 507.91 ng/ml

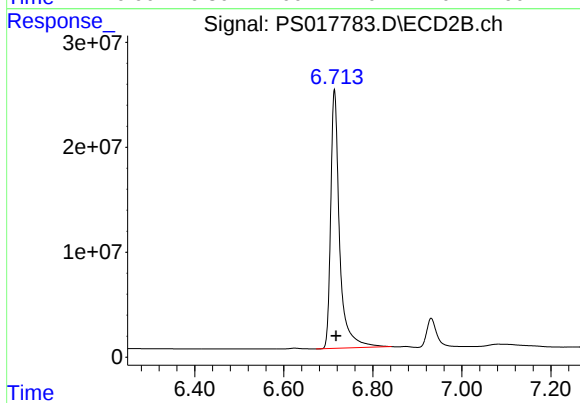

#4 2,4-DCAA


R.T.: 6.714 min
Delta R.T.: -0.004 min
Response: 341396746
Conc: 572.72 ng/ml

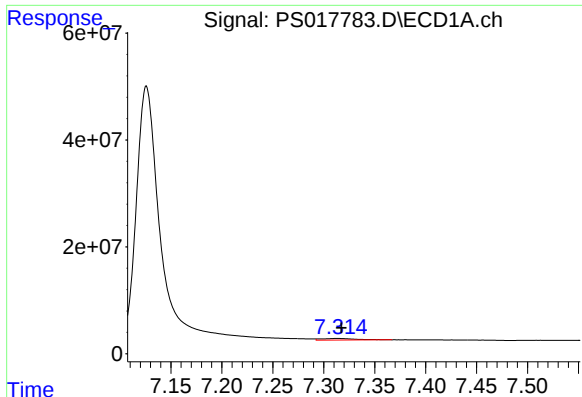

#5 DICAMBA


R.T.: 7.315 min
Delta R.T.: -0.003 min
Response: 6891674
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

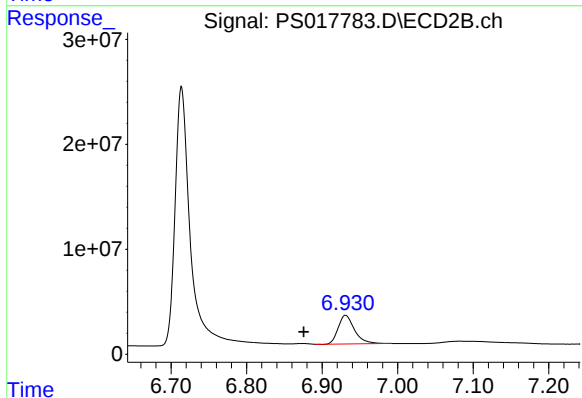


#5 DICAMBA

R.T.: 6.931 min
Delta R.T.: 0.055 min
Response: 40947773
Conc: 15.37 ng/ml

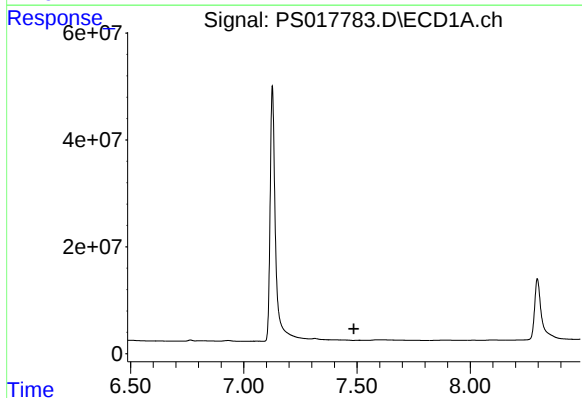


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

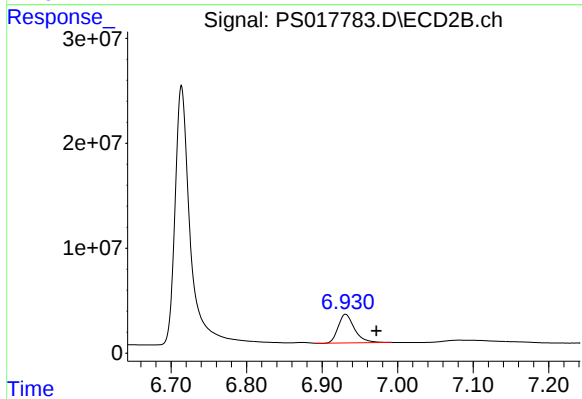

#6 MCPP


R.T.: 6.931 min
Delta R.T.: -0.041 min
Response: 40947773
Conc: 18.81 ug/ml

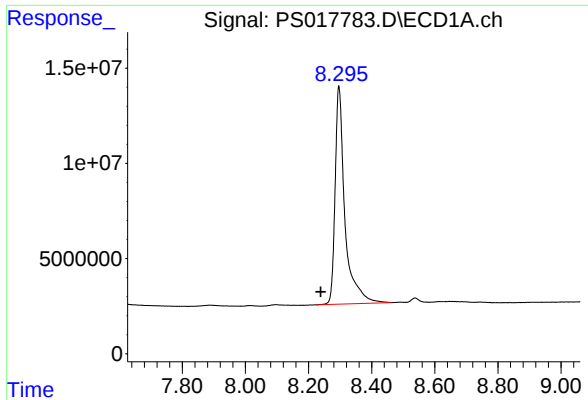

#9 2,4-D


R.T.: 8.296 min
Delta R.T.: 0.057 min
Response: 247546895
Conc: 140.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

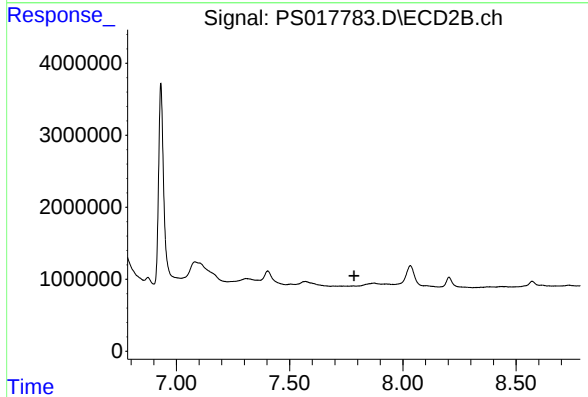


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

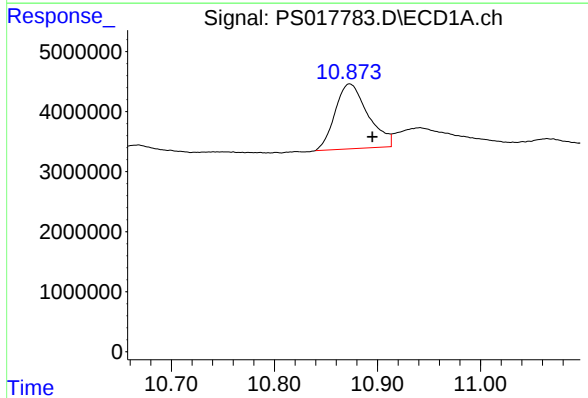

#15 Picloram

R.T.: 10.873 min
Delta R.T.: -0.022 min
Response: 23975454
Conc: 2.21 ng/ml

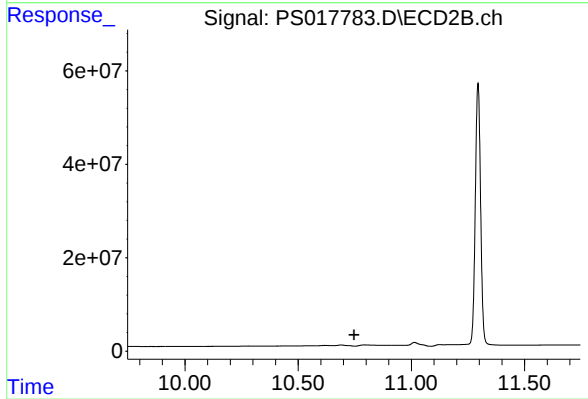

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.747 min
Response: 0
Conc: N.D.