

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122022\
 Data File : PS021470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 08:33
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 11:37:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.406	0.000	1016187	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.516	0.000	1140517	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.747	0.000	1101908	0	<MDL	N.D. #
3) T	4-Nitroph...	6.215	0.000	2399019	0	1.334	N.D. #
5) T	DICAMBA	6.528	0.000	347674	0	<MDL	N.D. #
8) T	DICHLORPROP	7.145	7.625	1443532	1265957	<MDL	<MDL #
9) T	2,4-D	7.343	0.000	16780710	0	4.392	N.D. #
10) T	Pentachlo...	7.551	8.322	1505969	1341237	<MDL	<MDL #
11) T	2,4,5-TP ...	8.085	8.642f	1059597	213854	<MDL	<MDL #
12) T	2,4,5-T	8.354	9.061	3788018	1103231	<MDL	<MDL #
13) T	2,4-DB	8.869	9.582	1188994	559241	<MDL	<MDL #
14) T	DINOSEB	9.906	0.000	1317658	0	<MDL	N.D. #
15) T	Picloram	9.765	10.873	53819738	33641531	1.879	2.069
16) T	DCPA	10.176	10.821	687085	3704654	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122022\
Data File : PS021470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 08:33
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 11:37:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

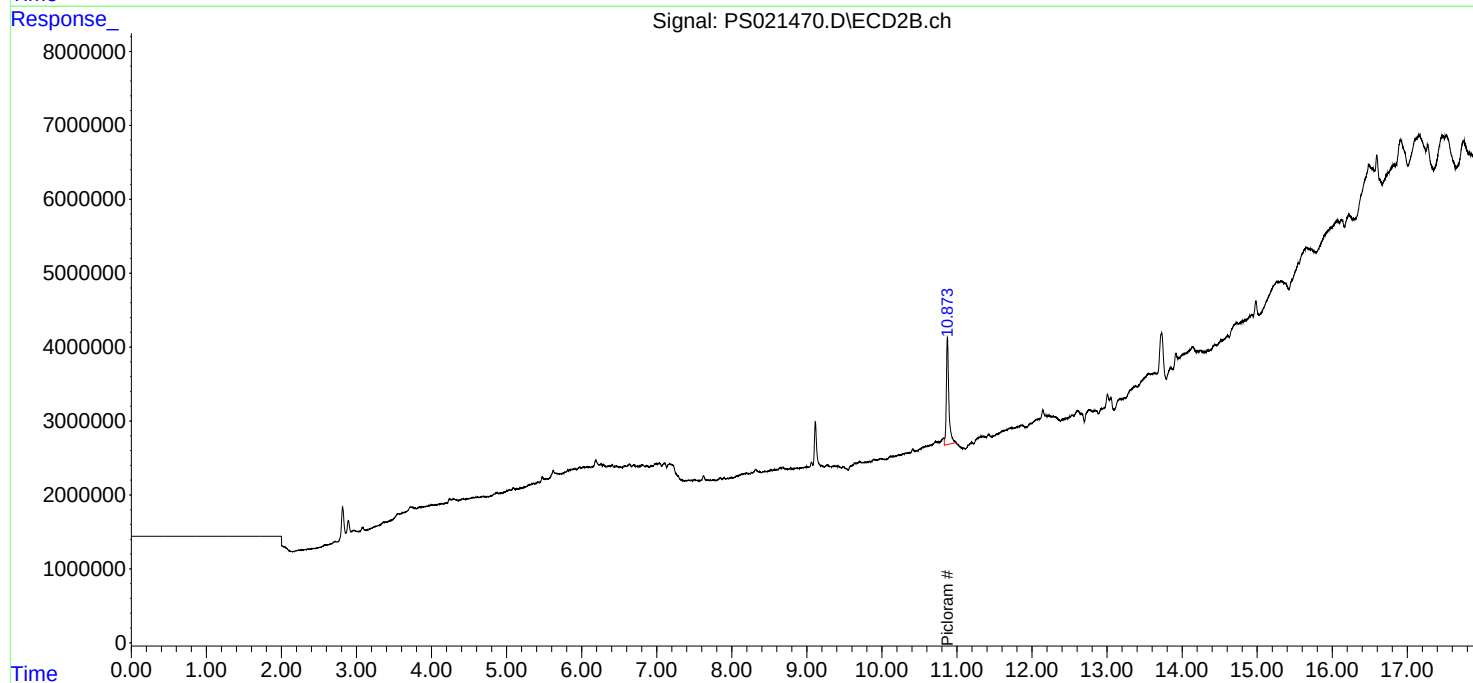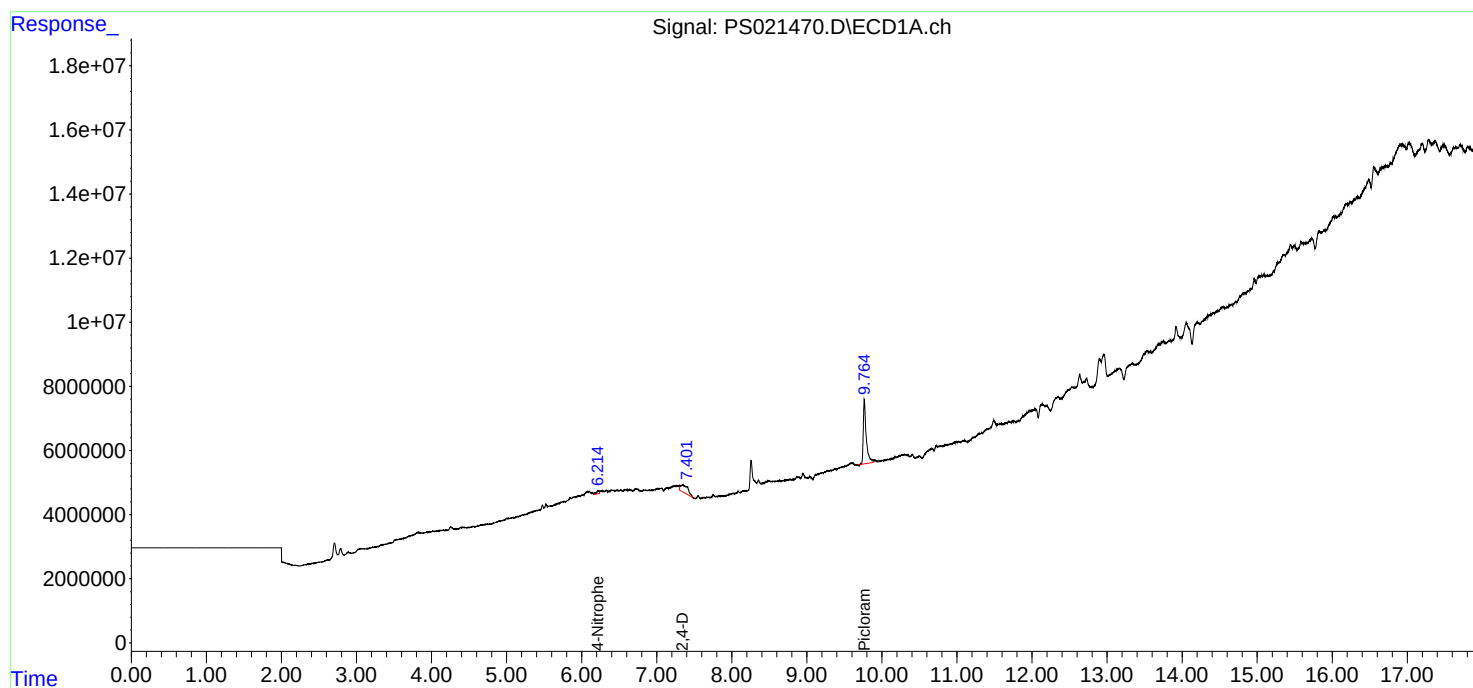


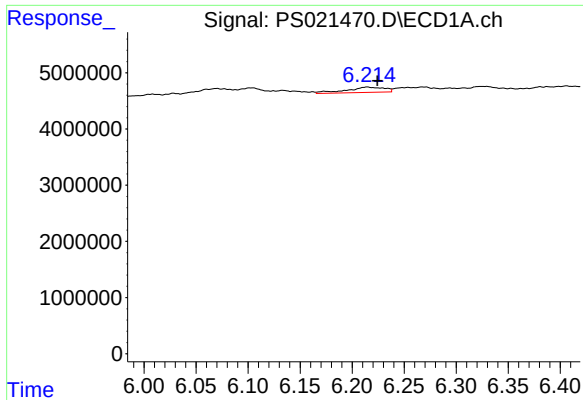

#3 4-Nitrophenol


R.T.: 6.215 min
Delta R.T.: -0.010 min
Response: 2399019
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

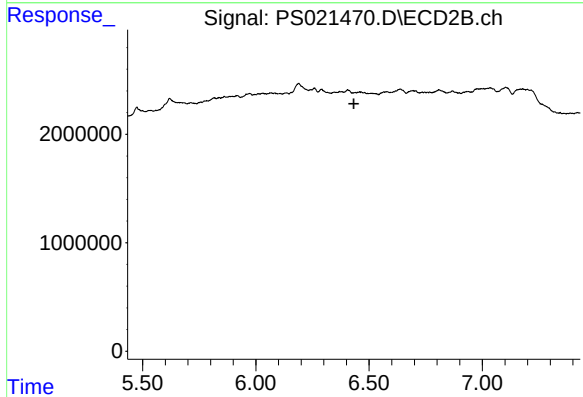


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

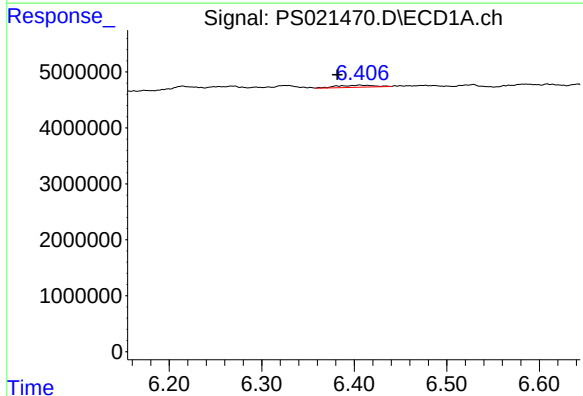


#4 2,4-DCAA

R.T.: 6.406 min
Delta R.T.: 0.024 min
Response: 1016187
Conc: N.D.

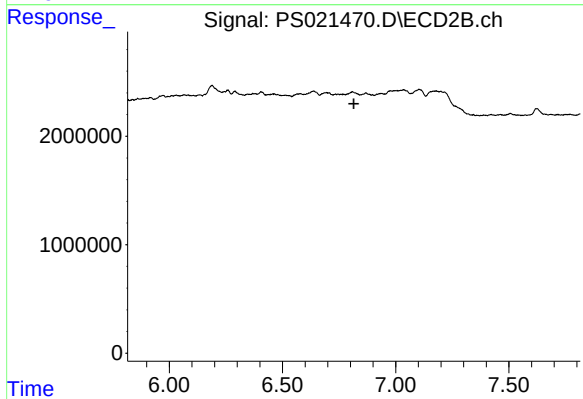

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

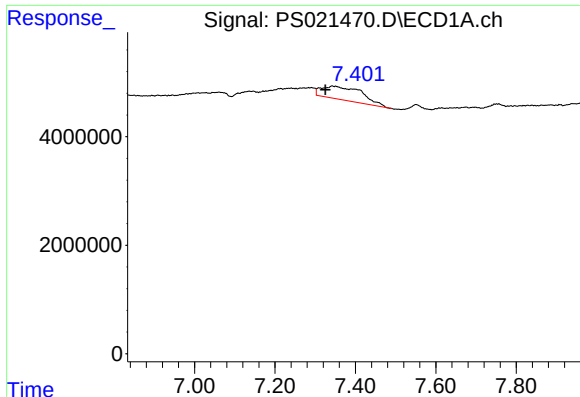

#9 2,4-D


R.T.: 7.343 min
Delta R.T.: 0.017 min
Response: 16780710
Conc: 4.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

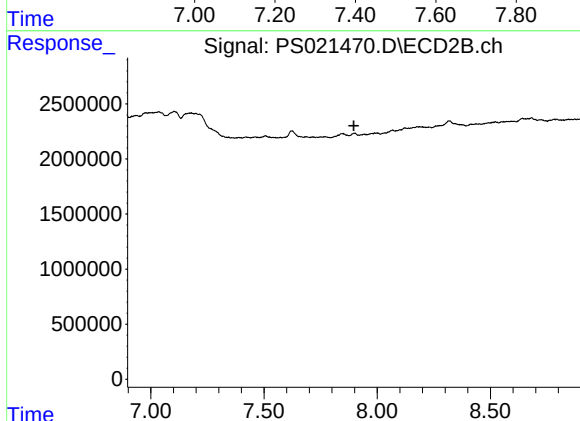


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.897 min
Response: 0
Conc: N.D.

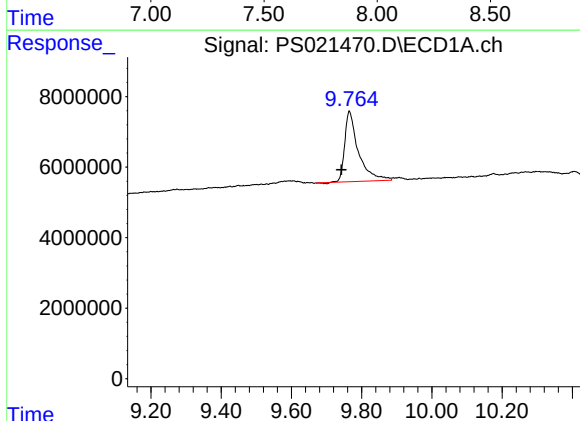

#15 Picloram

R.T.: 9.765 min
Delta R.T.: 0.023 min
Response: 53819738
Conc: 1.88 ng/ml

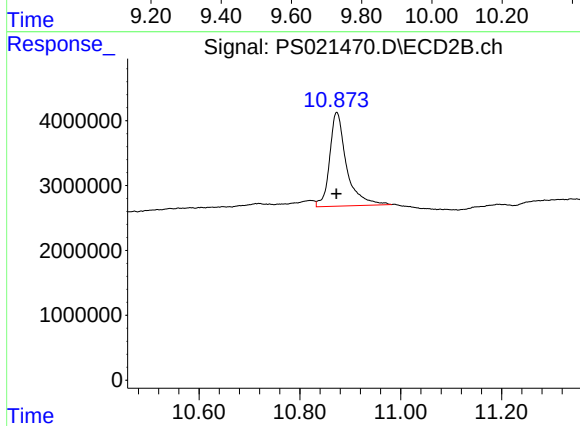

#15 Picloram

R.T.: 10.873 min
Delta R.T.: 0.001 min
Response: 33641531
Conc: 2.07 ng/ml