

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122022\
 Data File : PS021471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 08:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 11:37:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.384	6.809	1300.7E6	912.4E6	447.683	529.250
Target Compounds							
1) T	Dalapon	2.434f	0.000	276555	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.734	0.000	4045371	0	1.018	N.D. #
3) T	4-Nitroph...	6.229	0.000	5092823	0	2.832	N.D. #
6) T	MCP	0.000	7.121f	0	638815	N.D.	<MDL
7) T	MCPA	6.761	7.215f	2250861	13315499	<MDL	1.506 #
8) T	DICHLORPROP	0.000	7.645f	0	2927762	N.D.	1.486
10) T	Pentachlo...	7.552	0.000	445316	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.089	8.653	11460260	1353130	<MDL	<MDL #
12) T	2,4,5-T	8.313	9.080	13413933	1547285	<MDL	<MDL #
13) T	2,4-DB	8.840	9.637f	2302674	2538835	<MDL	1.766 #
14) T	DINOSEB	0.000	9.892	0	1471211	N.D.	<MDL
15) T	Picloram	9.734	10.900	2085365	24214948	<MDL	1.489 #
16) T	DCPA	10.170	10.821	1320876	491948	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122022\
Data File : PS021471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 08:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 11:37:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

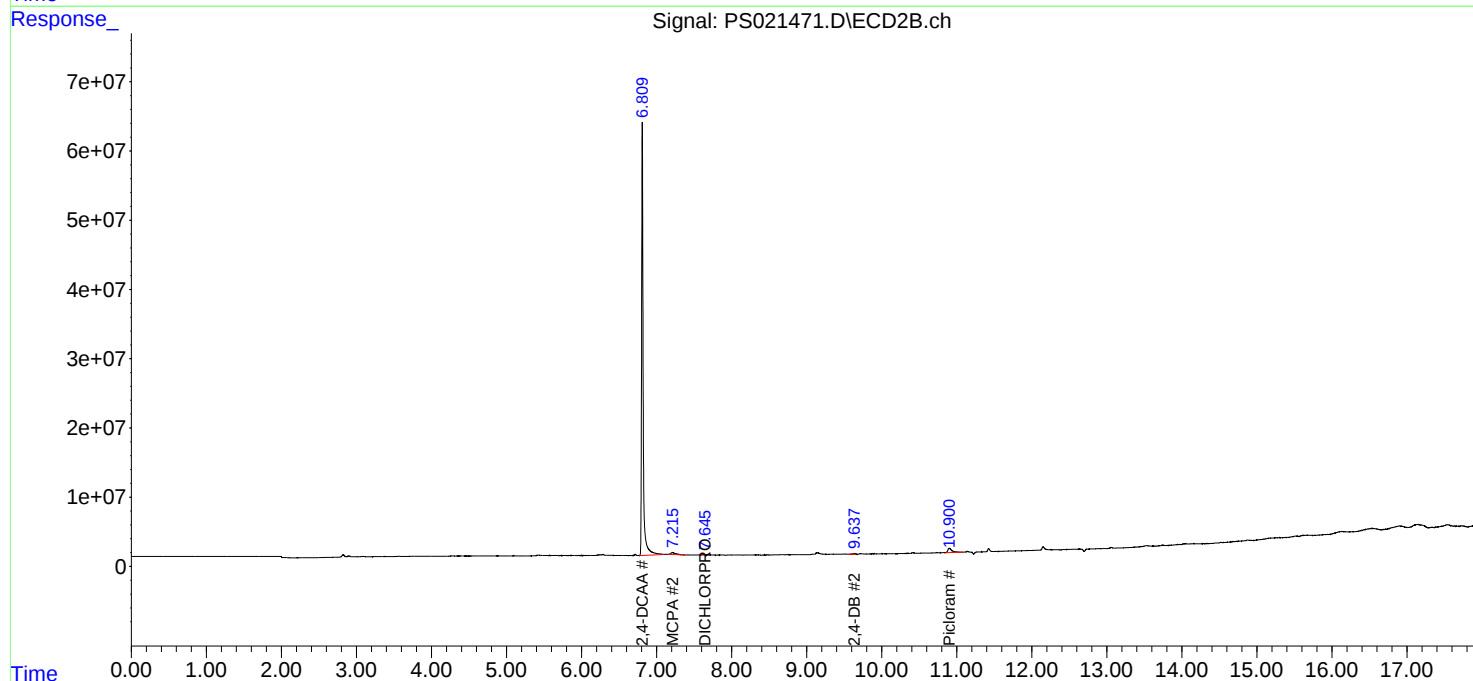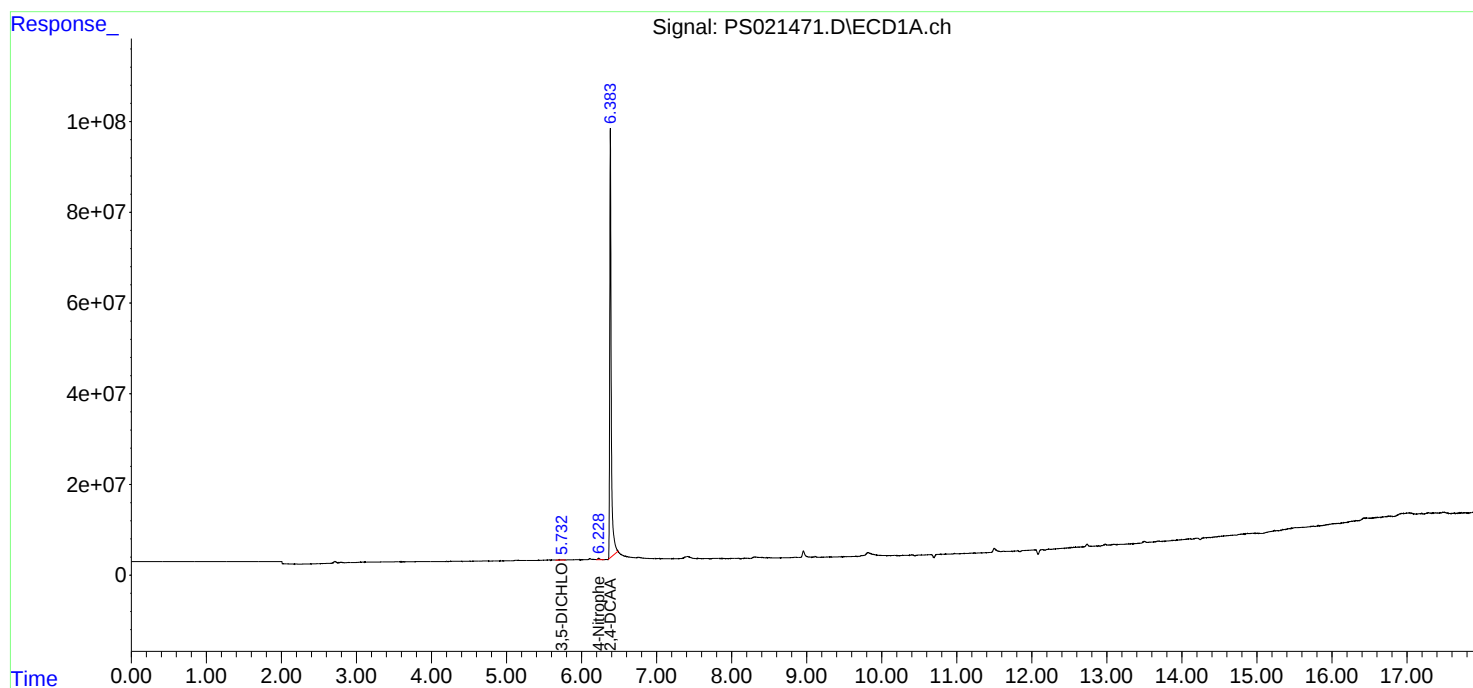


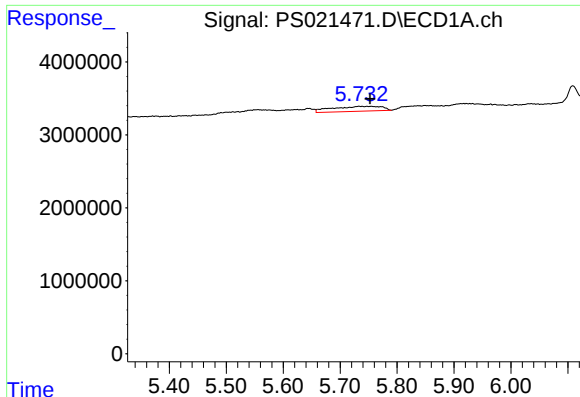

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.734 min
Delta R.T.: -0.018 min
Response: 4045371
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

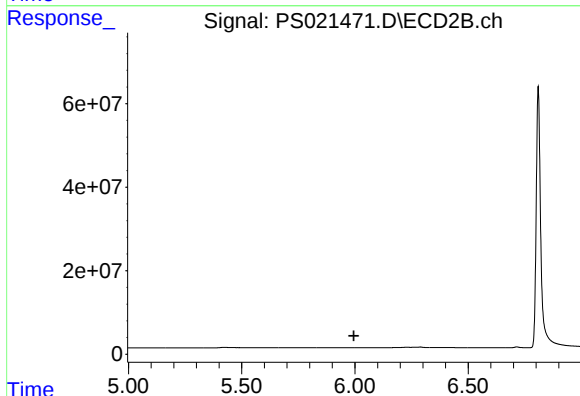


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

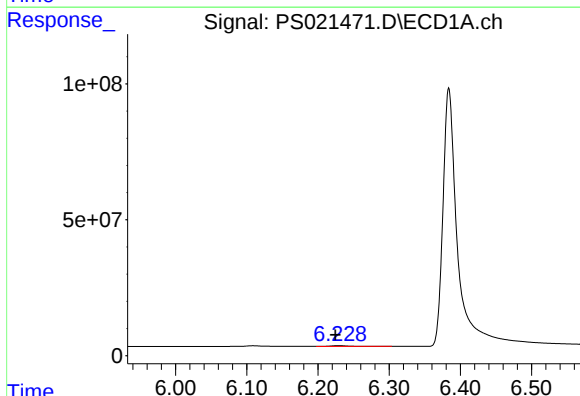


#3 4-Nitrophenol

R.T.: 6.229 min
Delta R.T.: 0.005 min
Response: 5092823
Conc: 2.83 ng/ml

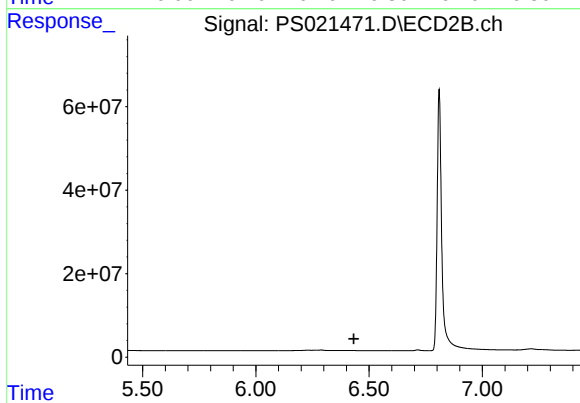

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

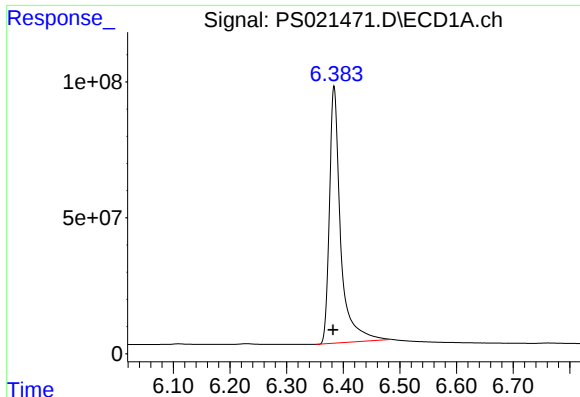

#4 2,4-DCAA


R.T.: 6.384 min
Delta R.T.: 0.002 min
Response: 1300740960
Conc: 447.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

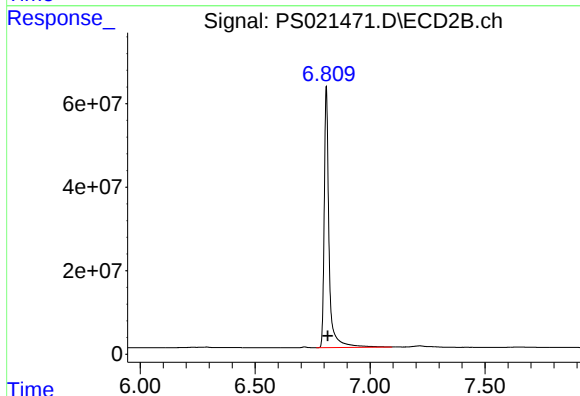


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.006 min
Response: 912424110
Conc: 529.25 ng/ml

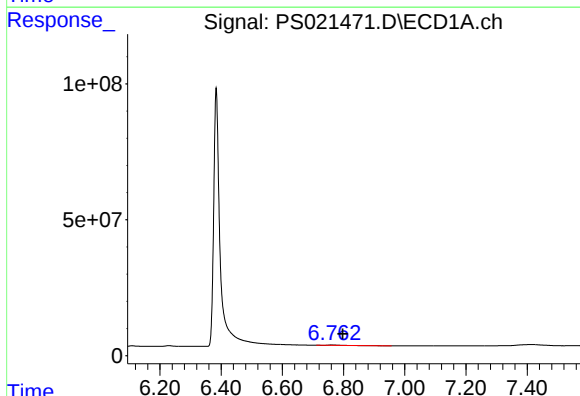


#7 MCPA

R.T.: 6.761 min
Delta R.T.: -0.036 min
Response: 2250861
Conc: N.D.

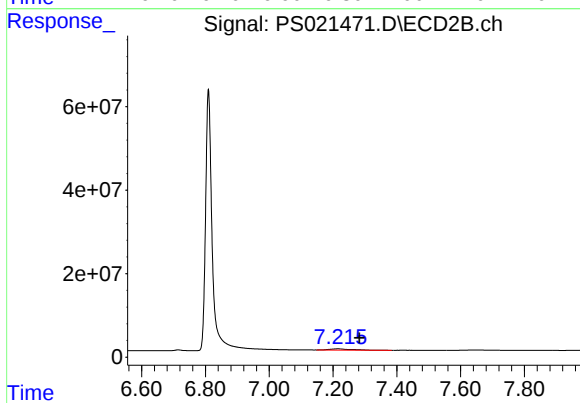

#7 MCPA


R.T.: 7.215 min
Delta R.T.: -0.067 min
Response: 13315499
Conc: 1.51 ug/ml

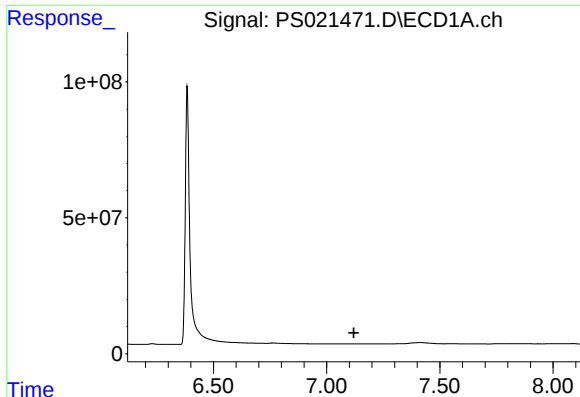

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

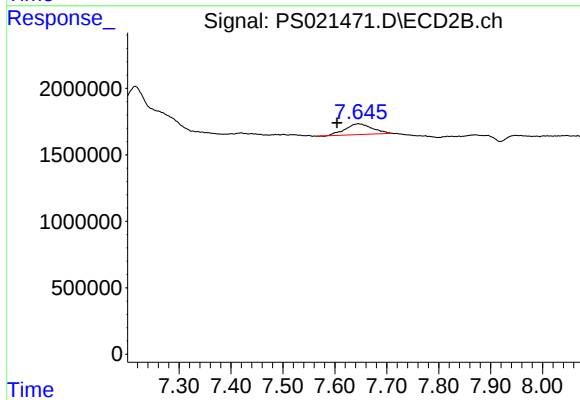


#8 DICHLORPROP

R.T.: 7.645 min
Delta R.T.: 0.041 min
Response: 2927762
Conc: 1.49 ng/ml

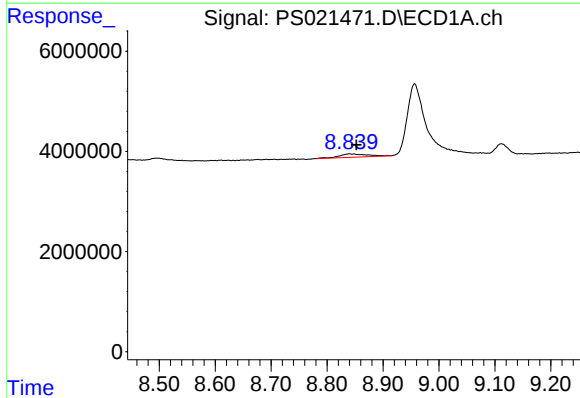


#13 2,4-DB

R.T.: 8.840 min
Delta R.T.: -0.012 min
Response: 2302674
Conc: N.D.

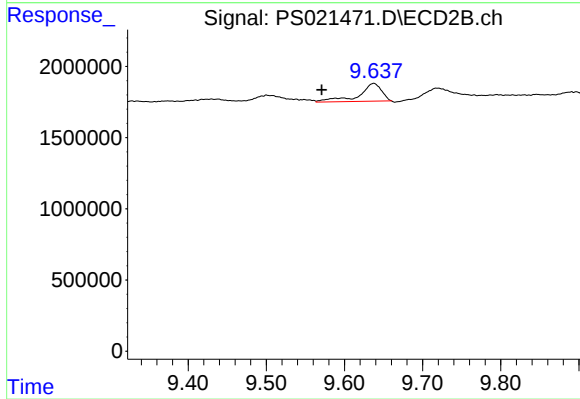

#13 2,4-DB


R.T.: 9.637 min
Delta R.T.: 0.066 min
Response: 2538835
Conc: 1.77 ng/ml

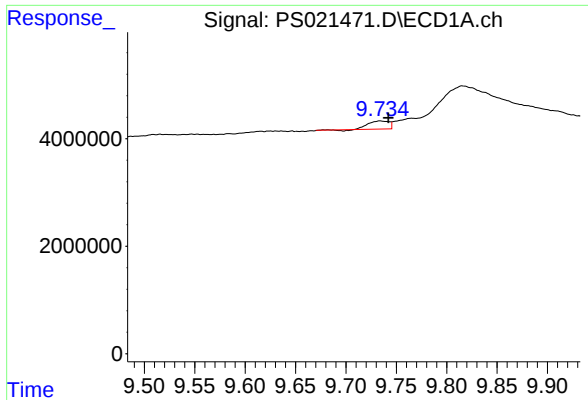

#15 Picloram

R.T.: 9.734 min
Delta R.T.: -0.008 min
Response: 2085365
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

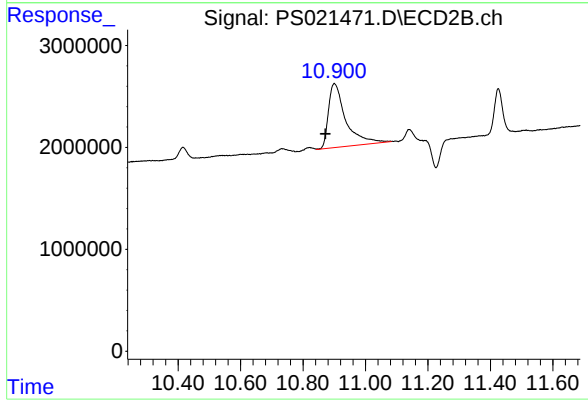

#15 Picloram

R.T.: 10.900 min
Delta R.T.: 0.028 min
Response: 24214948
Conc: 1.49 ng/ml