

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122022\
 Data File : PS021495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 20:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 03:33:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.377	6.810	1328.6E6	932.6E6	457.258	540.931
Target Compounds							
1) T	Dalapon	2.510	0.000	2232	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.727	0.000	2133624	0	<MDL	N.D. #
3) T	4-Nitroph...	6.223	0.000	4646514	0	2.584	N.D. #
6) T	MCP	0.000	7.121f	0	2748650	N.D.	<MDL
7) T	MCPA	6.757f	7.214f	7331677	35329963	<MDL	3.995 #
8) T	DICHLORPROP	7.132	7.650f	351671	5904268	<MDL	2.998 #
11) T	2,4,5-TP ...	8.085	8.687	5447203	1173575	<MDL	<MDL #
12) T	2,4,5-T	8.337	9.088	3835849	1703451	<MDL	<MDL #
13) T	2,4-DB	8.841	9.638f	1158115	1776936	<MDL	1.236 #
14) T	DINOSEB	9.899	0.000	2461089	0	<MDL	N.D. #
15) T	Picloram	9.754	10.920f	6180465	1212550	<MDL	<MDL #
16) T	DCPA	10.165	10.820	2241833	1182513	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122022\
Data File : PS021495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 20:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 03:33:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

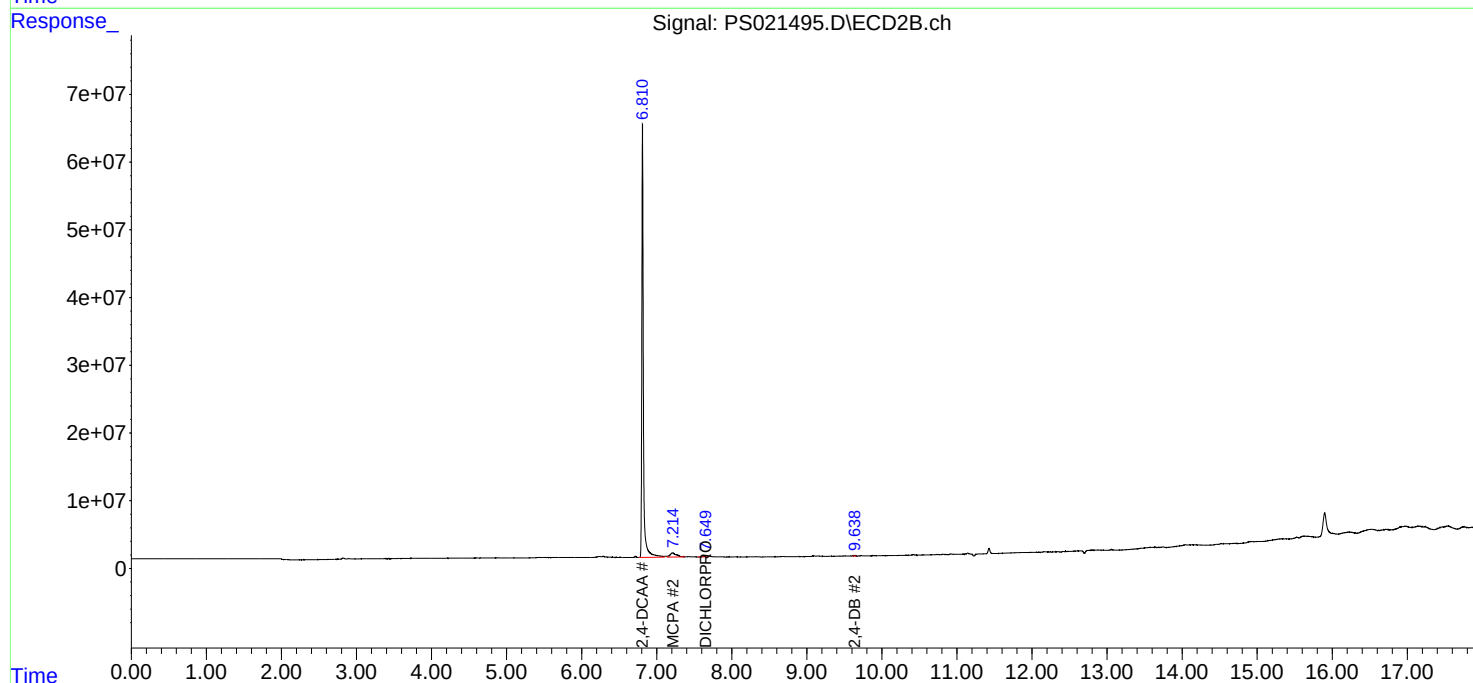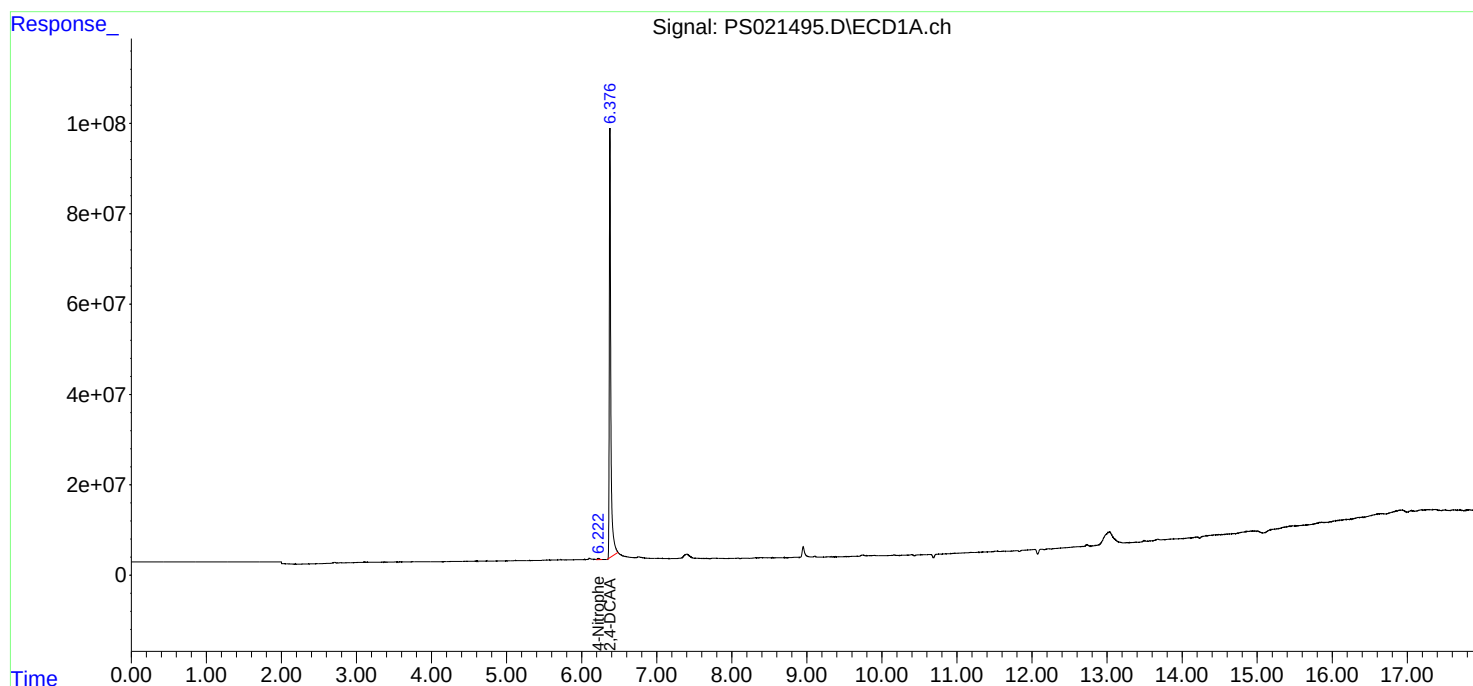


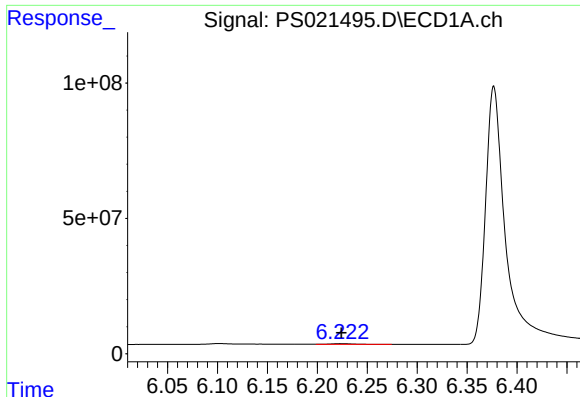

#3 4-Nitrophenol


R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 4646514
Conc: 2.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

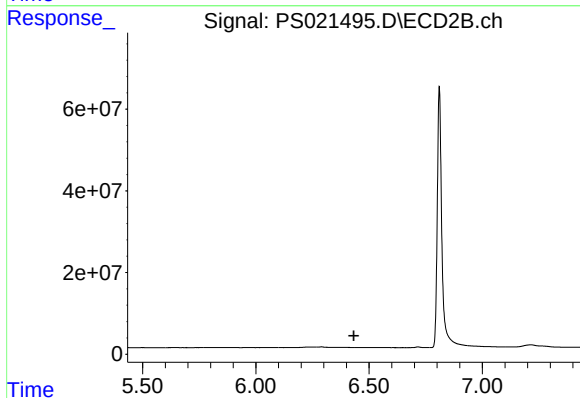


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

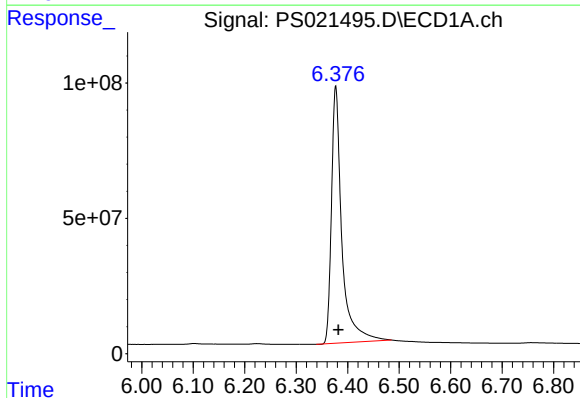


#4 2,4-DCAA

R.T.: 6.377 min
Delta R.T.: -0.005 min
Response: 1328561414
Conc: 457.26 ng/ml

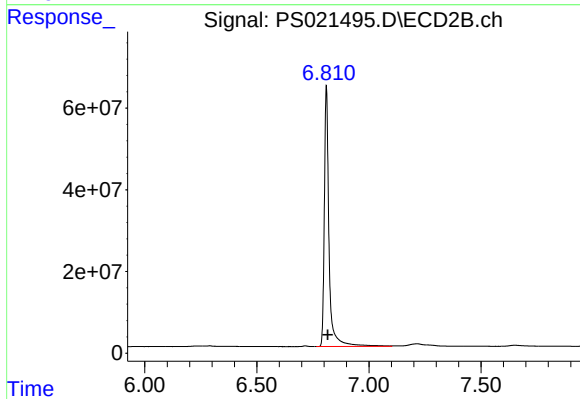

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.006 min
Response: 932561996
Conc: 540.93 ng/ml

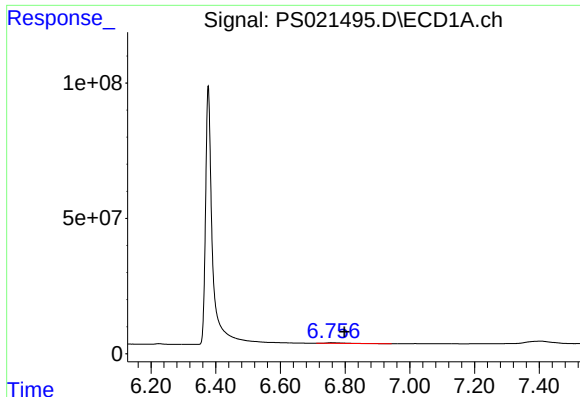

#7 MCPA


R.T.: 6.757 min
Delta R.T.: -0.040 min
Response: 7331677
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

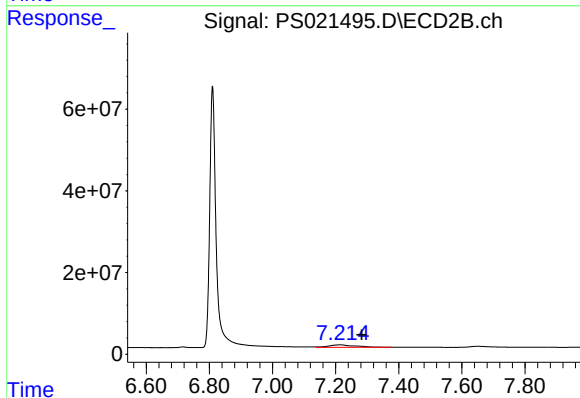


#7 MCPA

R.T.: 7.214 min
Delta R.T.: -0.068 min
Response: 35329963
Conc: 4.00 ug/ml

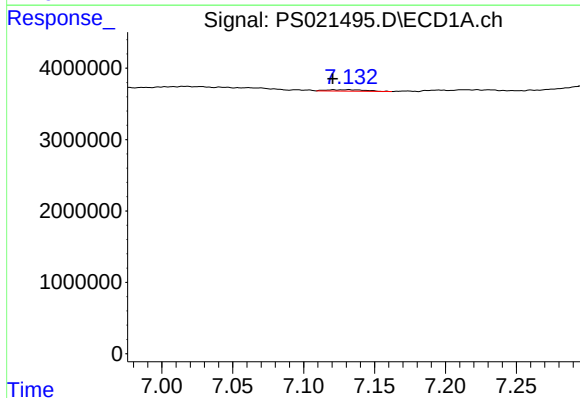


#8 DICHLORPROP

R.T.: 7.132 min
Delta R.T.: 0.011 min
Response: 351671
Conc: N.D.

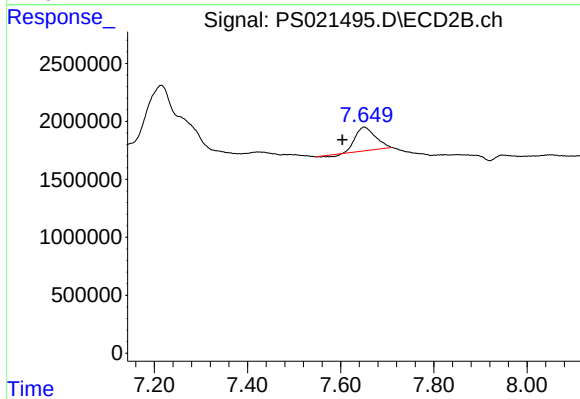

#8 DICHLORPROP


R.T.: 7.650 min
Delta R.T.: 0.046 min
Response: 5904268
Conc: 3.00 ng/ml

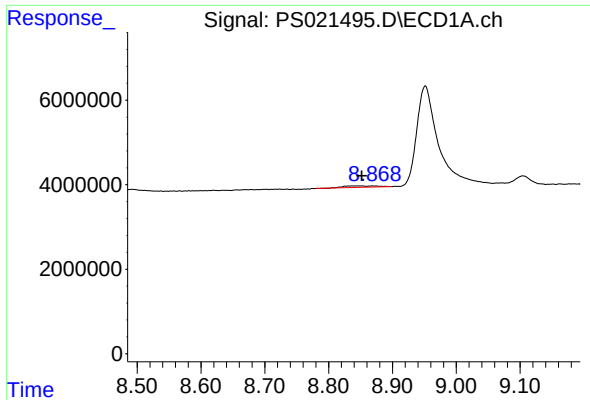

#13 2,4-DB

R.T.: 8.841 min
Delta R.T.: -0.011 min
Response: 1158115
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

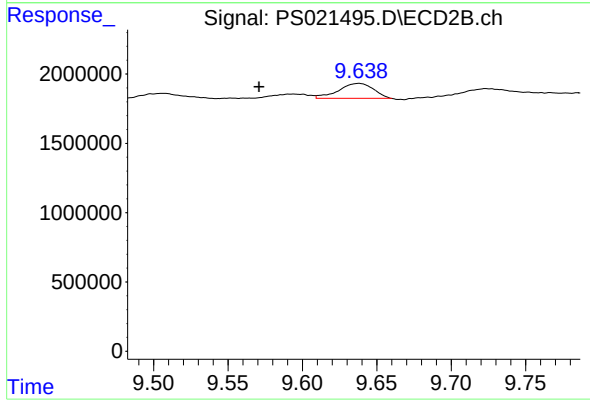

#13 2,4-DB

R.T.: 9.638 min
Delta R.T.: 0.067 min
Response: 1776936
Conc: 1.24 ng/ml