

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122120\
 Data File : PS013567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2020 12:30
 Operator : DD\AJ
 Sample : PB133689BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 13:34:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.912	587.9E6	267.9E6	631.396	680.944
Target Compounds							
1) T	Dalapon	3.028	2.621	629.5E6	325.2E6	586.059	618.730
2) T	3,5-DICHL...	6.426	6.066	764.3E6	346.7E6	596.312	558.030
3) T	4-Nitroph...	7.044	6.525	253.3E6	118.3E6	562.250	496.507
5) T	DICAMBA	7.400	7.078	2064.0E6	952.3E6	558.904	566.646
6) T	MCPD	7.566	7.171	180.6E6	77994271	66.517	58.856
7) T	MCPA	7.715	7.385	236.5E6	142.7E6	60.517	68.619
8) T	DICHLORPROP	8.091	7.703	528.8E6	271.5E6	571.320	607.511
9) T	2,4-D	8.323	8.000	631.4E6	332.2E6	627.221	615.574
10) T	Pentachlo...	8.629	8.425	8173.8E6	3472.6E6	609.867	615.810
11) T	2,4,5-TP ...	9.177	8.784	3251.9E6	1485.5E6	610.020	632.748
12) T	2,4,5-T	9.464	9.167	3190.0E6	1367.6E6	576.969	612.971
13) T	2,4-DB	10.017	9.673	367.5E6	178.0E6	400.093	608.447 #
14) T	DINOSEB	11.171	10.001	2313.3E6	936.1E6	545.869	566.369
15) T	Picloram	11.007	10.996	3281.6E6	1696.0E6	476.428	487.105
16) T	DCPA	11.438	10.928	3775.4E6	1814.7E6	556.701	596.700



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122120\
Data File : PS013567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2020 12:30
Operator : DD\AJ
Sample : PB133689BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 13:34:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

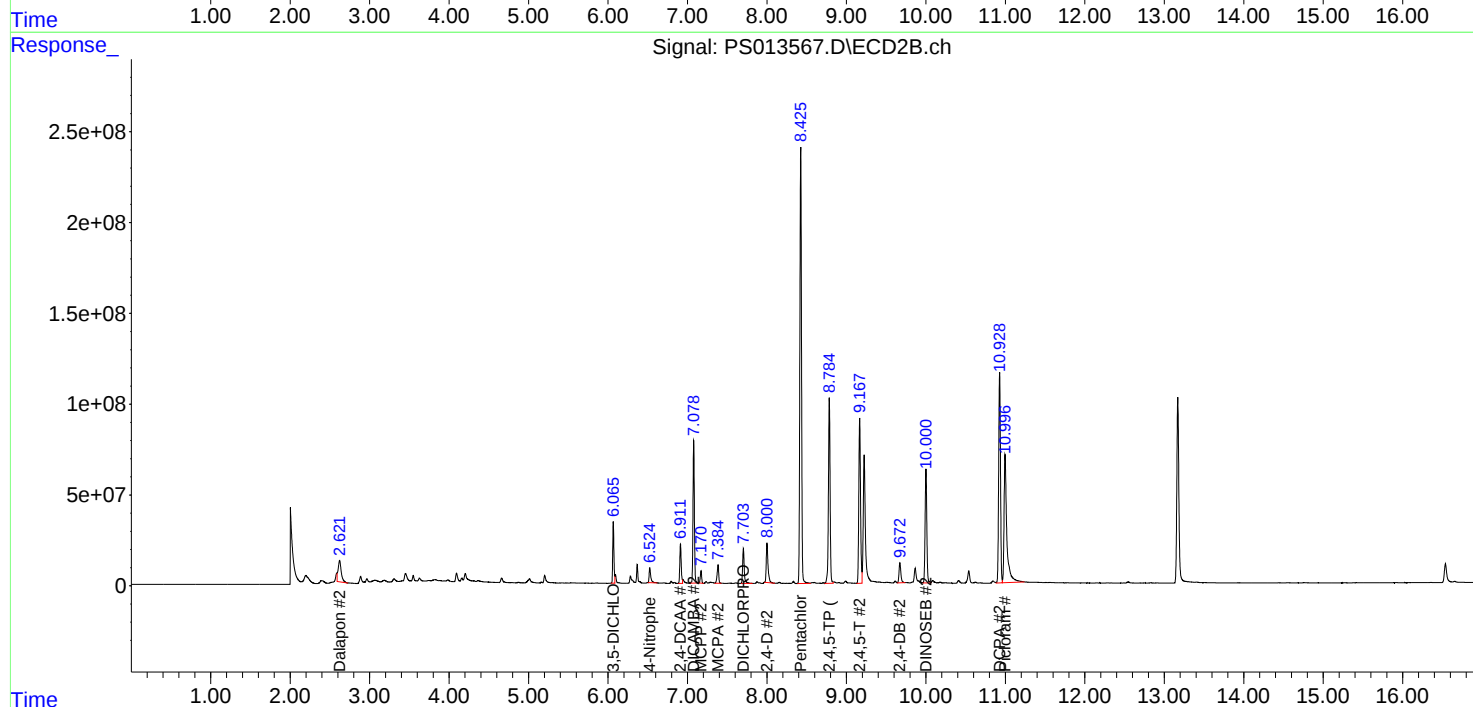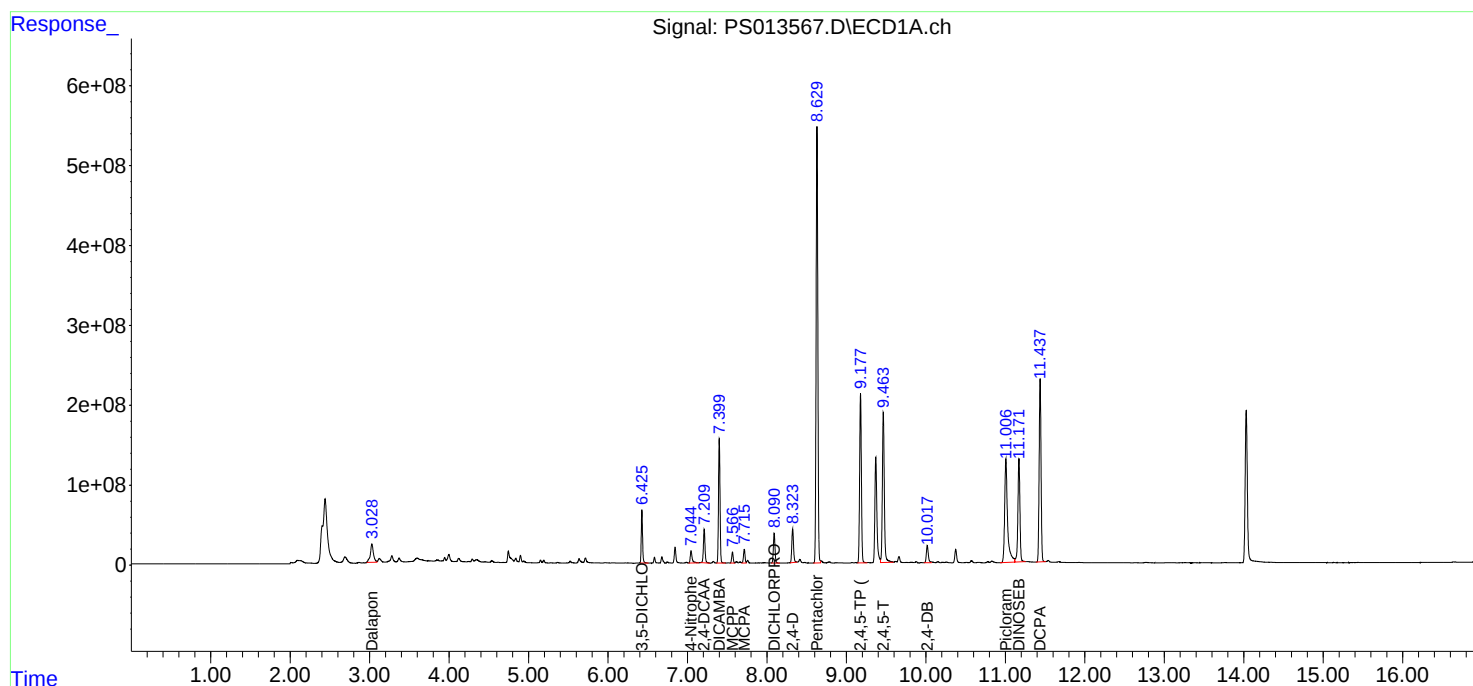


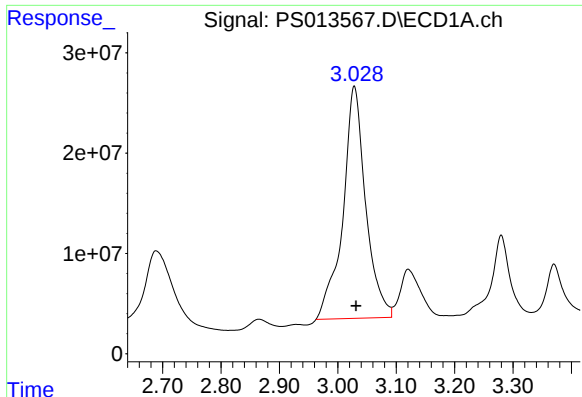

#1 Dalapon


R.T.: 3.028 min
Delta R.T.: -0.003 min
Response: 629546070
Conc: 586.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

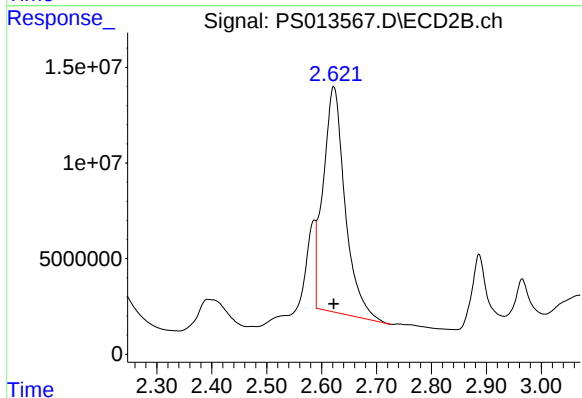


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 325161744
Conc: 618.73 ng/ml

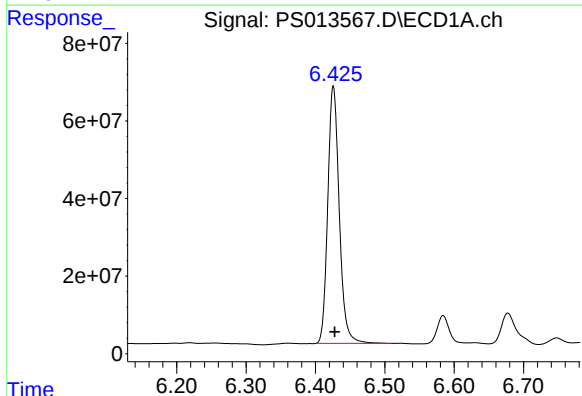


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.426 min
Delta R.T.: -0.002 min
Response: 764296564
Conc: 596.31 ng/ml

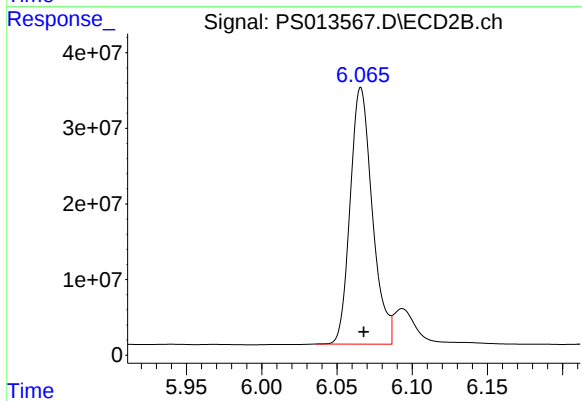

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.066 min
Delta R.T.: -0.002 min
Response: 346741686
Conc: 558.03 ng/ml

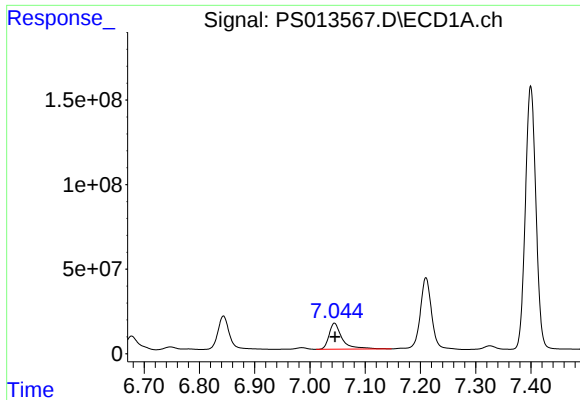

#3 4-Nitrophenol


R.T.: 7.044 min
Delta R.T.: -0.001 min
Response: 253334257
Conc: 562.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

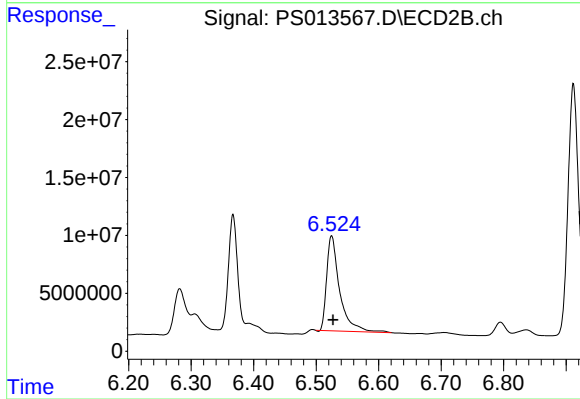


#3 4-Nitrophenol

R.T.: 6.525 min
Delta R.T.: -0.002 min
Response: 118342242
Conc: 496.51 ng/ml

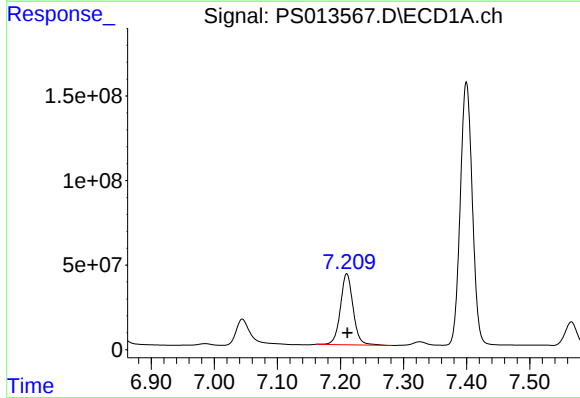


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 587866706
Conc: 631.40 ng/ml

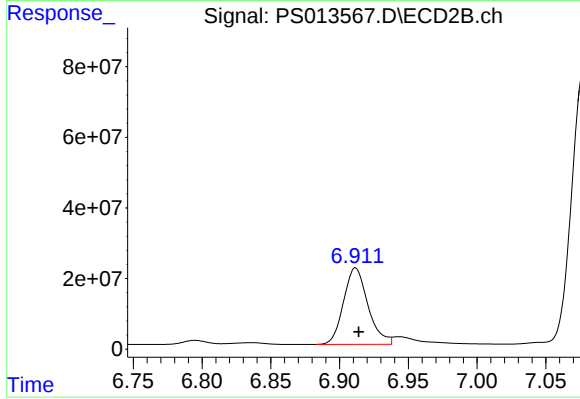

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: -0.002 min
Response: 267857084
Conc: 680.94 ng/ml

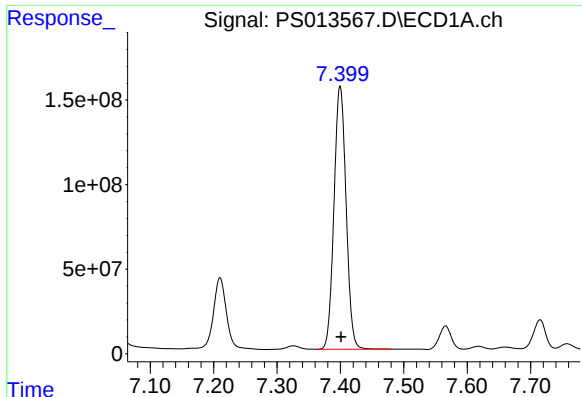

#5 DICAMBA


R.T.: 7.400 min
Delta R.T.: -0.001 min
Response: 2063969127
Conc: 558.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

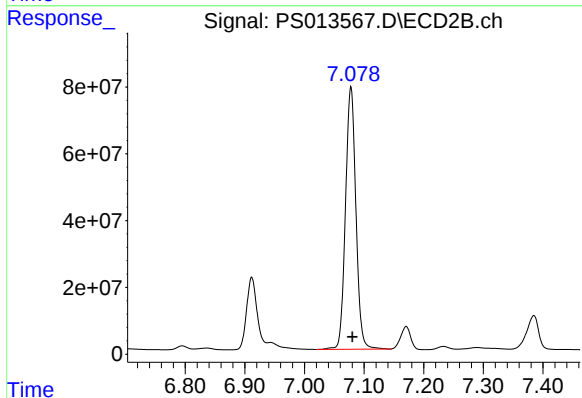


#5 DICAMBA

R.T.: 7.078 min
Delta R.T.: -0.002 min
Response: 952314425
Conc: 566.65 ng/ml

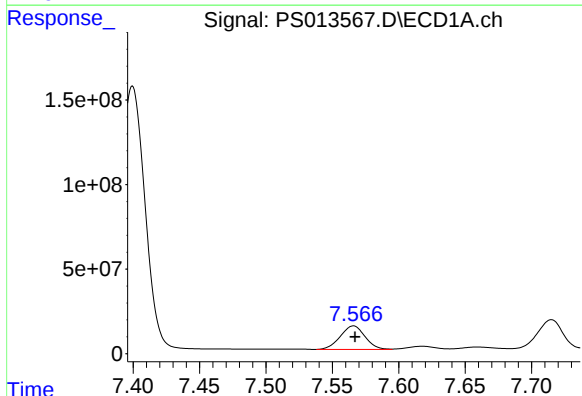


#6 MCPP

R.T.: 7.566 min
Delta R.T.: -0.001 min
Response: 180613578
Conc: 66.52 ug/ml

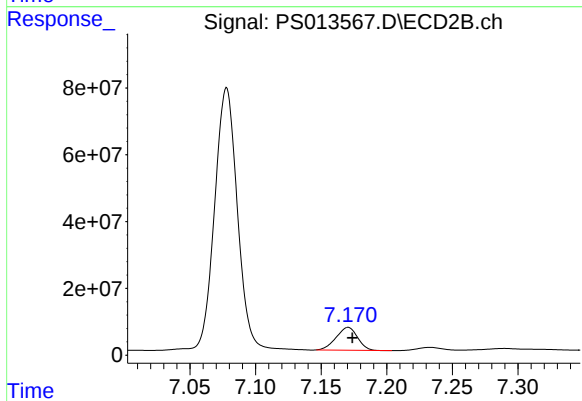

#6 MCPP


R.T.: 7.171 min
Delta R.T.: -0.003 min
Response: 77994271
Conc: 58.86 ug/ml

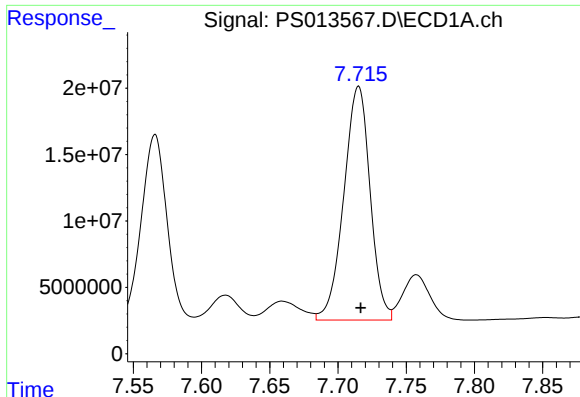

#7 MCPA


R.T.: 7.715 min
Delta R.T.: -0.001 min
Response: 236535993
Conc: 60.52 ug/ml

Instrument :
ECD_S
ClientSampleId :

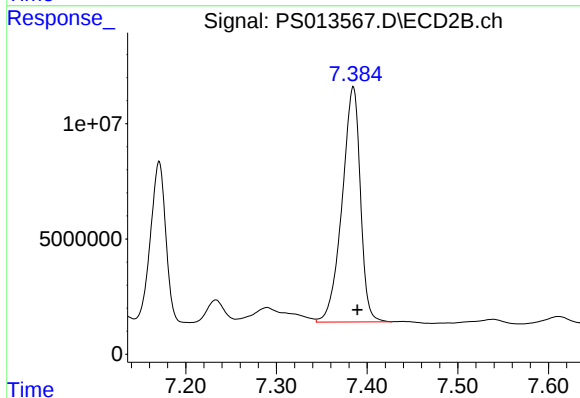


#7 MCPA

R.T.: 7.385 min
Delta R.T.: -0.005 min
Response: 142704159
Conc: 68.62 ug/ml

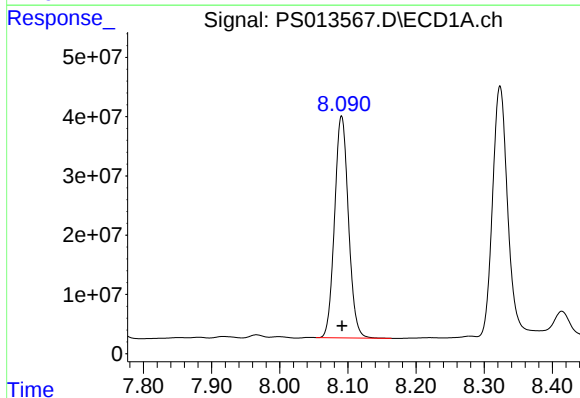


#8 DICHLORPROP

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 528788748
Conc: 571.32 ng/ml

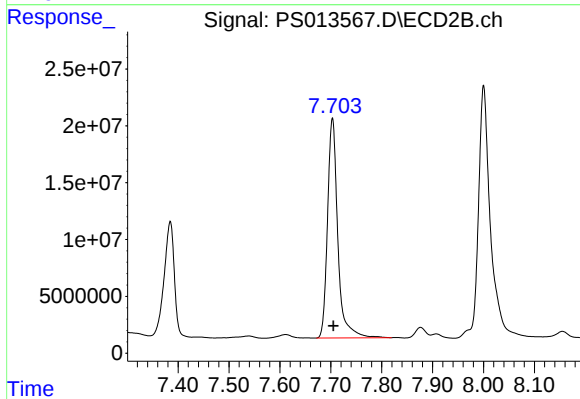

#8 DICHLORPROP


R.T.: 7.703 min
Delta R.T.: -0.002 min
Response: 271504142
Conc: 607.51 ng/ml

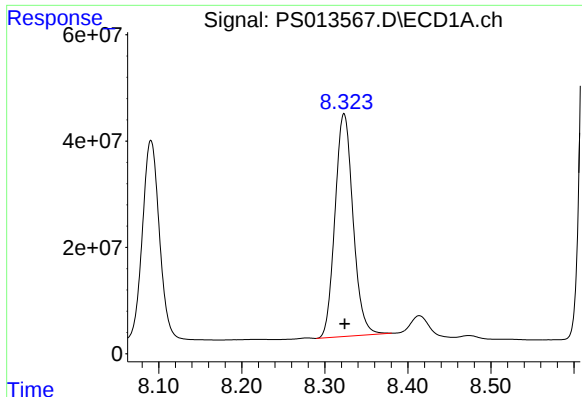

#9 2,4-D


R.T.: 8.323 min
Delta R.T.: 0.000 min
Response: 631400917
Conc: 627.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

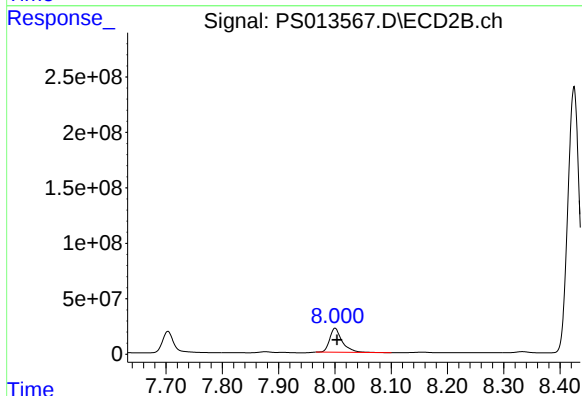


#9 2,4-D

R.T.: 8.000 min
Delta R.T.: -0.003 min
Response: 332162593
Conc: 615.57 ng/ml

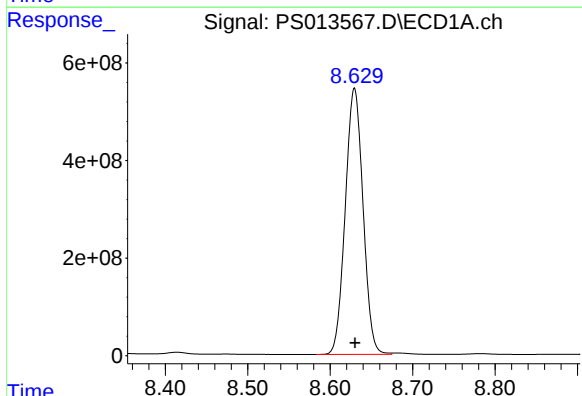


#10 Pentachlorophenol

R.T.: 8.629 min
Delta R.T.: 0.000 min
Response: 8173804469
Conc: 609.87 ng/ml

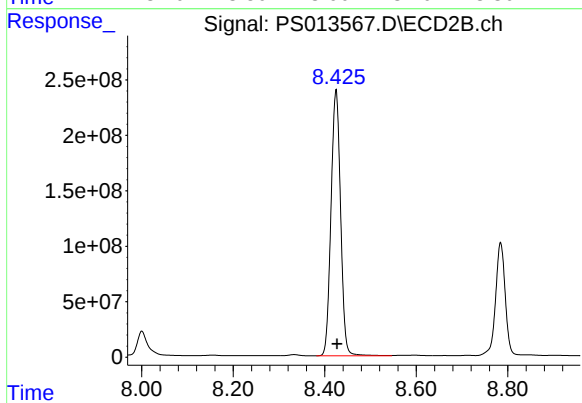

#10 Pentachlorophenol


R.T.: 8.425 min
Delta R.T.: -0.002 min
Response: 3472592838
Conc: 615.81 ng/ml

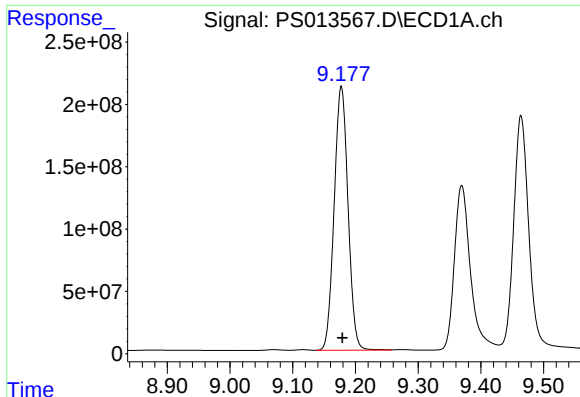

#11 2,4,5-TP (SILVEX)


R.T.: 9.177 min
Delta R.T.: -0.002 min
Response: 3251885326
Conc: 610.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

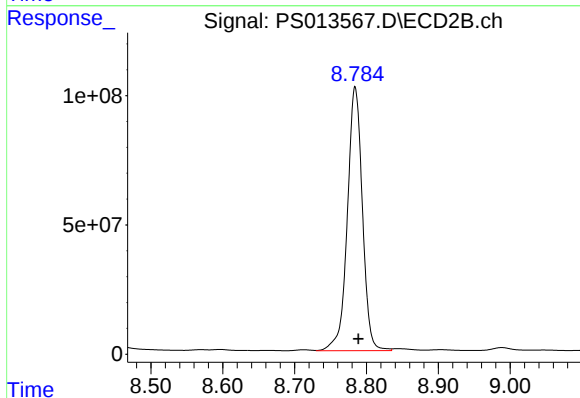


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: -0.004 min
Response: 1485496796
Conc: 632.75 ng/ml

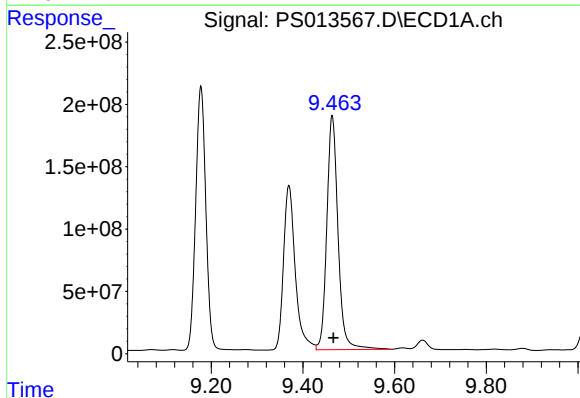


#12 2,4,5-T

R.T.: 9.464 min
Delta R.T.: -0.003 min
Response: 3189998581
Conc: 576.97 ng/ml

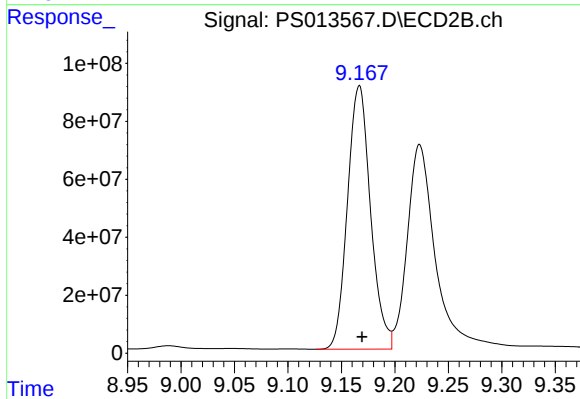

#12 2,4,5-T


R.T.: 9.167 min
Delta R.T.: -0.003 min
Response: 1367589023
Conc: 612.97 ng/ml

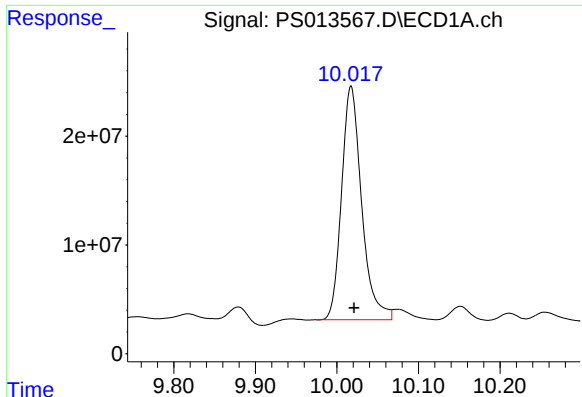

#13 2,4-DB


R.T.: 10.017 min
Delta R.T.: -0.004 min
Response: 367535967
Conc: 400.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

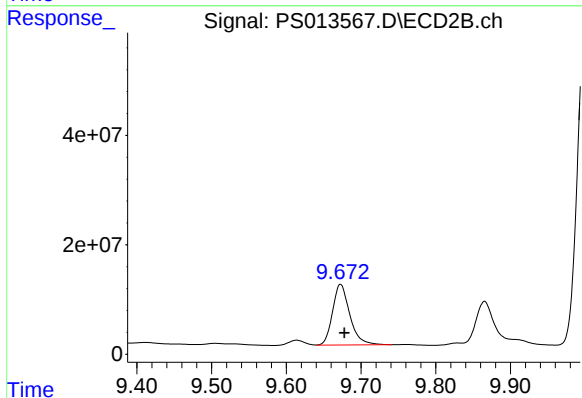


#13 2,4-DB

R.T.: 9.673 min
Delta R.T.: -0.005 min
Response: 177962983
Conc: 608.45 ng/ml

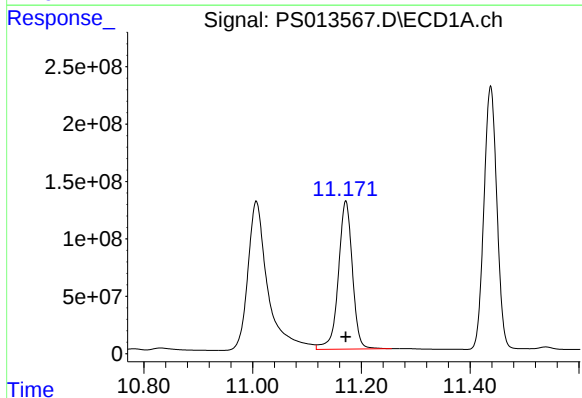


#14 DINOSEB

R.T.: 11.171 min
Delta R.T.: 0.000 min
Response: 2313310956
Conc: 545.87 ng/ml

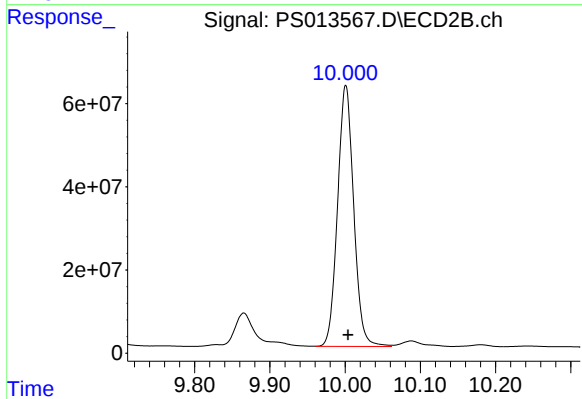

#14 DINOSEB


R.T.: 10.001 min
Delta R.T.: -0.003 min
Response: 936148274
Conc: 566.37 ng/ml

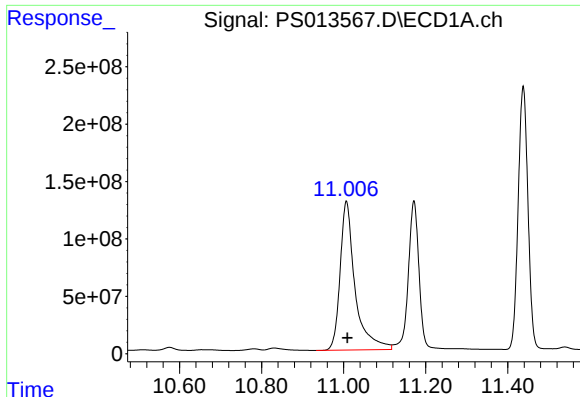

#15 Picloram


R.T.: 11.007 min
Delta R.T.: -0.002 min
Response: 3281613679
Conc: 476.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

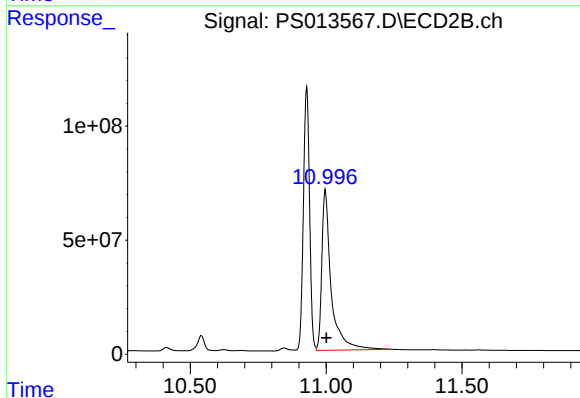


#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.005 min
Response: 1695991934
Conc: 487.11 ng/ml

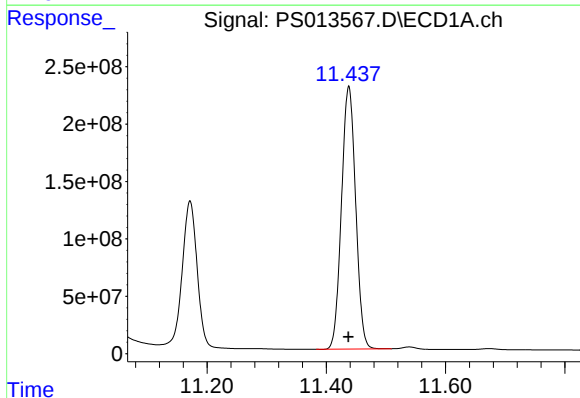

#16 DCPA

R.T.: 11.438 min
Delta R.T.: 0.000 min
Response: 3775354192
Conc: 556.70 ng/ml

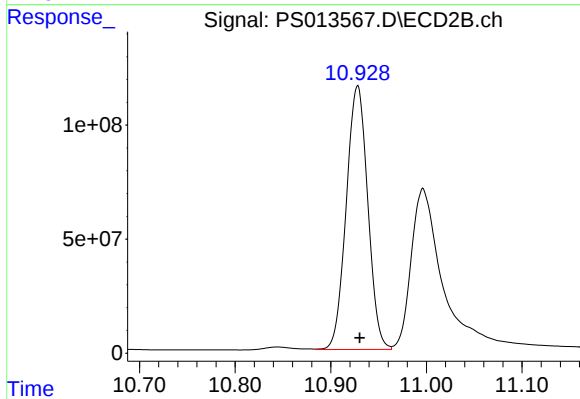

#16 DCPA

R.T.: 10.928 min
Delta R.T.: -0.002 min
Response: 1814710645
Conc: 596.70 ng/ml