

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122121\
 Data File : PS017786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2021 09:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 15:27:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.127	6.714	778.2E6	336.2E6	497.879	563.992
Target Compounds							
2) T	3,5-DICHL...	6.391	0.000	184.6E6	0	82.617	N.D. #
5) T	DICAMBA	7.316	6.931f	10507161	49824807	1.662	18.703 #
6) T	MCP	0.000	6.931f	0	49824807	N.D.	22.891
9) T	2,4-D	8.297f	0.000	260.6E6	0	147.427	N.D. #
11) T	2,4,5-TP ...	9.095	0.000	5725113	0	<MDL	N.D. #
12) T	2,4,5-T	9.406	0.000	21872964	0	2.514	N.D. #
14) T	DINOSEB	11.065	0.000	24375629	0	3.565	N.D. #
15) T	Picloram	10.878	10.779	22913937	59280111	2.112	12.070 #
16) T	DCPA	11.332	0.000	8172026	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122121\
Data File : PS017786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2021 09:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 15:27:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

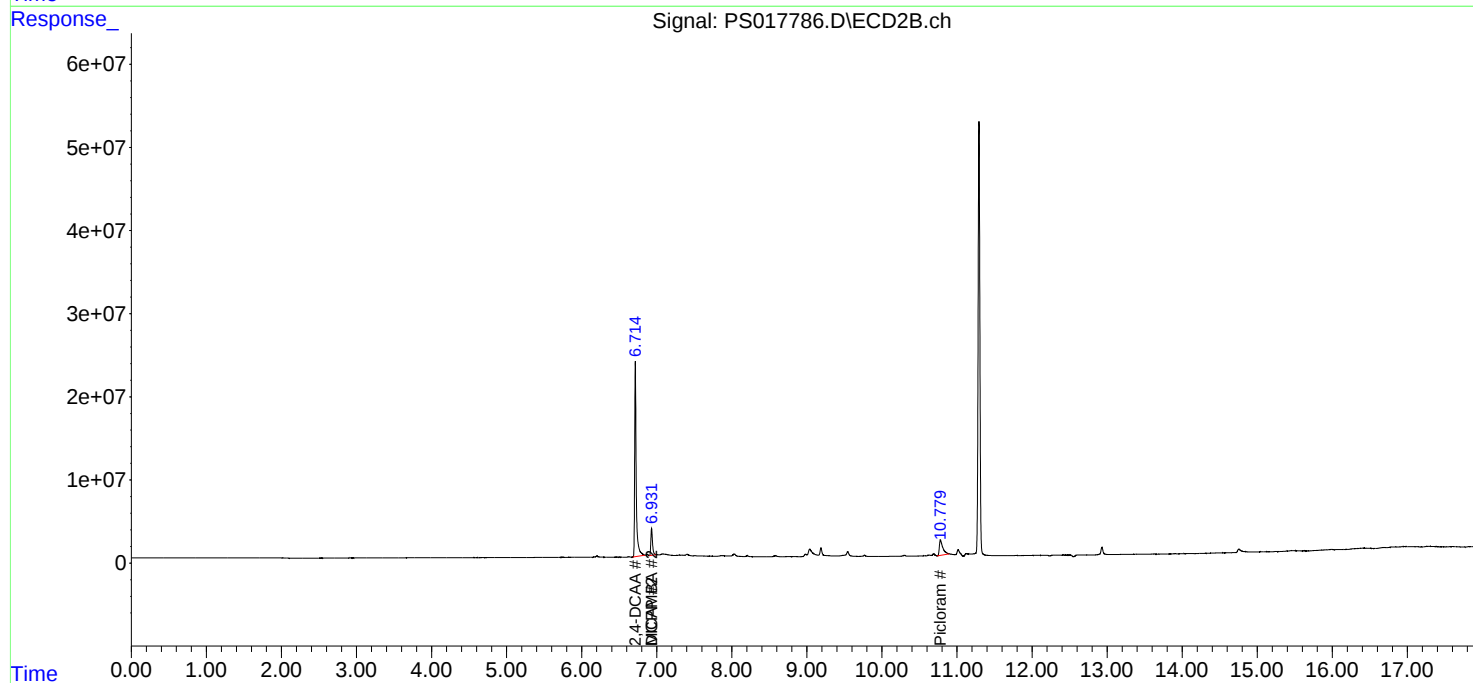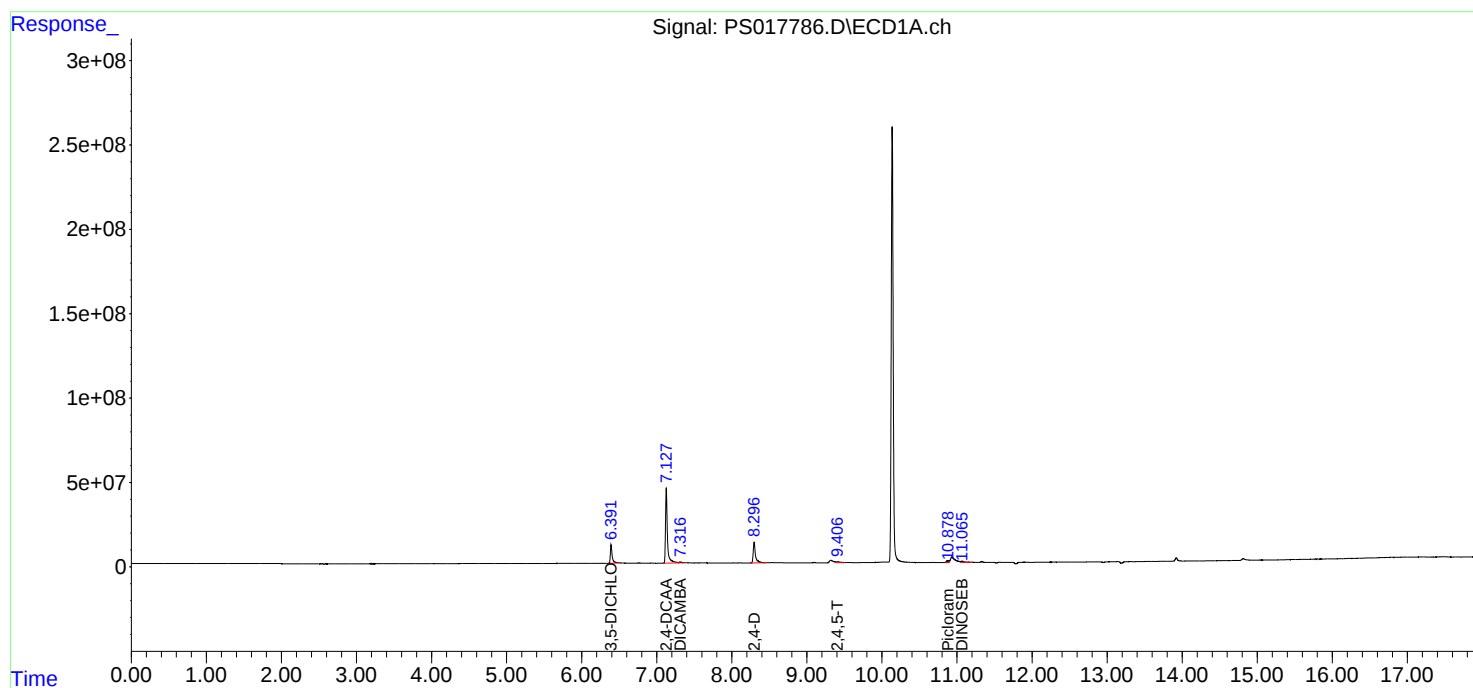


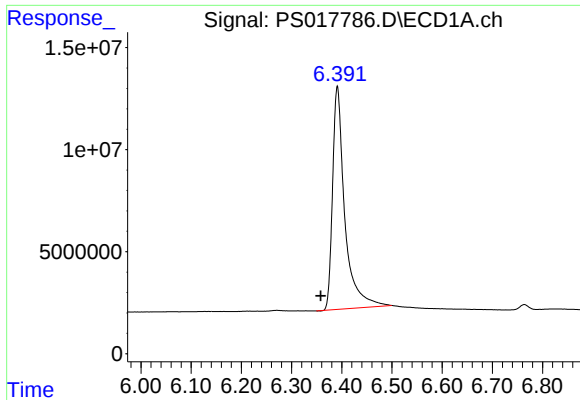

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.391 min
Delta R.T.: 0.033 min
Response: 184579050
Conc: 82.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

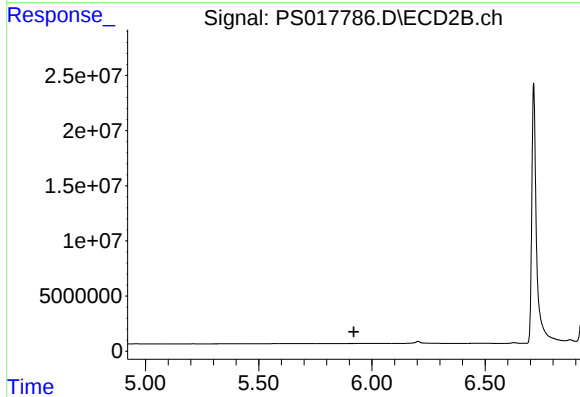


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

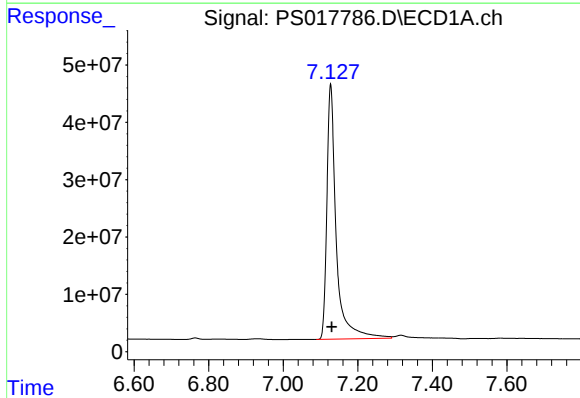


#4 2,4-DCAA

R.T.: 7.127 min
Delta R.T.: -0.003 min
Response: 778157184
Conc: 497.88 ng/ml

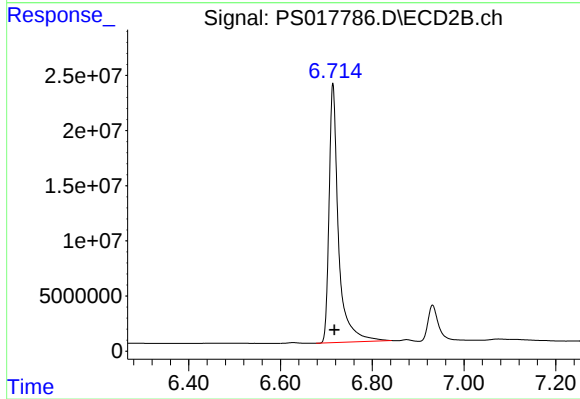

#4 2,4-DCAA


R.T.: 6.714 min
Delta R.T.: -0.003 min
Response: 336196509
Conc: 563.99 ng/ml

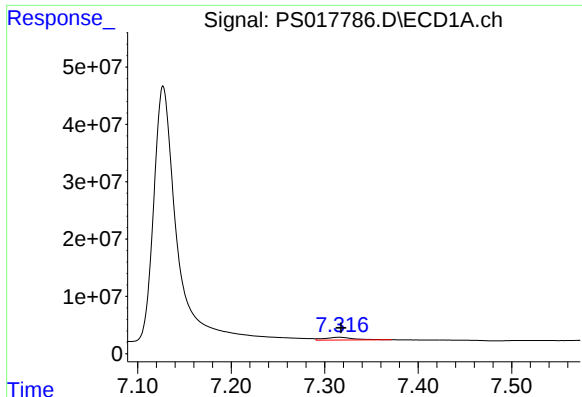

#5 DICAMBA


R.T.: 7.316 min
Delta R.T.: -0.001 min
Response: 10507161
Conc: 1.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

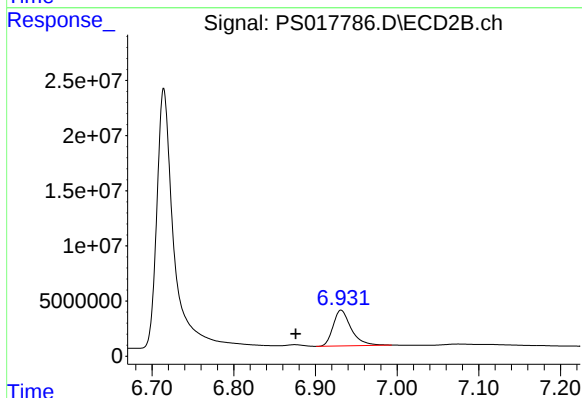


#5 DICAMBA

R.T.: 6.931 min
Delta R.T.: 0.056 min
Response: 49824807
Conc: 18.70 ng/ml

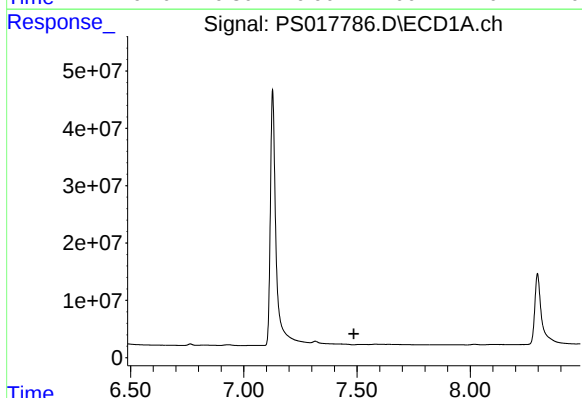


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

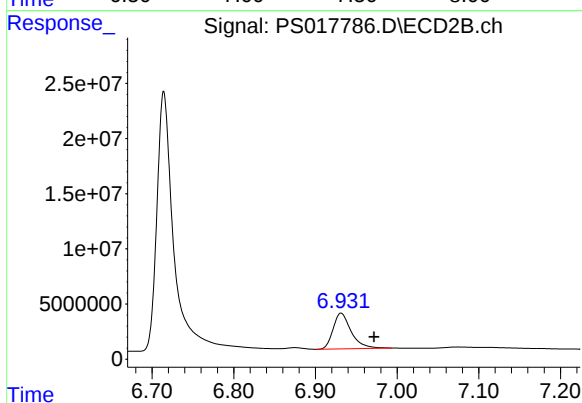

#6 MCP


R.T.: 6.931 min
Delta R.T.: -0.040 min
Response: 49824807
Conc: 22.89 ug/ml

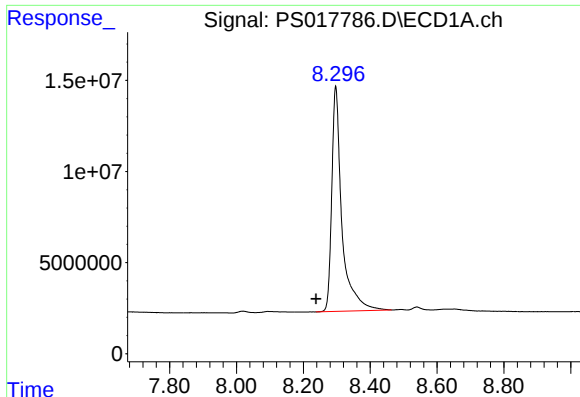

#9 2,4-D


R.T.: 8.297 min
Delta R.T.: 0.058 min
Response: 260632335
Conc: 147.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

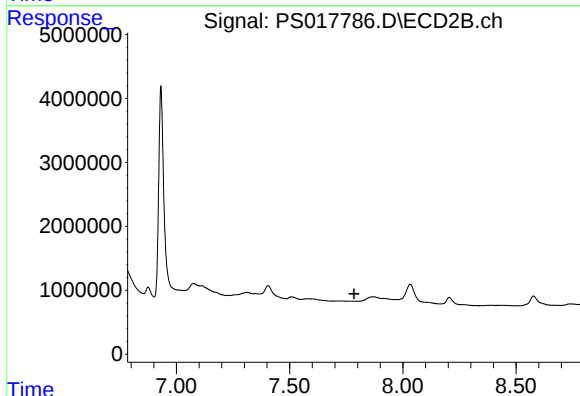


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

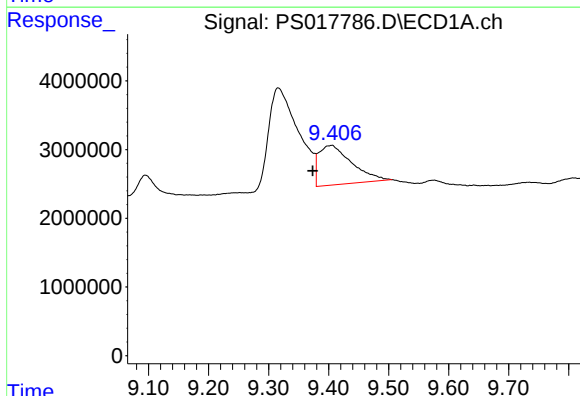


#12 2,4,5-T

R.T.: 9.406 min
Delta R.T.: 0.032 min
Response: 21872964
Conc: 2.51 ng/ml

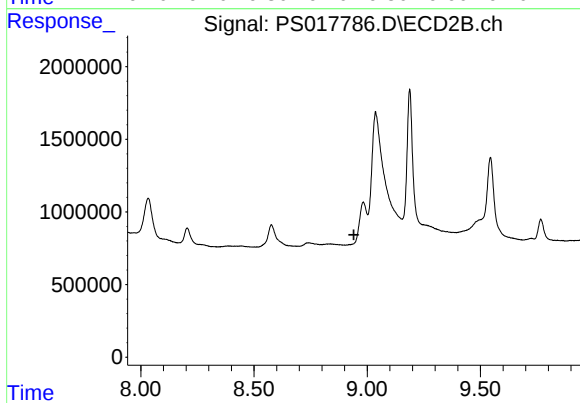

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

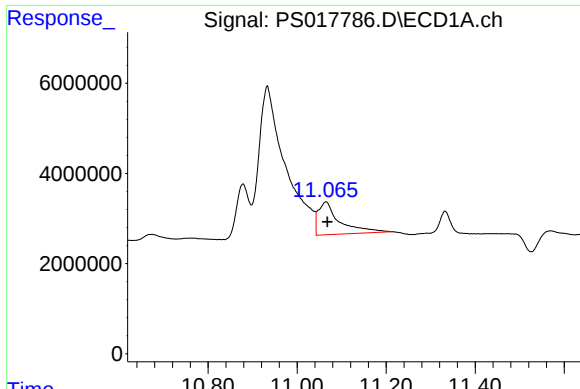

#14 DINOSEB


R.T.: 11.065 min
Delta R.T.: -0.003 min
Response: 24375629
Conc: 3.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

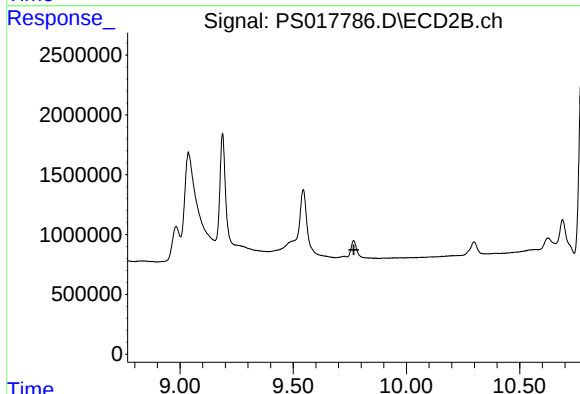


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

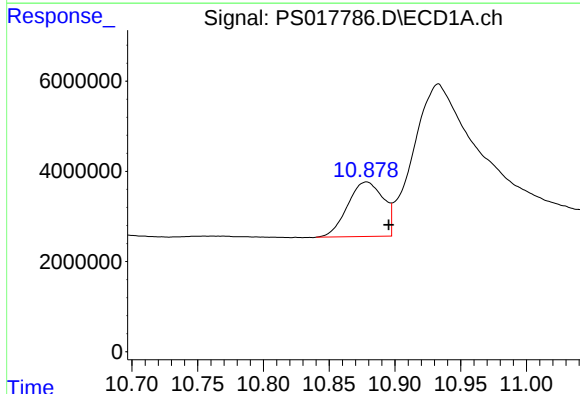

#15 Picloram

R.T.: 10.878 min
Delta R.T.: -0.017 min
Response: 22913937
Conc: 2.11 ng/ml

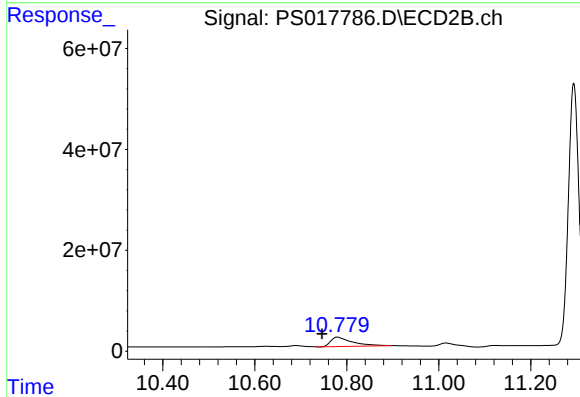

#15 Picloram

R.T.: 10.779 min
Delta R.T.: 0.032 min
Response: 59280111
Conc: 12.07 ng/ml