

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122121\
 Data File : PS017796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2021 15:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 16:44:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.128	6.716	845.4E6	356.9E6	540.881	598.772
Target Compounds							
2) T	3,5-DICHL...	6.394	0.000	114.0E6	0	51.041	N.D. #
5) T	DICAMBA	7.317	6.934f	12941869	34299096	2.047	12.875 #
6) T	MCP	0.000	6.934	0	34299096	N.D.	15.758
9) T	2,4-D	8.301f	0.000	242.4E6	0	137.092	N.D. #
10) T	Pentachlo...	8.541	0.000	11226482	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.100	0.000	7214928	0	<MDL	N.D. #
12) T	2,4,5-T	9.424f	0.000	15951059	0	1.834	N.D. #
14) T	DINOSEB	11.067	0.000	8637203	0	1.263	N.D. #
15) T	Picloram	10.886	0.000	28145970	0	2.594	N.D. #
16) T	DCPA	11.334	0.000	14787073	0	1.362	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122121\
Data File : PS017796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2021 15:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 16:44:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

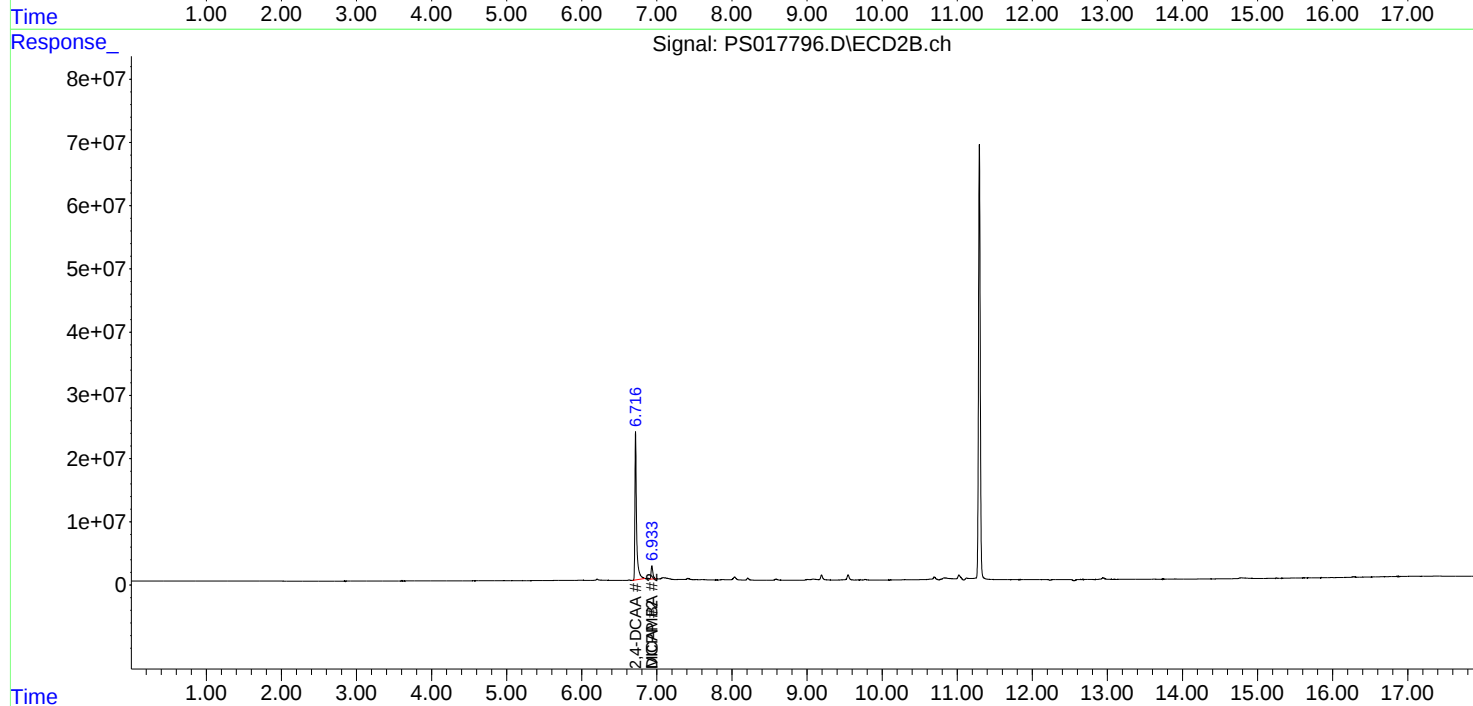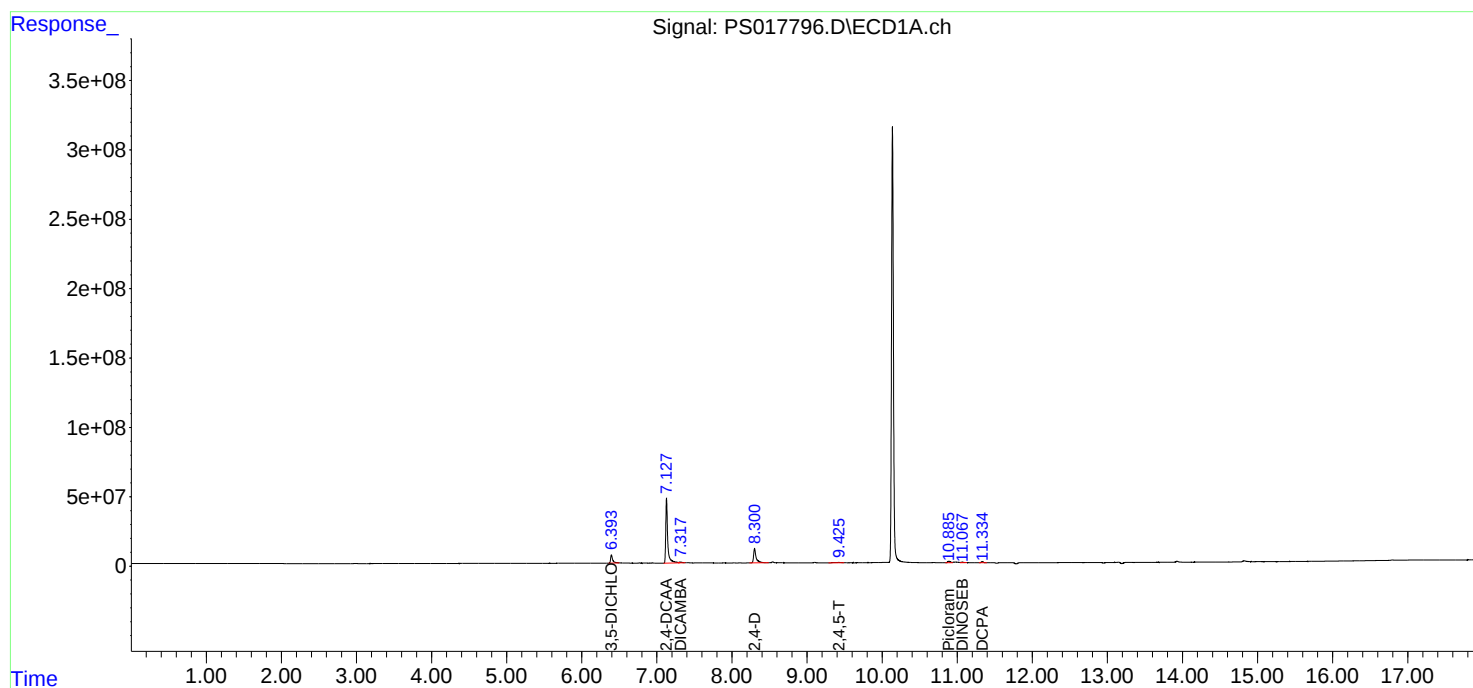


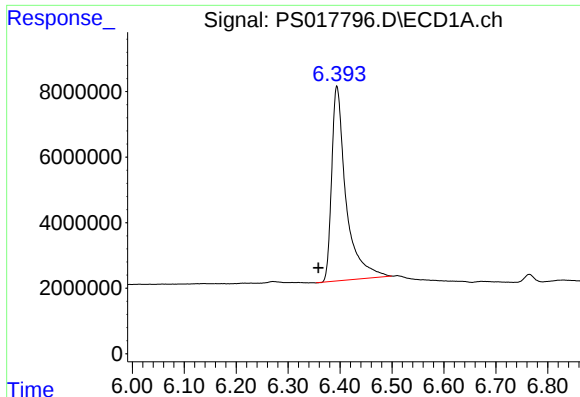

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.394 min
Delta R.T.: 0.036 min
Response: 114032942
Conc: 51.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

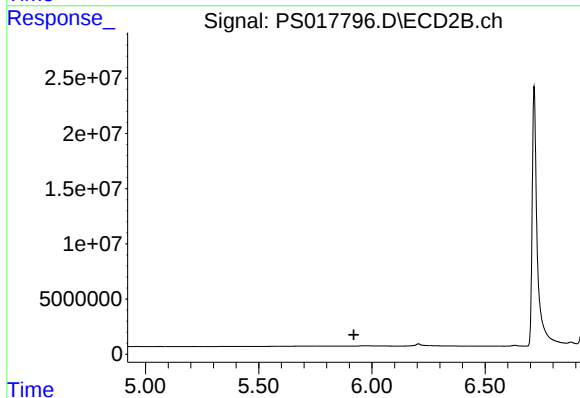


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.921 min
Response: 0
Conc: N.D.

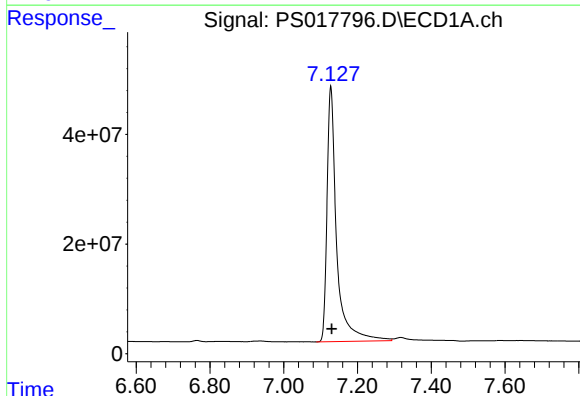


#4 2,4-DCAA

R.T.: 7.128 min
Delta R.T.: -0.002 min
Response: 845367067
Conc: 540.88 ng/ml

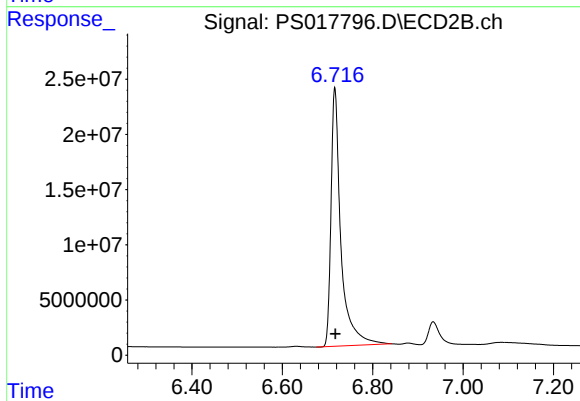

#4 2,4-DCAA


R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 356928986
Conc: 598.77 ng/ml

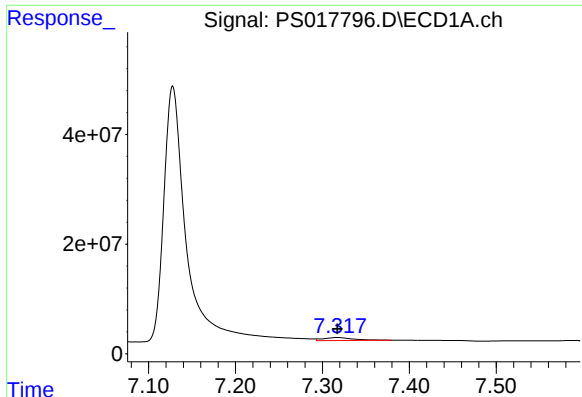

#5 DICAMBA


R.T.: 7.317 min
Delta R.T.: 0.000 min
Response: 12941869
Conc: 2.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

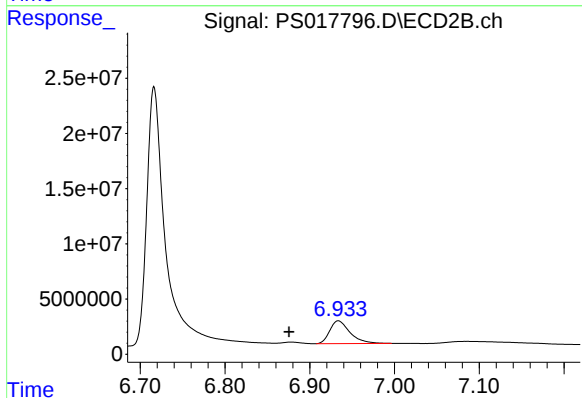


#5 DICAMBA

R.T.: 6.934 min
Delta R.T.: 0.058 min
Response: 34299096
Conc: 12.88 ng/ml

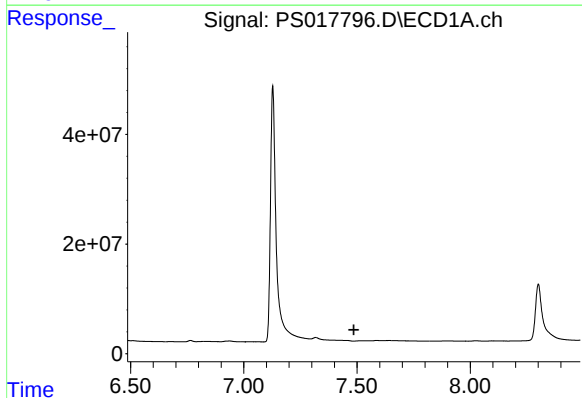


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

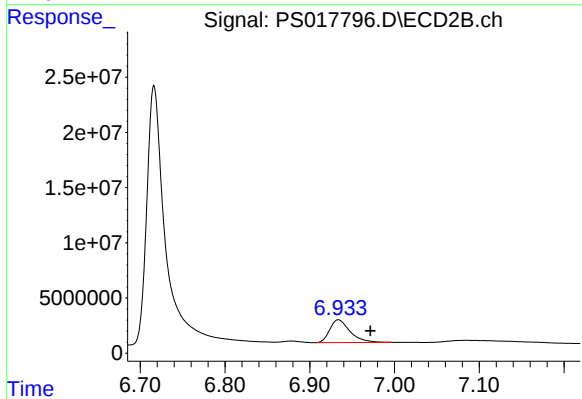

#6 MCPP


R.T.: 6.934 min
Delta R.T.: -0.038 min
Response: 34299096
Conc: 15.76 ug/ml

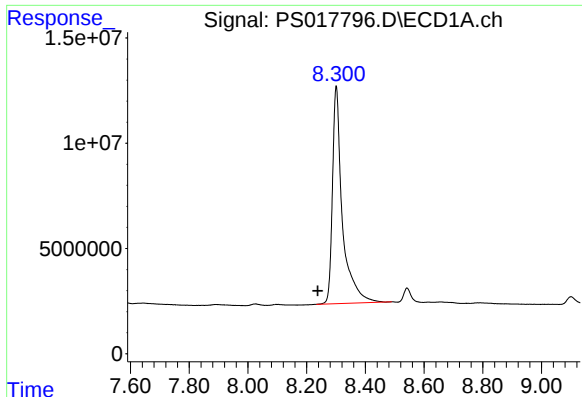

#9 2,4-D


R.T.: 8.301 min
Delta R.T.: 0.062 min
Response: 242362215
Conc: 137.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

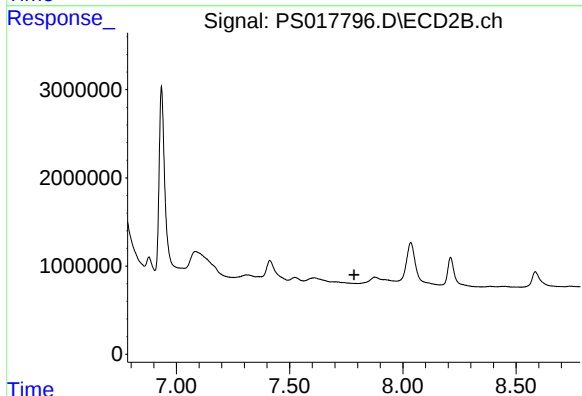


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.784 min
Response: 0
Conc: N.D.

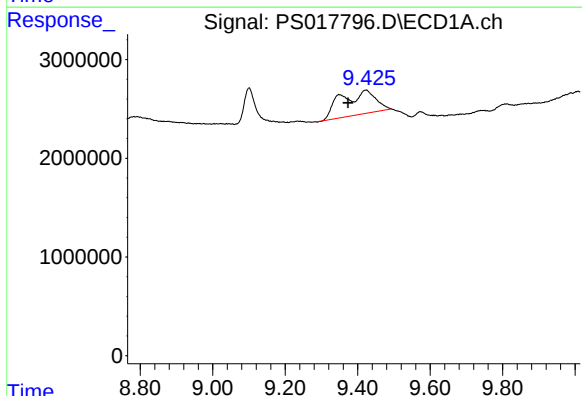


#12 2,4,5-T

R.T.: 9.424 min
Delta R.T.: 0.051 min
Response: 15951059
Conc: 1.83 ng/ml

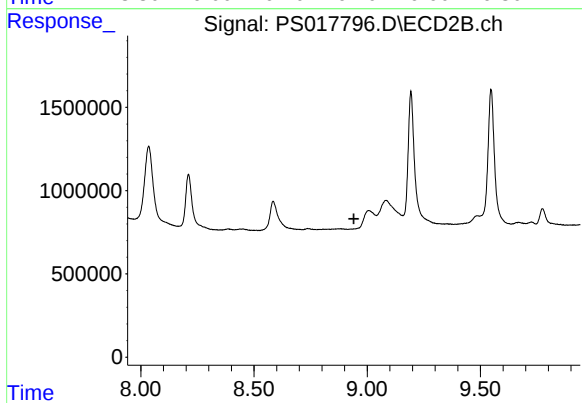

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

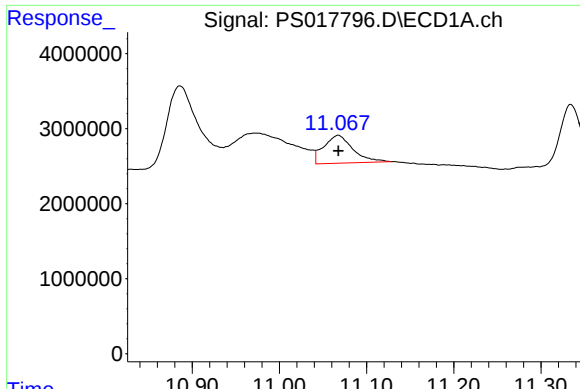

#14 DINOSEB


R.T.: 11.067 min
Delta R.T.: 0.000 min
Response: 8637203
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

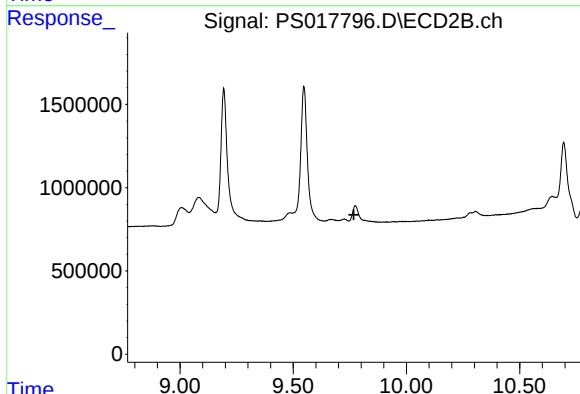


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.768 min
Response: 0
Conc: N.D.

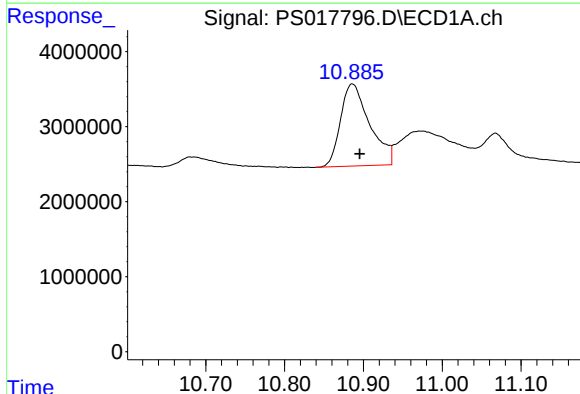


#15 Picloram

R.T.: 10.886 min
Delta R.T.: -0.009 min
Response: 28145970
Conc: 2.59 ng/ml

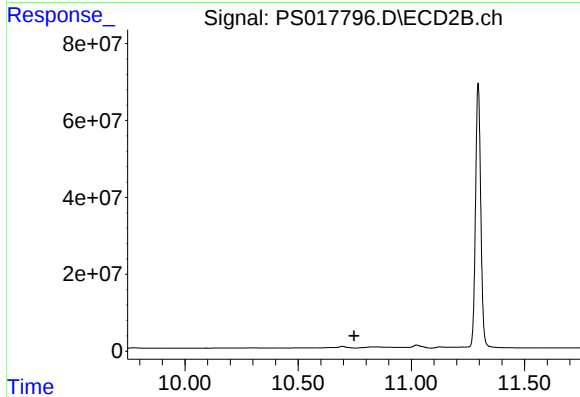

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 10.747 min
Response: 0
Conc: N.D.

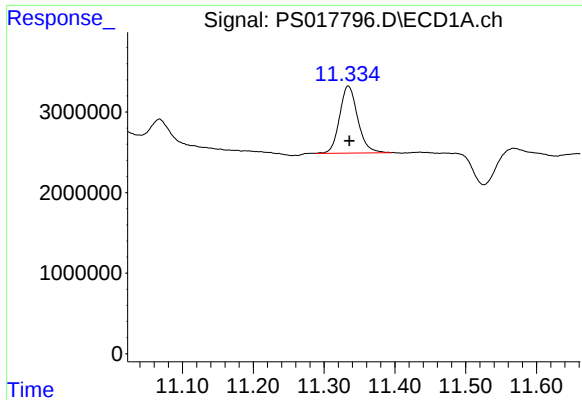

#16 DCPA

R.T.: 11.334 min
Delta R.T.: -0.002 min
Response: 14787073
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

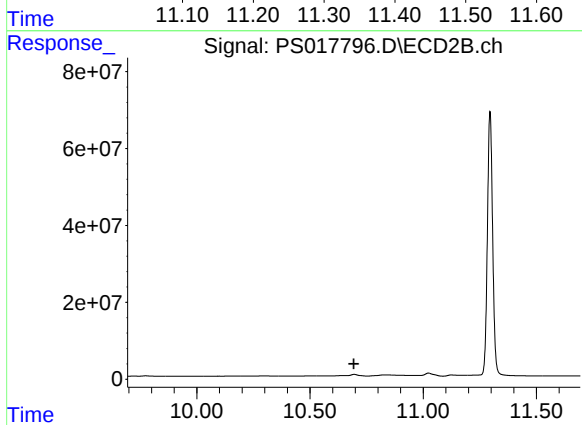

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.694 min
Response: 0
Conc: N.D.